

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX081522\
 Data File : VX030632.D
 Acq On : 15 Aug 2022 16:58
 Operator : JC/MD
 Sample : N4168-05
 Misc : 11.00g/5mL/100uL/5.00mL/MSVOA_X/MEOH
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 EX9B4

Quant Time: Aug 16 04:31:50 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML080422WMA.M
 Quant Title : VOC Analysis
 QLast Update : Tue Aug 16 04:27:08 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	6.763	114	358653	50.000	ug/L	0.00
28) Chlorobenzene-d5	10.055	117	315458	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	12.030	152	134299	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.367	65	95294	41.374	ug/L	0.00
Spiked Amount	50.000	Range	60 - 135	Recovery	=	82.740%
7) Chloroethane-d5	1.666	69	49890	30.727	ug/L	0.00
Spiked Amount	50.000	Range	70 - 130	Recovery	=	61.460%#
11) 1,1-Dichloroethene-d2	2.276	63	161573	37.086	ug/L	-0.03
Spiked Amount	50.000	Range	60 - 125	Recovery	=	74.180%
21) 2-Butanone-d5	4.513	46	163816	76.763	ug/L	0.04
Spiked Amount	100.000	Range	40 - 130	Recovery	=	76.760%
24) Chloroform-d	5.068	84	206269	43.505	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	87.020%
26) 1,2-Dichloroethane-d4	5.958	65	146238	45.425	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	90.860%
32) Benzene-d6	5.970	84	416519	46.095	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	92.180%
36) 1,2-Dichloropropane-d6	7.312	67	133608	45.573	ug/L	0.00
Spiked Amount	50.000	Range	70 - 120	Recovery	=	91.140%
41) Toluene-d8	8.653	98	375689	44.107	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	88.220%
43) trans-1,3-Dichloroprop...	8.951	79	55894	38.323	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	76.640%
47) 2-Hexanone-d5	9.403	63	110846	74.176	ug/L	0.02
Spiked Amount	100.000	Range	45 - 130	Recovery	=	74.180%
56) 1,1,2,2-Tetrachloroeth...	11.201	84	152807	39.676	ug/L	0.00
Spiked Amount	50.000	Range	65 - 120	Recovery	=	79.360%
66) 1,2-Dichlorobenzene-d4	12.323	152	111684	42.875	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	85.760%
Target Compounds						Qvalue
6) Bromomethane	1.611	94	1158	0.994	ug/L	90


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX081522\
Data File : VX030632.D
Acq On : 15 Aug 2022 16:58
Operator : JC/MD
Sample : N4168-05
Misc : 11.00g/5mL/100uL/5.00mL/MSVOA_X/MEOH
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
EX9B4

Quant Time: Aug 16 04:31:50 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML080422WMA.M
Quant Title : VOC Analysis
QLast Update : Tue Aug 16 04:27:08 2022
Response via : Initial Calibration

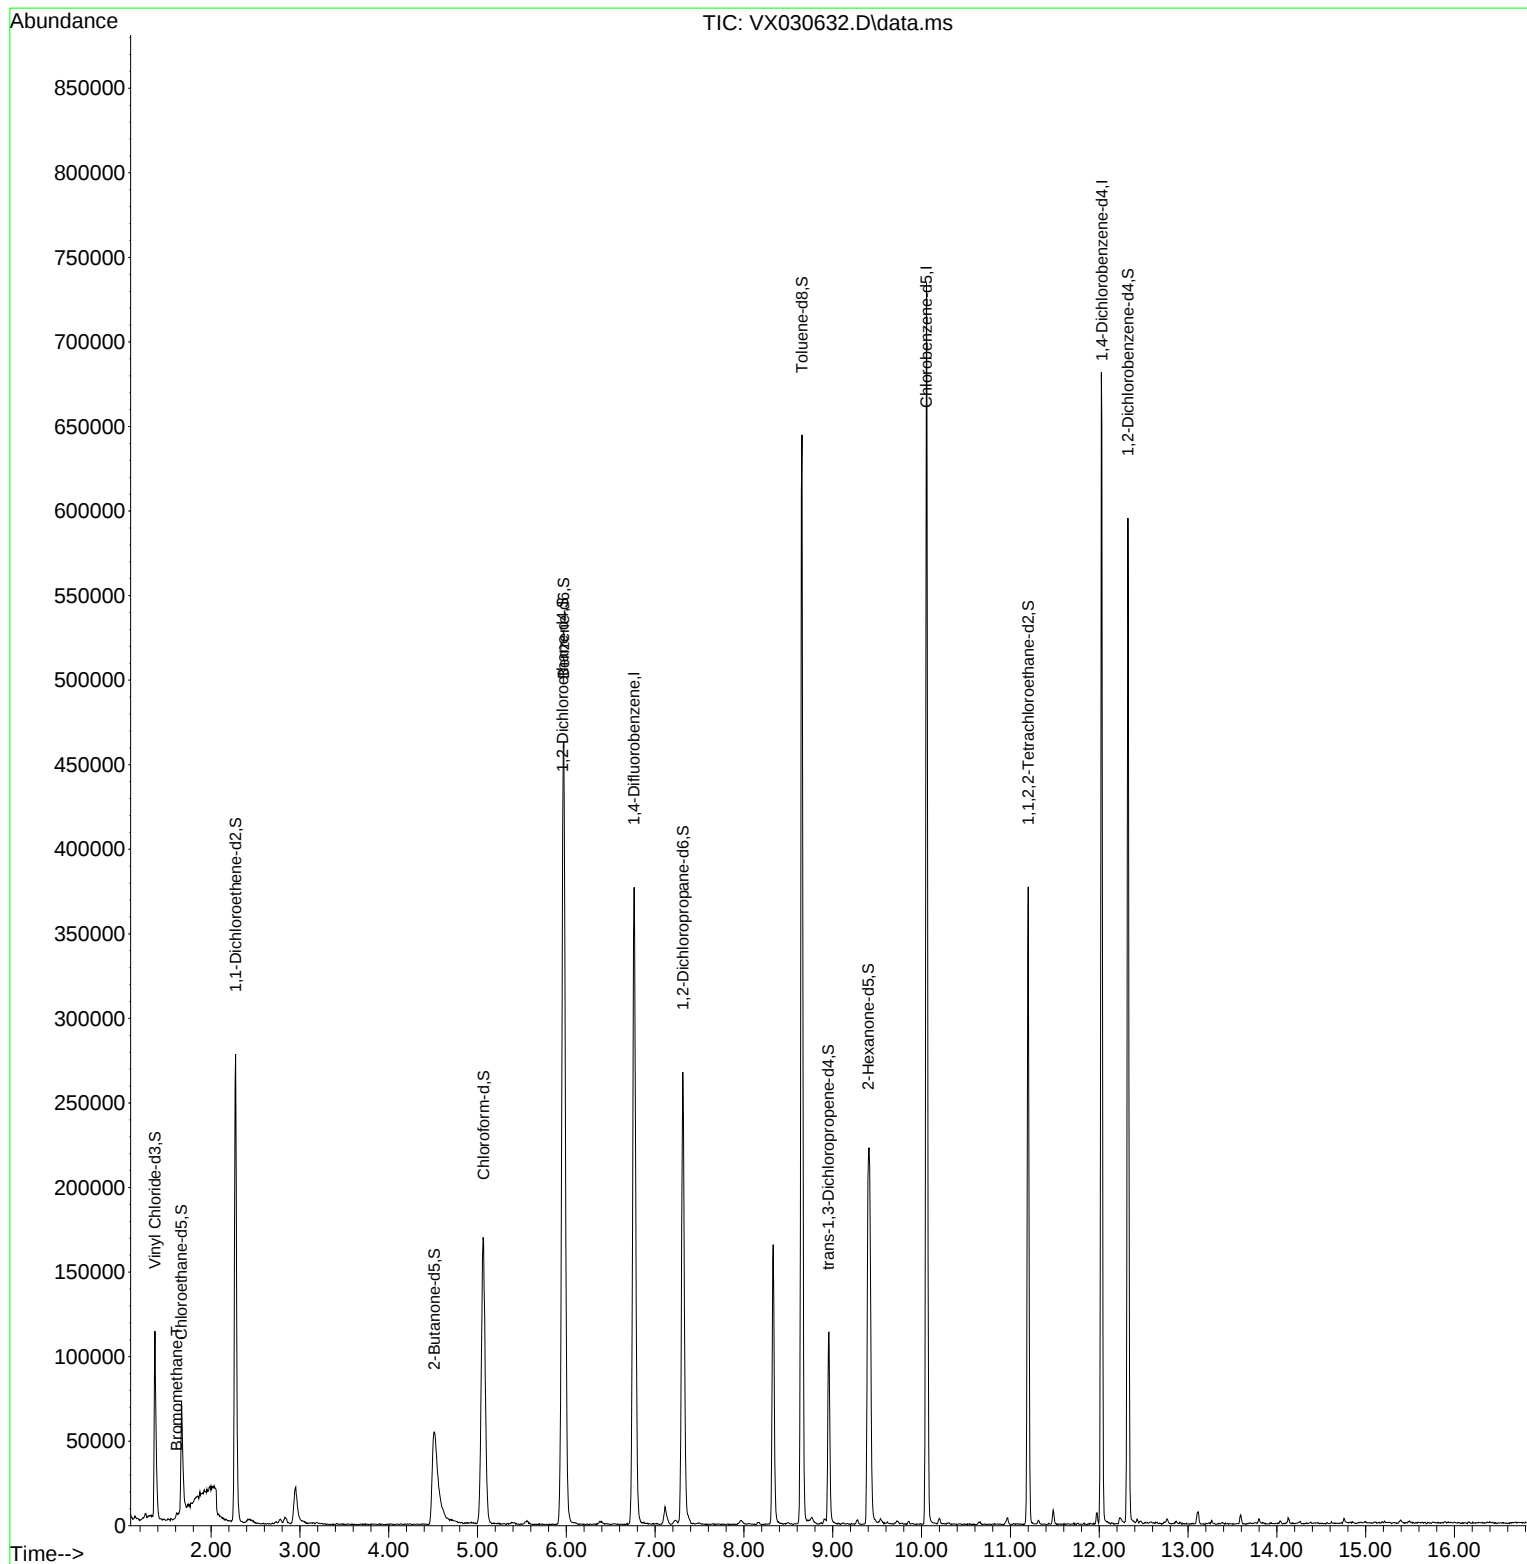

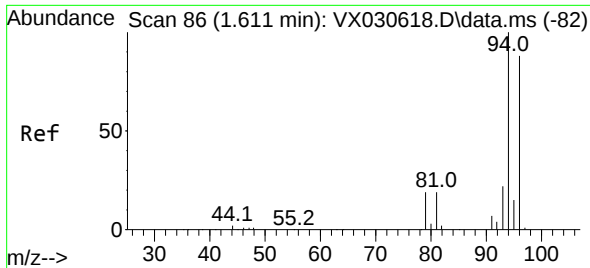

#6
 Bromomethane
 Concen: 0.994 ug/L
 RT: 1.611 min Scan# 80
 Delta R.T. -0.000 min
 Lab File: VX030632.D
 Acq: 15 Aug 2022 16:58

Instrument :
 MSVOA_X
 ClientSampleId :
 EX9B4

Tgt Ion: 94 Resp: 1158
 Ion Ratio Lower Upper
 94 100
 96 101.1 63.8 118.6

