

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX081522\
 Data File : VX030634.D
 Acq On : 15 Aug 2022 18:32
 Operator : JC/MD
 Sample : N4168-10
 Misc : 10.61g/5mL/100uL/5.00mL/MSVOA_X/MEOH
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 EX9B7

Quant Time: Aug 16 04:32:16 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML080422WMA.M
 Quant Title : VOC Analysis
 QLast Update : Tue Aug 16 04:27:08 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	6.763	114	285442	50.000	ug/L	0.00
28) Chlorobenzene-d5	10.055	117	248979	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	12.024	152	110499	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.368	65	90523	49.384	ug/L	0.00
Spiked Amount	50.000	Range	60 - 135	Recovery	=	98.760%
7) Chloroethane-d5	1.654	69	35061	27.133	ug/L	-0.02
Spiked Amount	50.000	Range	70 - 130	Recovery	=	54.260%#
11) 1,1-Dichloroethene-d2	2.270	63	156536	45.145	ug/L	-0.04
Spiked Amount	50.000	Range	60 - 125	Recovery	=	90.280%
21) 2-Butanone-d5	4.507	46	168203	99.035	ug/L	0.04
Spiked Amount	100.000	Range	40 - 130	Recovery	=	99.030%
24) Chloroform-d	5.062	84	195590	51.834	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	103.660%
26) 1,2-Dichloroethane-d4	5.958	65	139512	54.451	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	108.900%
32) Benzene-d6	5.971	84	395086	55.397	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	110.800%
36) 1,2-Dichloropropane-d6	7.312	67	127298	55.014	ug/L	0.00
Spiked Amount	50.000	Range	70 - 120	Recovery	=	110.020%
41) Toluene-d8	8.653	98	358266	53.293	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	106.580%
43) trans-1,3-Dichloroprop...	8.952	79	54194	47.079	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	94.160%
47) 2-Hexanone-d5	9.403	63	111288	94.356	ug/L	0.02
Spiked Amount	100.000	Range	45 - 130	Recovery	=	94.360%
56) 1,1,2,2-Tetrachloroeth...	11.201	84	149652	49.232	ug/L	0.00
Spiked Amount	50.000	Range	65 - 120	Recovery	=	98.460%
66) 1,2-Dichlorobenzene-d4	12.323	152	120065	56.020	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	112.040%
Target Compounds						Qvalue
44) trans-1,3-Dichloropropene	8.952	75	2551	0.823	ug/L	90


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX081522\
Data File : VX030634.D
Acq On : 15 Aug 2022 18:32
Operator : JC/MD
Sample : N4168-10
Misc : 10.61g/5mL/100uL/5.00mL/MSVOA_X/MEOH
ALS Vial : 20 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
EX9B7

Quant Time: Aug 16 04:32:16 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM080422WMA.M
Quant Title : VOC Analysis
QLast Update : Tue Aug 16 04:27:08 2022
Response via : Initial Calibration

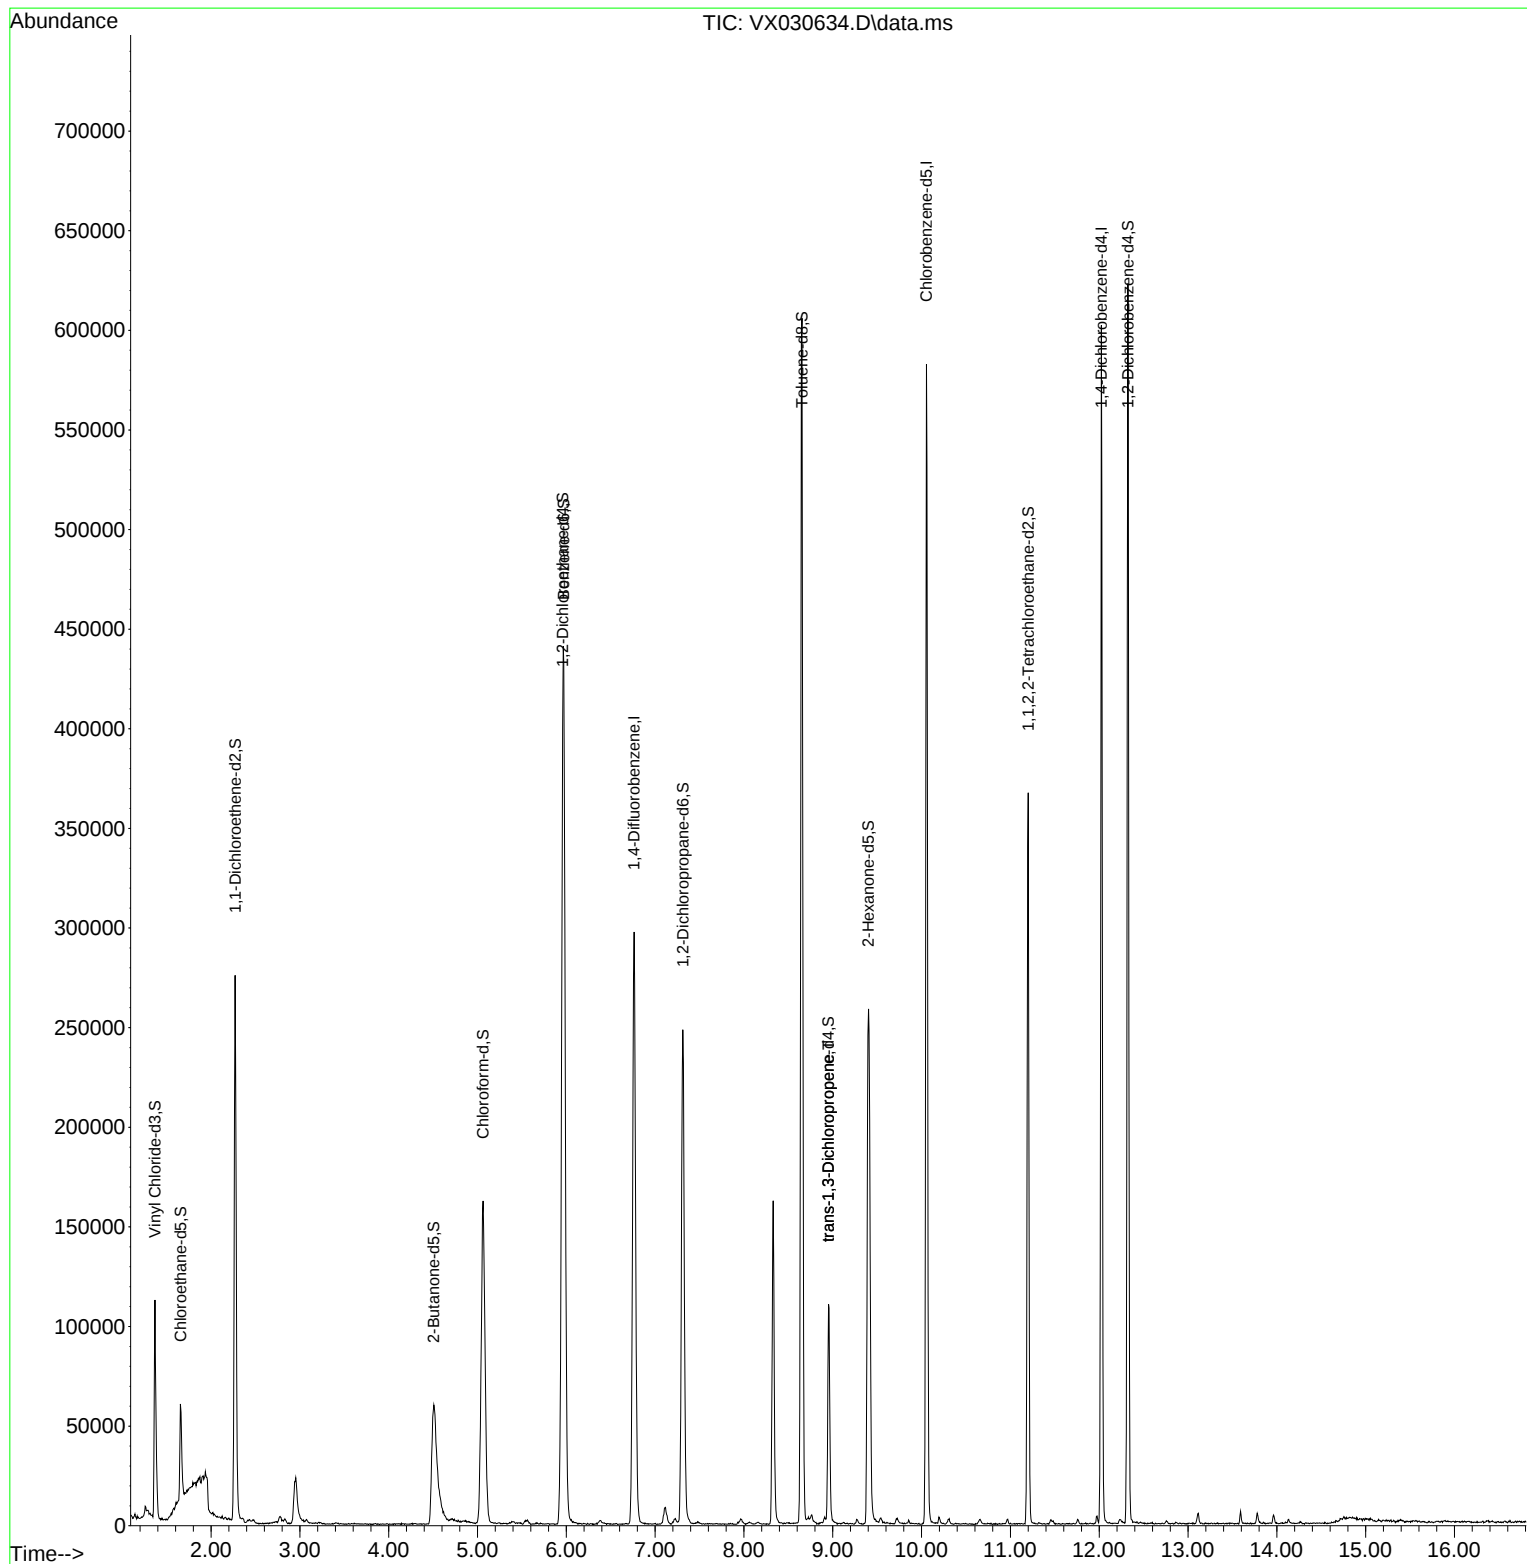

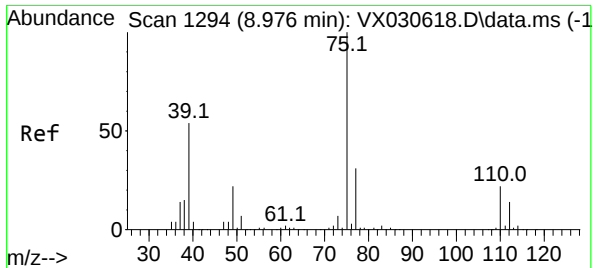

#44

trans-1,3-Dichloropropene

Concen: 0.823 ug/L

RT: 8.952 min Scan# 11

Delta R.T. -0.024 min

Lab File: VX030634.D


Acq: 15 Aug 2022 18:32

Instrument :

MSVOA_X

ClientSampleId :

EX9B7

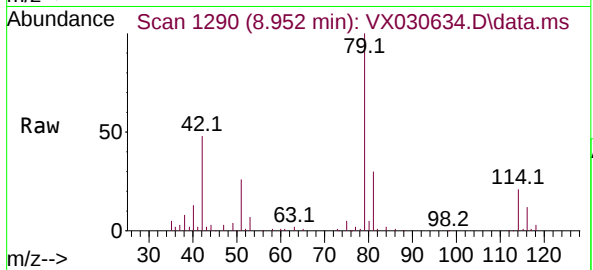

Tgt Ion: 75 Resp: 2551

Ion Ratio Lower Upper

75 100

77 37.6 22.5 41.7

