

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX081522\
 Data File : VX030636.D
 Acq On : 15 Aug 2022 19:18
 Operator : JC/MD
 Sample : N4168-12
 Misc : 11.27g/5mL/100uL/5.00mL/MSVOA_X/MEOH
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 EX9B9

Quant Time: Aug 16 04:32:40 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML080422WMA.M
 Quant Title : VOC Analysis
 QLast Update : Tue Aug 16 04:27:08 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	6.763	114	305766	50.000	ug/L	0.00
28) Chlorobenzene-d5	10.055	117	263911	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	12.030	152	120755	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.368	65	66139	33.683	ug/L	0.00
Spiked Amount	50.000	Range	60 - 135	Recovery	=	67.360%
7) Chloroethane-d5	1.654	69	24862	17.961	ug/L	-0.02
Spiked Amount	50.000	Range	70 - 130	Recovery	=	35.920%#
11) 1,1-Dichloroethene-d2	2.270	63	108075	29.097	ug/L	-0.04
Spiked Amount	50.000	Range	60 - 125	Recovery	=	58.200%#
21) 2-Butanone-d5	4.501	46	111455	61.261	ug/L	0.03
Spiked Amount	100.000	Range	40 - 130	Recovery	=	61.260%
24) Chloroform-d	5.062	84	136143	33.681	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	67.360%#
26) 1,2-Dichloroethane-d4	5.958	65	97414	35.493	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	70.980%
32) Benzene-d6	5.970	84	272925	36.103	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	72.200%
36) 1,2-Dichloropropane-d6	7.312	67	87099	35.512	ug/L	0.00
Spiked Amount	50.000	Range	70 - 120	Recovery	=	71.020%
41) Toluene-d8	8.653	98	246496	34.592	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	69.180%#
43) trans-1,3-Dichloroprop...	8.958	79	34339	28.143	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	56.280%#
47) 2-Hexanone-d5	9.409	63	71936	57.541	ug/L	0.02
Spiked Amount	100.000	Range	45 - 130	Recovery	=	57.540%
56) 1,1,2,2-Tetrachloroeth...	11.201	84	102413	31.785	ug/L	0.00
Spiked Amount	50.000	Range	65 - 120	Recovery	=	63.580%#
66) 1,2-Dichlorobenzene-d4	12.323	152	78335	33.445	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	66.900%#
Target Compounds						Qvalue
37) 1,2-Dichloropropane	7.312	63	10290	4.574	ug/L	# 89


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX081522\
Data File : VX030636.D
Acq On : 15 Aug 2022 19:18
Operator : JC/MD
Sample : N4168-12
Misc : 11.27g/5mL/100uL/5.00mL/MSVOA_X/MEOH
ALS Vial : 22 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
EX9B9

Quant Time: Aug 16 04:32:40 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML080422WMA.M
Quant Title : VOC Analysis
QLast Update : Tue Aug 16 04:27:08 2022
Response via : Initial Calibration

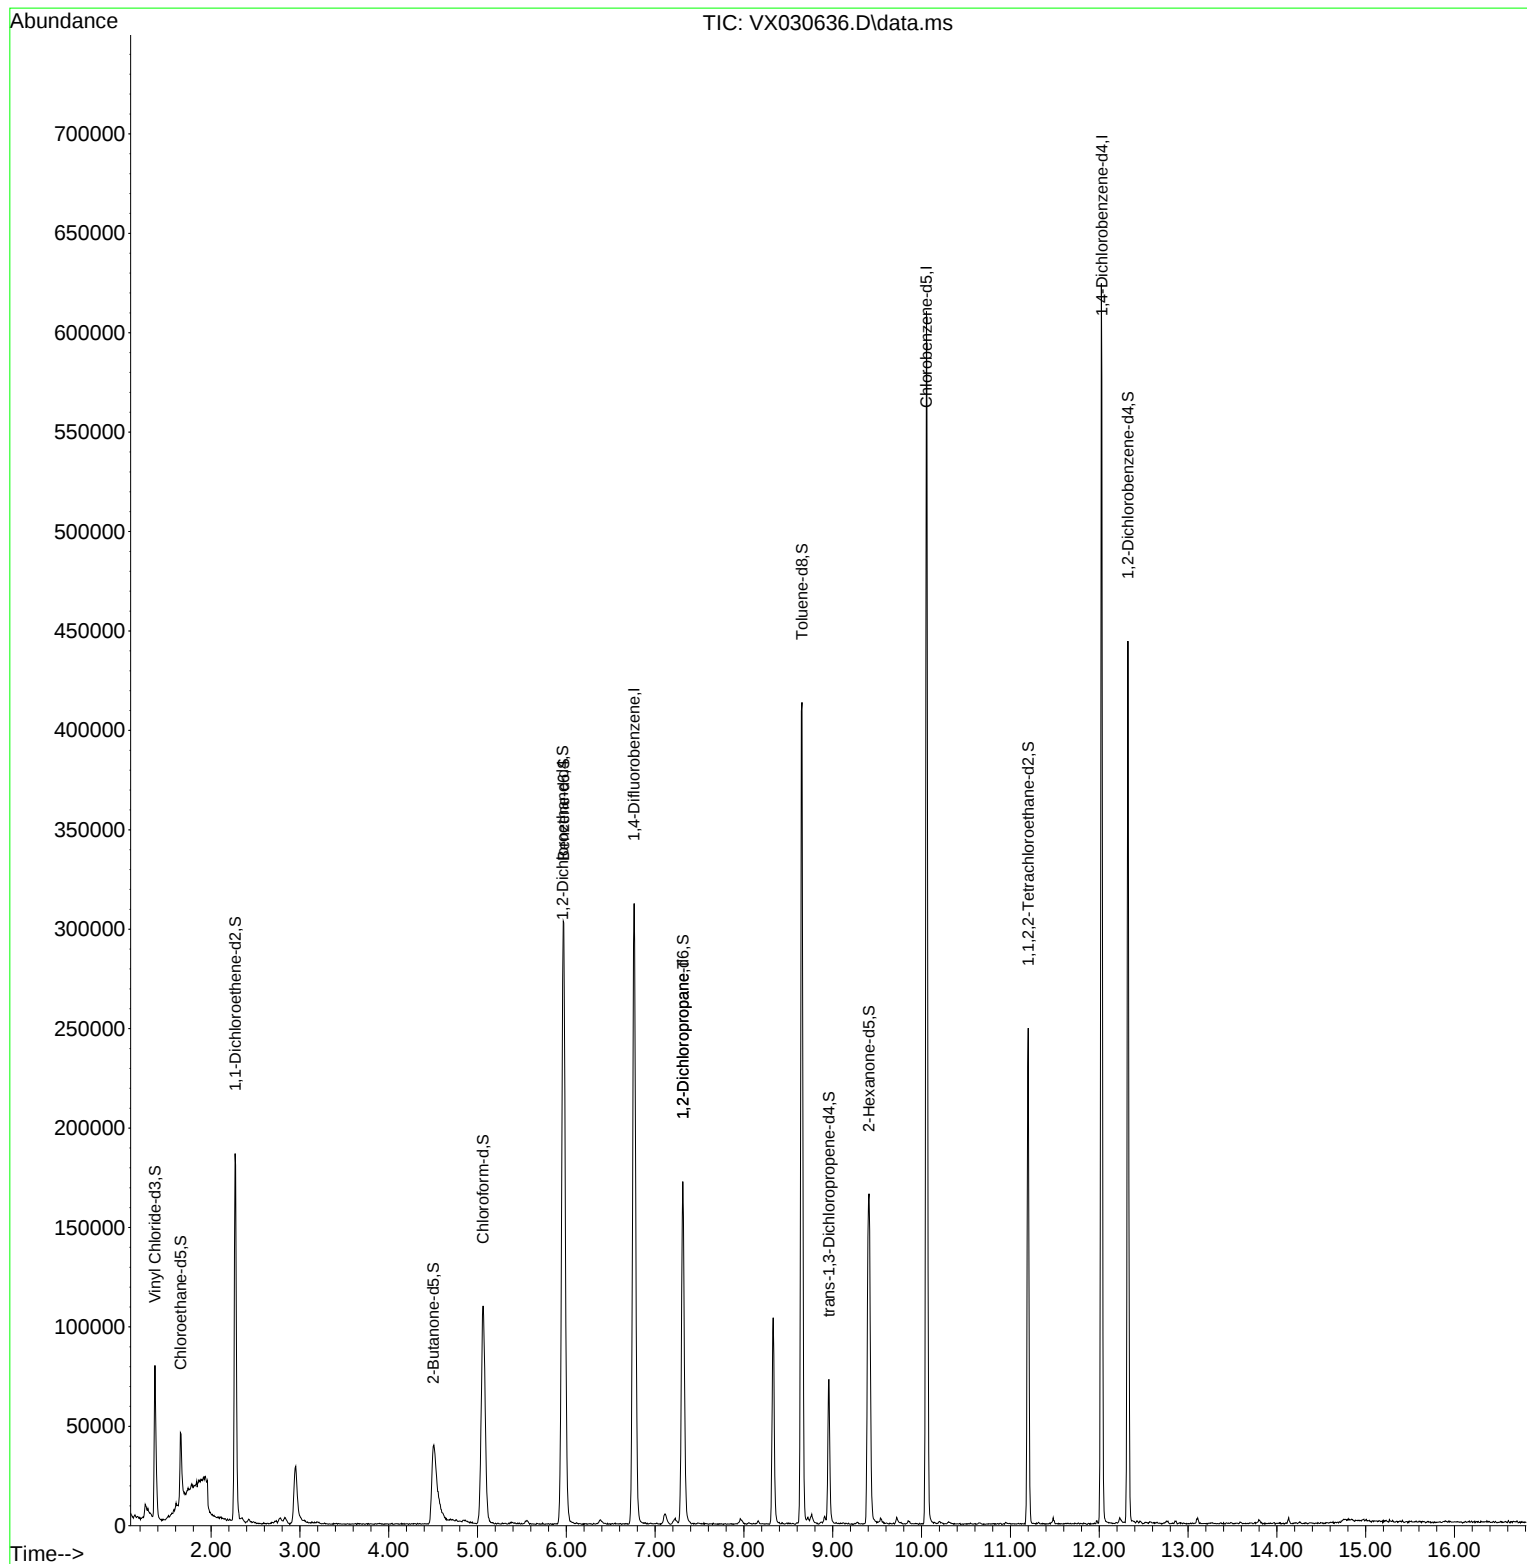

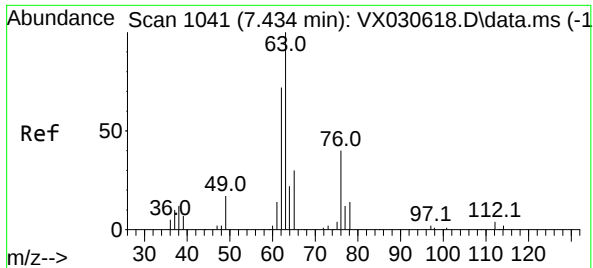

#37
 1,2-Dichloropropane
 Concen: 4.574 ug/L
 RT: 7.312 min Scan# 10
 Delta R.T. -0.122 min
 Lab File: VX030636.D
 Acq: 15 Aug 2022 19:18

Instrument :
 MSVOA_X
 ClientSampleId :
 EX9B9

Tgt Ion: 63 Resp: 10290
 Ion Ratio Lower Upper
 63 100
 112 0.0 3.0 4.4#

