

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX081522\
 Data File : VX030620.D
 Acq On : 15 Aug 2022 11:18
 Operator : JC/MD
 Sample : VX0815WBL01
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VBLK685

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML080422WMA.M
 Title : VOC Analysis

Signal : TIC: VX030620.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.367	43	46	56	rVB	89415	95926	10.11%	1.278%
2	1.672	92	96	103	rBV	83187	96562	10.18%	1.287%
3	2.166	175	177	179	rBV3	842	620	0.07%	0.008%
4	2.306	194	200	212	rBV	168025	267671	28.21%	3.567%
5	2.392	212	214	215	rBV2	612	481	0.05%	0.006%
6	2.562	241	242	245	rBV2	463	446	0.05%	0.006%
7	2.794	274	280	286	rVB4	2231	4400	0.46%	0.059%
8	2.855	286	290	292	rBV2	226	293	0.03%	0.004%
9	2.946	298	305	314	rBV2	13460	32492	3.42%	0.433%
10	3.166	340	341	347	rVB	536	649	0.07%	0.009%
11	3.452	385	388	389	rVB	429	377	0.04%	0.005%
12	3.489	392	394	396	rVV2	433	436	0.05%	0.006%
13	3.666	420	423	425	rBV	454	468	0.05%	0.006%
14	3.745	430	436	437	rBV	536	685	0.07%	0.009%
15	3.806	443	446	449	rVB2	443	362	0.04%	0.005%
16	3.977	472	474	479	rVB	600	836	0.09%	0.011%
17	4.019	479	481	484	rBV2	602	737	0.08%	0.010%
18	4.215	511	513	516	rVB	521	376	0.04%	0.005%
19	4.245	516	518	521	rBV2	325	358	0.04%	0.005%
20	4.355	535	536	539	rBV	589	465	0.05%	0.006%
21	4.471	545	555	569	rBV	95568	291779	30.75%	3.888%
22	4.800	607	609	612	rBV	427	322	0.03%	0.004%
23	5.062	640	652	672	rVV	135295	414503	43.68%	5.524%
24	5.251	681	683	689	rVB2	435	677	0.07%	0.009%
25	5.397	700	707	709	rBV3	1294	3080	0.32%	0.041%
26	5.446	713	715	717	rBV	307	320	0.03%	0.004%
27	5.556	726	733	738	rBV3	1678	4004	0.42%	0.053%
28	5.726	759	761	763	rBV2	383	387	0.04%	0.005%
29	5.976	790	802	819	rVV2	321735	948863	100.00%	12.645%
30	6.214	838	841	842	rVB	369	319	0.03%	0.004%
31	6.232	842	844	846	rBV	256	297	0.03%	0.004%
32	6.300	854	855	858	rBV	333	344	0.04%	0.005%
33	6.367	864	866	870	rVB2	449	397	0.04%	0.005%
34	6.513	888	890	893	rBV2	541	544	0.06%	0.007%
35	6.549	894	896	898	rVV	498	408	0.04%	0.005%
36	6.592	902	903	905	rBV2	378	307	0.03%	0.004%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX081522\
 Data File : VX030620.D
 Acq On : 15 Aug 2022 11:18
 Operator : JC/MD
 Sample : VX0815WBL01
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VBLK685

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML080422WMA.M
 Title : VOC Analysis

37	6.677	915	917	919	rBV2	355	334	0.04%	0.004%
38	6.769	919	932	945	rVV	249046	600705	63.31%	8.005%
39	7.116	981	989	997	rBV7	9207	21596	2.28%	0.288%
40	7.312	1011	1021	1039	rVV	206754	459768	48.45%	6.127%
41	7.464	1042	1046	1047	rBV2	378	515	0.05%	0.007%
42	7.482	1047	1049	1050	rBV	747	344	0.04%	0.005%
43	7.708	1085	1086	1090	rBV2	252	315	0.03%	0.004%
44	7.872	1109	1113	1115	rBV	394	509	0.05%	0.007%
45	7.927	1120	1122	1125	rBV3	1426	1877	0.20%	0.025%
46	8.025	1136	1138	1139	rBV2	488	292	0.03%	0.004%
47	8.092	1146	1149	1152	rVB2	480	515	0.05%	0.007%
48	8.214	1168	1169	1171	rBV	436	315	0.03%	0.004%
49	8.275	1176	1179	1181	rBV	421	561	0.06%	0.007%
50	8.330	1181	1188	1201	rVV	144812	232244	24.48%	3.095%
51	8.482	1210	1213	1218	rVB5	1399	2542	0.27%	0.034%
52	8.580	1226	1229	1231	rBV2	561	783	0.08%	0.010%
53	8.653	1234	1241	1252	rBV	436887	686312	72.33%	9.146%
54	8.951	1284	1290	1300	rBV	104268	154905	16.33%	2.064%
55	9.384	1354	1361	1374	rBV	433361	633304	66.74%	8.439%
56	9.518	1382	1383	1385	rBV2	512	318	0.03%	0.004%
57	9.659	1404	1406	1408	rVB	784	508	0.05%	0.007%
58	9.701	1408	1413	1419	rBV4	2399	4137	0.44%	0.055%
59	9.921	1447	1449	1451	rVV2	333	371	0.04%	0.005%
60	10.055	1465	1471	1482	rBV	520848	704664	74.26%	9.390%
61	10.305	1508	1512	1518	rBV2	697	866	0.09%	0.012%
62	10.445	1532	1535	1537	rBV	386	420	0.04%	0.006%
63	10.585	1556	1558	1562	rVB2	476	369	0.04%	0.005%
64	10.634	1564	1566	1568	rVV2	473	530	0.06%	0.007%
65	10.677	1572	1573	1576	rVB2	616	365	0.04%	0.005%
66	10.829	1597	1598	1601	rBV2	535	481	0.05%	0.006%
67	10.878	1604	1606	1607	rVB	449	315	0.03%	0.004%
68	11.195	1652	1658	1667	rBV	407295	518901	54.69%	6.915%
69	11.445	1693	1699	1700	rBV3	479	667	0.07%	0.009%
70	11.530	1711	1713	1716	rVB3	328	343	0.04%	0.005%
71	11.591	1719	1723	1724	rVB	413	408	0.04%	0.005%
72	11.628	1724	1729	1732	rBV	440	749	0.08%	0.010%
73	11.756	1746	1750	1752	rBV4	756	993	0.10%	0.013%
74	11.884	1770	1771	1773	rVB	530	340	0.04%	0.005%
75	11.969	1783	1785	1788	rBV2	415	405	0.04%	0.005%
76	12.024	1788	1794	1802	rBV	504445	640062	67.46%	8.529%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX081522\
 Data File : VX030620.D
 Acq On : 15 Aug 2022 11:18
 Operator : JC/MD
 Sample : VX0815WBL01
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VBLK685

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML080422WMA.M
 Title : VOC Analysis

77	12.128	1807	1811	1812	rBV2	564	762	0.08%	0.010%
78	12.170	1816	1818	1822	rVB2	738	588	0.06%	0.008%
79	12.219	1822	1826	1827	rBV	674	787	0.08%	0.010%
80	12.323	1837	1843	1850	rBV	510454	645894	68.07%	8.607%
81	12.475	1865	1868	1869	rVB	665	488	0.05%	0.007%
82	12.634	1890	1894	1895	rVB2	356	309	0.03%	0.004%
83	12.762	1913	1915	1917	rVB2	456	387	0.04%	0.005%
84	12.878	1932	1934	1935	rVV	604	379	0.04%	0.005%
85	13.402	2017	2020	2024	rBV2	516	616	0.06%	0.008%
86	13.445	2024	2027	2028	rBV2	326	352	0.04%	0.005%
87	13.591	2049	2051	2053	rBV	652	545	0.06%	0.007%
88	13.646	2059	2060	2063	rVB2	569	390	0.04%	0.005%
89	13.688	2066	2067	2069	rBV	578	500	0.05%	0.007%
90	13.969	2110	2113	2114	rVB2	458	383	0.04%	0.005%
91	14.079	2129	2131	2136	rBV2	337	724	0.08%	0.010%
92	14.133	2137	2140	2143	rVB2	1151	1369	0.14%	0.018%
93	14.164	2143	2145	2146	rBV	637	425	0.04%	0.006%
94	14.231	2154	2156	2159	rBV2	288	347	0.04%	0.005%
95	14.268	2159	2162	2164	rBV	495	530	0.06%	0.007%
96	14.505	2198	2201	2204	rBV2	531	705	0.07%	0.009%
97	14.700	2231	2233	2236	rBV	897	603	0.06%	0.008%
98	14.798	2248	2249	2251	rVB	742	442	0.05%	0.006%
99	15.115	2299	2301	2305	rVB3	718	838	0.09%	0.011%
100	15.548	2370	2372	2376	rBV3	610	650	0.07%	0.009%




Sum of corrected areas: 7504152

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX081522\
Data File : VX030620.D
Acq On : 15 Aug 2022 11:18
Operator : JC/MD
Sample : VX0815WBL01
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VBLK685

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML080422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

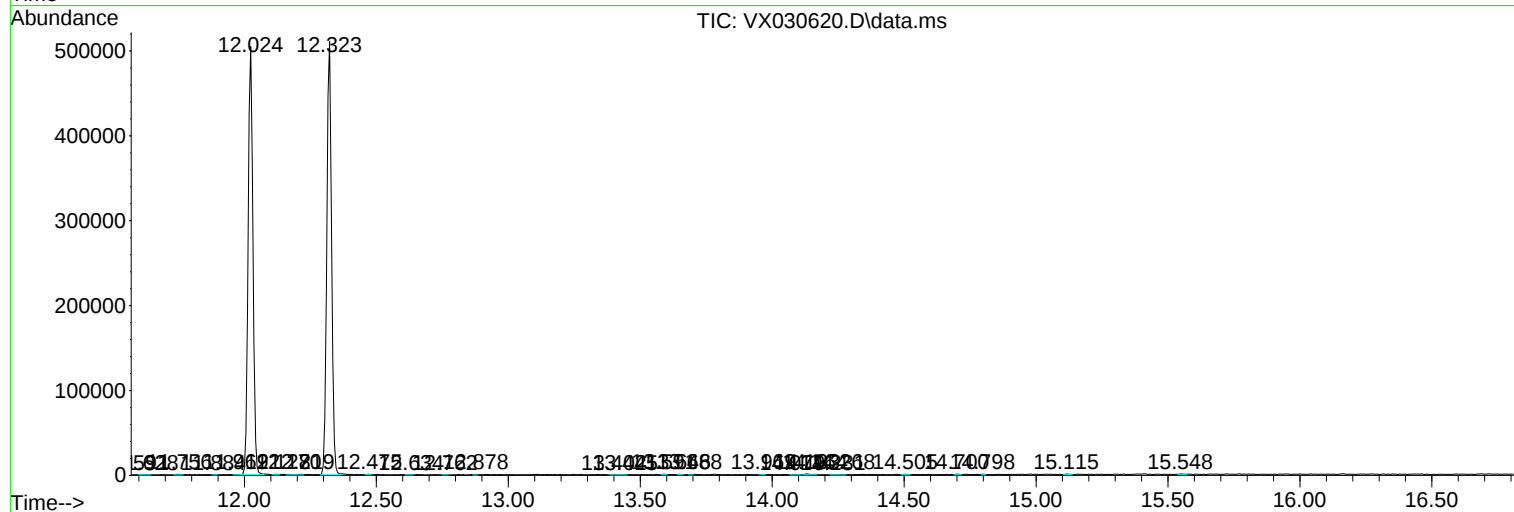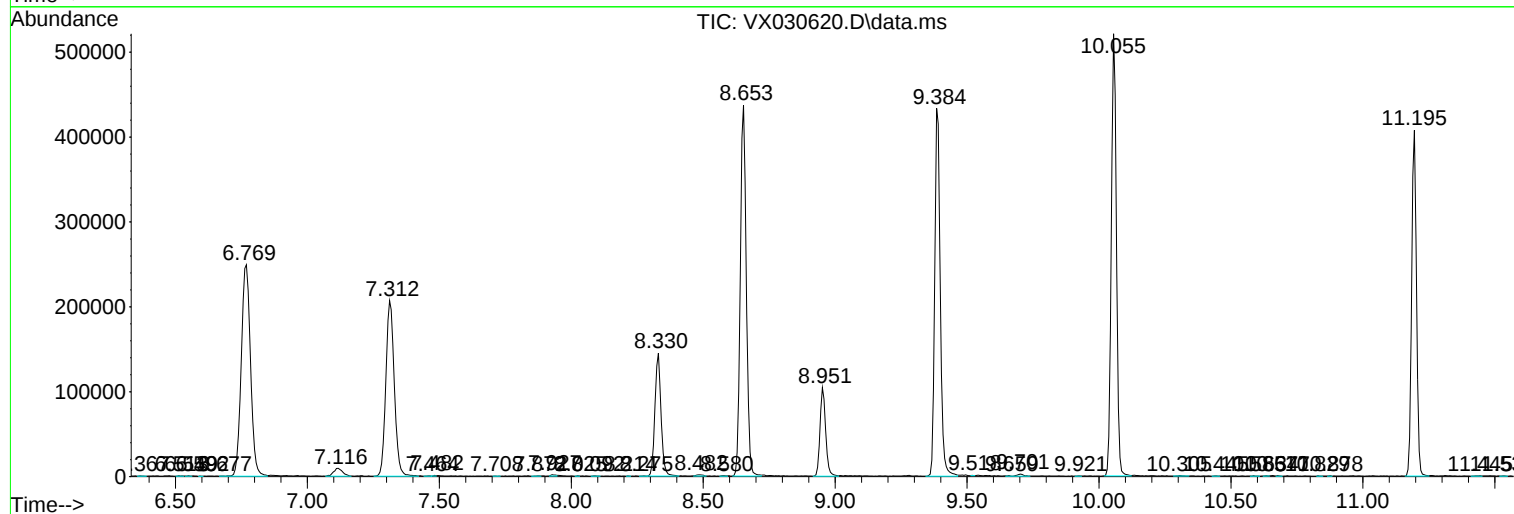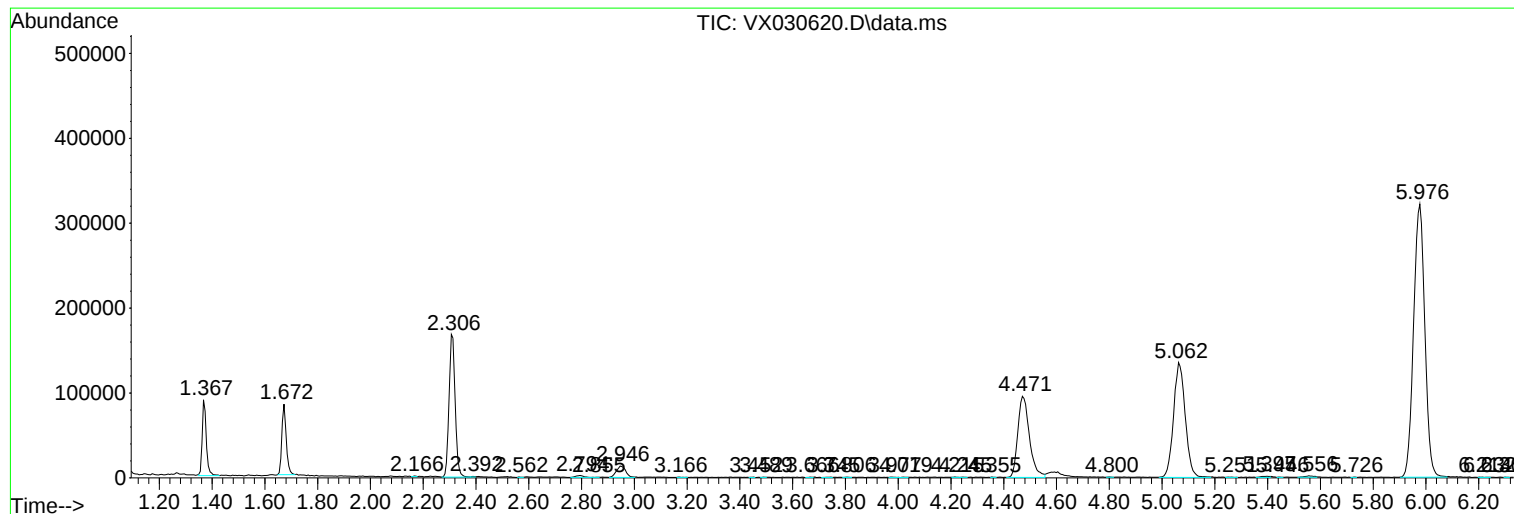

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX081522\
Data File : VX030620.D
Acq On : 15 Aug 2022 11:18
Operator : JC/MD
Sample : VX0815WBL01
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VBLK685

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXMLM080422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX081522\
Data File : VX030620.D
Acq On : 15 Aug 2022 11:18
Operator : JC/MD
Sample : VX0815WBL01
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VBLK685

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML080422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc