

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX081522\
 Data File : VX030623.D
 Acq On : 15 Aug 2022 13:14
 Operator : JC/MD
 Sample : N4110-07
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VHBLK001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXMLM080422WMA.M
 Title : VOC Analysis

Signal : TIC: VX030623.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.368	42	46	54	rVB	150907	156792	13.46%	1.829%
2	1.666	91	95	107	rVB	112104	145248	12.47%	1.694%
3	2.307	194	200	211	rVB	267859	405902	34.84%	4.734%
4	2.575	241	244	245	rBV	385	472	0.04%	0.006%
5	2.678	256	261	264	rBV3	606	1083	0.09%	0.013%
6	2.745	269	272	274	rVB2	349	352	0.03%	0.004%
7	2.770	274	276	277	rBV	736	699	0.06%	0.008%
8	2.788	277	279	285	rVB5	1600	2460	0.21%	0.029%
9	2.855	288	290	291	rBV2	377	340	0.03%	0.004%
10	2.947	298	305	314	rBV	12352	28898	2.48%	0.337%
11	3.440	384	386	388	rBV2	536	496	0.04%	0.006%
12	3.696	423	428	429	rBV2	380	448	0.04%	0.005%
13	4.026	480	482	489	rBV	507	648	0.06%	0.008%
14	4.312	528	529	533	rBV2	493	638	0.05%	0.007%
15	4.471	546	555	569	rBV	87750	267440	22.96%	3.119%
16	5.062	640	652	668	rBV2	156610	472935	40.60%	5.515%
17	5.221	674	678	679	rBV3	457	654	0.06%	0.008%
18	5.324	693	695	696	rBV	571	373	0.03%	0.004%
19	5.404	700	708	712	rVB5	1240	3185	0.27%	0.037%
20	5.440	712	714	717	rBV2	259	328	0.03%	0.004%
21	5.501	721	724	726	rBV	507	533	0.05%	0.006%
22	5.525	726	728	730	rBV2	717	638	0.05%	0.007%
23	5.721	757	760	762	rBB2	360	421	0.04%	0.005%
24	5.977	788	802	814	rBV2	394101	1164948	100.00%	13.586%
25	6.172	833	834	839	rVB2	672	588	0.05%	0.007%
26	6.300	854	855	858	rVB	590	335	0.03%	0.004%
27	6.330	858	860	863	rVB	611	427	0.04%	0.005%
28	6.361	863	865	867	rBV2	441	438	0.04%	0.005%
29	6.483	884	885	889	rVV2	490	414	0.04%	0.005%
30	6.544	894	895	898	rBV	537	434	0.04%	0.005%
31	6.763	920	931	945	rBV	270567	648878	55.70%	7.567%
32	6.922	956	957	960	rBV2	523	452	0.04%	0.005%
33	6.946	960	961	965	rVV2	334	442	0.04%	0.005%
34	7.117	981	989	996	rBV4	8412	19979	1.72%	0.233%
35	7.312	1012	1021	1039	rVV	238138	532384	45.70%	6.209%
36	7.434	1039	1041	1045	rVV4	471	673	0.06%	0.008%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX081522\
 Data File : VX030623.D
 Acq On : 15 Aug 2022 13:14
 Operator : JC/MD
 Sample : N4110-07
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VHBLK001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML080422WMA.M
 Title : VOC Analysis

37	7.501	1045	1052	1056	rVV4	970	2214	0.19%	0.026%
38	7.708	1083	1086	1088	rBV2	671	763	0.07%	0.009%
39	7.836	1105	1107	1110	rVB2	387	334	0.03%	0.004%
40	7.940	1120	1124	1130	rVV4	930	1868	0.16%	0.022%
41	8.043	1138	1141	1144	rBV2	381	684	0.06%	0.008%
42	8.129	1151	1155	1158	rBV	310	386	0.03%	0.005%
43	8.153	1158	1159	1162	rVB2	460	371	0.03%	0.004%
44	8.330	1180	1188	1197	rBV	165889	271584	23.31%	3.167%
45	8.470	1209	1211	1212	rBV	532	431	0.04%	0.005%
46	8.653	1234	1241	1250	rBV	598317	917222	78.74%	10.697%
47	8.952	1285	1290	1307	rVB	118668	176269	15.13%	2.056%
48	9.104	1314	1315	1318	rBV2	402	367	0.03%	0.004%
49	9.159	1322	1324	1329	rVV2	418	540	0.05%	0.006%
50	9.281	1342	1344	1347	rVB2	709	480	0.04%	0.006%
51	9.384	1356	1361	1376	rBV	404872	593061	50.91%	6.916%
52	9.665	1405	1407	1410	rVB3	463	416	0.04%	0.005%
53	9.708	1410	1414	1419	rBV3	1847	3169	0.27%	0.037%
54	9.811	1429	1431	1434	rVB2	418	391	0.03%	0.005%
55	10.055	1464	1471	1484	rBV	568811	767977	65.92%	8.956%
56	10.244	1500	1502	1505	rBV2	349	345	0.03%	0.004%
57	10.390	1522	1526	1529	rBV2	453	847	0.07%	0.010%
58	10.470	1535	1539	1541	rBV	540	550	0.05%	0.006%
59	10.543	1549	1551	1553	rVB2	638	423	0.04%	0.005%
60	10.567	1553	1555	1556	rBV	537	447	0.04%	0.005%
61	10.744	1582	1584	1586	rVV	499	456	0.04%	0.005%
62	10.787	1589	1591	1593	rVV	454	422	0.04%	0.005%
63	10.811	1593	1595	1597	rVV	443	382	0.03%	0.004%
64	10.915	1610	1612	1616	rVB	555	596	0.05%	0.007%
65	10.982	1619	1623	1627	rVB2	482	828	0.07%	0.010%
66	11.195	1652	1658	1673	rVB	404331	521338	44.75%	6.080%
67	11.908	1774	1775	1778	rVB2	514	392	0.03%	0.005%
68	12.024	1789	1794	1802	rBV	575344	687371	59.00%	8.016%
69	12.213	1823	1825	1828	rBV	333	401	0.03%	0.005%
70	12.323	1837	1843	1850	rBV	595797	740607	63.57%	8.637%
71	12.506	1871	1873	1877	rBV2	357	454	0.04%	0.005%
72	12.689	1901	1903	1907	rVB	421	456	0.04%	0.005%
73	12.756	1912	1914	1916	rVB2	467	359	0.03%	0.004%
74	13.103	1969	1971	1974	rVB	451	388	0.03%	0.005%
75	13.152	1977	1979	1983	rBV2	508	555	0.05%	0.006%
76	13.347	2009	2011	2013	rVB	652	448	0.04%	0.005%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX081522\
 Data File : VX030623.D
 Acq On : 15 Aug 2022 13:14
 Operator : JC/MD
 Sample : N4110-07
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VHBLK001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML080422WMA.M
 Title : VOC Analysis

77	13.457	2026	2029	2032	rVB	530	567	0.05%	0.007%
78	13.494	2032	2035	2036	rBV2	422	527	0.05%	0.006%
79	13.646	2055	2060	2061	rVB2	415	512	0.04%	0.006%
80	13.731	2072	2074	2076	rBV	577	487	0.04%	0.006%
81	13.780	2080	2082	2084	rVV	495	447	0.04%	0.005%
82	13.969	2111	2113	2117	rBV	600	532	0.05%	0.006%
83	14.036	2122	2124	2126	rBV2	409	457	0.04%	0.005%
84	14.134	2137	2140	2147	rBV3	1606	2223	0.19%	0.026%
85	14.317	2167	2170	2171	rBV2	411	476	0.04%	0.006%
86	14.463	2191	2194	2196	rBV3	469	412	0.04%	0.005%
87	14.487	2196	2198	2201	rVB2	629	662	0.06%	0.008%
88	14.536	2201	2206	2208	rBV2	589	975	0.08%	0.011%
89	14.682	2228	2230	2234	rBV2	605	767	0.07%	0.009%
90	14.719	2234	2236	2238	rVB2	583	459	0.04%	0.005%
91	14.749	2238	2241	2242	rBV2	901	782	0.07%	0.009%
92	14.920	2267	2269	2270	rBV	497	343	0.03%	0.004%
93	14.944	2270	2273	2275	rBV3	571	756	0.06%	0.009%
94	14.987	2278	2280	2284	rVV2	652	707	0.06%	0.008%
95	15.329	2332	2336	2339	rBV3	621	715	0.06%	0.008%
96	15.383	2343	2345	2352	rVB5	1189	2201	0.19%	0.026%
97	15.950	2437	2438	2441	rBV2	696	569	0.05%	0.007%
98	16.097	2460	2462	2463	rBV	719	408	0.04%	0.005%
99	16.322	2497	2499	2500	rVB2	799	433	0.04%	0.005%
100	16.560	2536	2538	2540	rVB	780	435	0.04%	0.005%




Sum of corrected areas: 8574819

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX081522\
Data File : VX030623.D
Acq On : 15 Aug 2022 13:14
Operator : JC/MD
Sample : N4110-07
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML080422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

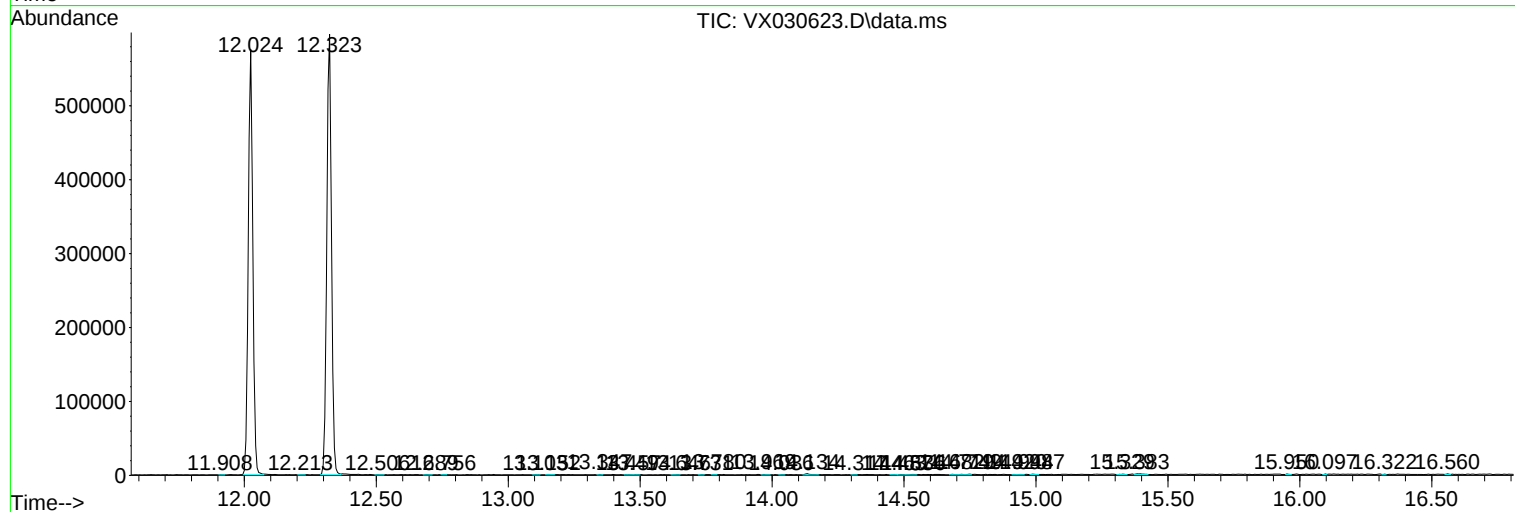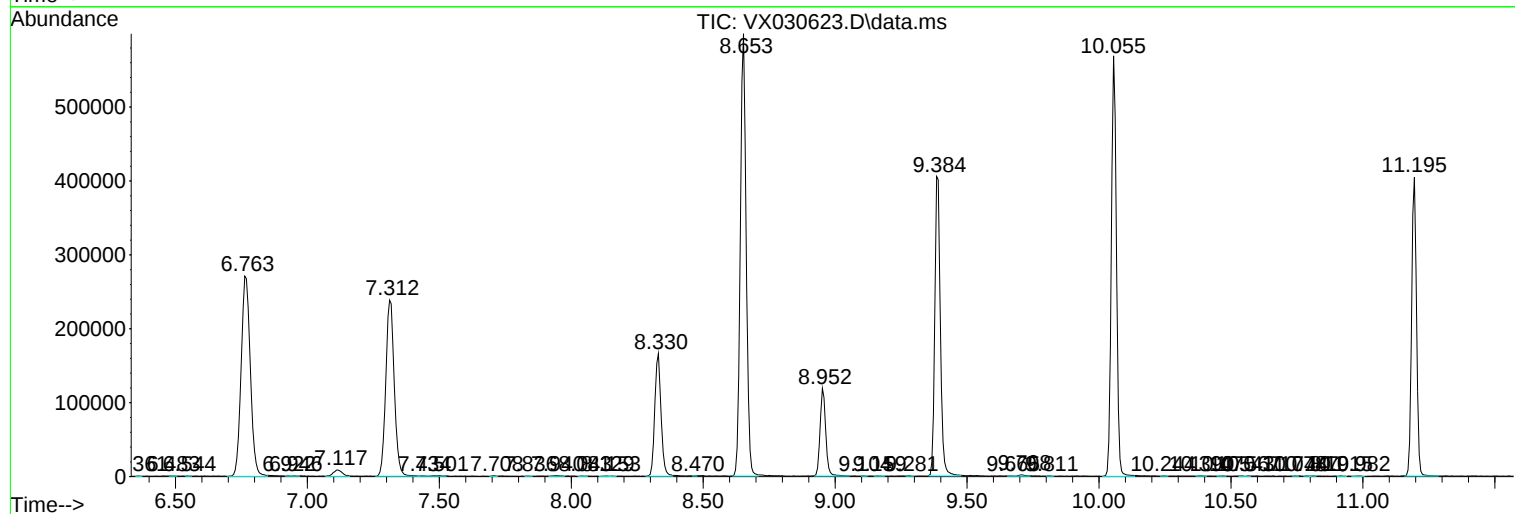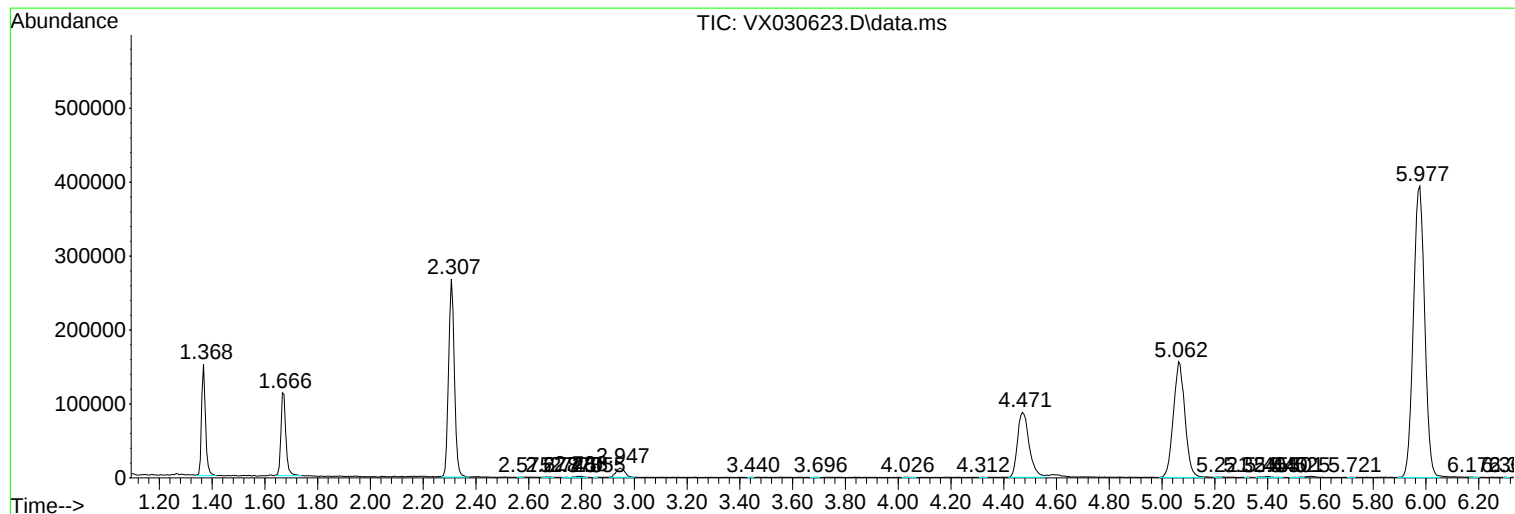

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX081522\
Data File : VX030623.D
Acq On : 15 Aug 2022 13:14
Operator : JC/MD
Sample : N4110-07
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXMLM080422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX081522\
Data File : VX030623.D
Acq On : 15 Aug 2022 13:14
Operator : JC/MD
Sample : N4110-07
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML080422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc