

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX081522\
 Data File : VX030624.D
 Acq On : 15 Aug 2022 13:42
 Operator : JC/MD
 Sample : N4193-03
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VHBLK001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML080422WMA.M
 Title : VOC Analysis

Signal : TIC: VX030624.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.368	42	46	56	rVB	137145	140191	12.66%	1.713%
2	1.666	91	95	111	rVB	102929	137396	12.40%	1.679%
3	2.306	193	200	211	rBV	241712	374491	33.81%	4.575%
4	2.502	230	232	233	rBV2	424	388	0.04%	0.005%
5	2.520	233	235	237	rVB2	610	454	0.04%	0.006%
6	2.697	260	264	265	rBV2	577	537	0.05%	0.007%
7	2.788	275	279	287	rVB5	1716	3601	0.33%	0.044%
8	2.861	287	291	292	rBV2	446	555	0.05%	0.007%
9	2.947	297	305	315	rBV	13332	33038	2.98%	0.404%
10	3.361	371	373	377	rVB2	381	431	0.04%	0.005%
11	3.977	471	474	477	rBV2	430	506	0.05%	0.006%
12	4.233	513	516	518	rBV2	362	445	0.04%	0.005%
13	4.282	521	524	525	rVV2	442	384	0.03%	0.005%
14	4.471	544	555	568	rBV	88521	265600	23.98%	3.245%
15	4.812	608	611	613	rVB2	491	458	0.04%	0.006%
16	4.843	615	616	618	rBV2	447	339	0.03%	0.004%
17	5.062	638	652	668	rBV2	149484	456930	41.25%	5.582%
18	5.391	702	706	710	rVB3	481	948	0.09%	0.012%
19	5.471	716	719	721	rBV	438	518	0.05%	0.006%
20	5.538	726	730	732	rBV3	1061	1691	0.15%	0.021%
21	5.635	744	746	749	rBV2	508	577	0.05%	0.007%
22	5.739	761	763	765	rBV	353	344	0.03%	0.004%
23	5.769	765	768	770	rBV	411	458	0.04%	0.006%
24	5.842	775	780	781	rVB2	359	468	0.04%	0.006%
25	5.855	781	782	786	rBV	446	509	0.05%	0.006%
26	5.970	789	801	817	rBV2	373676	1107601	100.00%	13.532%
27	6.178	832	835	836	rBV2	517	410	0.04%	0.005%
28	6.275	849	851	856	rBB2	443	487	0.04%	0.006%
29	6.422	873	875	878	rBV2	377	530	0.05%	0.006%
30	6.672	914	916	920	rBV2	401	479	0.04%	0.006%
31	6.763	920	931	950	rBV	256249	610257	55.10%	7.456%
32	6.982	963	967	968	rVB2	321	380	0.03%	0.005%
33	7.001	968	970	972	rBV2	470	512	0.05%	0.006%
34	7.117	982	989	1000	rVB3	7716	18365	1.66%	0.224%
35	7.190	1000	1001	1005	rBV2	513	346	0.03%	0.004%
36	7.312	1011	1021	1037	rBV	233460	508484	45.91%	6.212%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX081522\
 Data File : VX030624.D
 Acq On : 15 Aug 2022 13:42
 Operator : JC/MD
 Sample : N4193-03
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VHBLK001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML080422WMA.M
 Title : VOC Analysis

37	7.482	1045	1049	1050	rBV2	935	1241	0.11%	0.015%
38	7.568	1061	1063	1065	rBV	374	439	0.04%	0.005%
39	7.616	1069	1071	1074	rVB2	435	525	0.05%	0.006%
40	7.653	1074	1077	1079	rBV2	470	556	0.05%	0.007%
41	7.684	1079	1082	1083	rVB2	374	367	0.03%	0.004%
42	7.860	1110	1111	1114	rBV2	314	351	0.03%	0.004%
43	7.933	1119	1123	1129	rBV4	975	1924	0.17%	0.024%
44	8.324	1181	1187	1199	rBV	150872	259281	23.41%	3.168%
45	8.421	1201	1203	1208	rVB4	771	1215	0.11%	0.015%
46	8.464	1208	1210	1211	rBV	524	451	0.04%	0.006%
47	8.574	1226	1228	1230	rBV4	507	397	0.04%	0.005%
48	8.653	1234	1241	1250	rBV	545680	867666	78.34%	10.601%
49	8.952	1284	1290	1299	rBV	115852	169704	15.32%	2.073%
50	9.183	1327	1328	1331	rBV	524	401	0.04%	0.005%
51	9.317	1347	1350	1353	rBV2	452	497	0.04%	0.006%
52	9.384	1356	1361	1375	rVV	390474	580979	52.45%	7.098%
53	9.634	1400	1402	1405	rVB2	461	437	0.04%	0.005%
54	9.701	1408	1413	1420	rVB3	2696	5028	0.45%	0.061%
55	9.769	1420	1424	1428	rVB2	865	1143	0.10%	0.014%
56	9.799	1428	1429	1431	rBV2	578	578	0.05%	0.007%
57	9.921	1447	1449	1452	rVB2	291	327	0.03%	0.004%
58	9.982	1455	1459	1460	rBV2	511	643	0.06%	0.008%
59	10.055	1465	1471	1483	rBV	530225	720237	65.03%	8.799%
60	10.256	1502	1504	1507	rBV2	364	409	0.04%	0.005%
61	10.610	1560	1562	1564	rBV2	382	428	0.04%	0.005%
62	10.671	1569	1572	1573	rBV2	411	505	0.05%	0.006%
63	10.713	1577	1579	1580	rBV	484	391	0.04%	0.005%
64	10.921	1611	1613	1619	rVB	414	715	0.06%	0.009%
65	10.976	1619	1622	1623	rBV2	310	335	0.03%	0.004%
66	11.098	1640	1642	1645	rVB3	591	565	0.05%	0.007%
67	11.128	1645	1647	1652	rBV2	440	703	0.06%	0.009%
68	11.195	1652	1658	1667	rBV	394014	510470	46.09%	6.237%
69	11.488	1704	1706	1708	rBV2	492	382	0.03%	0.005%
70	11.597	1723	1724	1726	rBV	556	400	0.04%	0.005%
71	11.689	1737	1739	1741	rVB2	646	491	0.04%	0.006%
72	11.719	1741	1744	1746	rBV	471	424	0.04%	0.005%
73	12.024	1789	1794	1804	rBV	540779	655882	59.22%	8.013%
74	12.323	1837	1843	1852	rBV	557577	716738	64.71%	8.757%
75	12.542	1876	1879	1882	rBV2	543	431	0.04%	0.005%
76	12.798	1920	1921	1924	rVB	538	391	0.04%	0.005%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX081522\
 Data File : VX030624.D
 Acq On : 15 Aug 2022 13:42
 Operator : JC/MD
 Sample : N4193-03
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VHBLK001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML080422WMA.M
 Title : VOC Analysis

77	12.829	1924	1926	1927	rBV	432	361	0.03%	0.004%
78	12.963	1946	1948	1950	rBV	352	434	0.04%	0.005%
79	13.012	1955	1956	1958	rVB	678	329	0.03%	0.004%
80	13.030	1958	1959	1962	rVB2	430	337	0.03%	0.004%
81	13.061	1962	1964	1965	rBV	573	344	0.03%	0.004%
82	13.335	2007	2009	2010	rBV	557	354	0.03%	0.004%
83	13.585	2046	2050	2051	rBV2	483	482	0.04%	0.006%
84	13.695	2066	2068	2070	rVB2	573	405	0.04%	0.005%
85	13.871	2095	2097	2100	rBV2	305	326	0.03%	0.004%
86	14.030	2121	2123	2125	rBV2	436	344	0.03%	0.004%
87	14.091	2131	2133	2135	rBV2	376	398	0.04%	0.005%
88	14.286	2164	2165	2169	rBV2	520	480	0.04%	0.006%
89	14.621	2218	2220	2223	rVB	577	413	0.04%	0.005%
90	14.652	2223	2225	2226	rBV2	525	354	0.03%	0.004%
91	14.908	2265	2267	2269	rBV	619	365	0.03%	0.004%
92	15.365	2340	2342	2344	rBV3	659	677	0.06%	0.008%
93	15.731	2400	2402	2406	rBV2	621	780	0.07%	0.010%
94	15.847	2418	2421	2423	rBV2	543	491	0.04%	0.006%
95	15.865	2423	2424	2427	rVV3	689	623	0.06%	0.008%
96	15.920	2431	2433	2434	rBV	1071	659	0.06%	0.008%
97	16.243	2484	2486	2487	rBV	647	409	0.04%	0.005%
98	16.267	2488	2490	2491	rBV	773	462	0.04%	0.006%
99	16.469	2522	2523	2529	rBV4	579	1080	0.10%	0.013%
100	16.658	2550	2554	2555	rBV4	853	1079	0.10%	0.013%




Sum of corrected areas: 8185141

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX081522\
Data File : VX030624.D
Acq On : 15 Aug 2022 13:42
Operator : JC/MD
Sample : N4193-03
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML080422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

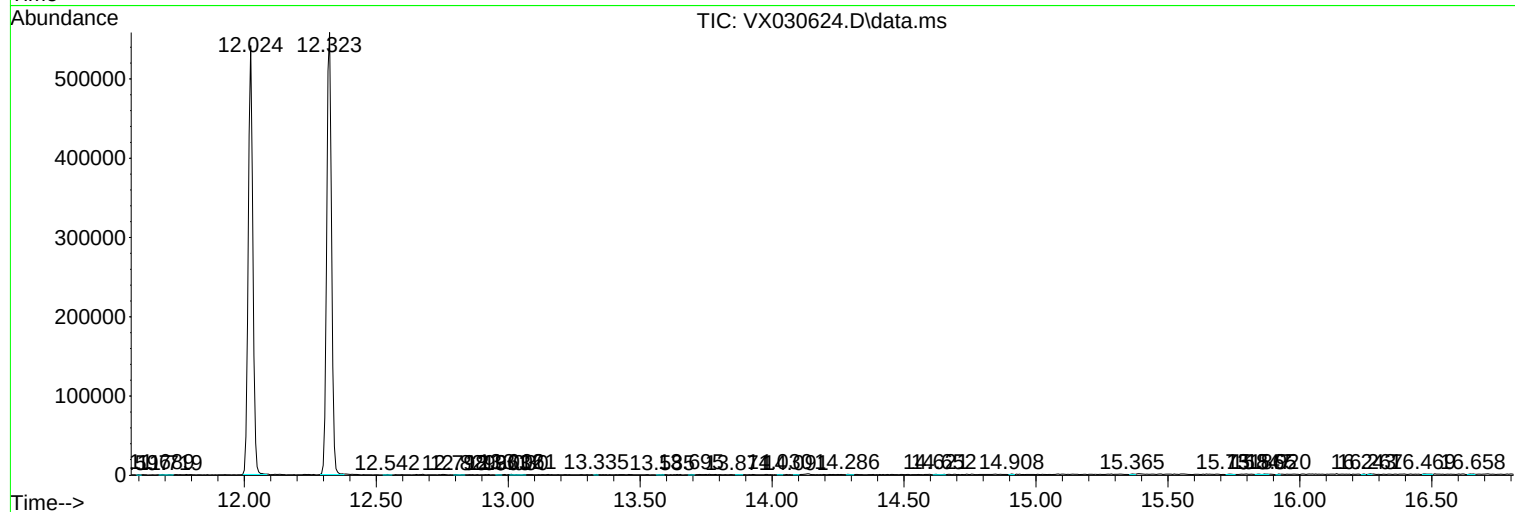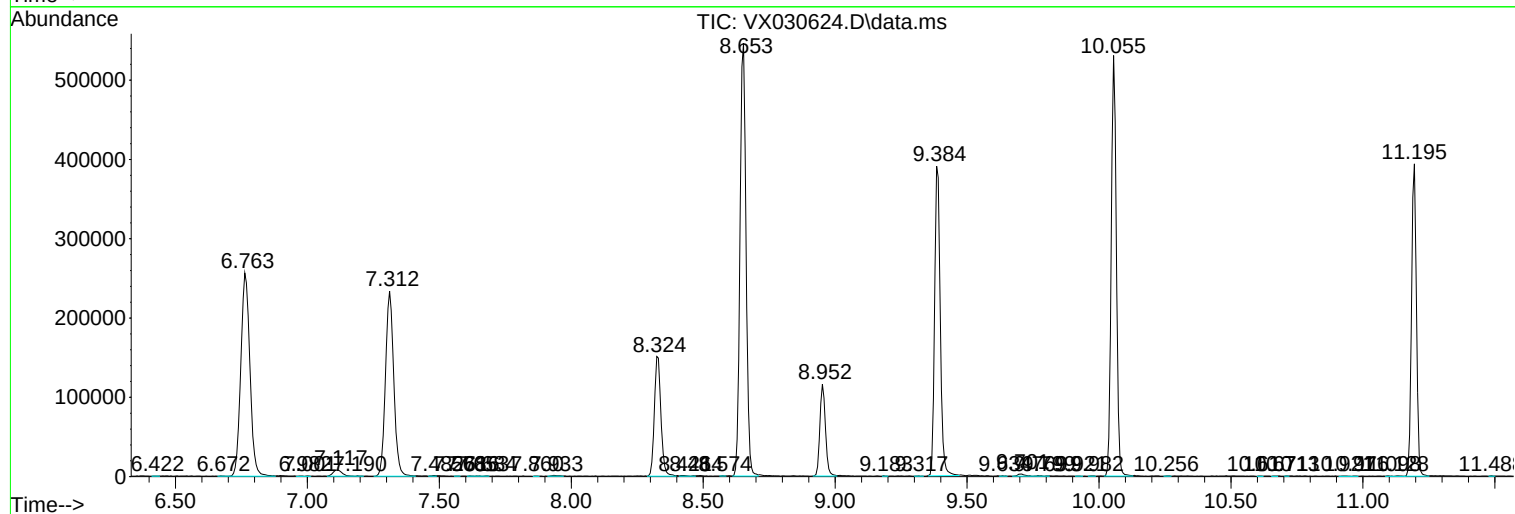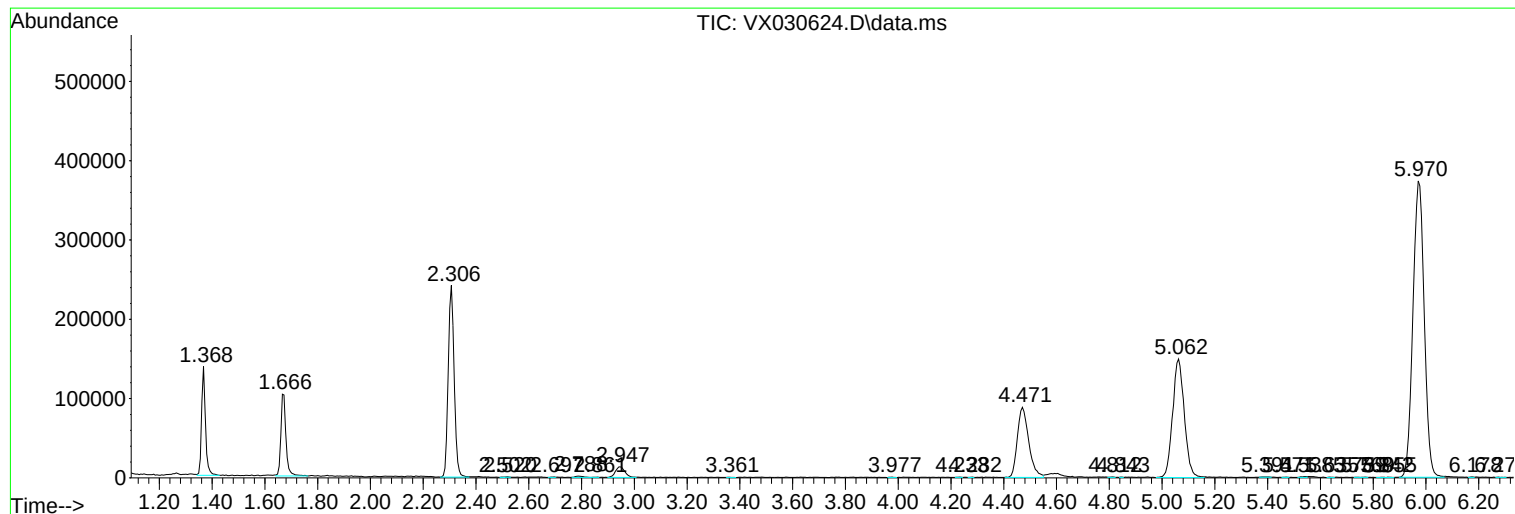

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX081522\
Data File : VX030624.D
Acq On : 15 Aug 2022 13:42
Operator : JC/MD
Sample : N4193-03
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXMLM080422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX081522\
Data File : VX030624.D
Acq On : 15 Aug 2022 13:42
Operator : JC/MD
Sample : N4193-03
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML080422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc