
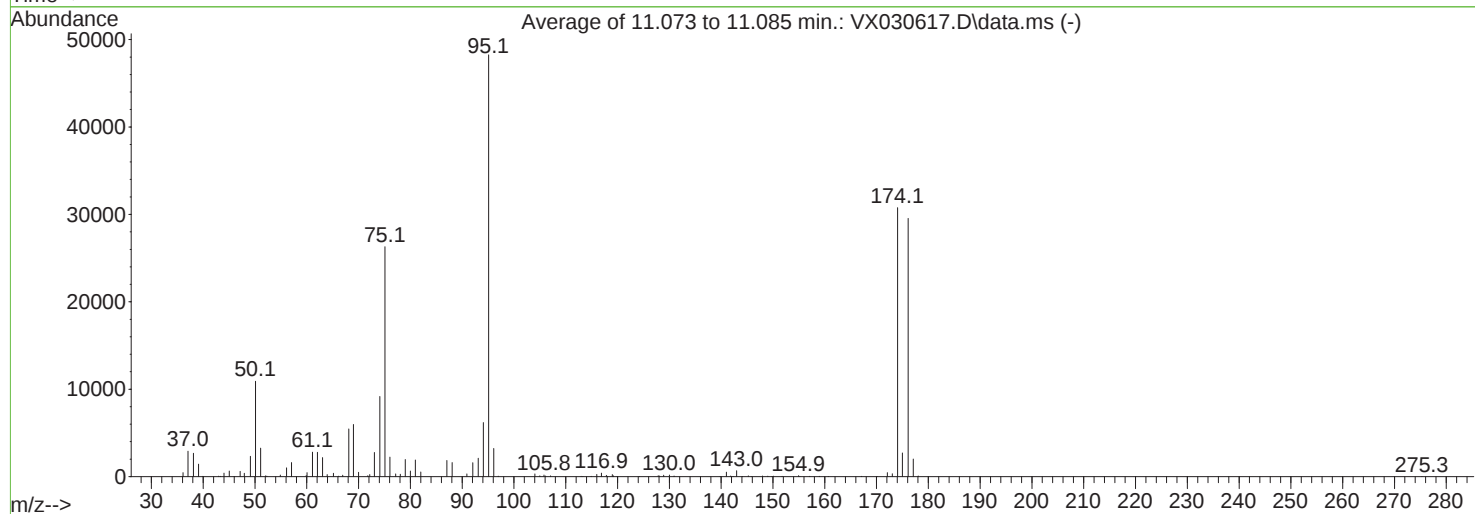


Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX081522\
 Data File : VX030617.D
 Acq On : 15 Aug 2022 09:49
 Operator : JC/MD
 Sample : BFB679
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 BFB679

Integration File: LSCINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM080422WMA.M
 Title : VOC Analysis
 Last Update : Wed Aug 17 02:19:30 2022

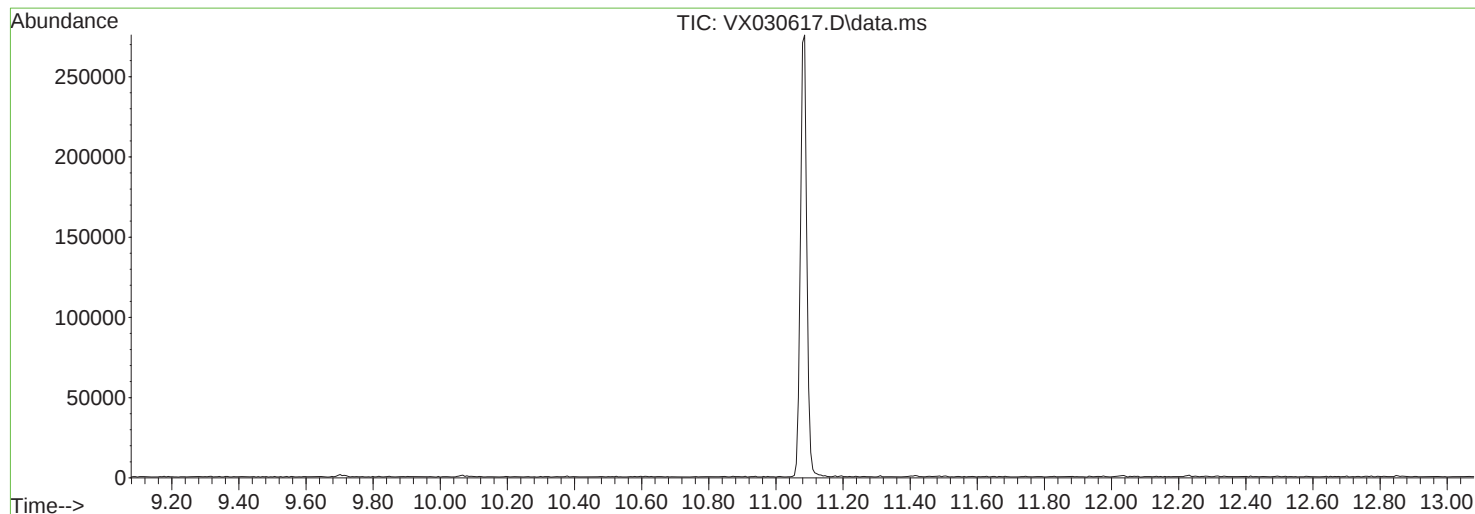

AutoFind: Scans 1638, 1639, 1640; Background Corrected with Scan 1633

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	22.6	10904	PASS
75	95	30	80	54.5	26299	PASS
95	95	100	100	100.0	48251	PASS
96	95	5	9	6.7	3217	PASS
173	174	0.00	2	1.1	335	PASS
174	95	50	120	63.8	30773	PASS
175	174	5	9	8.8	2715	PASS
176	174	95	101	96.0	29536	PASS
177	176	5	9	6.8	2013	PASS

m/z	Abundance
39.90	448.0
44.00	220.0

Instrument :
MSVOA_X
ClientSampleId :
BFB679

m/z	Abundance
36.10	379.0
37.10	3400.0
38.10	2940.0
39.10	2001.0
40.00	473.0
43.00	78.0
44.00	853.0
45.00	738.0
47.10	724.0
47.90	538.0
49.10	2660.0
50.10	13208.0
51.10	3938.0
52.30	143.0
54.90	230.0
56.10	890.0
57.10	1976.0
60.10	719.0
61.10	3099.0
62.10	2985.0
63.10	2483.0
63.90	312.0
65.20	418.0
66.20	99.0
66.90	173.0
68.10	6238.0
69.00	7299.0
70.10	609.0
72.20	363.0
73.10	3049.0
74.10	11052.0
75.10	31088.0
76.10	2682.0
77.10	352.0
78.10	305.0
79.00	2066.0
80.00	673.0
80.90	2145.0
82.00	606.0
87.10	2218.0
88.00	1708.0
90.90	308.0
92.00	2056.0
93.10	2317.0
94.10	7611.0
95.10	56496.0
96.10	3974.0
96.90	75.0
104.00	454.0
105.00	109.0
105.80	299.0
107.10	100.0
113.00	75.0
114.90	50.0
116.00	316.0
116.90	449.0
117.80	251.0
119.20	303.0
128.10	240.0
128.80	148.0
130.00	268.0
130.90	70.0
139.80	57.0
141.00	514.0
141.80	79.0
142.30	56.0
143.00	782.0
144.10	83.0
145.20	118.0
148.00	96.0
149.00	74.0
149.80	62.0
150.10	77.0
151.70	60.0
155.00	128.0
157.10	52.0
158.90	51.0
170.10	54.0
172.10	607.0
173.10	412.0
174.10	35280.0
175.00	2830.0
176.10	33216.0
177.10	2523.0
178.00	81.0

Instrument :
MSVOA_X
ClientSampleId :
BFB679

m/z	Abundance
36.10	405.0
37.00	2002.0
38.10	1780.0
39.00	1137.0
40.10	535.0
43.00	86.0
44.00	572.0
45.10	424.0
47.20	395.0
48.00	244.0
49.10	1641.0
50.10	8466.0
51.10	2305.0
52.00	100.0
54.90	143.0
56.10	824.0
57.00	1014.0
59.90	407.0
61.10	2156.0
62.00	2206.0
63.10	1356.0
64.00	172.0
65.10	318.0
67.00	183.0
68.10	4042.0
69.00	4351.0
70.10	316.0
72.10	342.0
73.00	1984.0
74.10	6288.0
75.10	17512.0
76.00	1555.0
77.20	193.0
78.10	213.0
79.00	1404.0
80.00	478.0
81.00	1129.0
82.00	387.0
87.00	1230.0
88.00	1326.0
91.00	322.0
92.10	1073.0
93.10	1281.0
94.10	3544.0
95.10	31944.0
96.10	2228.0
104.10	144.0
104.90	94.0
105.80	231.0
107.00	74.0
113.30	56.0
114.90	74.0
116.00	146.0
117.00	373.0
118.10	120.0
119.00	300.0
127.80	96.0
128.90	75.0
130.00	153.0
141.10	374.0
143.00	383.0
145.20	62.0
149.00	75.0
151.80	51.0
155.00	81.0
172.10	272.0
173.10	225.0
174.00	17328.0
175.00	1783.0
176.10	16280.0
177.10	1087.0
275.30	52.0

Instrument :
MSVOA_X
ClientSampleId :
BFB679

m/z	Abundance
36.10	565.0
37.10	3325.0
38.10	3280.0
39.20	1133.0
40.10	425.0
43.30	107.0
44.00	451.0
45.00	747.0
46.00	68.0
47.10	719.0
47.90	363.0
49.10	2679.0
50.10	11037.0
51.10	3558.0
52.10	199.0
54.90	168.0
56.10	1304.0
57.00	1831.0
60.00	656.0
61.10	3126.0
62.00	3166.0
63.00	2699.0
64.00	227.0
65.10	443.0
66.10	53.0
66.90	125.0
68.10	6100.0
69.00	6276.0
69.90	584.0
71.80	334.0
73.10	3249.0
74.10	10183.0
75.10	30296.0
76.10	2462.0
77.10	366.0
78.00	295.0
79.00	2422.0
80.00	789.0
81.00	2439.0
82.00	605.0
87.00	2078.0
88.10	1788.0
90.80	289.0
92.10	1673.0
93.10	2731.0
94.10	7382.0
95.10	56312.0
96.10	3448.0
97.00	103.0
104.10	366.0
105.10	55.0
106.10	224.0
107.10	92.0
112.90	59.0
116.00	289.0
116.80	386.0
117.90	215.0
119.00	437.0
119.90	56.0
124.20	62.0
127.90	220.0
128.90	261.0
130.00	131.0
130.90	135.0
140.90	664.0
141.90	141.0
143.00	846.0
145.30	94.0
145.80	51.0
148.00	110.0
150.10	89.0
154.80	121.0
155.20	100.0
157.10	69.0
159.00	72.0
160.70	61.0
167.10	136.0
172.10	500.0
173.00	368.0
174.10	39712.0
175.00	3531.0
176.10	39112.0
177.10	2429.0
178.10	125.0

Instrument :
MSVOA_X
ClientSampleId :
BFB679