

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX081523\
 Data File : VX036979.D
 Acq On : 15 Aug 2023 11:30
 Operator : JC/MD
 Sample : VX0815MBL01
 Misc : 5.00g/10mL/100uL/5.00mL/MSVOA_X/MEOH
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VX0815MBL01

Quant Time: Aug 15 16:52:55 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X072123W.M
 Quant Title : SW846 8260
 QLast Update : Fri Jul 21 12:14:12 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Pentafluorobenzene	5.556	168	127561	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	6.763	114	234181	50.000	ug/l	0.00
63) Chlorobenzene-d5	10.055	117	231260	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	12.024	152	109825	50.000	ug/l	0.00

System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	5.952	65	89461	47.398	ug/l	0.00
Spiked Amount	50.000	Range	78 - 117	Recovery	=	94.800%
35) Dibromofluoromethane	5.385	113	75934	47.175	ug/l	0.00
Spiked Amount	50.000	Range	75 - 124	Recovery	=	94.340%
50) Toluene-d8	8.646	98	284227	49.794	ug/l	0.00
Spiked Amount	50.000	Range	92 - 112	Recovery	=	99.580%
62) 4-Bromofluorobenzene	11.079	95	115521	53.642	ug/l	0.00
Spiked Amount	50.000	Range	83 - 123	Recovery	=	107.280%


Target Compounds	Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX081523\
Data File : VX036979.D
Acq On : 15 Aug 2023 11:30
Operator : JC/MD
Sample : VX0815MBL01
Misc : 5.00g/10mL/100uL/5.00mL/MSVOA_X/MEOH
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VX0815MBL01

Quant Time: Aug 15 16:52:55 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X072123W.M
Quant Title : SW846 8260
QLast Update : Fri Jul 21 12:14:12 2023
Response via : Initial Calibration




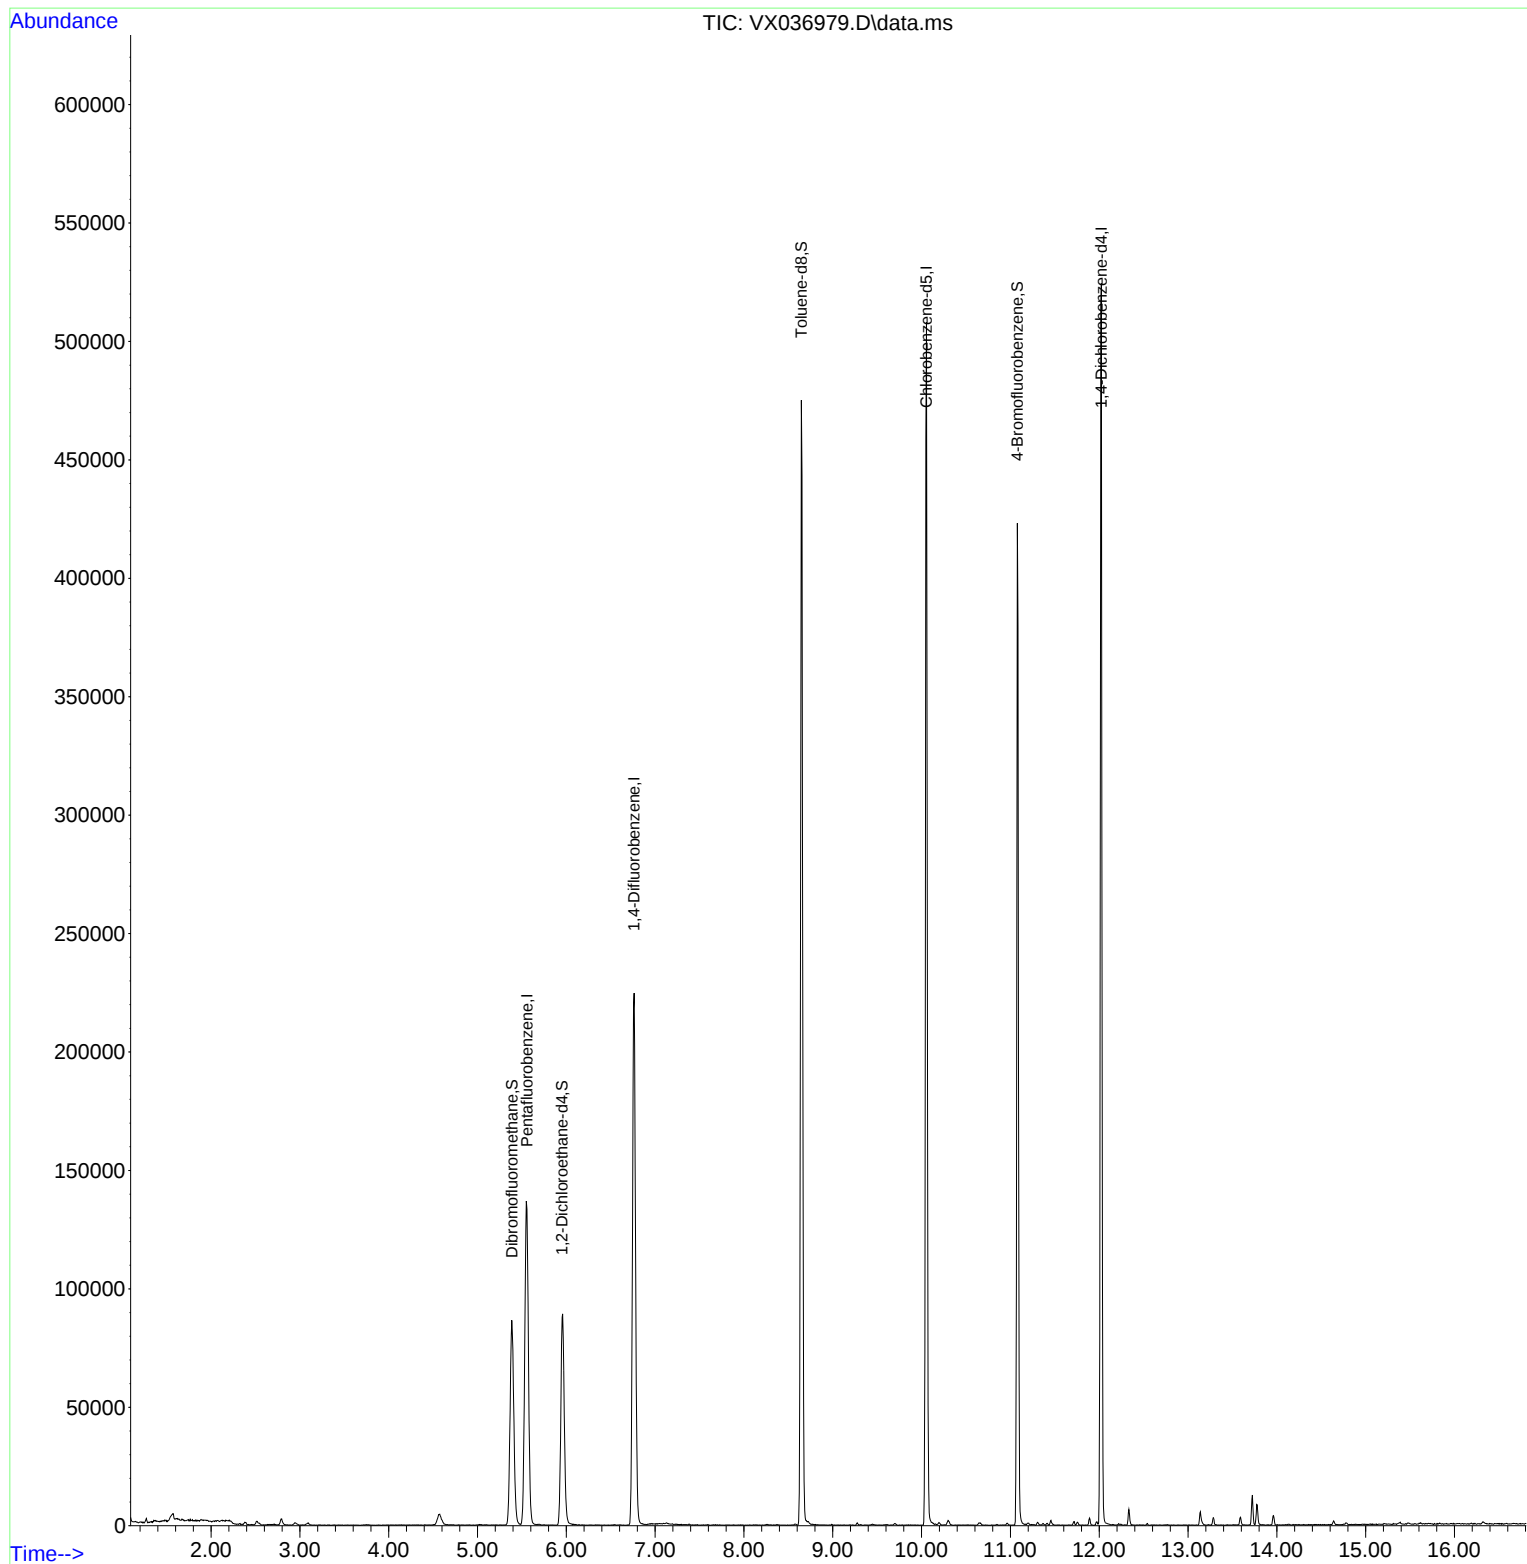


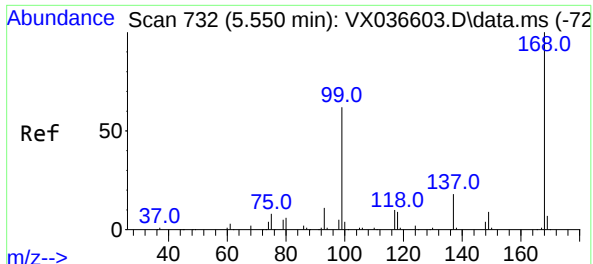

#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 5.556 min Scan# 71
Delta R.T. 0.006 min
Lab File: VX036979.D
Acq: 15 Aug 2023 11:30




Instrument :
MSVOA_X
ClientSampleId :
VX0815MBL01


Tgt Ion:168 Resp: 127561
Ion Ratio Lower Upper
168 100
99 60.8 56.6 85.0

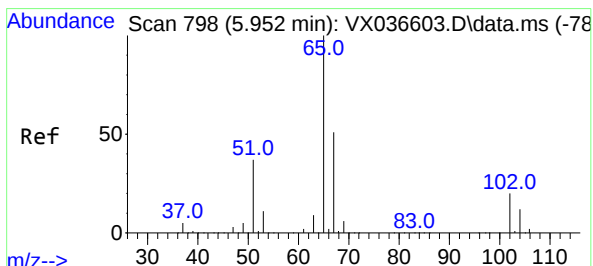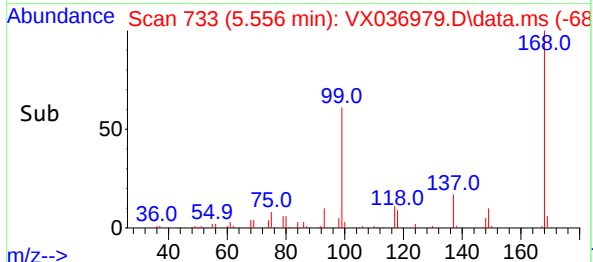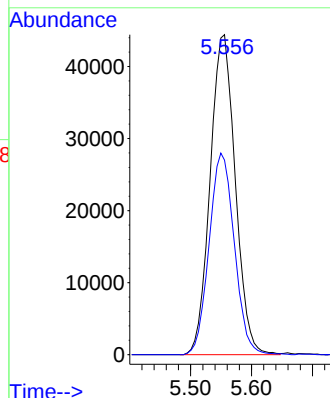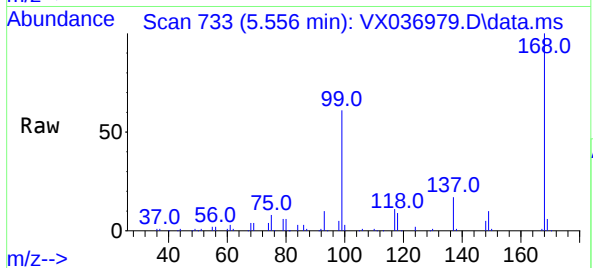

#33
1,2-Dichloroethane-d4
Concen: 47.398 ug/l
RT: 5.952 min Scan# 798
Delta R.T. -0.000 min
Lab File: VX036979.D
Acq: 15 Aug 2023 11:30

Tgt Ion: 65 Resp: 89461
Ion Ratio Lower Upper
65 100
67 50.5 0.0 100.2


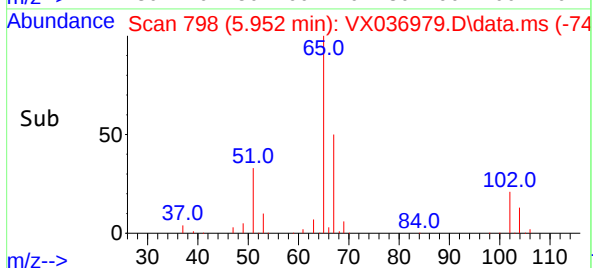
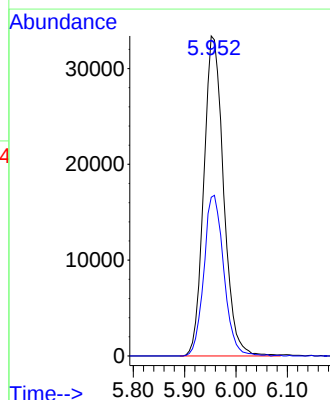
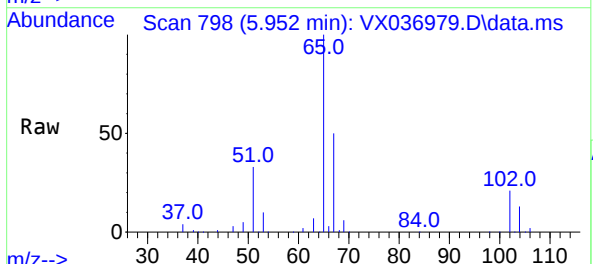


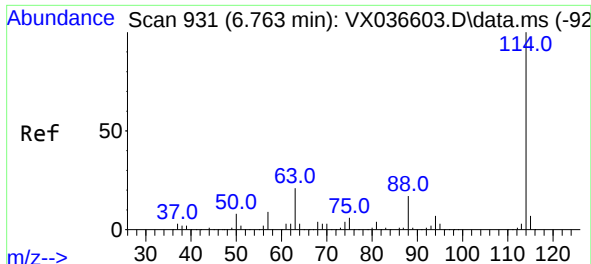

#34
1,4-Difluorobenzene
Concen: 50.000 ug/l
RT: 6.763 min Scan# 91
Delta R.T. -0.000 min
Lab File: VX036979.D
Acq: 15 Aug 2023 11:30




Instrument :
MSVOA_X
ClientSampleId :
VX0815MBL01


Tgt Ion:114 Resp: 234181
Ion Ratio Lower Upper
114 100
63 20.0 0.0 45.0
88 16.8 0.0 36.6

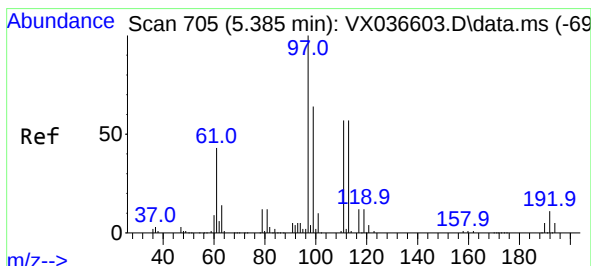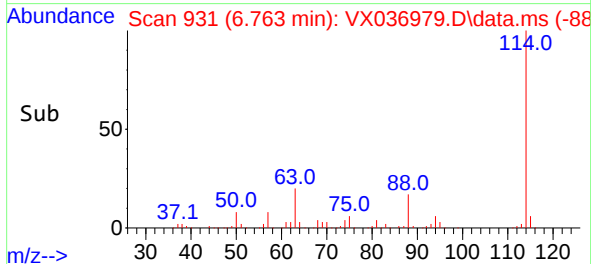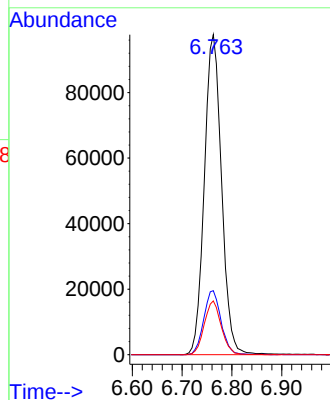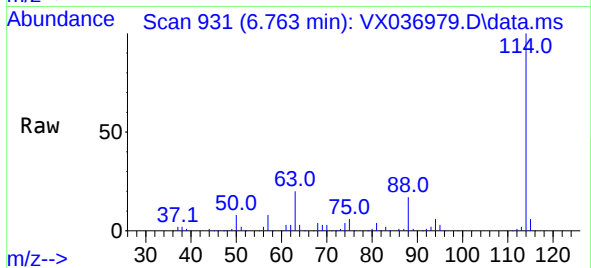

#35
Dibromofluoromethane
Concen: 47.175 ug/l
RT: 5.385 min Scan# 705
Delta R.T. -0.000 min
Lab File: VX036979.D
Acq: 15 Aug 2023 11:30

Tgt Ion:113 Resp: 75934
Ion Ratio Lower Upper
113 100
111 102.0 82.9 124.3
192 18.5 13.3 19.9


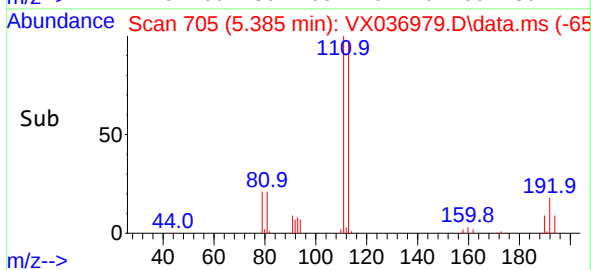
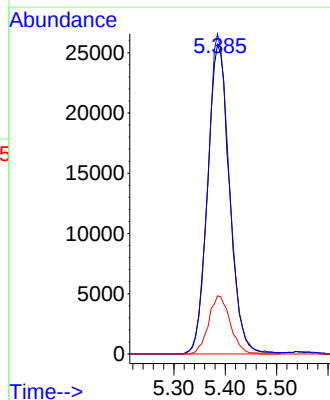
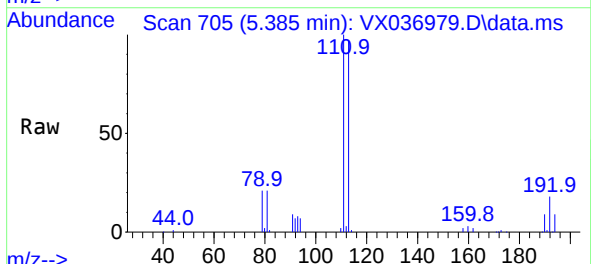


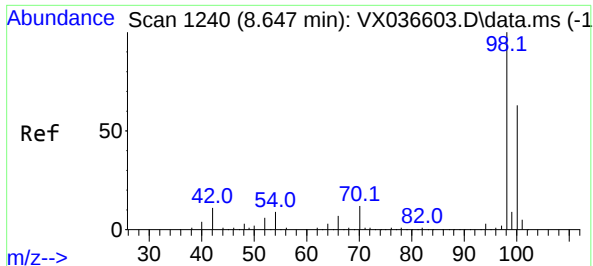

#50
Toluene-d8
Concen: 49.794 ug/l
RT: 8.646 min Scan# 11
Delta R.T. -0.000 min
Lab File: VX036979.D
Acq: 15 Aug 2023 11:30




Instrument :
MSVOA_X
ClientSampleId :
VX0815MBL01


Tgt Ion: 98 Resp: 284227
Ion Ratio Lower Upper
98 100
100 65.8 53.1 79.7

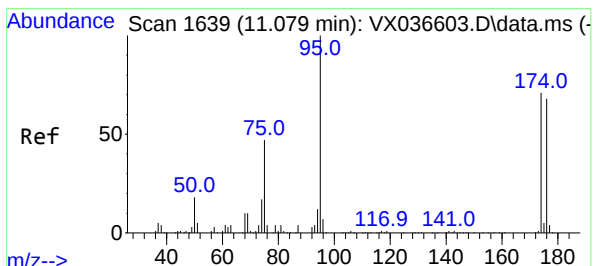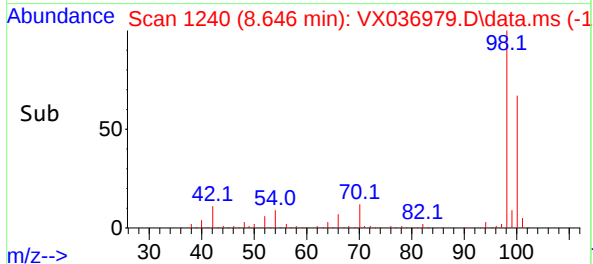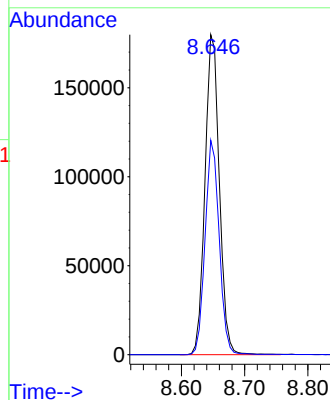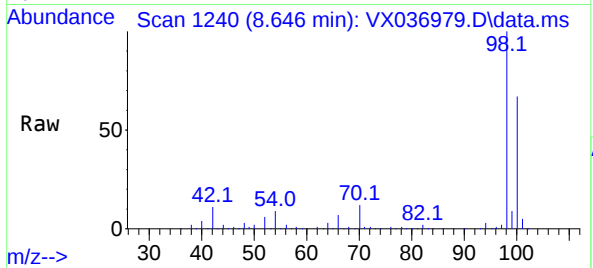

#62
4-Bromofluorobenzene
Concen: 53.642 ug/l
RT: 11.079 min Scan# 1639
Delta R.T. -0.000 min
Lab File: VX036979.D
Acq: 15 Aug 2023 11:30

Tgt Ion: 95 Resp: 115521
Ion Ratio Lower Upper
95 100
174 73.3 0.0 135.6
176 71.0 0.0 131.0


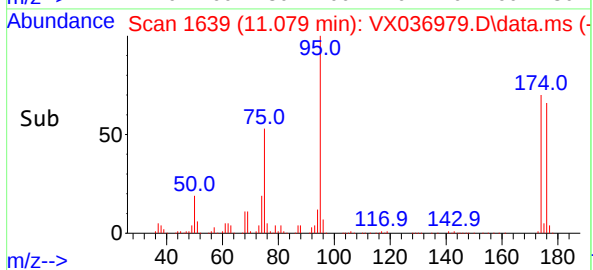
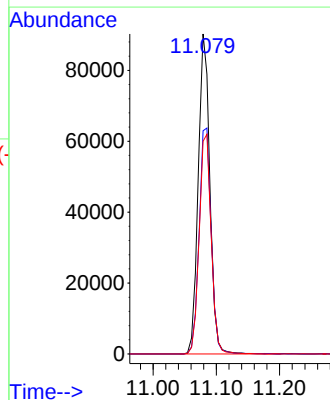
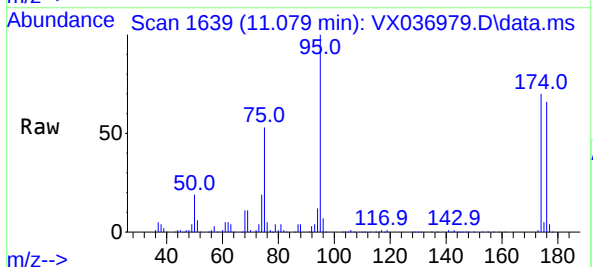


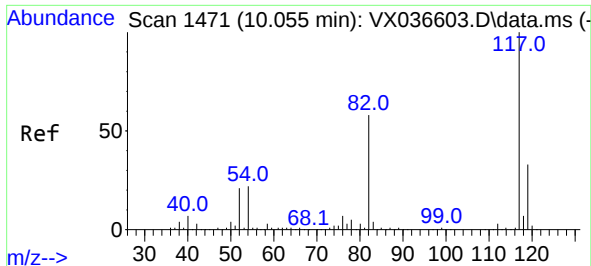

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 10.055 min Scan# 1471
Delta R.T. -0.000 min
Lab File: VX036979.D
Acq: 15 Aug 2023 11:30

Instrument :
MSVOA_X
ClientSampleId :
VX0815MBL01

Tgt Ion:117 Resp: 231260
Ion Ratio Lower Upper
117 100
82 55.3 46.2 69.4
119 32.6 25.5 38.3

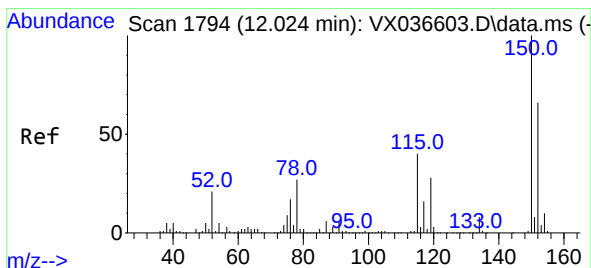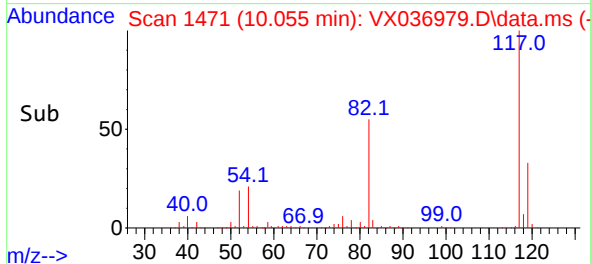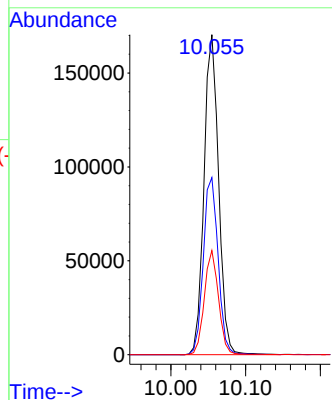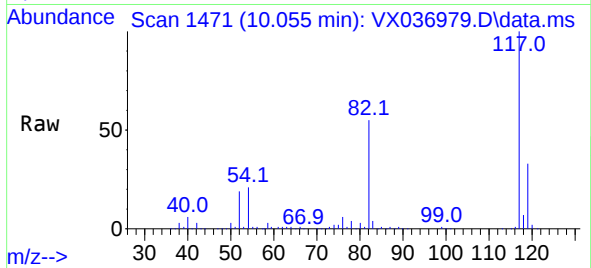

#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 12.024 min Scan# 1794
Delta R.T. -0.000 min
Lab File: VX036979.D
Acq: 15 Aug 2023 11:30

Tgt Ion:152 Resp: 109825
Ion Ratio Lower Upper
152 100
115 62.4 43.3 129.9
150 155.1 0.0 345.0

