

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX081524\
 Data File : VX043049.D
 Acq On : 15 Aug 2024 09:42
 Operator : JC/MD
 Sample : VX0815MBL01
 Misc : 5.00g/10mL/100uL/5.00mL/MSVOA_X/MEOH
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VX0815MBL01

Quant Time: Aug 16 01:35:46 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X081424W.M
 Quant Title : SW846 8260
 QLast Update : Thu Aug 15 04:22:11 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) Pentafluorobenzene	5.544	168	91451	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	6.757	114	162363	50.000	ug/l	0.00
63) Chlorobenzene-d5	10.055	117	141491	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	12.024	152	63156	50.000	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	5.952	65	56390	46.926	ug/l	0.00
Spiked Amount 50.000	Range 74 - 125		Recovery =	93.860%		
35) Dibromofluoromethane	5.385	113	48948	48.732	ug/l	0.00
Spiked Amount 50.000	Range 75 - 124		Recovery =	97.460%		
50) Toluene-d8	8.647	98	192113	49.548	ug/l	0.00
Spiked Amount 50.000	Range 86 - 113		Recovery =	99.100%		
62) 4-Bromofluorobenzene	11.079	95	65727	46.750	ug/l	0.00
Spiked Amount 50.000	Range 77 - 121		Recovery =	93.500%		
Target Compounds						Qvalue
3) Chloromethane	1.301	50	368	0.269	ug/l	94
5) Bromomethane	1.605	94	335	0.804	ug/l	96
10) Methyl Iodide	2.441	142	286	0.693	ug/l #	34
11) Tert butyl alcohol	2.947	59	4298	13.863	ug/l #	80
13) Acrolein	2.239	56	478	1.525	ug/l #	14
14) Allyl chloride	2.660	41	684	0.331	ug/l #	53
15) Acrylonitrile	3.087	53	580	0.755	ug/l #	81
16) Acetone	2.386	43	980	1.644	ug/l	100
17) Carbon Disulfide	2.502	76	2676	0.846	ug/l #	88
18) Methyl Acetate	2.715	43	612	0.311	ug/l #	60
20) Methylene Chloride	2.776	84	776	0.563	ug/l #	82
21) trans-1,2-Dichloroethene	3.093	96	476	0.414	ug/l #	70
29) Tetrahydrofuran	5.050	42	496	0.685	ug/l #	37
36) 1,1-Dichloropropene	5.544	75	7082	5.075	ug/l #	49
38) Carbon Tetrachloride	5.544	117	8885	6.297	ug/l #	14
48) Methyl methacrylate	7.708	41	165	0.515	ug/l #	41
51) 4-Methyl-2-Pentanone	8.586	43	709	0.352	ug/l #	68
68) m/p-Xylenes	10.311	106	519	0.254	ug/l	84
76) 1,2,3-Trichloropropane	11.079	75	32702	22.593	ug/l #	39
81) trans-1,4-Dichloro-2-b...	11.079	75	32702	49.281	ug/l #	5
82) 4-Chlorotoluene	11.463	91	1062	0.279	ug/l	93
87) 1,3-Dichlorobenzene	11.975	146	646	0.310	ug/l	88
88) 1,4-Dichlorobenzene	11.975	146	646	0.303	ug/l	89
89) n-Butylbenzene	12.335	91	1084	0.307	ug/l	92
91) 1,2-Dichlorobenzene	12.335	146	465	0.222	ug/l	99
93) 1,2,4-Trichlorobenzene	13.591	180	1032	0.874	ug/l	89
94) Hexachlorobutadiene	13.719	225	130	0.295	ug/l	81
95) Naphthalene	13.780	128	6382	1.368	ug/l	98
96) 1,2,3-Trichlorobenzene	13.963	180	1066	0.882	ug/l	93


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX081524\
Data File : VX043049.D
Acq On : 15 Aug 2024 09:42
Operator : JC/MD
Sample : VX0815MBL01
Misc : 5.00g/10mL/100uL/5.00mL/MSVOA_X/MEOH
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VX0815MBL01

Quant Time: Aug 16 01:35:46 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X081424W.M
Quant Title : SW846 8260
QLast Update : Thu Aug 15 04:22:11 2024
Response via : Initial Calibration




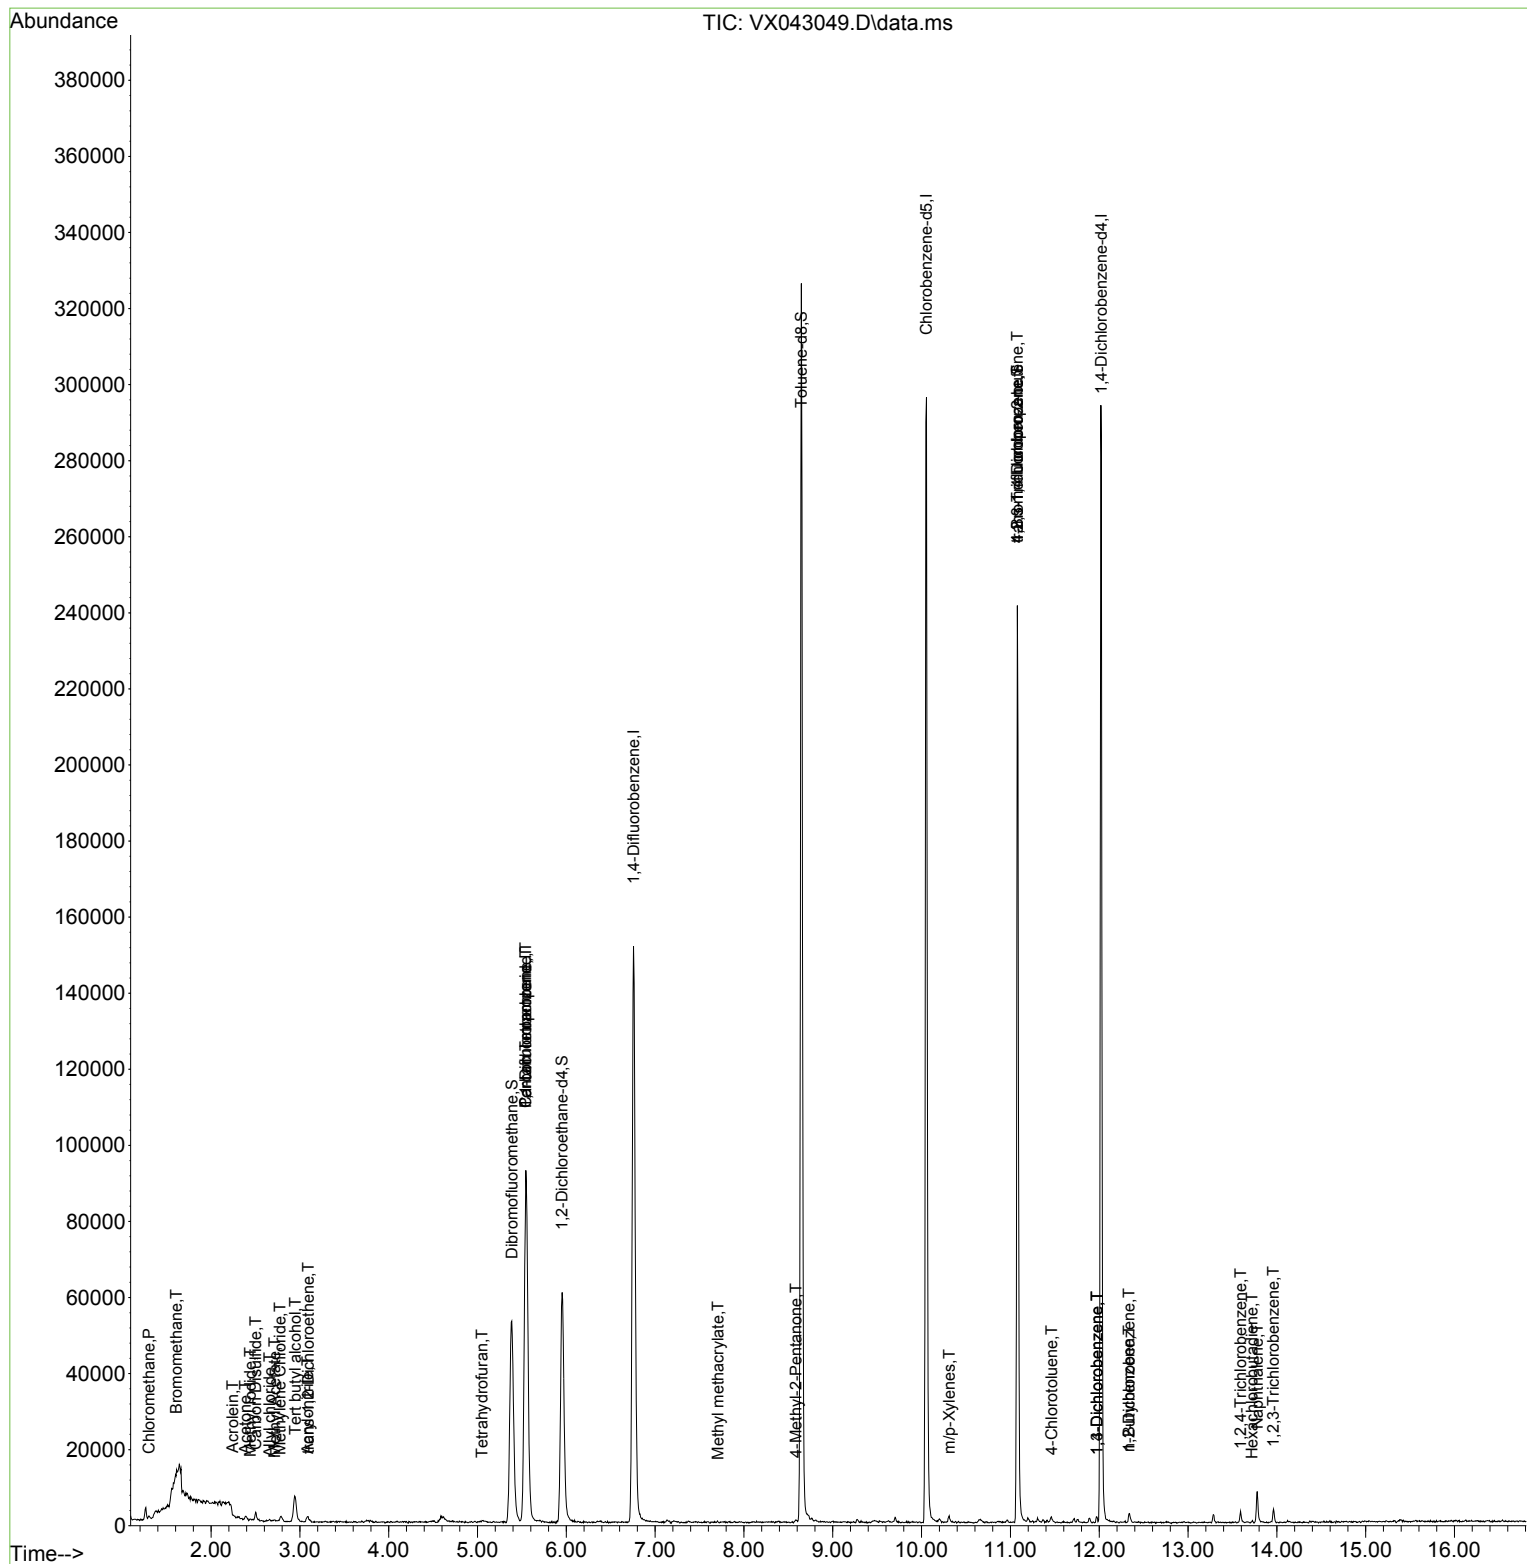




#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 5.544 min Scan# 71
Delta R.T. -0.006 min
Lab File: VX043049.D
Acq: 15 Aug 2024 09:42




Instrument :
MSVOA_X
ClientSampleId :
VX0815MBL01


Tgt Ion:168 Resp: 91451
Ion Ratio Lower Upper
168 100
99 57.6 56.6 85.0

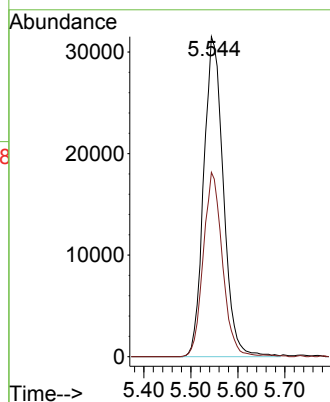

#3
Chloromethane
Concen: 0.269 ug/l
RT: 1.301 min Scan# 35
Delta R.T. -0.000 min
Lab File: VX043049.D
Acq: 15 Aug 2024 09:42

Tgt Ion: 50 Resp: 368
Ion Ratio Lower Upper
50 100
52 28.6 25.5 38.3


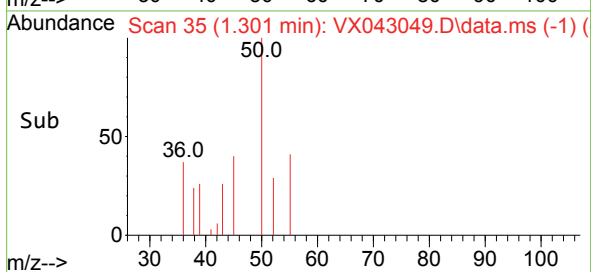
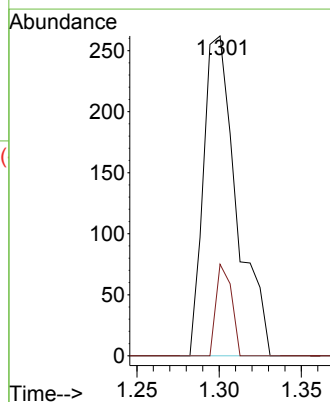



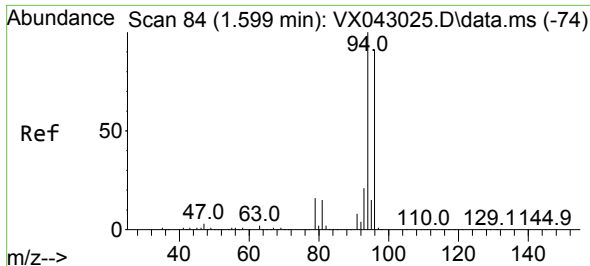

#5
Bromomethane
Concen: 0.804 ug/l
RT: 1.605 min Scan# 81
Delta R.T. 0.006 min
Lab File: VX043049.D
Acq: 15 Aug 2024 09:42




Instrument :
MSVOA_X
ClientSampleId :
VX0815MBL01


Tgt Ion: 94 Resp: 335
Ion Ratio Lower Upper
94 100
96 89.2 74.6 111.8

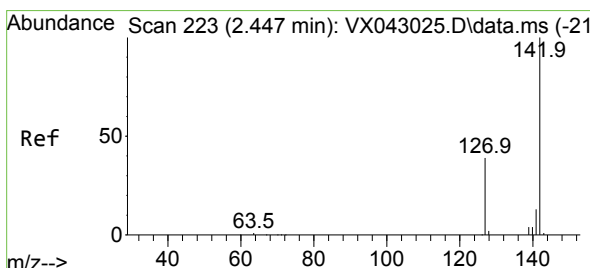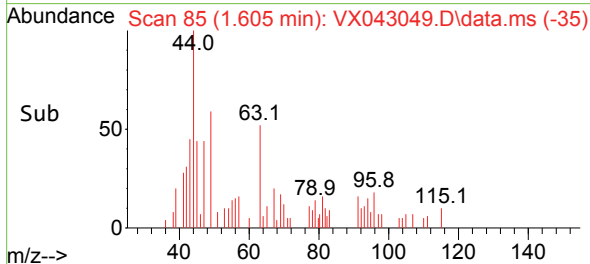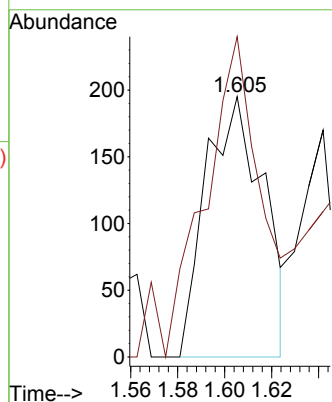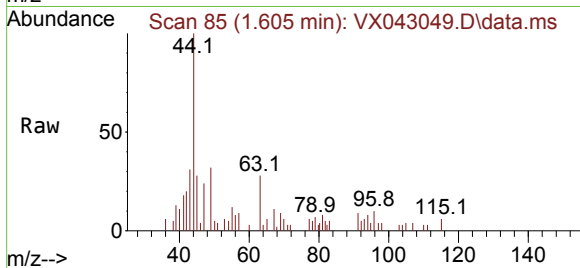

#10
Methyl Iodide
Concen: 0.693 ug/l
RT: 2.441 min Scan# 222
Delta R.T. -0.006 min
Lab File: VX043049.D
Acq: 15 Aug 2024 09:42

Tgt Ion: 142 Resp: 286
Ion Ratio Lower Upper
142 100
127 0.0 41.6 62.4#
141 0.0 11.6 17.4#


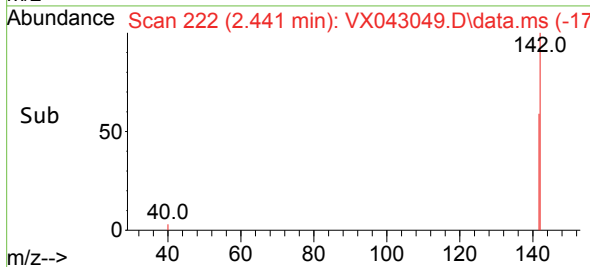
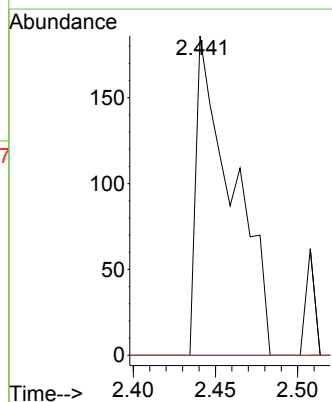
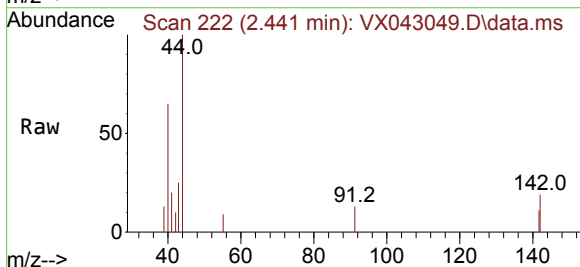




#11
Tert butyl alcohol
Concen: 13.863 ug/l
RT: 2.947 min Scan# 305
Delta R.T. -0.055 min
Lab File: VX043049.D
Acq: 15 Aug 2024 09:42




Instrument :
MSVOA_X
ClientSampleId :
VX0815MBL01


Tgt Ion: 59 Resp: 4298
Ion Ratio Lower Upper
59 100
57 0.5 6.0 9.0#

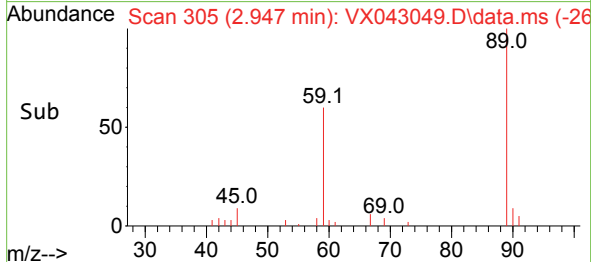

#13
Acrolein
Concen: 1.525 ug/l
RT: 2.239 min Scan# 189
Delta R.T. -0.000 min
Lab File: VX043049.D
Acq: 15 Aug 2024 09:42

Tgt Ion: 56 Resp: 478
Ion Ratio Lower Upper
56 100
55 0.0 57.1 85.7#




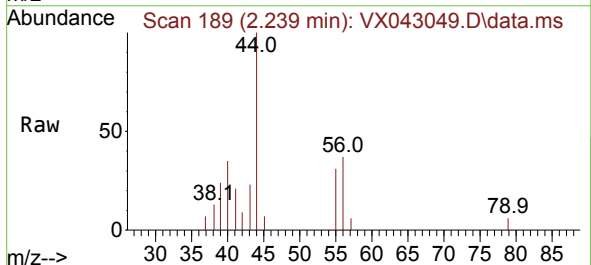




#14
 Allyl chloride
 Concen: 0.331 ug/l
 RT: 2.660 min Scan# 21
 Delta R.T. -0.000 min
 Lab File: VX043049.D
 Acq: 15 Aug 2024 09:42




Instrument :
 MSVOA_X
 ClientSampleId :
 VX0815MBL01


Tgt Ion:	41	Resp:	684
Ion	Ratio	Lower	Upper
41	100		
39	34.4	55.8	83.6#
76	0.0	24.3	36.5#

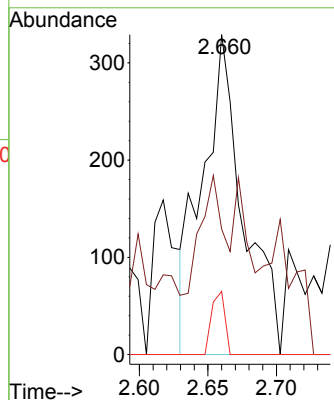

#15
 Acrylonitrile
 Concen: 0.755 ug/l
 RT: 3.087 min Scan# 328
 Delta R.T. 0.012 min
 Lab File: VX043049.D
 Acq: 15 Aug 2024 09:42

Tgt Ion:	53	Resp:	580
Ion	Ratio	Lower	Upper
53	100		
52	85.5	66.0	99.0
51	5.9	29.8	44.6#



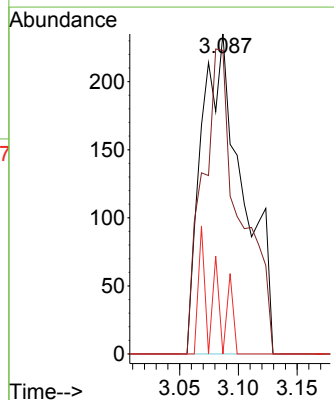





#16
Acetone
Concen: 1.644 ug/l
RT: 2.386 min Scan# 214
Delta R.T. -0.006 min
Lab File: VX043049.D
Acq: 15 Aug 2024 09:42




Instrument :
MSVOA_X
ClientSampleId :
VX0815MBL01


Tgt Ion: 43 Resp: 980
Ion Ratio Lower Upper
43 100
58 27.4 21.9 32.9

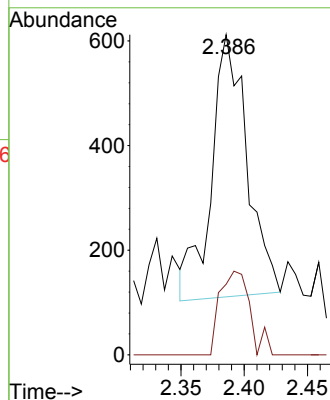

#17
Carbon Disulfide
Concen: 0.846 ug/l
RT: 2.502 min Scan# 232
Delta R.T. -0.000 min
Lab File: VX043049.D
Acq: 15 Aug 2024 09:42

Tgt Ion: 76 Resp: 2676
Ion Ratio Lower Upper
76 100
78 13.2 7.0 10.6#



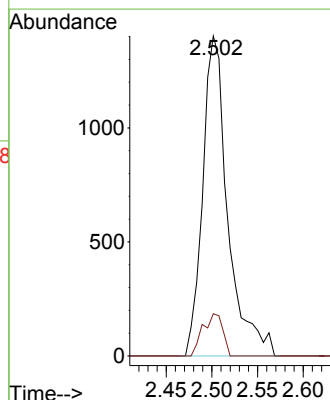





#18
Methyl Acetate
Concen: 0.311 ug/l
RT: 2.715 min Scan# 20
Delta R.T. 0.006 min
Lab File: VX043049.D
Acq: 15 Aug 2024 09:42




Instrument :
MSVOA_X
ClientSampleId :
VX0815MBL01


Tgt Ion: 43 Resp: 612
Ion Ratio Lower Upper
43 100
74 3.1 17.8 26.8#

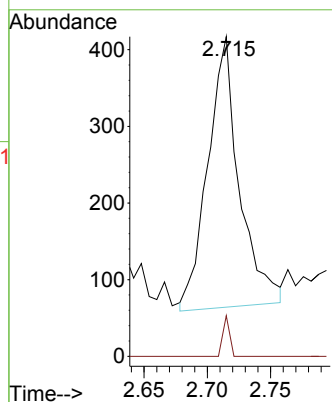

#20
Methylene Chloride
Concen: 0.563 ug/l
RT: 2.776 min Scan# 277
Delta R.T. -0.012 min
Lab File: VX043049.D
Acq: 15 Aug 2024 09:42

Tgt Ion: 84 Resp: 776
Ion Ratio Lower Upper
84 100
49 101.2 103.6 155.4#
51 42.4 33.8 50.6
86 48.1 49.4 74.0#









#21
trans-1,2-Dichloroethene
Concen: 0.414 ug/l
RT: 3.093 min Scan# 31
Delta R.T. 0.006 min
Lab File: VX043049.D
Acq: 15 Aug 2024 09:42




Instrument :
MSVOA_X
ClientSampleId :
VX0815MBL01


Tgt Ion: 96 Resp: 476
Ion Ratio Lower Upper
96 100
61 98.8 119.2 178.8#
98 64.7 48.7 73.1



#29
Tetrahydrofuran
Concen: 0.685 ug/l
RT: 5.050 min Scan# 650
Delta R.T. 0.037 min
Lab File: VX043049.D
Acq: 15 Aug 2024 09:42

Tgt Ion: 42 Resp: 496
Ion Ratio Lower Upper
42 100
72 4.0 34.2 51.4#
71 0.0 32.2 48.2#



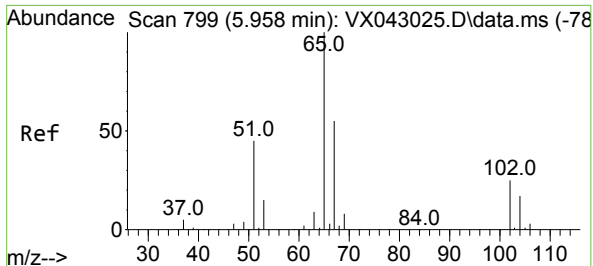

#33

1,2-Dichloroethane-d4

Concen: 46.926 ug/l

RT: 5.952 min Scan# 799

Delta R.T. -0.006 min

Lab File: VX043049.D

Acq: 15 Aug 2024 09:42

Instrument :

MSVOA_X

ClientSampleId :





VX0815MBL01

Tgt Ion: 65 Resp: 56390

Ion Ratio Lower Upper

65 100

67 53.7 0.0 100.2

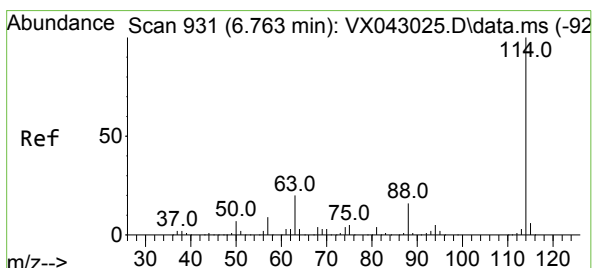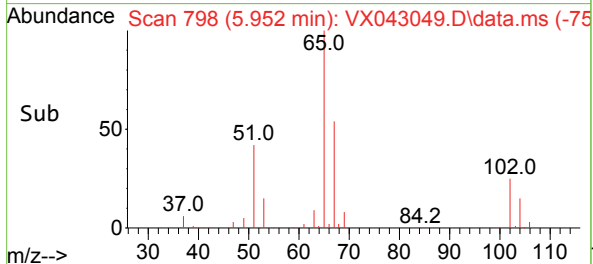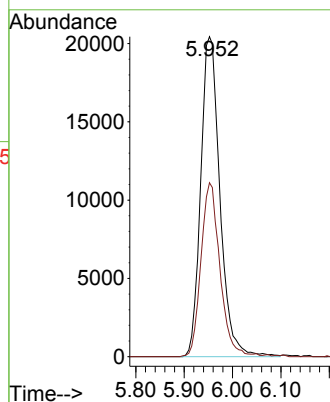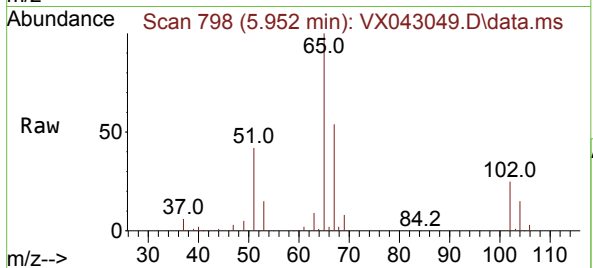

#34

1,4-Difluorobenzene

Concen: 50.000 ug/l

RT: 6.757 min Scan# 930

Delta R.T. -0.006 min

Lab File: VX043049.D

Acq: 15 Aug 2024 09:42




Tgt Ion: 114 Resp: 162363


Ion Ratio Lower Upper

114 100

63 20.4 0.0 45.0

88 15.7 0.0 36.6


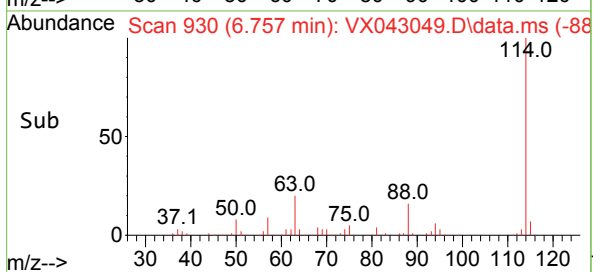
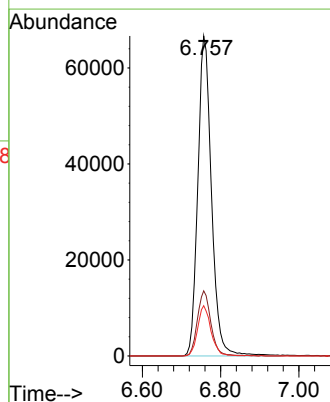
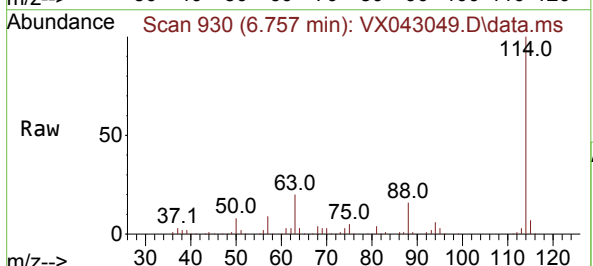




#35
Dibromofluoromethane
Concen: 48.732 ug/l
RT: 5.385 min Scan# 705
Delta R.T. 0.000 min
Lab File: VX043049.D
Acq: 15 Aug 2024 09:42




Instrument :
MSVOA_X
ClientSampleId :
VX0815MBL01


Tgt Ion:113 Resp: 48948
Ion Ratio Lower Upper
113 100
111 101.9 82.9 124.3
192 18.5 13.3 19.9

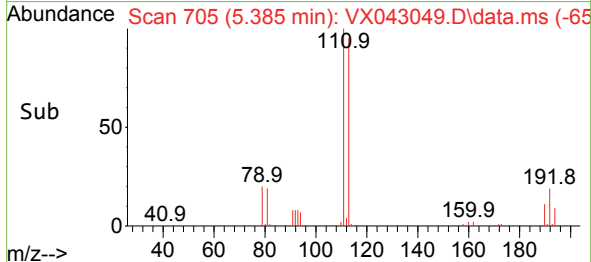

#36
1,1-Dichloropropene
Concen: 5.075 ug/l
RT: 5.544 min Scan# 731
Delta R.T. -0.146 min
Lab File: VX043049.D
Acq: 15 Aug 2024 09:42


Tgt Ion: 75 Resp: 7082
Ion Ratio Lower Upper
75 100
110 8.0 17.0 50.9#
77 0.0 24.7 37.1#

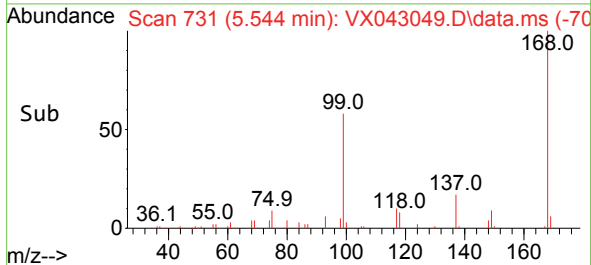






#38
Carbon Tetrachloride
Concen: 6.297 ug/l
RT: 5.544 min Scan# 71
Delta R.T. -0.128 min
Lab File: VX043049.D
Acq: 15 Aug 2024 09:42

Instrument :
MSVOA_X
ClientSampleId :
VX0815MBL01







Tgt Ion:117 Resp: 8885
Ion Ratio Lower Upper
117 100
119 4.0 78.2 117.2#
121 0.0 24.4 36.6#



#48
Methyl methacrylate
Concen: 0.515 ug/l
RT: 7.708 min Scan# 1086
Delta R.T. 0.012 min
Lab File: VX043049.D
Acq: 15 Aug 2024 09:42

Tgt Ion: 41 Resp: 165
Ion Ratio Lower Upper
41 100
69 0.0 59.2 88.8#
39 77.6 47.7 71.5#









#50
Toluene-d8
Concen: 49.548 ug/l
RT: 8.647 min Scan# 11
Delta R.T. -0.000 min
Lab File: VX043049.D
Acq: 15 Aug 2024 09:42




Instrument :
MSVOA_X
ClientSampleId :
VX0815MBL01


Tgt Ion: 98 Resp: 192113
Ion Ratio Lower Upper
98 100
100 67.0 53.1 79.7

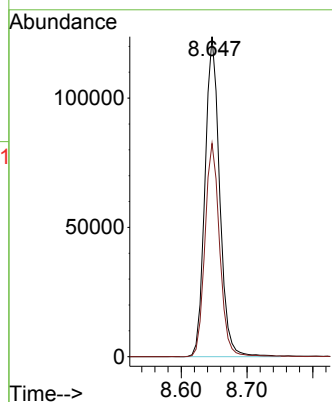

#51
4-Methyl-2-Pentanone
Concen: 0.352 ug/l
RT: 8.586 min Scan# 1230
Delta R.T. 0.006 min
Lab File: VX043049.D
Acq: 15 Aug 2024 09:42

Tgt Ion: 43 Resp: 709
Ion Ratio Lower Upper
43 100
58 18.5 30.4 45.6#



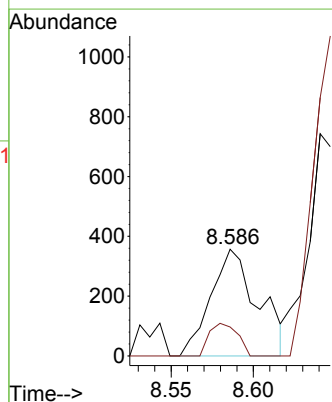





#62
4-Bromofluorobenzene
Concen: 46.750 ug/l
RT: 11.079 min Scan# 1639
Delta R.T. 0.000 min
Lab File: VX043049.D
Acq: 15 Aug 2024 09:42




Instrument :
MSVOA_X
ClientSampleId :
VX0815MBL01


Tgt Ion: 95 Resp: 65727
Ion Ratio Lower Upper
95 100
174 77.4 0.0 135.6
176 73.8 0.0 131.0

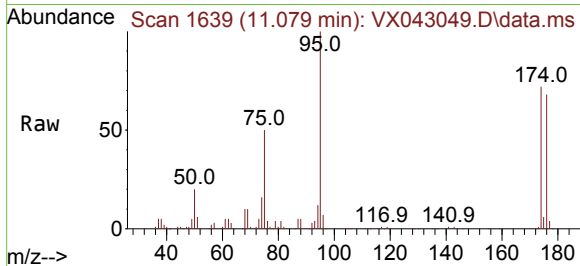

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 10.055 min Scan# 1471
Delta R.T. -0.000 min
Lab File: VX043049.D
Acq: 15 Aug 2024 09:42

Tgt Ion: 117 Resp: 141491
Ion Ratio Lower Upper
117 100
82 52.4 46.2 69.4
119 32.9 25.5 38.3



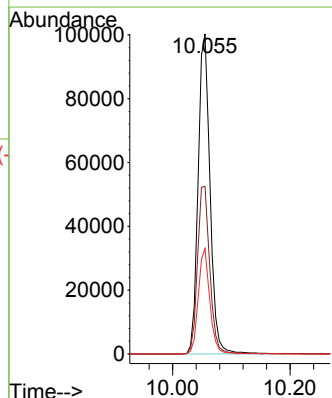
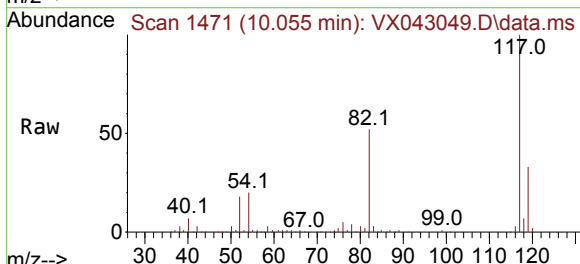




#68
m/p-Xylenes
Concen: 0.254 ug/l
RT: 10.311 min Scan# 1511
Delta R.T. 0.012 min
Lab File: VX043049.D
Acq: 15 Aug 2024 09:42




Instrument :
MSVOA_X
ClientSampleId :
VX0815MBL01


Tgt Ion:106 Resp: 519
Ion Ratio Lower Upper
106 100
91 231.8 165.5 248.3

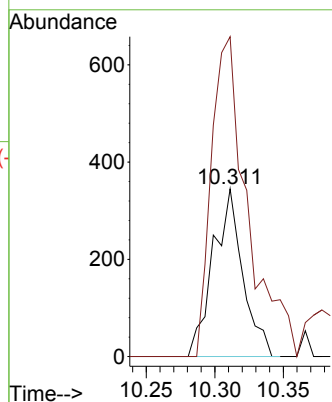

#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 12.024 min Scan# 1794
Delta R.T. -0.000 min
Lab File: VX043049.D
Acq: 15 Aug 2024 09:42

Tgt Ion:152 Resp: 63156
Ion Ratio Lower Upper
152 100
115 58.9 43.3 129.9
150 157.5 0.0 345.0

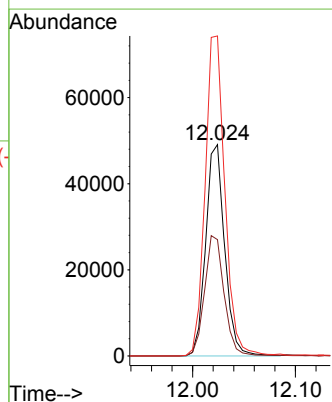



#76

1,2,3-Trichloropropane

Concen: 22.593 ug/l

RT: 11.079 min Scan# 1639

Delta R.T. -0.159 min

Lab File: VX043049.D

Acq: 15 Aug 2024 09:42

Instrument :

MSVOA_X

ClientSampleId :





VX0815MBL01

Tgt Ion: 75 Resp: 32702

Ion Ratio Lower Upper

75 100

77 1.5 19.1 57.5#

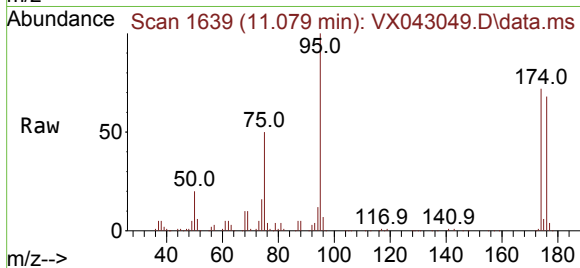

#81

trans-1,4-Dichloro-2-butene

Concen: 49.281 ug/l

RT: 11.079 min Scan# 1639

Delta R.T. 0.061 min

Lab File: VX043049.D

Acq: 15 Aug 2024 09:42




Tgt Ion: 75 Resp: 32702


Ion Ratio Lower Upper

75 100

53 0.0 90.5 135.7#


89 0.0 36.9 55.3#

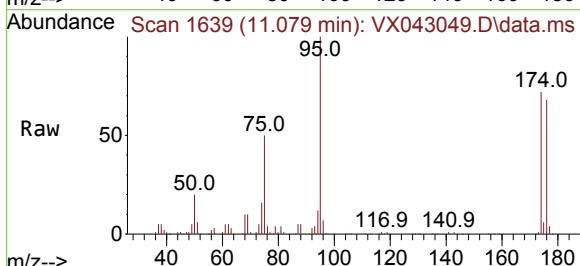





#82
4-Chlorotoluene
Concen: 0.279 ug/l
RT: 11.463 min Scan# 1702
Delta R.T. 0.012 min
Lab File: VX043049.D
Acq: 15 Aug 2024 09:42


Instrument :
MSVOA_X
ClientSampleId :
VX0815MBL01

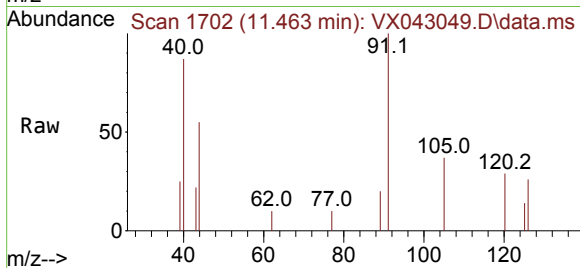



Tgt Ion: 91 Resp: 1062
Ion Ratio Lower Upper
91 100
126 24.5 14.2 42.6

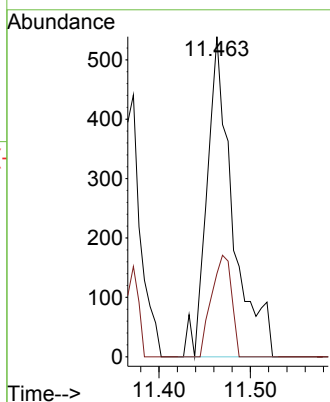


#87
1,3-Dichlorobenzene
Concen: 0.310 ug/l
RT: 11.975 min Scan# 1786
Delta R.T. 0.006 min
Lab File: VX043049.D
Acq: 15 Aug 2024 09:42

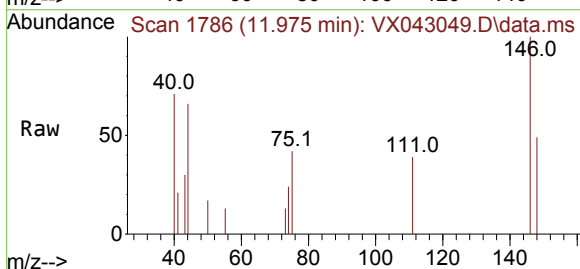


Tgt Ion: 146 Resp: 646
Ion Ratio Lower Upper
146 100
111 35.9 22.1 66.1
148 54.8 31.8 95.3

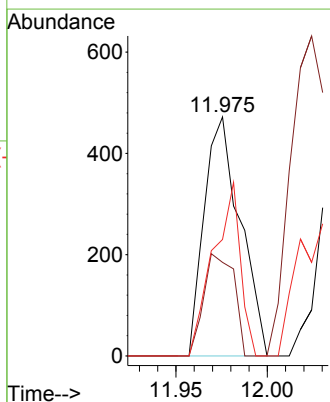






#88
1,4-Dichlorobenzene
Concen: 0.303 ug/l
RT: 11.975 min Scan# 1786
Delta R.T. -0.067 min
Lab File: VX043049.D
Acq: 15 Aug 2024 09:42

Instrument :
MSVOA_X
ClientSampleId :
VX0815MBL01



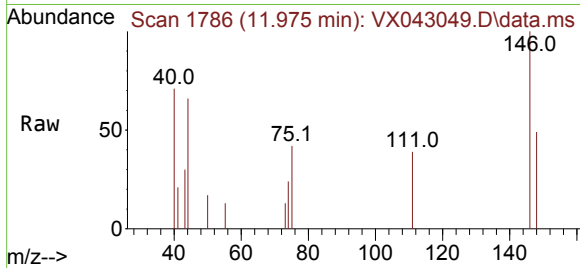



Tgt Ion:146 Resp: 646
Ion Ratio Lower Upper
146 100
111 35.9 21.3 63.7
148 54.8 31.8 95.4

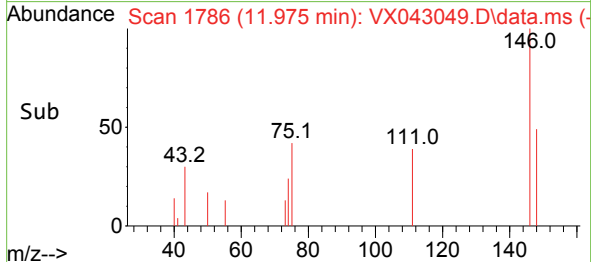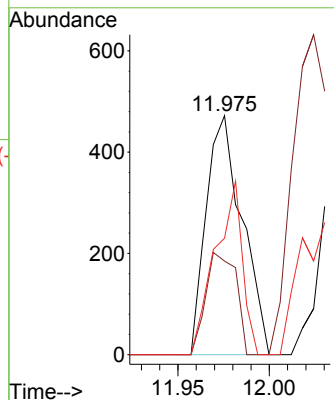

#89
n-Butylbenzene
Concen: 0.307 ug/l
RT: 12.335 min Scan# 1845
Delta R.T. 0.006 min
Lab File: VX043049.D
Acq: 15 Aug 2024 09:42

Tgt Ion: 91 Resp: 1084
Ion Ratio Lower Upper
91 100
92 52.0 27.4 82.0
134 17.3 12.6 37.8

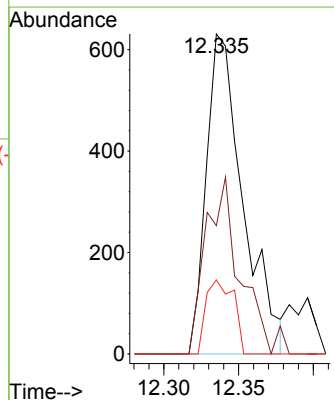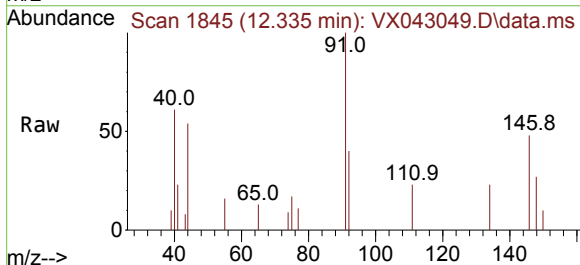



#91

1,2-Dichlorobenzene

Concen: 0.222 ug/l

RT: 12.335 min Scan# 1845

Delta R.T. -0.000 min

Lab File: VX043049.D

Acq: 15 Aug 2024 09:42

Instrument :

MSVOA_X

ClientSampleId :

VX0815MBL01





Tgt Ion:146 Resp: 465

Ion Ratio Lower Upper

146 100

111 45.2 22.4 67.0

148 64.7 31.6 95.0



#93

1,2,4-Trichlorobenzene

Concen: 0.874 ug/l

RT: 13.591 min Scan# 2051

Delta R.T. 0.006 min

Lab File: VX043049.D

Acq: 15 Aug 2024 09:42




Tgt Ion:180 Resp: 1032


Ion Ratio Lower Upper

180 100

182 87.8 48.3 144.8

145 25.8 18.0 54.0





#94

Hexachlorobutadiene

Concen: 0.295 ug/l

RT: 13.719 min Scan# 2072

Delta R.T. -0.006 min

Lab File: VX043049.D

Acq: 15 Aug 2024 09:42





Instrument :

MSVOA_X

ClientSampleId :

VX0815MBL01

Tgt Ion:225	Resp:	130
Ion	Ratio	Lower Upper
225	100	
223	53.1	31.1 93.2
227	44.6	32.5 97.5

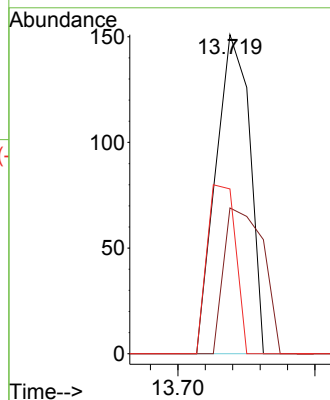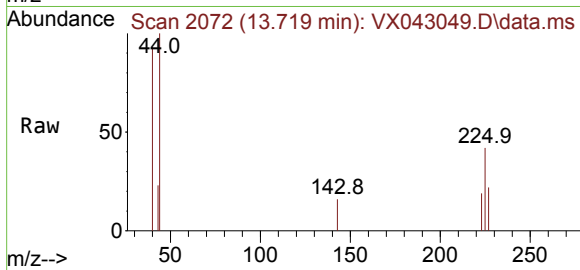

#95

Naphthalene

Concen: 1.368 ug/l




RT: 13.780 min Scan# 2082


Delta R.T. 0.006 min

Lab File: VX043049.D

Acq: 15 Aug 2024 09:42


Tgt Ion:128	Resp:	6382
Ion	Ratio	Lower Upper
128	100	
127	11.6	10.3 15.5
129	11.0	8.8 13.2

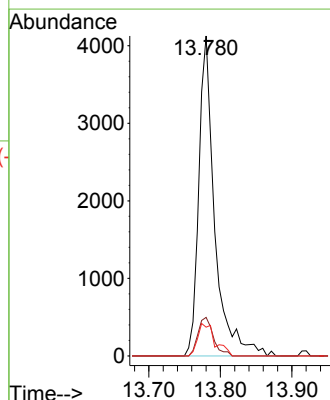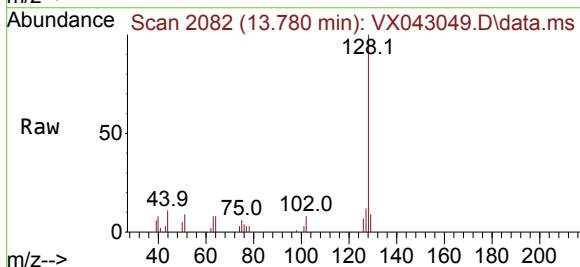



#96
 1,2,3-Trichlorobenzene
 Concen: 0.882 ug/l
 RT: 13.963 min Scan# 2112
 Delta R.T. -0.000 min
 Lab File: VX043049.D
 Acq: 15 Aug 2024 09:42

Instrument :
 MSVOA_X
 ClientSampleId :
 VX0815MBL01



Tgt Ion:	180	Resp:	1066
Ion	Ratio	Lower	Upper
180	100		
182	98.9	46.9	140.6
145	30.1	17.8	53.5

