
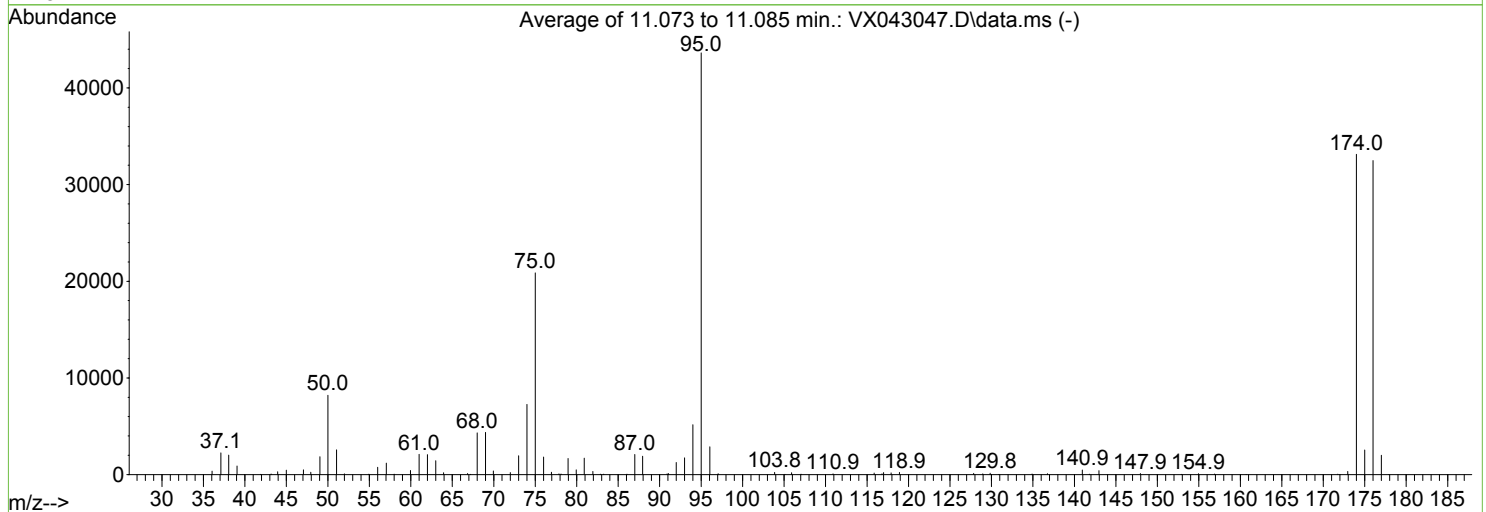


Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX081524\
Data File : VX043047.D
Acq On : 15 Aug 2024 08:06
Operator : JC/MD
Sample : BFB
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X081424W.M
Title : SW846 8260
Last Update : Thu Aug 15 04:22:11 2024

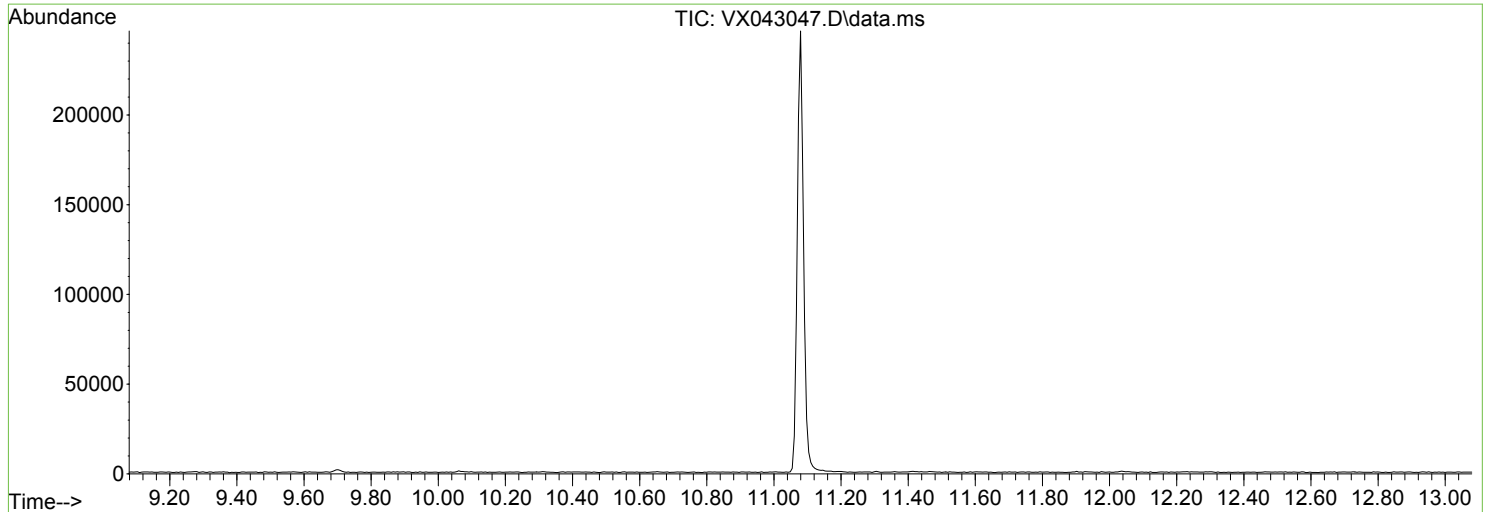

AutoFind: Scans 1638, 1639, 1640; Background Corrected with Scan 1632

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	18.8	8209	PASS
75	95	30	60	47.8	20867	PASS
95	95	100	100	100.0	43629	PASS
96	95	5	9	6.6	2884	PASS
173	174	0.00	2	1.0	325	PASS
174	95	50	100	75.9	33133	PASS
175	174	5	9	7.7	2556	PASS
176	174	95	101	98.1	32496	PASS
177	176	5	9	6.1	1997	PASS