

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX081525\
 Data File : VX047359.D
 Acq On : 15 Aug 2025 14:00
 Operator : JC/MD
 Sample : VX0815MBL01
 Misc : 5.00g/10mL/100uL/5.00mL/MSVOA_X/MEOH
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VX0815MBL01

Quant Time: Aug 18 04:32:27 2025
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X081525W.M
 Quant Title : SW846 8260
 QLast Update : Mon Aug 18 04:18:28 2025
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Pentafluorobenzene	5.562	168	297007	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	6.769	114	578456	50.000	ug/l	0.00
63) Chlorobenzene-d5	10.055	117	574386	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	12.018	152	286462	50.000	ug/l	0.00

System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	5.964	65	236619	56.925	ug/l	0.00
Spiked Amount	50.000	Range	78 - 117	Recovery	=	113.840%
35) Dibromofluoromethane	5.397	113	196532	52.349	ug/l	0.00
Spiked Amount	50.000	Range	75 - 124	Recovery	=	104.700%
50) Toluene-d8	8.653	98	715242	53.302	ug/l	0.00
Spiked Amount	50.000	Range	92 - 112	Recovery	=	106.600%
62) 4-Bromofluorobenzene	11.079	95	300945	60.776	ug/l	0.00
Spiked Amount	50.000	Range	83 - 123	Recovery	=	121.560%


Target Compounds	Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX081525\
Data File : VX047359.D
Acq On : 15 Aug 2025 14:00
Operator : JC/MD
Sample : VX0815MBL01
Misc : 5.00g/10mL/100uL/5.00mL/MSVOA_X/MEOH
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VX0815MBL01

Quant Time: Aug 18 04:32:27 2025
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X081525W.M
Quant Title : SW846 8260
QLast Update : Mon Aug 18 04:18:28 2025
Response via : Initial Calibration




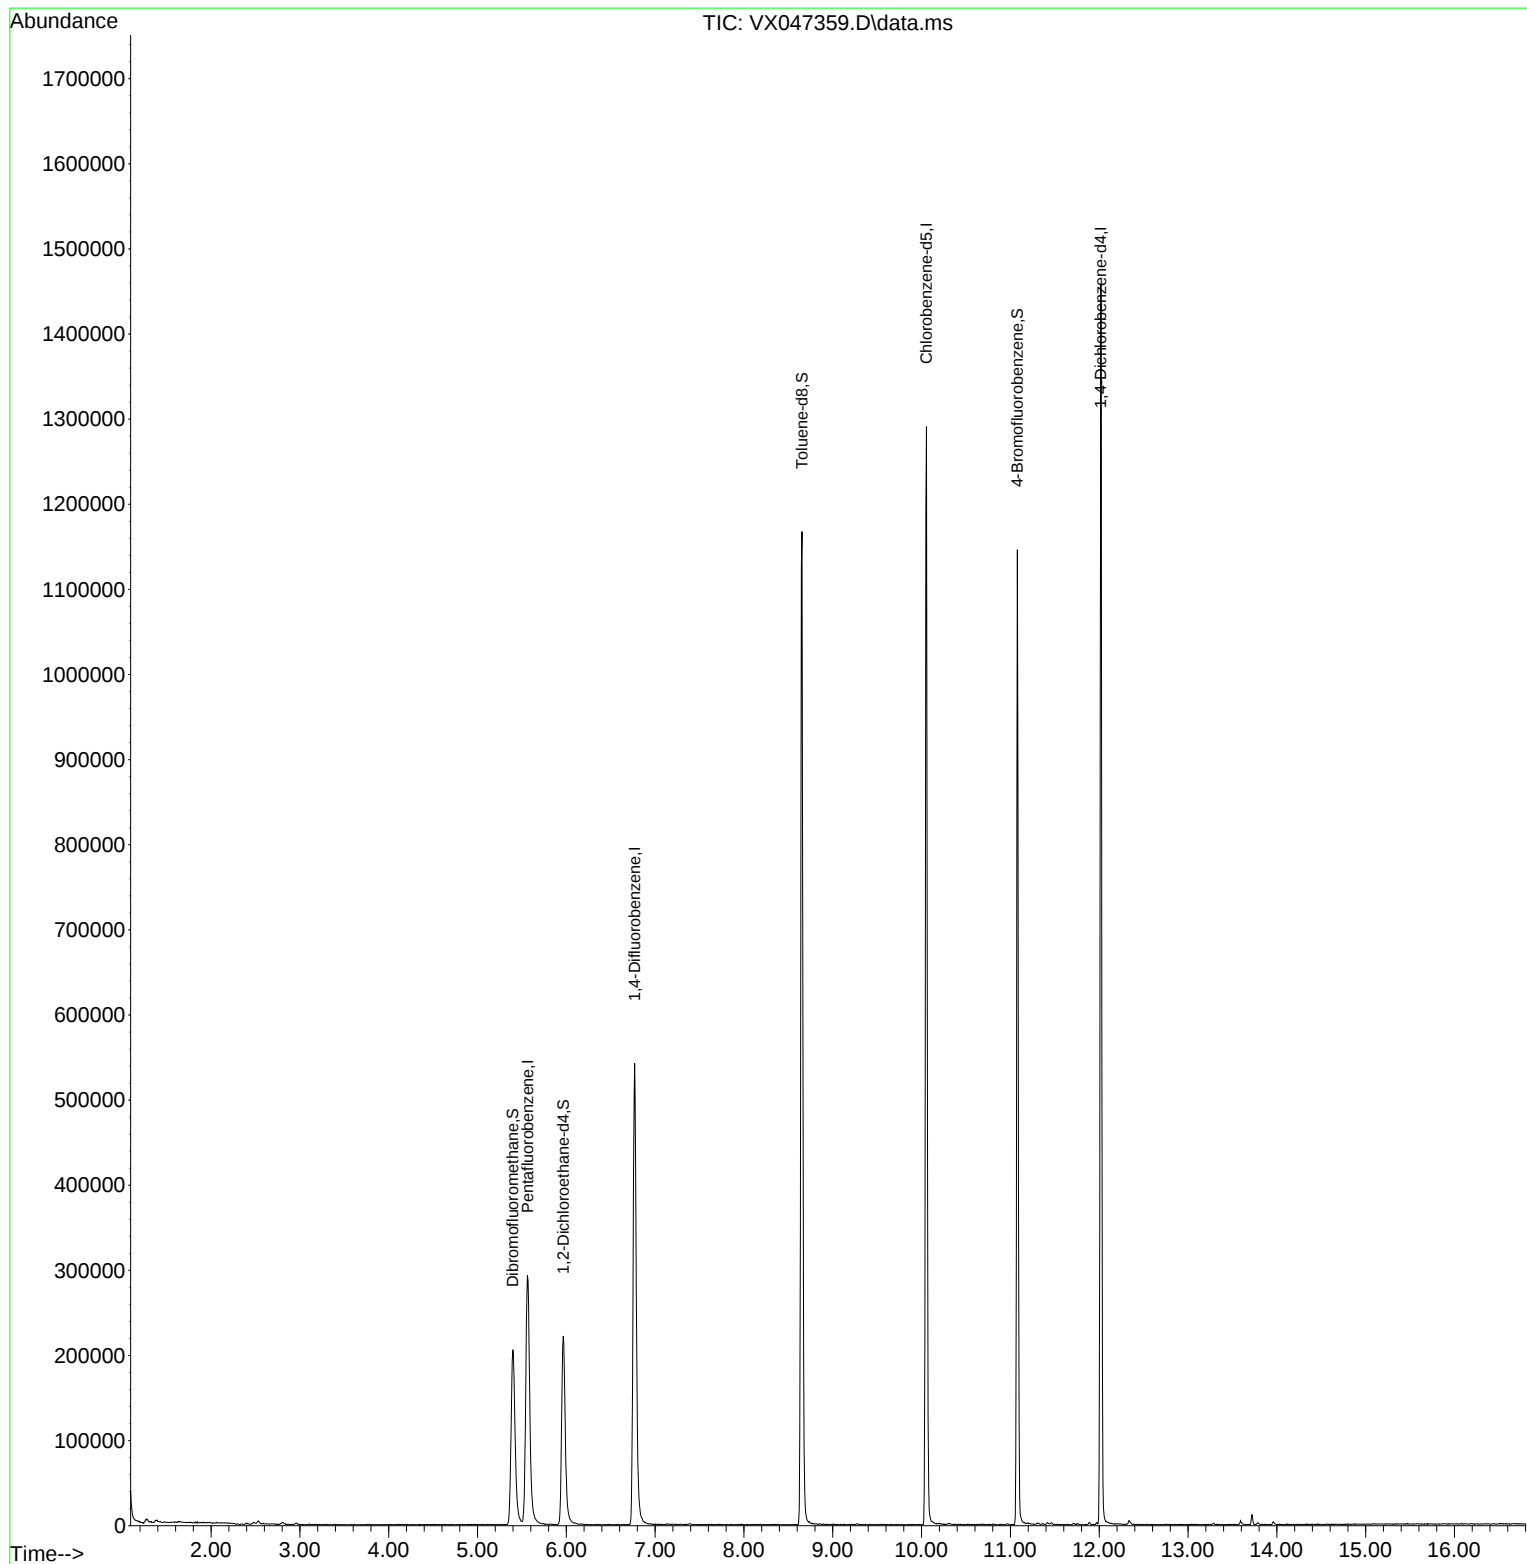


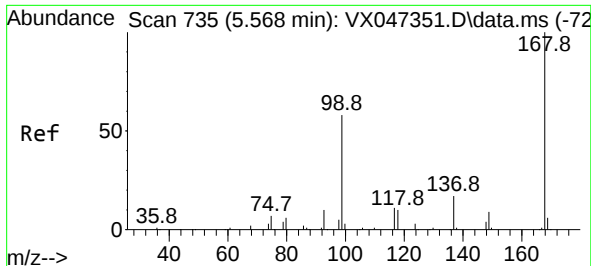

#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 5.562 min Scan# 71
Delta R.T. -0.006 min
Lab File: VX047359.D
Acq: 15 Aug 2025 14:00




Instrument :
MSVOA_X
ClientSampleId :
VX0815MBL01


Tgt Ion:168 Resp: 297007
Ion Ratio Lower Upper
168 100
99 61.4 47.9 71.9

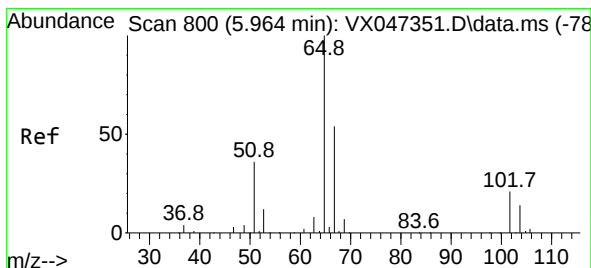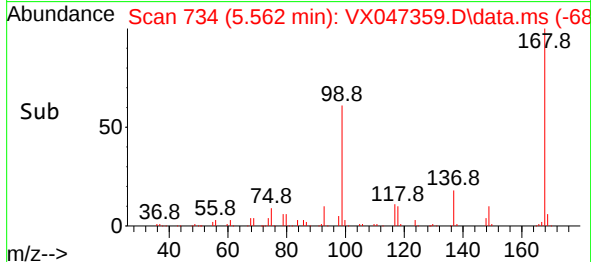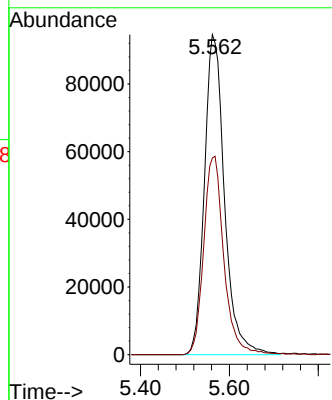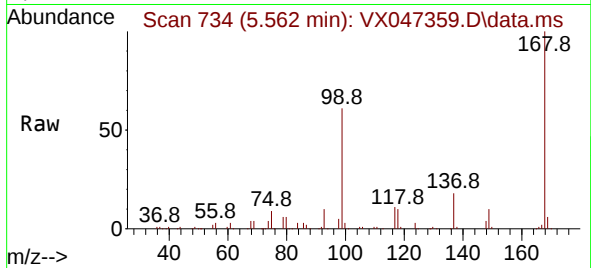

#33
1,2-Dichloroethane-d4
Concen: 56.925 ug/l
RT: 5.964 min Scan# 800
Delta R.T. -0.000 min
Lab File: VX047359.D
Acq: 15 Aug 2025 14:00

Tgt Ion: 65 Resp: 236619
Ion Ratio Lower Upper
65 100
67 51.3 0.0 106.0


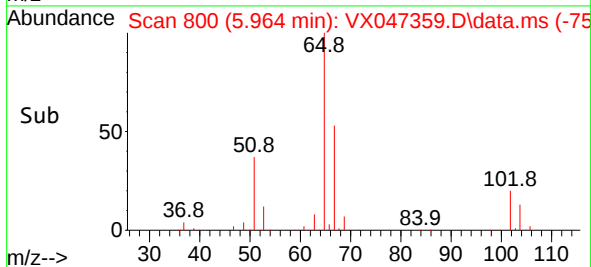
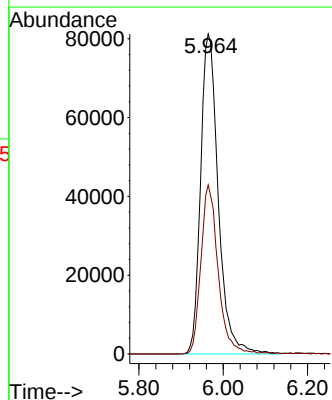
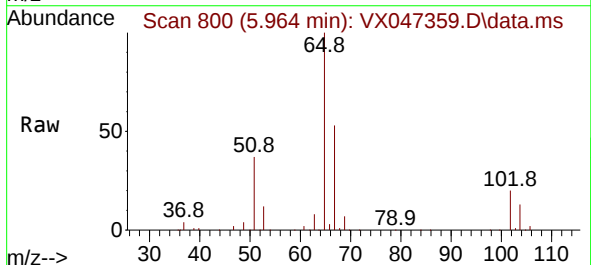


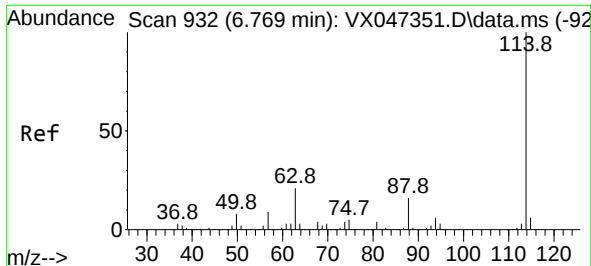

#34
1,4-Difluorobenzene
Concen: 50.000 ug/l
RT: 6.769 min Scan# 911
Delta R.T. -0.000 min
Lab File: VX047359.D
Acq: 15 Aug 2025 14:00




Instrument :
MSVOA_X
ClientSampleId :
VX0815MBL01


Tgt Ion:114 Resp: 578456
Ion Ratio Lower Upper
114 100
63 21.4 0.0 42.4
88 16.8 0.0 33.0

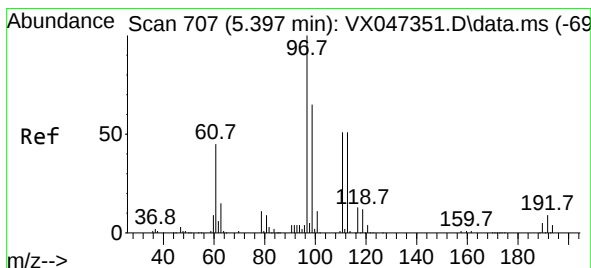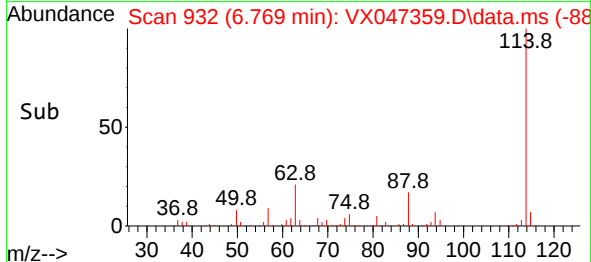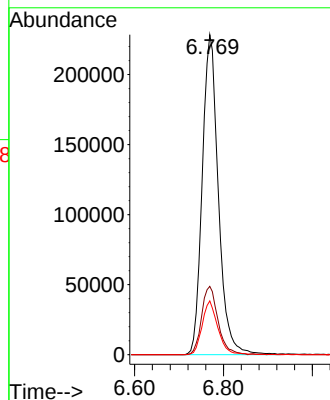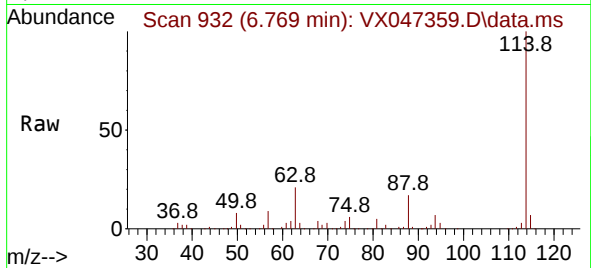

#35
Dibromofluoromethane
Concen: 52.349 ug/l
RT: 5.397 min Scan# 707
Delta R.T. -0.000 min
Lab File: VX047359.D
Acq: 15 Aug 2025 14:00

Tgt Ion:113 Resp: 196532
Ion Ratio Lower Upper
113 100
111 103.4 81.4 122.2
192 18.4 14.1 21.1


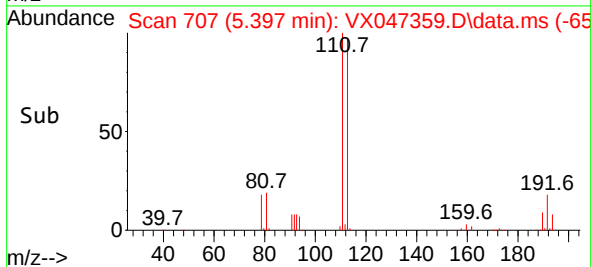
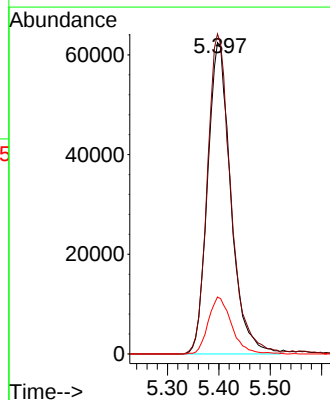
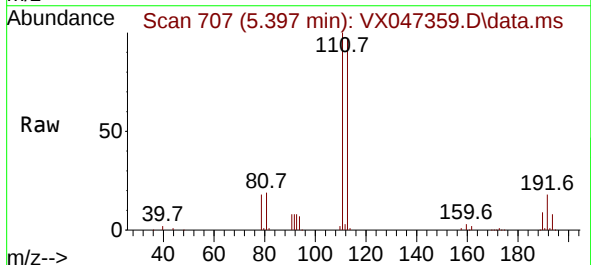


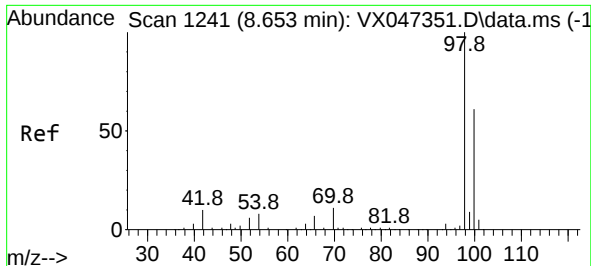

#50
Toluene-d8
Concen: 53.302 ug/l
RT: 8.653 min Scan# 11
Delta R.T. -0.000 min
Lab File: VX047359.D
Acq: 15 Aug 2025 14:00




Instrument :
MSVOA_X
ClientSampleId :
VX0815MBL01


Tgt Ion: 98 Resp: 715242
Ion Ratio Lower Upper
98 100
100 66.7 53.9 80.9

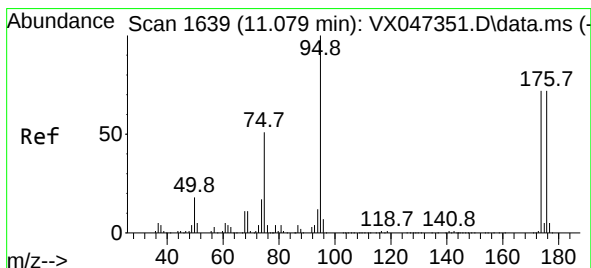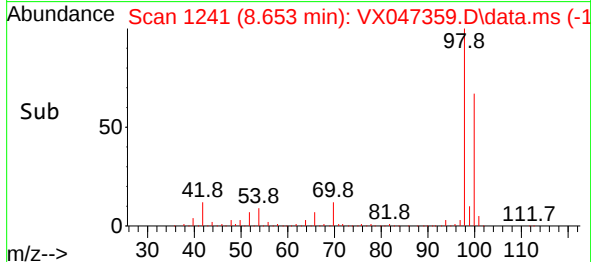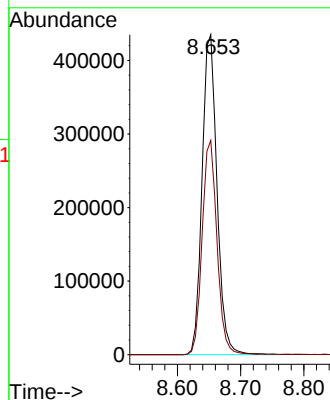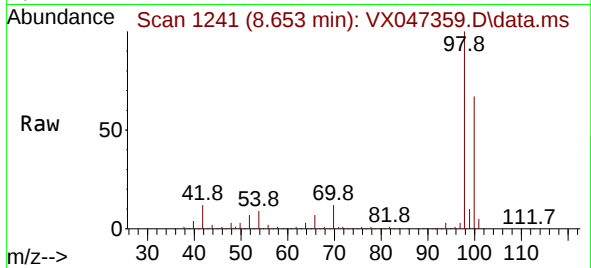

#62
4-Bromofluorobenzene
Concen: 60.776 ug/l
RT: 11.079 min Scan# 1639
Delta R.T. -0.000 min
Lab File: VX047359.D
Acq: 15 Aug 2025 14:00

Tgt Ion: 95 Resp: 300945
Ion Ratio Lower Upper
95 100
174 72.7 0.0 148.0
176 69.7 0.0 145.4


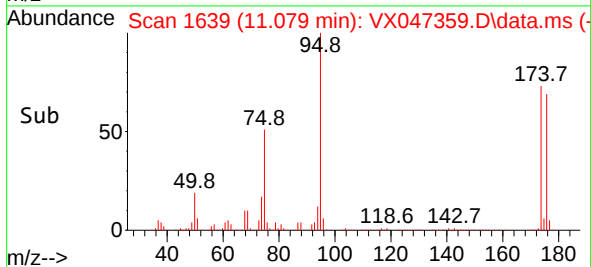
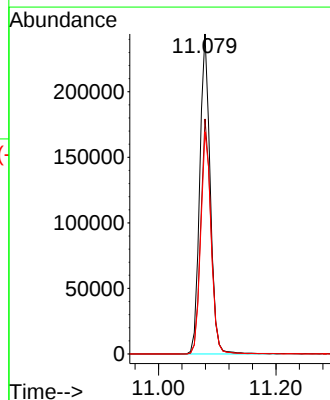
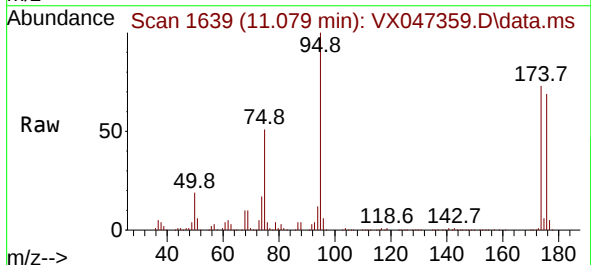


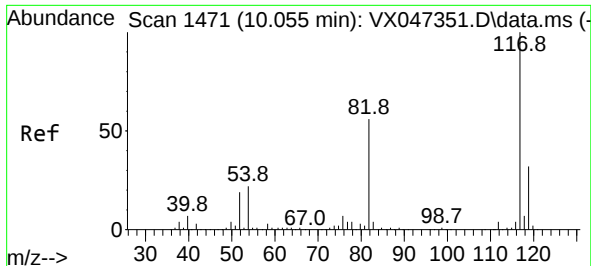

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 10.055 min Scan# 1471
Delta R.T. -0.000 min
Lab File: VX047359.D
Acq: 15 Aug 2025 14:00

Instrument :
MSVOA_X
ClientSampleId :
VX0815MBL01

Tgt Ion:117 Resp: 574386
Ion Ratio Lower Upper
117 100
82 56.5 45.0 67.4
119 32.3 25.8 38.8

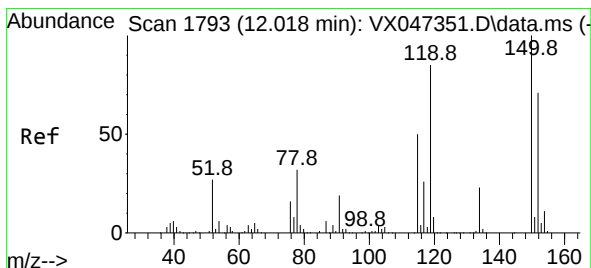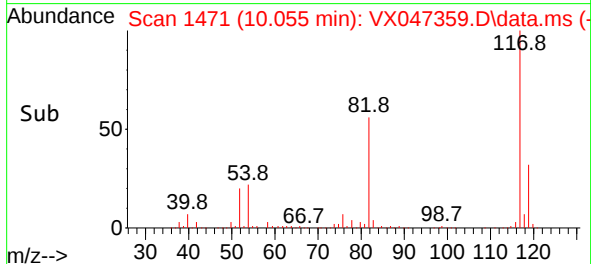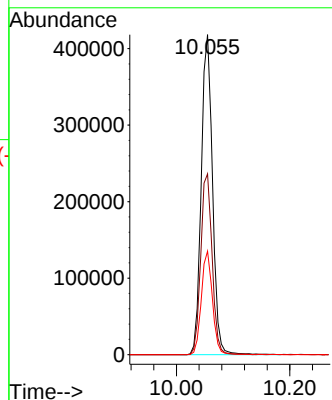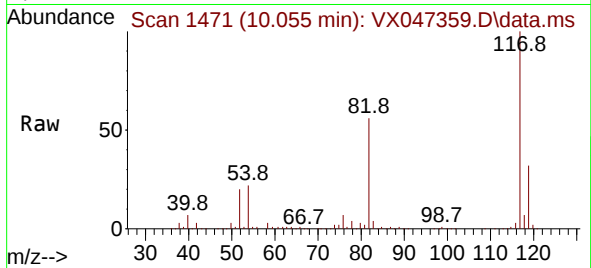

#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 12.018 min Scan# 1793
Delta R.T. -0.000 min
Lab File: VX047359.D
Acq: 15 Aug 2025 14:00

Tgt Ion:152 Resp: 286462
Ion Ratio Lower Upper
152 100
115 61.9 44.6 133.8
150 159.0 0.0 349.8

