

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX081525\
 Data File : VX047368.D
 Acq On : 15 Aug 2025 17:19
 Operator : JC/MD
 Sample : Q2837-01
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 TW-WTS-13

Integration Parameters: RTEINT.P

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X081525W.M
 Title : SW846 8260

Signal : TIC: VX047368.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	2.392	207	214	233	rBV	214104	464733	21.52%	3.510%
2	5.403	695	708	724	rBV3	195685	622816	28.84%	4.704%
3	5.568	724	735	760	rVB	325624	1024582	47.45%	7.739%
4	5.970	788	801	812	rBV	250485	724599	33.55%	5.473%
5	6.769	921	932	954	rBV	612754	1551295	71.84%	11.717%
6	8.653	1234	1241	1249	rBV	1346881	2159478	100.00%	16.311%
7	8.726	1249	1253	1264	rVB	20464	40461	1.87%	0.306%
8	10.055	1465	1471	1488	rBV	1461267	2022437	93.65%	15.276%
9	10.195	1488	1494	1502	rVB	25621	38464	1.78%	0.291%
10	10.305	1508	1512	1521	rVB	14068	21940	1.02%	0.166%
11	11.079	1634	1639	1655	rBV	1260050	1594324	73.83%	12.042%
12	12.018	1788	1793	1801	rBV	1659626	2042053	94.56%	15.424%
13	12.244	1824	1830	1840	rVB	103871	141641	6.56%	1.070%
14	12.414	1853	1858	1863	rBV	38559	51074	2.37%	0.386%
15	13.426	2019	2024	2029	rBV2	22942	31658	1.47%	0.239%
16	13.774	2076	2081	2092	rBV	384979	485403	22.48%	3.666%
17	13.865	2092	2096	2104	rVB	25163	35213	1.63%	0.266%
18	14.634	2218	2222	2231	rVB	63328	85008	3.94%	0.642%
19	14.780	2241	2246	2252	rBV	74381	102204	4.73%	0.772%




Sum of corrected areas: 13239383

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX081525\
Data File : VX047368.D
Acq On : 15 Aug 2025 17:19
Operator : JC/MD
Sample : Q2837-01
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 24 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
TW-WTS-13

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X081525W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

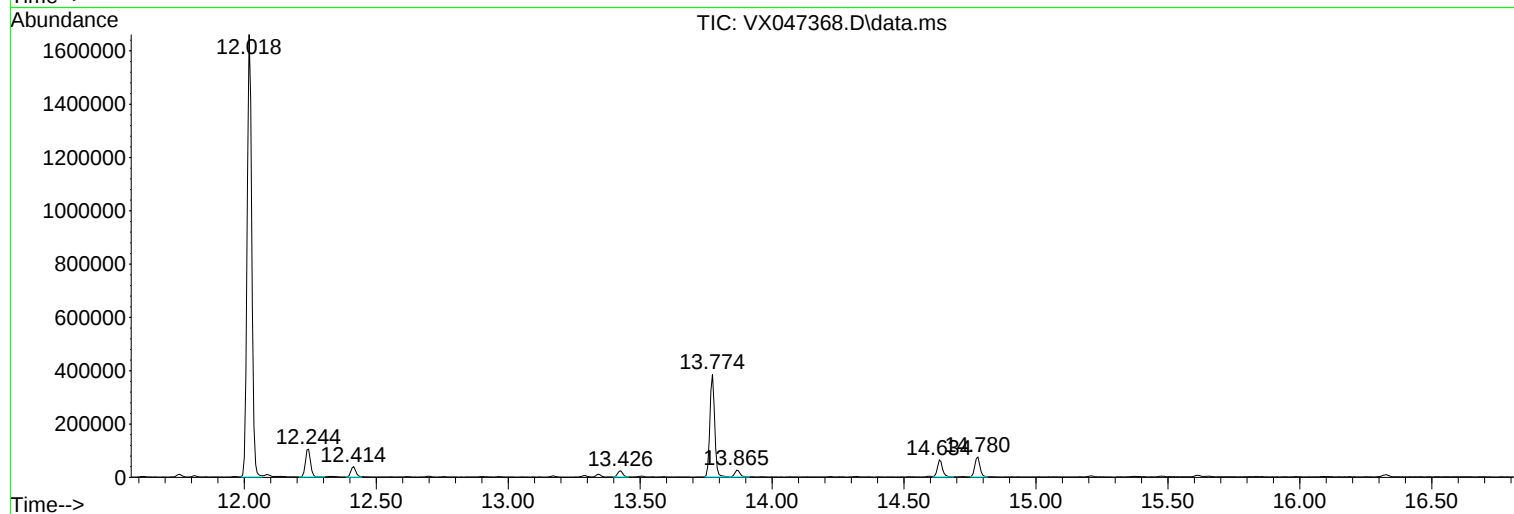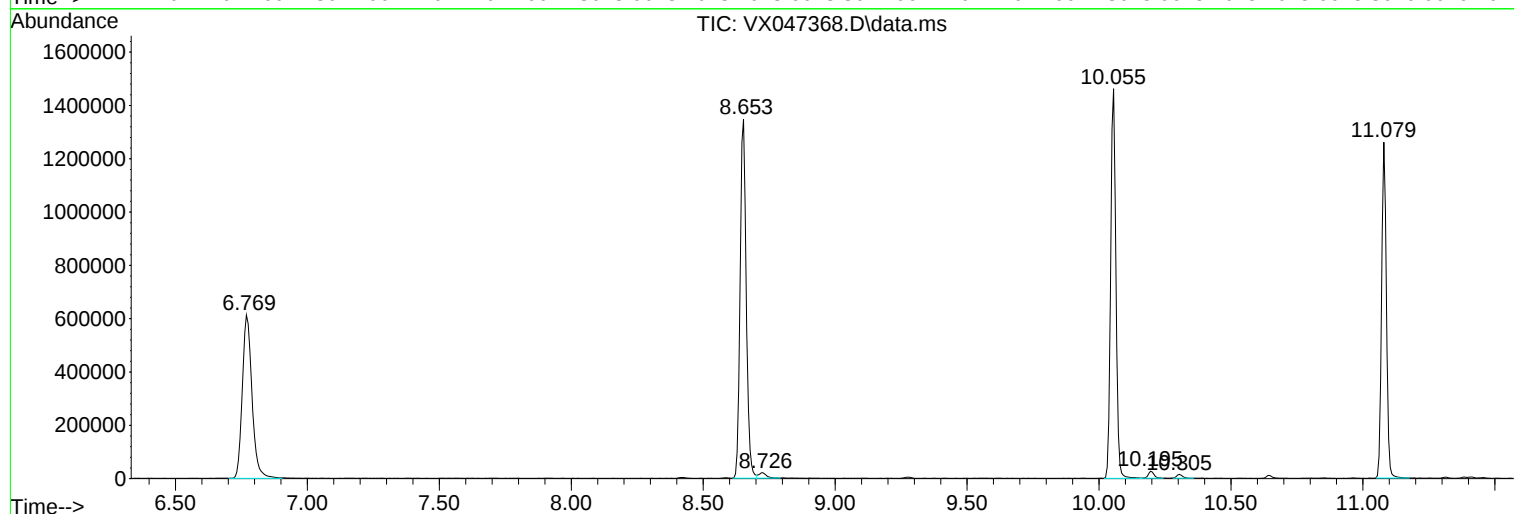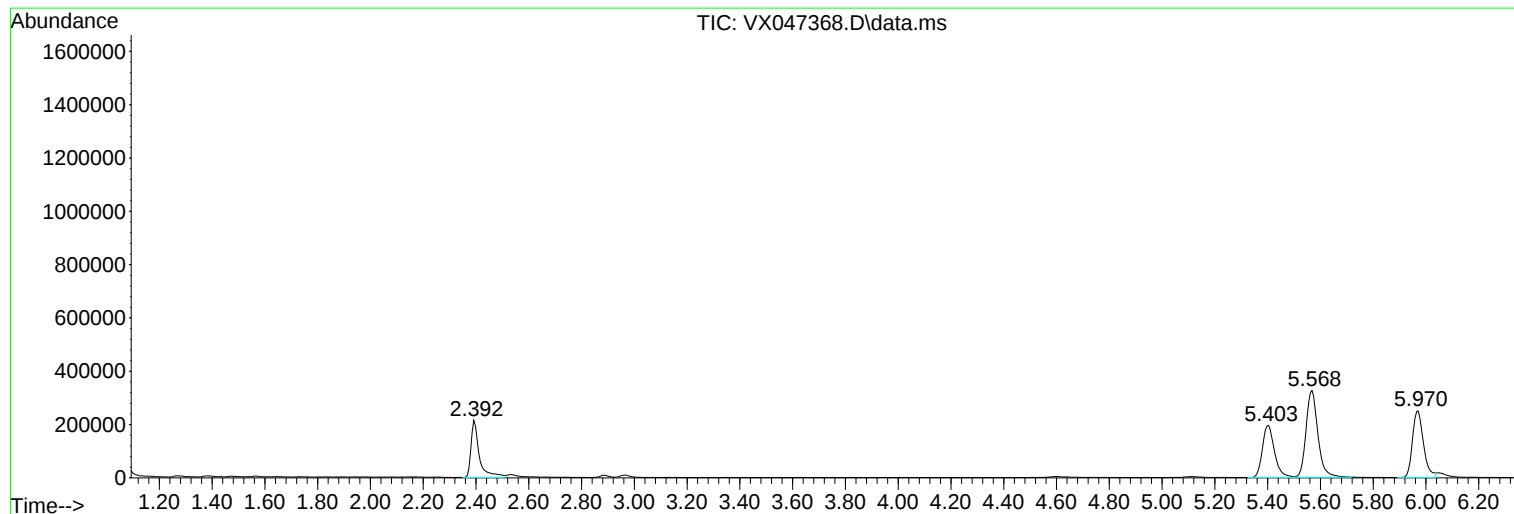

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX081525\
Data File : VX047368.D
Acq On : 15 Aug 2025 17:19
Operator : JC/MD
Sample : Q2837-01
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 24 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
TW-WTS-13

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X081525W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX081525\
Data File : VX047368.D
Acq On : 15 Aug 2025 17:19
Operator : JC/MD
Sample : Q2837-01
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 24 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
TW-WTS-13

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X081525W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc