

Data Path : Z:\VOASRV\HPCHEM1\MSVOA X\DATA\VX081619\
 Data File : VX011603.D
 Acq On : 17 Aug 2019 01:00
 Operator : JC/SP
 Sample : K4272-04
 Misc : 5.0mL/MSVOA X/WATER
 ALS Vial : 37 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 2S-G3-(0)

Quant Time: Aug 19 04:02:28 2019
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82X081519W.M
 Quant Title : SW846 8260
 QLast Update : Fri Aug 16 04:15:26 2019
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) Pentafluorobenzene	5.66	168	440056	50.00	ug/l	0.00
34) 1,4-Difluorobenzene	6.85	114	609673	50.00	ug/l	0.00
63) Chlorobenzene-d5	10.11	117	541402	50.00	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	12.08	152	261139	50.00	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	6.06	65	209559	51.35	ug/l	0.00
Spiked Amount 50.000			Recovery	=	102.70%	
35) Dibromofluoromethane	5.49	113	182569	45.78	ug/l	0.00
Spiked Amount 50.000			Recovery	=	91.56%	
50) Toluene-d8	8.71	98	699621	56.31	ug/l	0.00
Spiked Amount 50.000			Recovery	=	112.62%	
62) 4-Bromofluorobenzene	11.13	95	242045	46.15	ug/l	0.00
Spiked Amount 50.000			Recovery	=	92.30%	
Target Compounds						
16) Acetone	2.43	43	11628	5.667	ug/l	98
20) Methylene Chloride	2.85	84	10702	2.484	ug/l	95
43) Isopropyl Acetate	6.44	43	80277	8.580	ug/l	100


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA X\DATA\VX081619\
Data File : VX011603.D
Acq On : 17 Aug 2019 01:00
Operator : JC/SP
Sample : K4272-04
Misc : 5.0mL/MSVOA X/WATER
ALS Vial : 37 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
2S-G3-(0)

Quant Time: Aug 19 04:02:28 2019
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_X\METHOD\82X081519W.M
Quant Title : SW846 8260
QLast Update : Fri Aug 16 04:15:26 2019
Response via : Initial Calibration

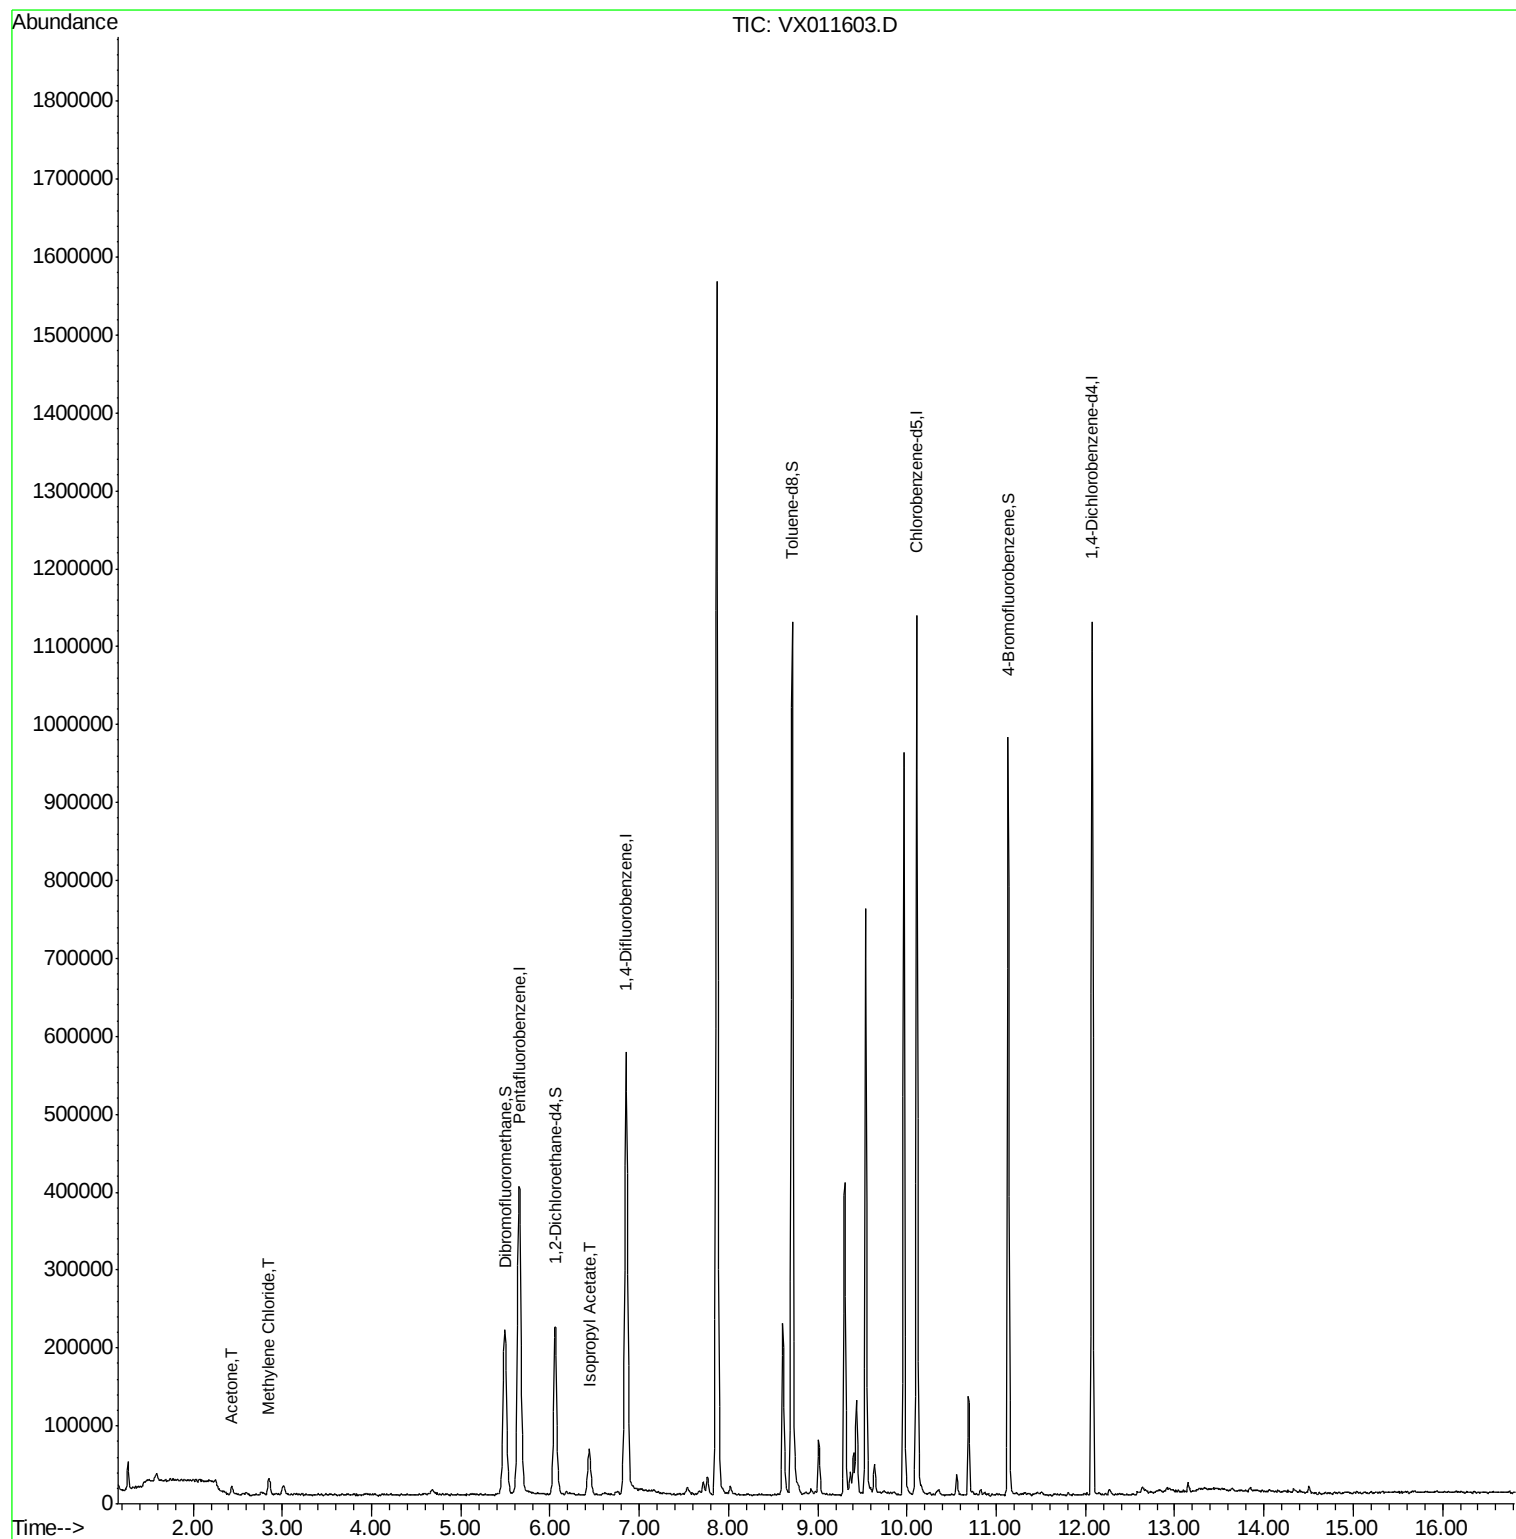

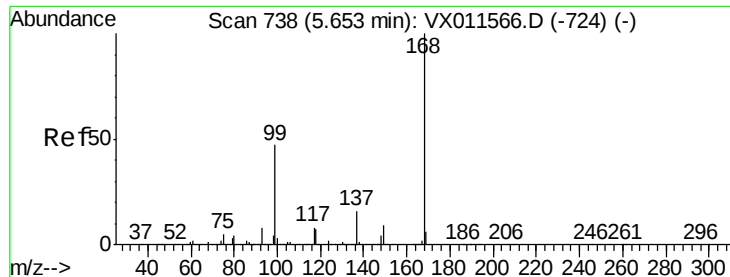

#1

Pentafluorobenzene

Concen: 50.000 ug/l

RT: 5.66 min Scan# 739

Delta R.T. 0.01 min

Lab File: VX011603.D

Acq: 17 Aug 2019 01:00

Instrument :

MSVOA_X

ClientSampleId :


2S-G3-(0)

Tot Ion:168 Resp: 440056

Ion Ratio Lower Upper

168 100

99 45.9 37.3 55.9

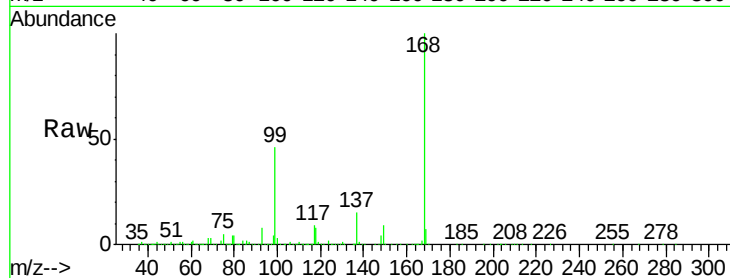

Abundance Ion 167.90 (167.60 to 168.60): V

Ion 98.90 (98.60 to 99.60): VX0

5.66



150000

100000

50000

0

Time-->

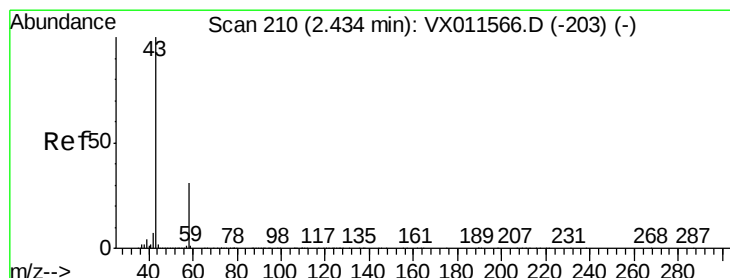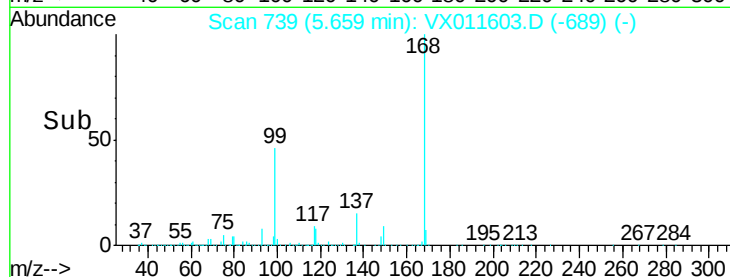

#16

Acetone

Concen: 5.667 ug/l

RT: 2.43 min Scan# 210

Delta R.T. 0.00 min

Lab File: VX011603.D


Acq: 17 Aug 2019 01:00

Tgt Ion: 43 Resp: 11628

Ion Ratio Lower Upper

43 100

58 30.4 25.2 37.8

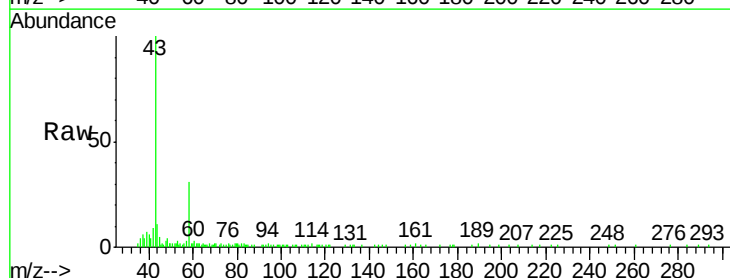

Abundance Ion 43.00 (42.70 to 43.70): VX0

Ion 58.00 (57.70 to 58.70): VX0

2.43

8000


6000


4000

2000

0

Time-->




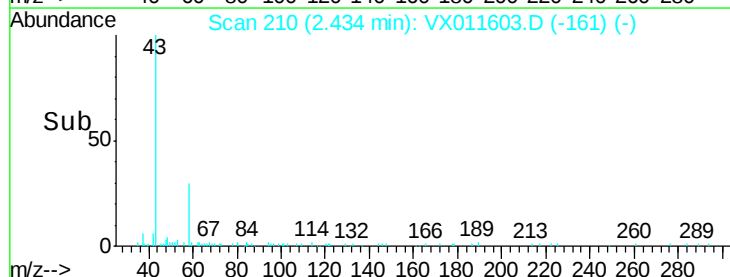


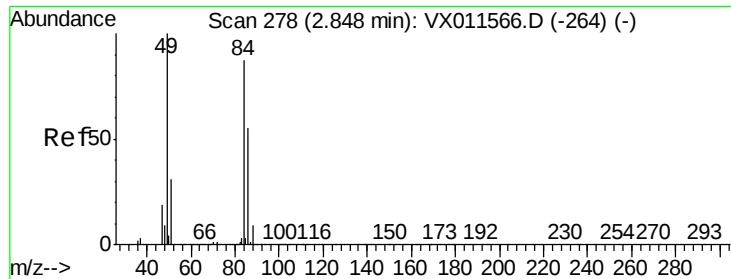

#20
Methvlene Chloride
Concen: 2.484 ug/l
RT: 2.85 min Scan# 278
Delta R.T. 0.00 min
Lab File: VX011603.D
Acq: 17 Aug 2019 01:00




Instrument :
MSVOA_X
ClientSampleId :
2S-G3-(0)


Tot Ion:	84	Resp:	10702
Ion	Ratio	Lower	Upper
84	100		
49	113.3	92.4	138.6
51	39.8	28.5	42.7
86	70.9	51.0	76.6

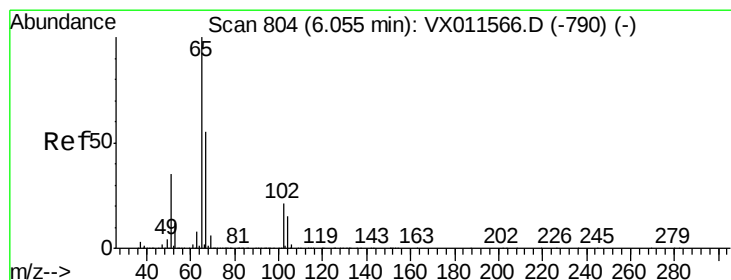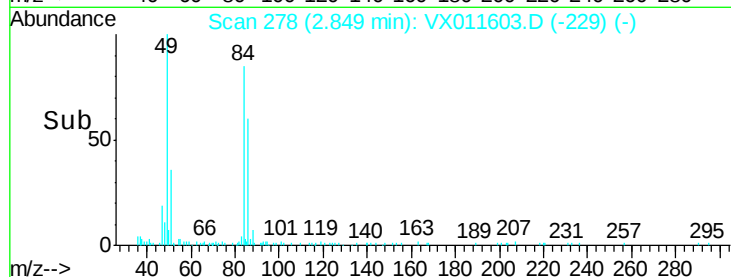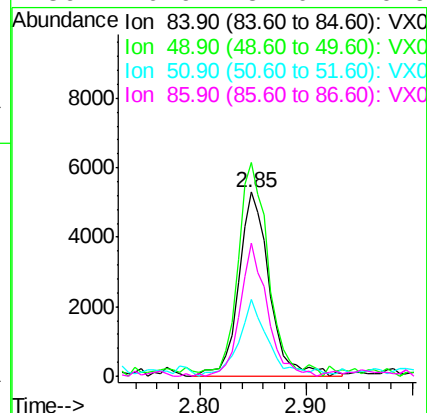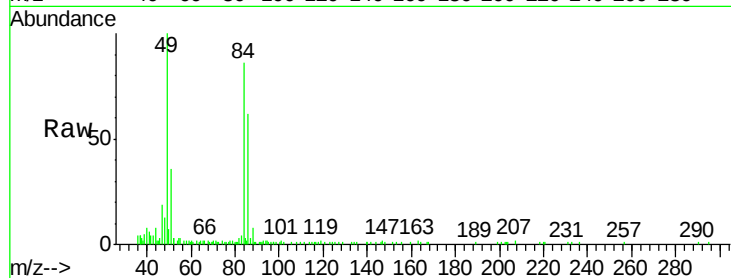

#33
1,2-Dichloroethane-d4
Concen: 51.351 ug/l
RT: 6.06 min Scan# 804
Delta R.T. 0.00 min
Lab File: VX011603.D
Acq: 17 Aug 2019 01:00

Tgt Ion:	65	Resp:	209559
Ion	Ratio	Lower	Upper
65	100		
67	53.2	0.0	107.6

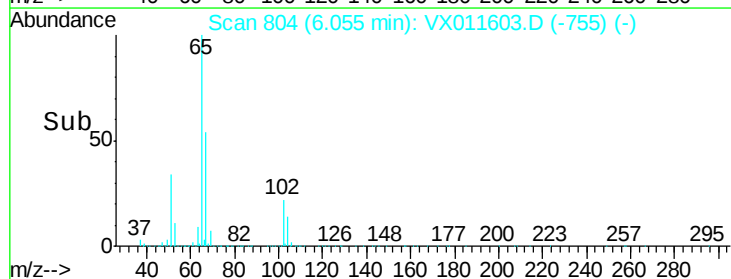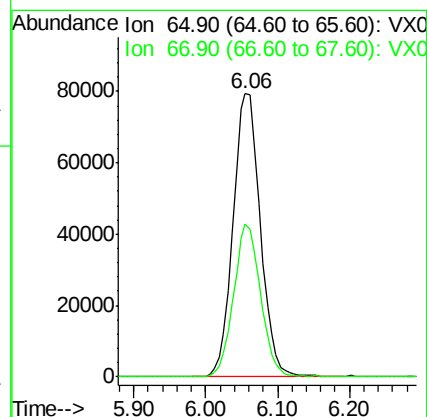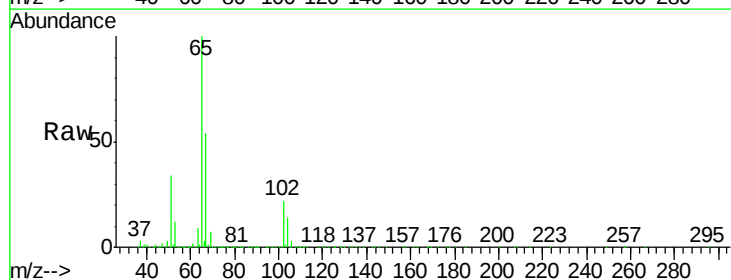

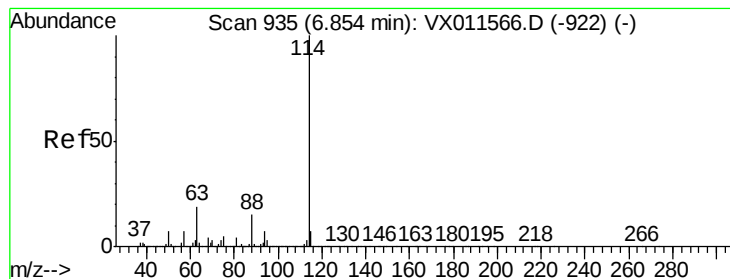

#34

1,4-Difluorobenzene

Concen: 50.000 ug/l

RT: 6.85 min Scan# 935

Delta R.T. 0.00 min

Lab File: VX011603.D

Acq: 17 Aug 2019 01:00

Instrument :

MSVOA_X

ClientSampleId :

2S-G3-(0)


Tot Ion:114 Resp: 609673

Ion Ratio Lower Upper

114 100

63 18.3 0.0 37.8




88 14.5 0.0 30.2

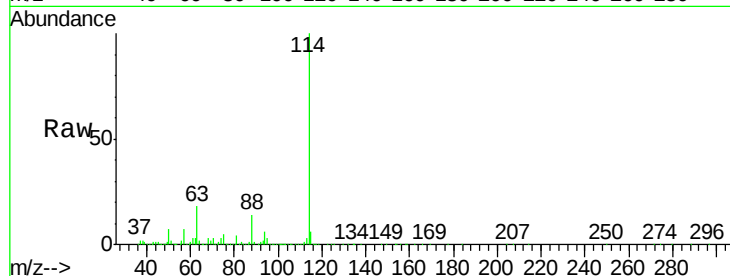

Abundance Ion 113.90 (113.60 to 114.60): V

Ion 63.00 (62.70 to 63.70): VX0

Ion 87.90 (87.60 to 88.60): VX0

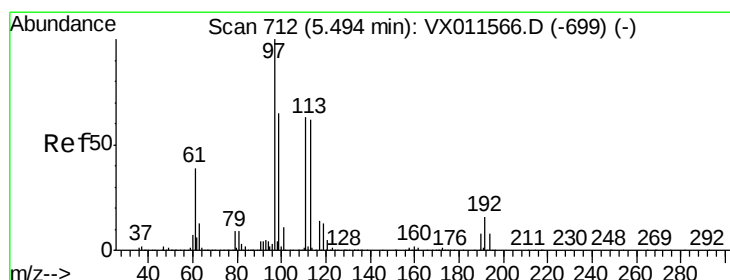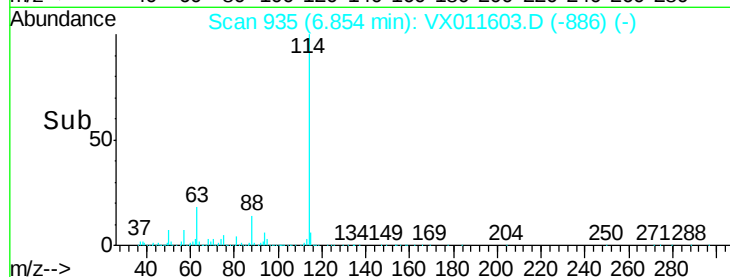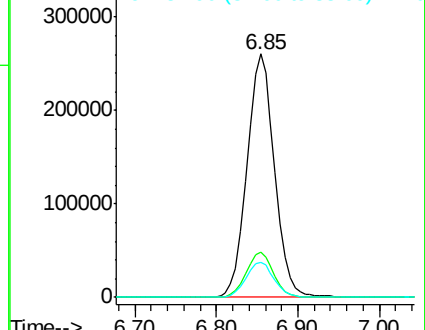

#35

Dibromofluoromethane

Concen: 45.784 ug/l

RT: 5.49 min Scan# 712

Delta R.T. 0.00 min

Lab File: VX011603.D

Acq: 17 Aug 2019 01:00


Tgt Ion:113 Resp: 182569

Ion Ratio Lower Upper

113 100

111 100.5 81.1 121.7



192 25.6 20.8 31.2

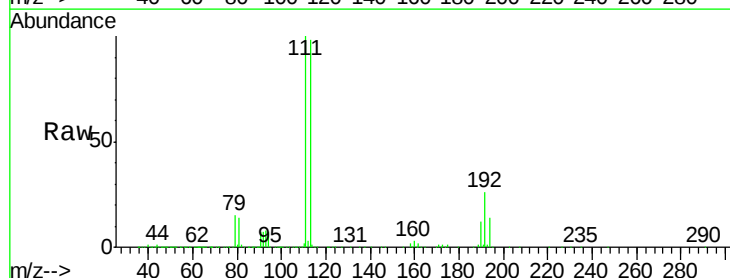


Abundance Ion 112.80 (112.50 to 113.50): V

Ion 110.80 (110.50 to 111.50): V

Ion 191.70 (191.40 to 192.40): V

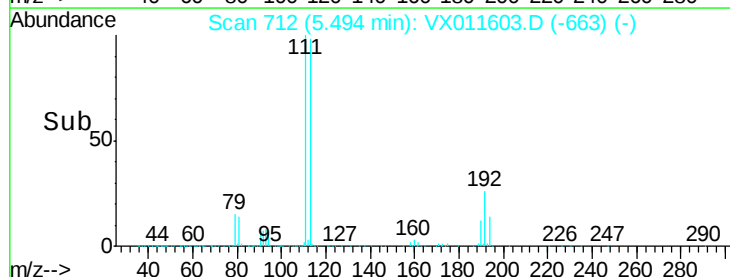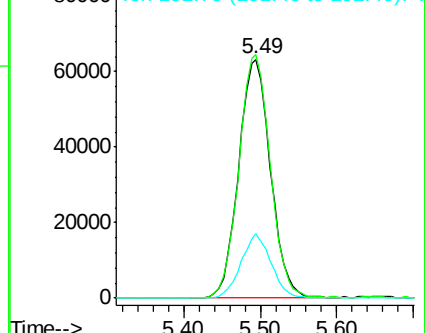

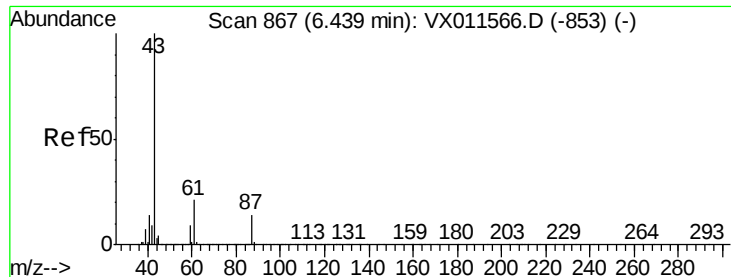

#43

Isopropyl Acetate

Concen: 8.580 ug/l

RT: 6.44 min Scan# 867

Delta R.T. 0.00 min

Lab File: VX011603.D

Acq: 17 Aug 2019 01:00

Instrument :

MSVOA_X

ClientSampleId :

2S-G3-(0)


Tot Ion: 43 Resp: 80277

Ion Ratio Lower Upper

43 100

61 20.9 16.6 24.8




87 14.5 11.4 17.2

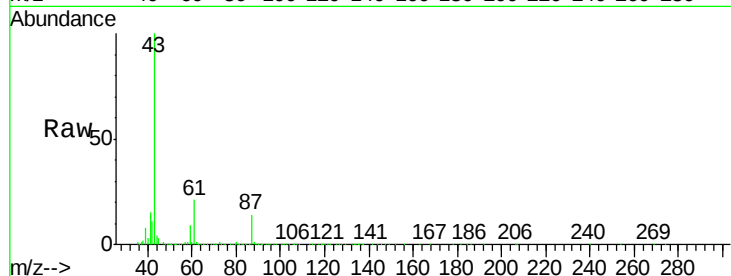

Abundance Ion 43.00 (42.70 to 43.70): VX0

Ion 61.00 (60.70 to 61.70): VX0

Ion 87.00 (86.70 to 87.70): VX0

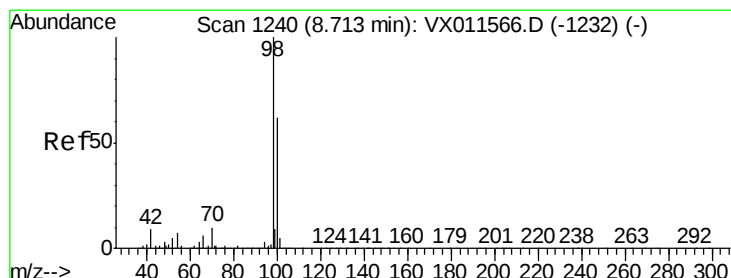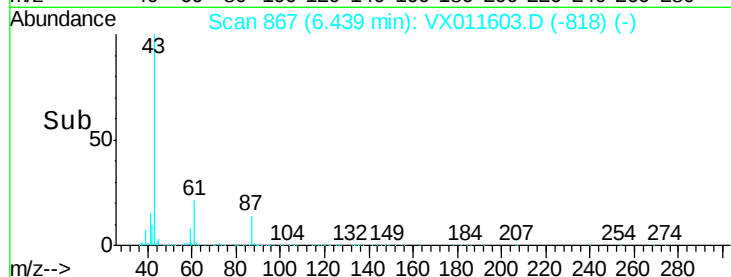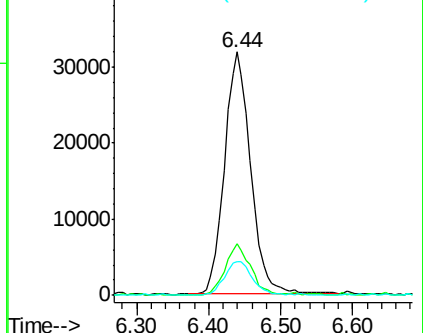

#50

Toluene-d8

Concen: 56.307 ug/l

RT: 8.71 min Scan# 1240

Delta R.T. 0.00 min

Lab File: VX011603.D


Acq: 17 Aug 2019 01:00

Tgt Ion: 98 Resp: 699621

Ion Ratio Lower Upper



98 100


100 64.3 52.4 78.6

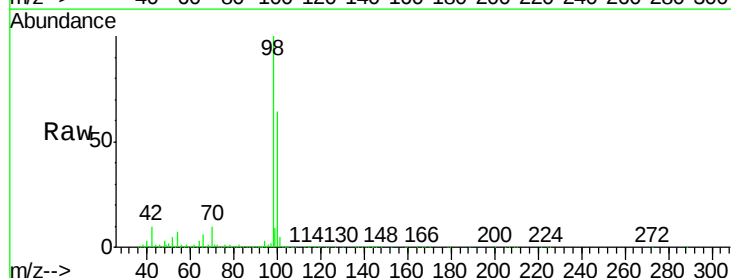

Abundance Ion 98.00 (97.70 to 98.70): VX0

Ion 100.00 (99.70 to 100.70): VX0

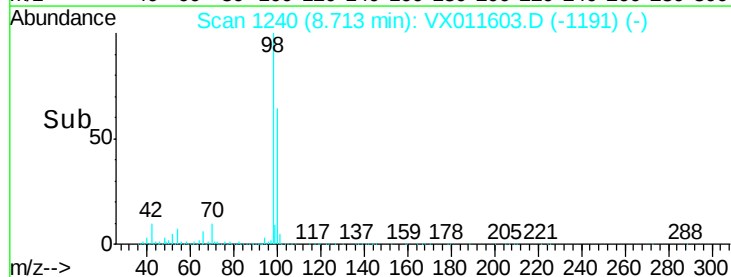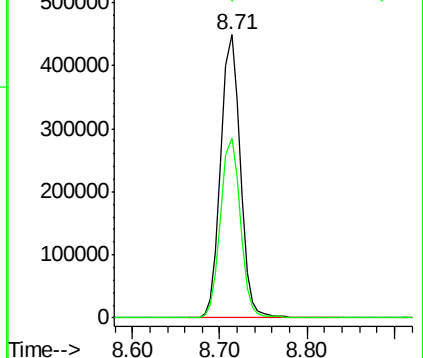

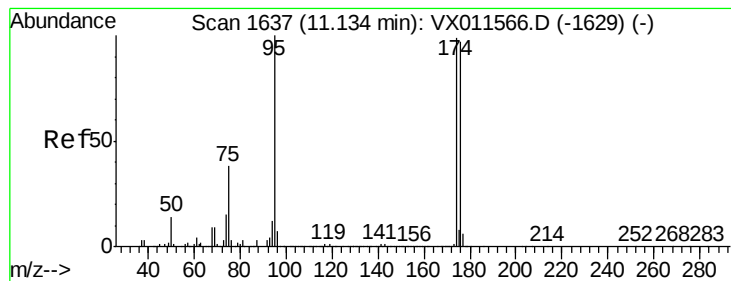

#62

4-Bromofluorobenzene

Concen: 46.153 ug/l

RT: 11.13 min Scan# 1637

Delta R.T. 0.00 min

Lab File: VX011603.D

Acq: 17 Aug 2019 01:00

Instrument :

MSVOA_X

ClientSampleId :

2S-G3-(0)


Tot Ion: 95 Resp: 242045

Ion Ratio Lower Upper

95 100

174 100.2 0.0 200.6




176 97.8 0.0 196.6

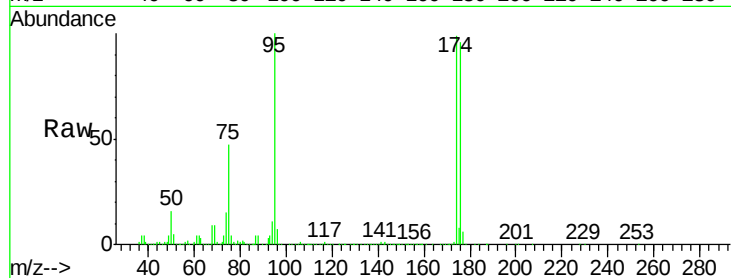

Abundance Ion 94.90 (94.60 to 95.60): VX011566.D (-1629) (-)

Ion 173.80 (173.50 to 174.50): VX011566.D (-1629) (-)

Ion 175.80 (175.50 to 176.50): VX011566.D (-1629) (-)

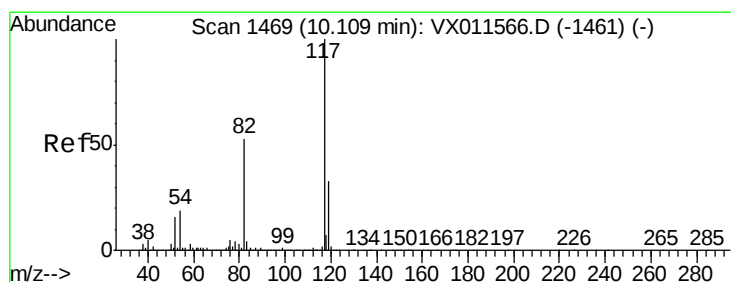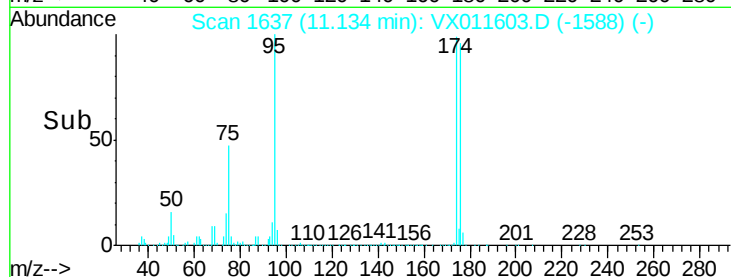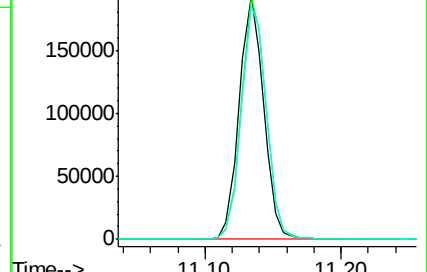

#63

Chlorobenzene-d5

Concen: 50.000 ug/l

RT: 10.11 min Scan# 1469

Delta R.T. 0.00 min

Lab File: VX011603.D

Acq: 17 Aug 2019 01:00


Tgt Ion: 117 Resp: 541402

Ion Ratio Lower Upper

117 100

82 52.3 42.0 63.0



119 32.3 26.5 39.7



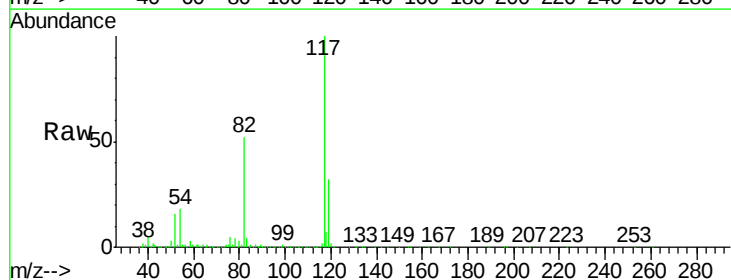


Abundance Ion 116.90 (116.60 to 117.60): VX011566.D (-1461) (-)

Ion 82.00 (81.70 to 82.70): VX011566.D (-1461) (-)

Ion 118.90 (118.60 to 119.60): VX011566.D (-1461) (-)

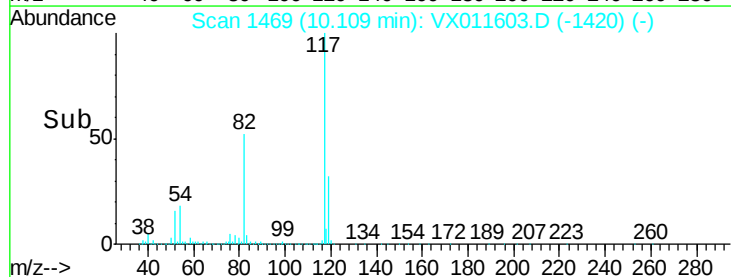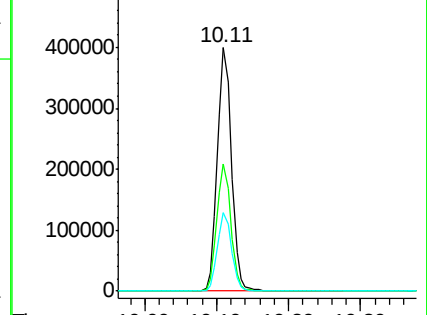

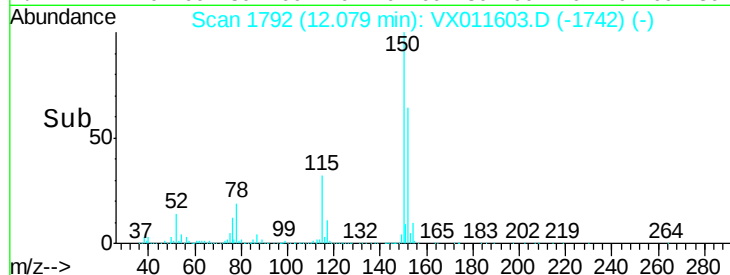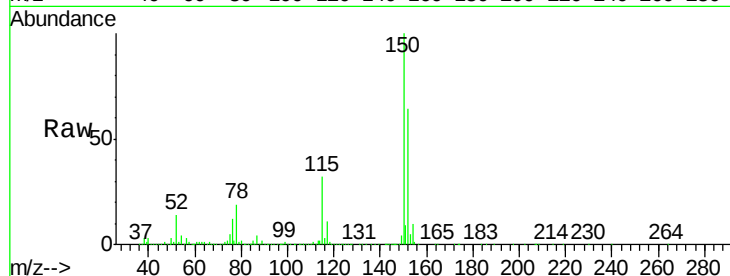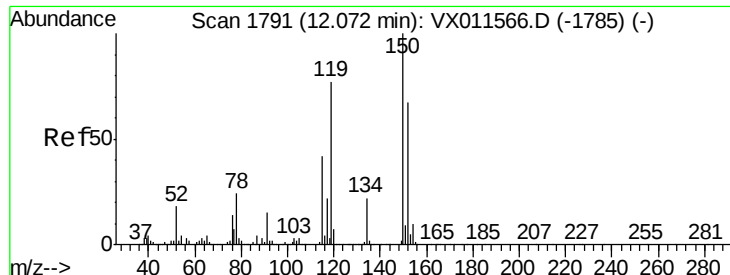

#72

1,4-Dichlorobenzene-d4

Concen: 50.000 ug/l

RT: 12.08 min Scan# 1792

Delta R.T. 0.01 min

Lab File: VX011603.D

Acq: 17 Aug 2019 01:00

Instrument :

MSVOA_X

ClientSampleId :

2S-G3-(0)

Tot Ion:152 Resp: 261139

Ion Ratio Lower Upper

152 100

115 52.5 37.3 111.9

150 155.3 0.0 346.2

Abundance Ion 151.90 (151.60 to 152.60): V

Ion 114.90 (114.60 to 115.60): V

Ion 149.90 (149.60 to 150.60): V

