


Data Path : Z:\voasrv\HPCHEM1\MSVOA X\Data\VX081619\
Data File : VX011595.D
Acq On : 16 Aug 2019 21:06
Operator : JC/SP
Sample : BFB
Misc : 5.0mL/MSVOA X/WATER
ALS Vial : 27 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82X081519W.M
Title : SW846 8260
Last Update : Fri Aug 16 04:15:26 2019

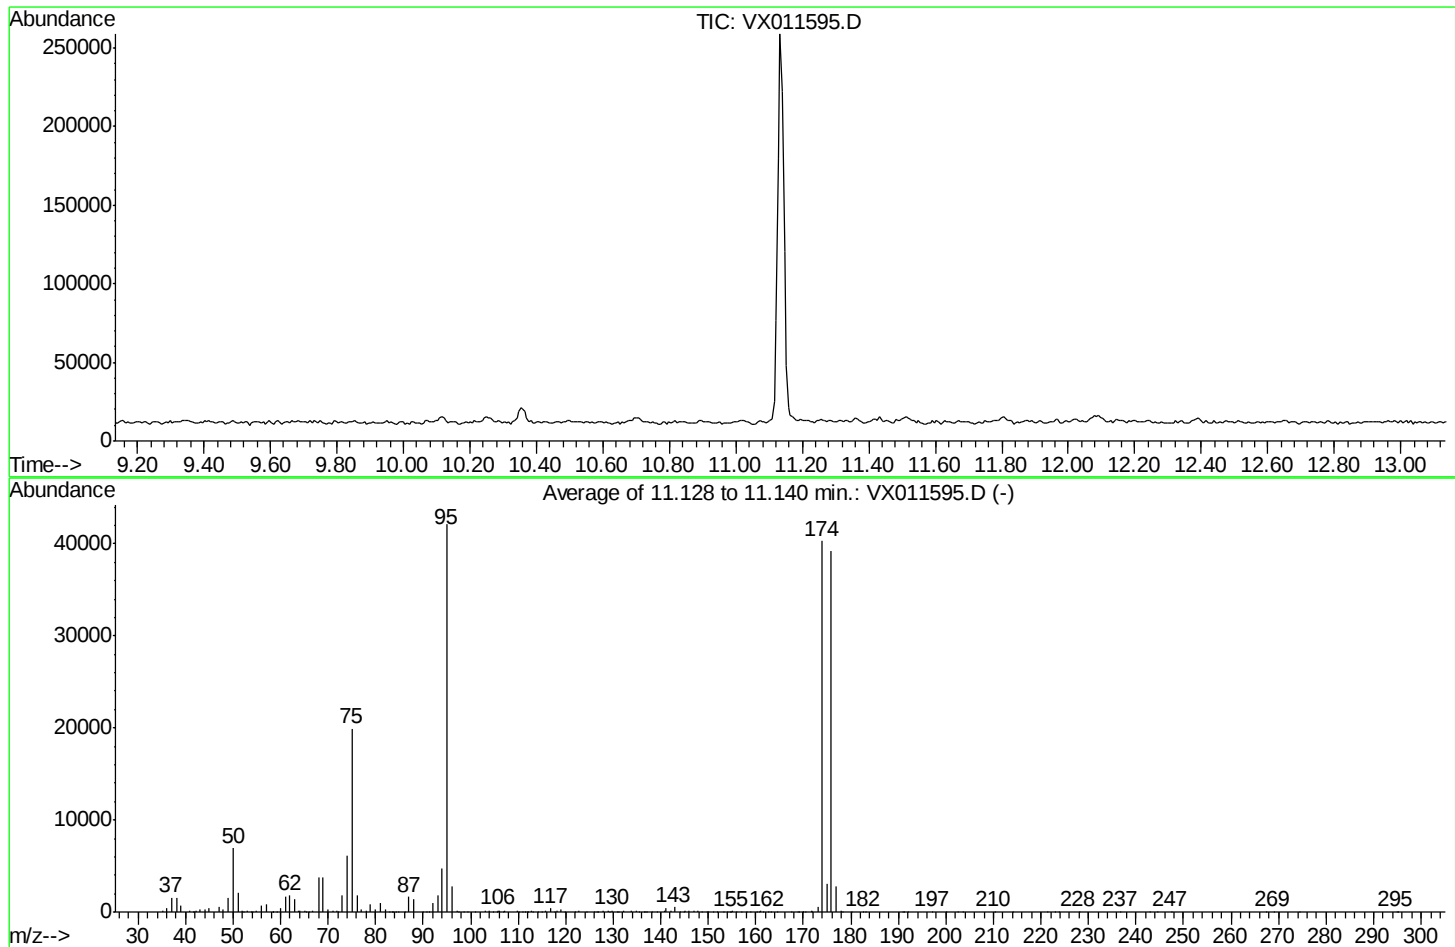

AutoFind: Scans 1636, 1637, 1638; Background Corrected with Scan 1629

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	16.5	6942	PASS
75	95	30	60	47.3	19921	PASS
95	95	100	100	100.0	42117	PASS
96	95	5	9	6.7	2801	PASS
173	174	0.00	2	1.5	603	PASS
174	95	50	100	95.6	40280	PASS
175	174	5	9	7.8	3133	PASS
176	174	95	101	97.4	39218	PASS
177	176	5	9	7.0	2750	PASS