

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX081622\
 Data File : VX030648.D
 Acq On : 16 Aug 2022 12:35
 Operator : JC/MD
 Sample : N4221-09
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 C0KQ3

Quant Time: Aug 17 02:22:09 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML080422WMA.M
 Quant Title : VOC Analysis
 QLast Update : Wed Aug 17 02:19:30 2022
 Response via : Initial Calibration

Compound	R.T. QIon		Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	6.763	114	295006	50.000	ug/L	0.00
28) Chlorobenzene-d5	10.055	117	268099	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	12.024	152	118103	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.368	65	94939	50.114	ug/L	0.00
Spiked Amount	50.000	Range 60 - 135	Recovery	= 100.220%		
7) Chloroethane-d5	1.666	69	77643	58.137	ug/L	0.00
Spiked Amount	50.000	Range 70 - 130	Recovery	= 116.280%		
11) 1,1-Dichloroethene-d2	2.307	63	153139	42.733	ug/L	0.00
Spiked Amount	50.000	Range 60 - 125	Recovery	= 85.460%		
21) 2-Butanone-d5	4.459	46	182830	104.157	ug/L	0.00
Spiked Amount	100.000	Range 40 - 130	Recovery	= 104.160%		
24) Chloroform-d	5.056	84	201292	51.615	ug/L	0.00
Spiked Amount	50.000	Range 70 - 125	Recovery	= 103.240%		
26) 1,2-Dichloroethane-d4	5.958	65	135676	51.237	ug/L	0.00
Spiked Amount	50.000	Range 70 - 125	Recovery	= 102.480%		
32) Benzene-d6	5.977	84	406734	52.963	ug/L	0.00
Spiked Amount	50.000	Range 70 - 125	Recovery	= 105.920%		
36) 1,2-Dichloropropane-d6	7.312	67	136261	54.688	ug/L	0.00
Spiked Amount	50.000	Range 70 - 120	Recovery	= 109.380%		
41) Toluene-d8	8.647	98	361330	49.915	ug/L	0.00
Spiked Amount	50.000	Range 80 - 120	Recovery	= 99.840%		
43) trans-1,3-Dichloroprop...	8.952	79	57416	46.321	ug/L	0.00
Spiked Amount	50.000	Range 60 - 125	Recovery	= 92.640%		
47) 2-Hexanone-d5	9.385	63	127391	100.307	ug/L	0.00
Spiked Amount	100.000	Range 45 - 130	Recovery	= 100.310%		
56) 1,1,2,2-Tetrachloroeth...	11.195	84	171171	52.295	ug/L	0.00
Spiked Amount	50.000	Range 65 - 120	Recovery	= 104.600%		
66) 1,2-Dichlorobenzene-d4	12.323	152	122936	53.667	ug/L	0.00
Spiked Amount	50.000	Range 80 - 120	Recovery	= 107.340%		
Target Compounds						Qvalue
13) Acetone	2.392	43	4493	3.492	ug/L	98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX081622\
Data File : VX030648.D
Acq On : 16 Aug 2022 12:35
Operator : JC/MD
Sample : N4221-09
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
C0KQ3

Quant Time: Aug 17 02:22:09 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML080422WMA.M
Quant Title : VOC Analysis
QLast Update : Wed Aug 17 02:19:30 2022
Response via : Initial Calibration

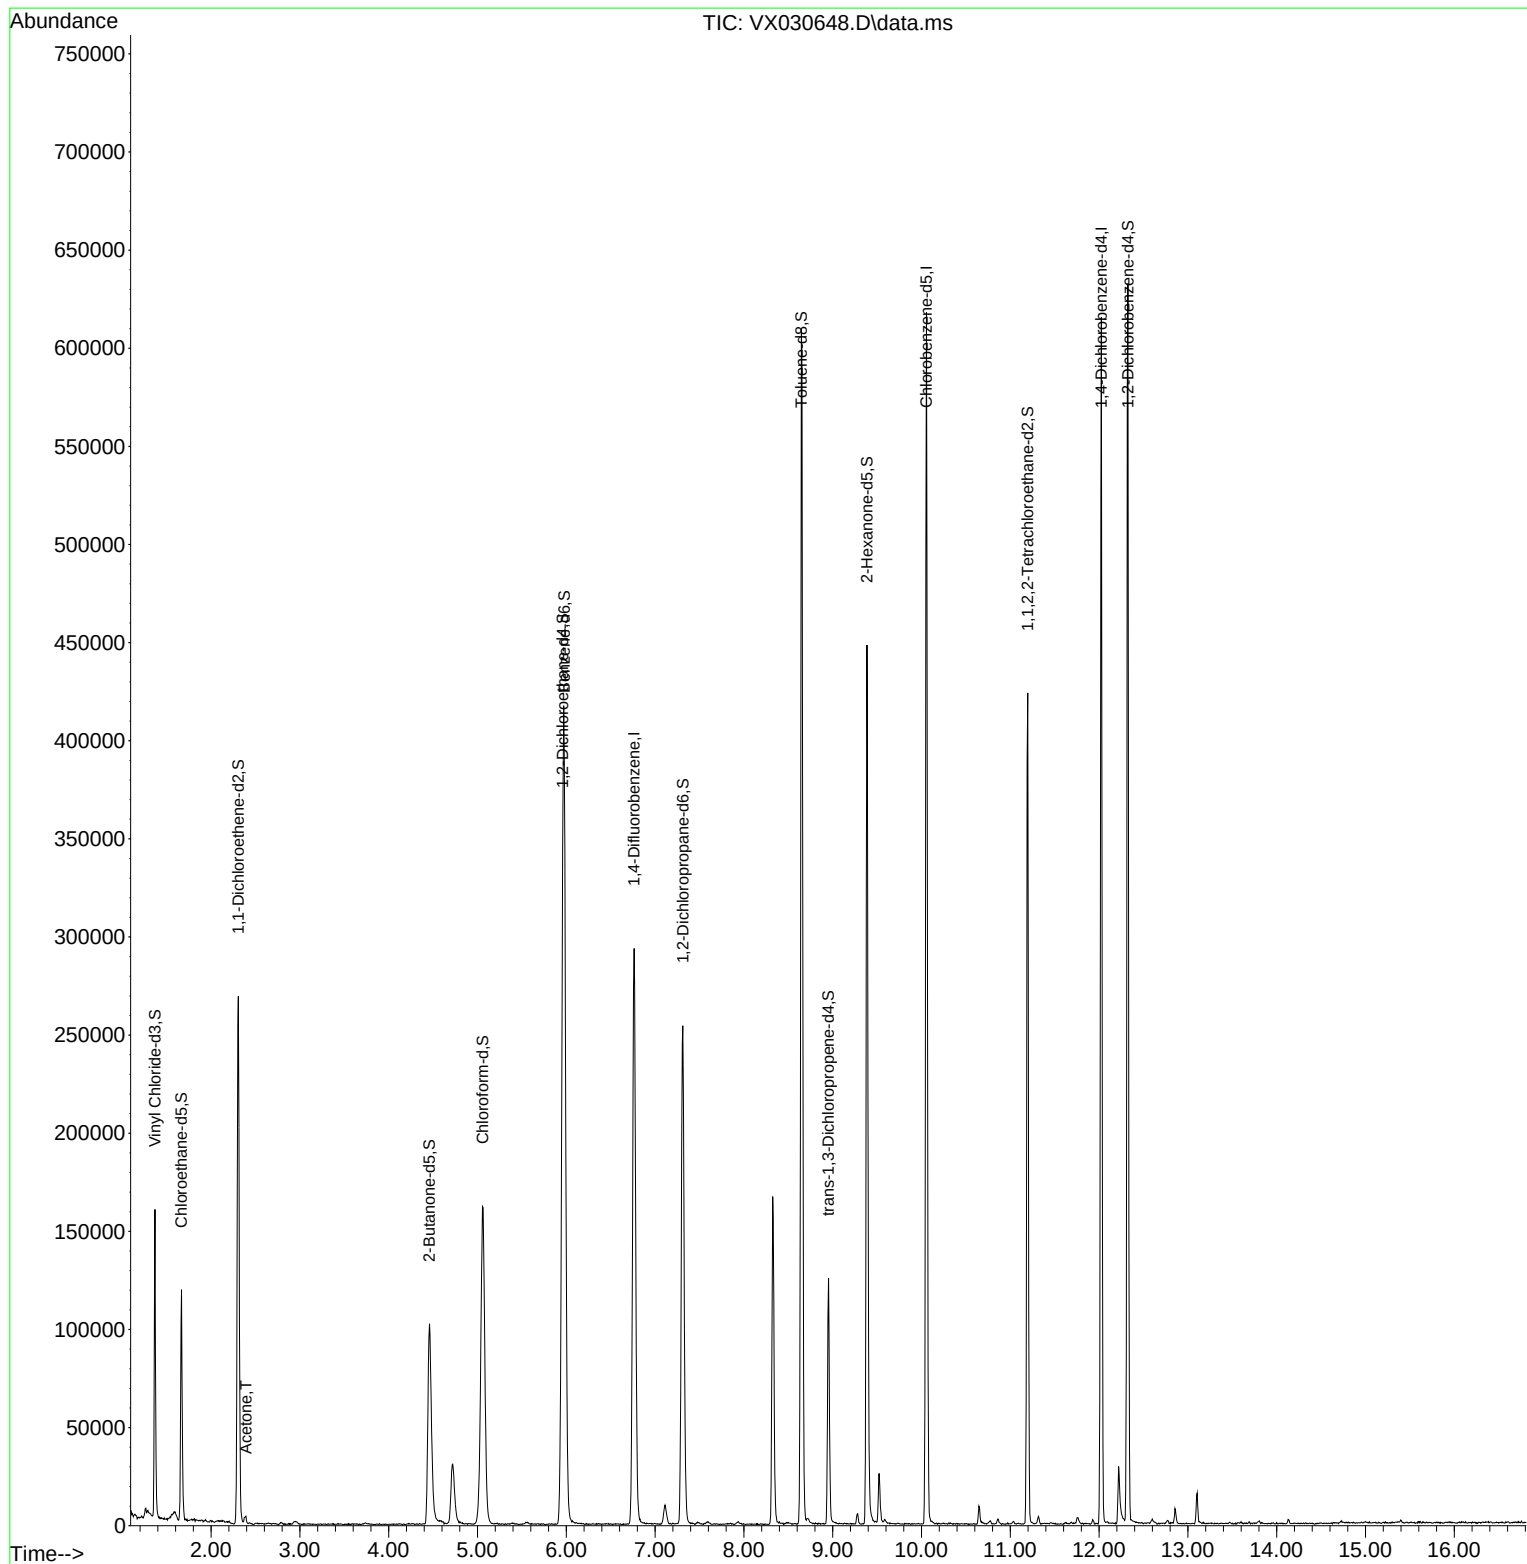

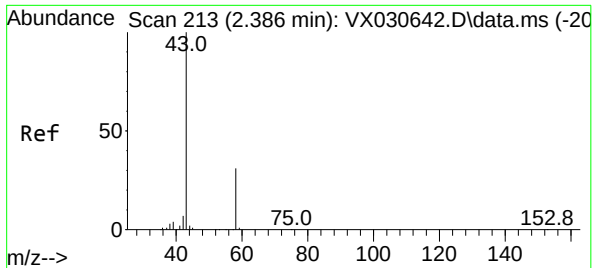

#13
 Acetone
 Concen: 3.492 ug/L
 RT: 2.392 min Scan# 21
 Delta R.T. 0.006 min
 Lab File: VX030648.D
 Acq: 16 Aug 2022 12:35

Instrument :
 MSVOA_X
 ClientSampleId :
 C0KQ3

Tgt Ion: 43 Resp: 4493
 Ion Ratio Lower Upper
 43 100
 58 30.1 0.0 57.8

