

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX081622\
 Data File : VX030644.D
 Acq On : 16 Aug 2022 10:37
 Operator : JC/MD
 Sample : VX0816WBL01
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VBLK687

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML080422WMA.M
 Title : VOC Analysis

Signal : TIC: VX030644.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.368	42	46	53	rVB	145737	153290	13.12%	1.720%
2	1.666	91	95	104	rVB	109892	138142	11.83%	1.550%
3	2.306	193	200	211	rBV	265324	405208	34.69%	4.547%
4	2.502	229	232	238	rVB3	1111	1966	0.17%	0.022%
5	2.556	239	241	242	rBV	472	307	0.03%	0.003%
6	2.648	254	256	257	rBV	429	415	0.04%	0.005%
7	2.788	274	279	285	rVV2	3716	6587	0.56%	0.074%
8	2.947	297	305	316	rVV	12711	31383	2.69%	0.352%
9	3.532	399	401	404	rVV2	262	372	0.03%	0.004%
10	3.721	429	432	433	rVB2	461	482	0.04%	0.005%
11	3.739	433	435	436	rBV2	564	402	0.03%	0.005%
12	3.818	445	448	451	rBV	350	472	0.04%	0.005%
13	4.251	516	519	522	rVB2	545	612	0.05%	0.007%
14	4.306	525	528	530	rBV2	242	327	0.03%	0.004%
15	4.385	538	541	543	rBV2	446	553	0.05%	0.006%
16	4.465	545	554	565	rBV	89861	258493	22.13%	2.901%
17	5.056	639	651	669	rBV	153178	474113	40.59%	5.320%
18	5.550	725	732	740	rVV4	2232	5464	0.47%	0.061%
19	5.788	769	771	772	rVB	521	355	0.03%	0.004%
20	5.806	772	774	776	rBV2	377	374	0.03%	0.004%
21	5.836	776	779	780	rBV2	414	398	0.03%	0.004%
22	5.970	788	801	820	rBV2	393713	1168133	100.00%	13.108%
23	6.233	843	844	848	rBV2	338	420	0.04%	0.005%
24	6.355	862	864	868	rVB2	369	479	0.04%	0.005%
25	6.550	893	896	897	rBV2	370	330	0.03%	0.004%
26	6.763	922	931	944	rBV	314473	726895	62.23%	8.157%
27	6.952	961	962	965	rBV	484	417	0.04%	0.005%
28	7.111	981	988	994	rBV4	8566	19957	1.71%	0.224%
29	7.312	1011	1021	1036	rBV	241326	532269	45.57%	5.973%
30	7.604	1067	1069	1071	rVB	420	331	0.03%	0.004%
31	7.629	1071	1073	1076	rBV2	468	699	0.06%	0.008%
32	7.677	1079	1081	1083	rVB2	659	504	0.04%	0.006%
33	7.708	1083	1086	1089	rBV	482	547	0.05%	0.006%
34	7.745	1089	1092	1094	rBV2	374	454	0.04%	0.005%
35	7.885	1112	1115	1117	rBV2	377	395	0.03%	0.004%
36	7.934	1120	1123	1127	rVV5	1087	1433	0.12%	0.016%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX081622\
 Data File : VX030644.D
 Acq On : 16 Aug 2022 10:37
 Operator : JC/MD
 Sample : VX0816WBL01
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VBLK687

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML080422WMA.M
 Title : VOC Analysis

37	8.171	1159	1162	1165	rBV2	421	541	0.05%	0.006%
38	8.324	1180	1187	1199	rBV	158603	268773	23.01%	3.016%
39	8.452	1205	1208	1211	rBV2	523	712	0.06%	0.008%
40	8.555	1224	1225	1227	rBV	441	391	0.03%	0.004%
41	8.574	1227	1228	1232	rVB3	617	567	0.05%	0.006%
42	8.647	1234	1240	1249	rBV	588182	915842	78.40%	10.277%
43	8.952	1285	1290	1301	rBV	121071	179207	15.34%	2.011%
44	9.055	1305	1307	1309	rVB	845	629	0.05%	0.007%
45	9.074	1309	1310	1313	rBV	416	343	0.03%	0.004%
46	9.098	1313	1314	1316	rBV2	445	444	0.04%	0.005%
47	9.275	1340	1343	1346	rBV4	456	586	0.05%	0.007%
48	9.384	1355	1361	1374	rBV	413641	575690	49.28%	6.460%
49	9.567	1390	1391	1394	rBV2	556	554	0.05%	0.006%
50	9.702	1408	1413	1419	rBV2	4101	6363	0.54%	0.071%
51	9.878	1440	1442	1444	rBV2	360	347	0.03%	0.004%
52	10.055	1465	1471	1479	rBV	649010	869850	74.46%	9.761%
53	10.214	1496	1497	1498	rBV	452	326	0.03%	0.004%
54	10.281	1506	1508	1511	rBV2	368	581	0.05%	0.007%
55	10.305	1511	1512	1514	rVV	688	364	0.03%	0.004%
56	10.677	1571	1573	1575	rBV	317	311	0.03%	0.003%
57	10.726	1579	1581	1584	rBV2	343	325	0.03%	0.004%
58	10.835	1596	1599	1601	rVB2	366	379	0.03%	0.004%
59	10.939	1614	1616	1618	rVB2	456	419	0.04%	0.005%
60	10.963	1618	1620	1621	rBV	363	320	0.03%	0.004%
61	11.000	1624	1626	1627	rBV	546	333	0.03%	0.004%
62	11.055	1634	1635	1640	rVB2	428	508	0.04%	0.006%
63	11.152	1648	1651	1652	rBV	337	377	0.03%	0.004%
64	11.195	1652	1658	1666	rBV	405170	523317	44.80%	5.872%
65	11.317	1674	1678	1680	rVB2	789	902	0.08%	0.010%
66	11.427	1694	1696	1699	rBV2	462	530	0.05%	0.006%
67	11.451	1699	1700	1703	rVV	699	511	0.04%	0.006%
68	11.500	1707	1708	1711	rBV	309	382	0.03%	0.004%
69	11.591	1721	1723	1725	rBV2	404	415	0.04%	0.005%
70	11.750	1747	1749	1752	rVB3	521	512	0.04%	0.006%
71	11.884	1767	1771	1772	rBV	284	349	0.03%	0.004%
72	12.024	1789	1794	1803	rVB	659263	807740	69.15%	9.064%
73	12.323	1837	1843	1849	rVV	635584	799558	68.45%	8.972%
74	12.494	1870	1871	1874	rVB	598	456	0.04%	0.005%
75	12.524	1874	1876	1878	rBV2	405	432	0.04%	0.005%
76	12.567	1881	1883	1886	rBV2	494	582	0.05%	0.007%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX081622\
 Data File : VX030644.D
 Acq On : 16 Aug 2022 10:37
 Operator : JC/MD
 Sample : VX0816WBL01
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VBLK687

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML080422WMA.M
 Title : VOC Analysis

77	12.756	1912	1914	1915	rBV	780	621	0.05%	0.007%
78	13.116	1971	1973	1978	rVB3	1075	1094	0.09%	0.012%
79	13.183	1982	1984	1985	rBV2	517	487	0.04%	0.005%
80	13.219	1989	1990	1992	rBV	465	334	0.03%	0.004%
81	13.384	2016	2017	2020	rBV2	464	338	0.03%	0.004%
82	13.414	2020	2022	2025	rVV2	453	412	0.04%	0.005%
83	13.457	2027	2029	2032	rVB2	572	666	0.06%	0.007%
84	13.573	2046	2048	2050	rBV2	418	414	0.04%	0.005%
85	13.780	2080	2082	2086	rVB2	897	961	0.08%	0.011%
86	13.908	2099	2103	2104	rBV2	565	704	0.06%	0.008%
87	14.060	2126	2128	2129	rBV2	433	309	0.03%	0.003%
88	14.134	2136	2140	2145	rVB	2156	2715	0.23%	0.030%
89	14.182	2146	2148	2149	rBV	633	360	0.03%	0.004%
90	14.402	2183	2184	2187	rBV	413	416	0.04%	0.005%
91	14.542	2205	2207	2208	rBV	568	396	0.03%	0.004%
92	14.646	2222	2224	2226	rBV	712	533	0.05%	0.006%
93	14.701	2229	2233	2235	rBV3	471	818	0.07%	0.009%
94	14.755	2239	2242	2244	rBV2	505	791	0.07%	0.009%
95	14.890	2262	2264	2265	rBV	703	620	0.05%	0.007%
96	15.383	2343	2345	2351	rVB4	1306	2025	0.17%	0.023%
97	15.694	2395	2396	2400	rVB	1009	955	0.08%	0.011%
98	16.072	2456	2458	2460	rBV	740	589	0.05%	0.007%
99	16.286	2491	2493	2495	rBV2	941	790	0.07%	0.009%
100	16.591	2541	2543	2545	rBV	759	579	0.05%	0.006%


Sum of corrected areas: 8911673

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX081622\
Data File : VX030644.D
Acq On : 16 Aug 2022 10:37
Operator : JC/MD
Sample : VX0816WBL01
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VBLK687

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML080422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

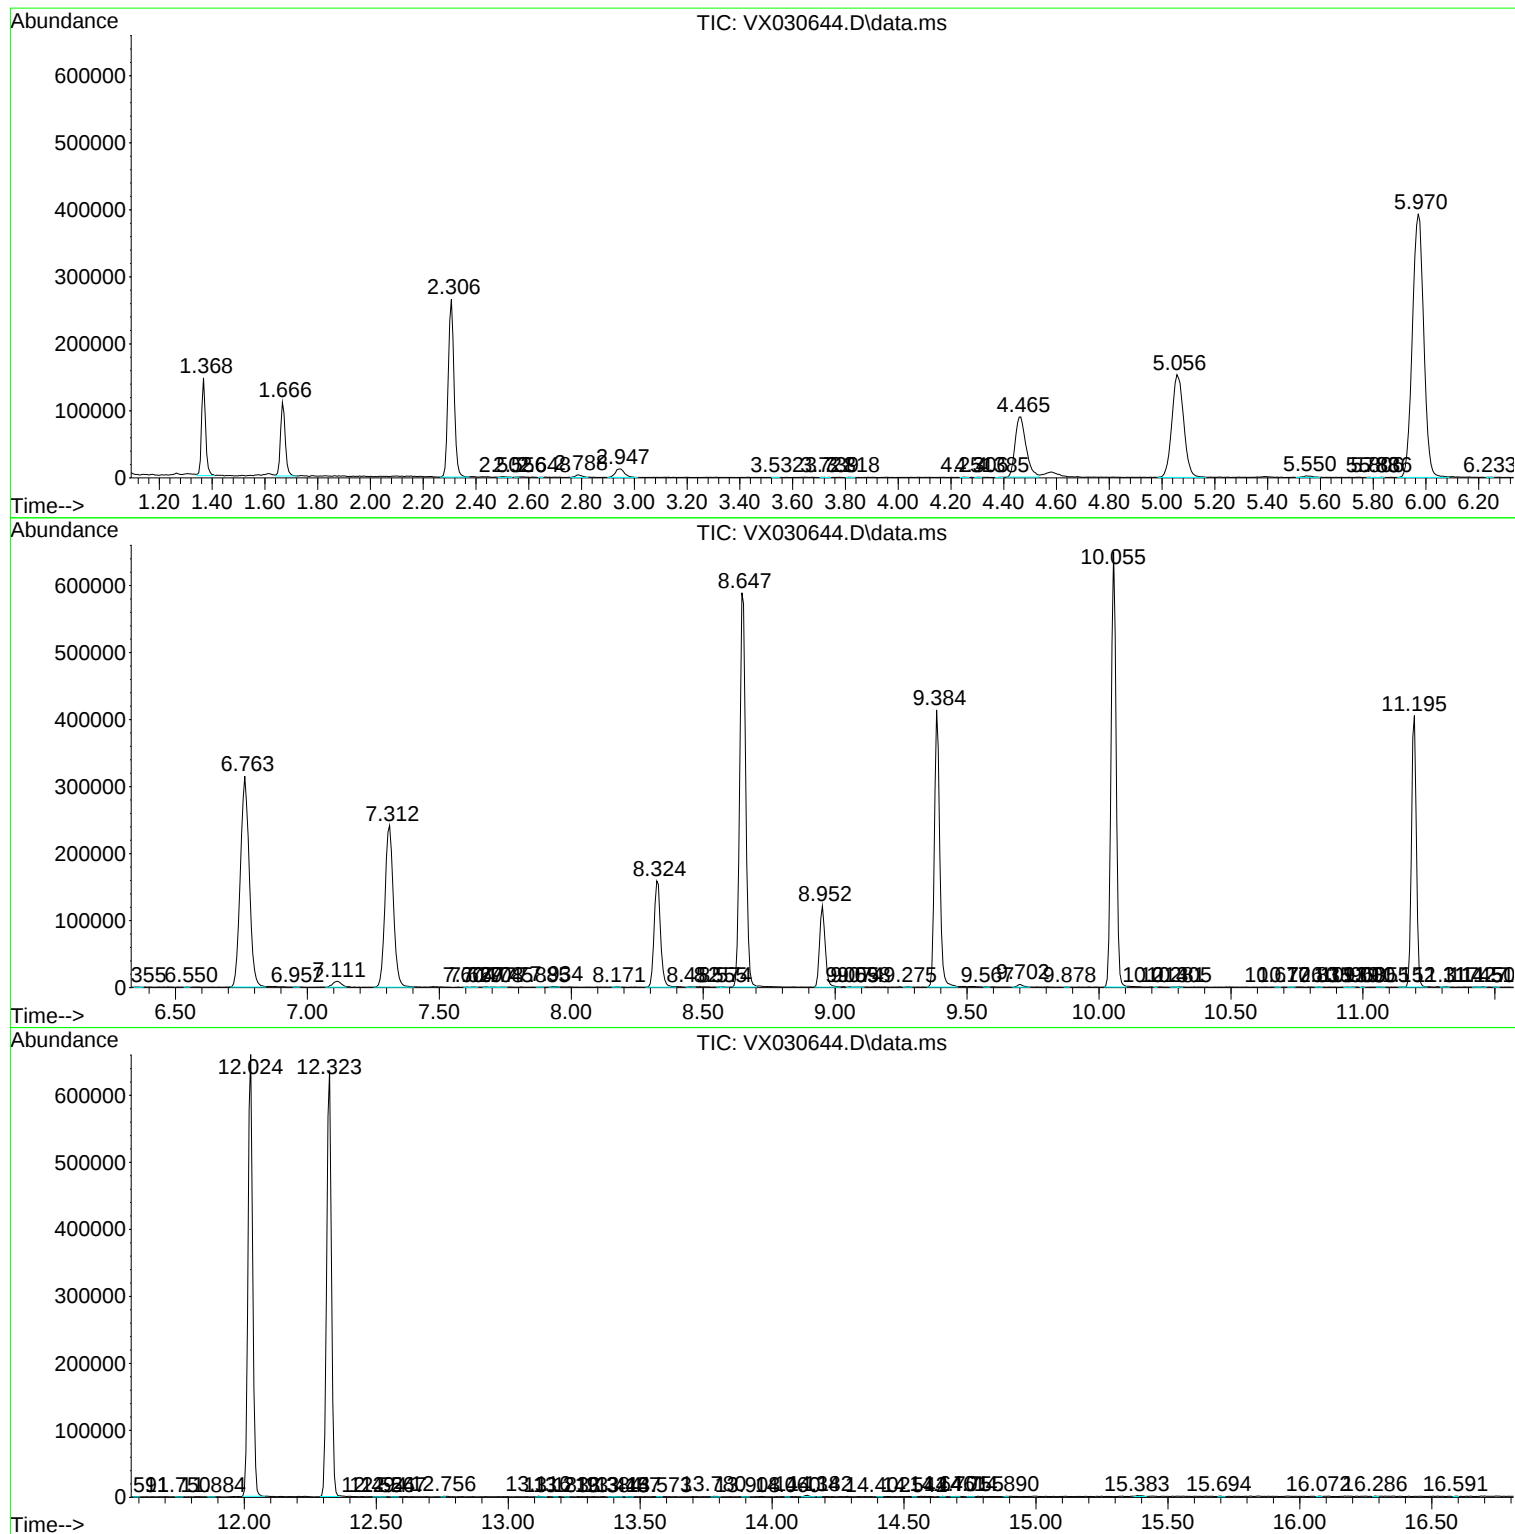

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX081622\
Data File : VX030644.D
Acq On : 16 Aug 2022 10:37
Operator : JC/MD
Sample : VX0816WBL01
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VBLK687

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXMLM080422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX081622\
Data File : VX030644.D
Acq On : 16 Aug 2022 10:37
Operator : JC/MD
Sample : VX0816WBL01
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VBLK687

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML080422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc