

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX081622\
 Data File : VX030650.D
 Acq On : 16 Aug 2022 13:21
 Operator : JC/MD
 Sample : N4220-02
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VHBLK001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML080422WMA.M
 Title : VOC Analysis

Signal : TIC: VX030650.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.240	23	25	33	rBV3	8814	14327	1.20%	0.161%
2	1.368	42	46	51	rBV	156956	151208	12.67%	1.696%
3	1.666	90	95	103	rVB	107877	141413	11.85%	1.586%
4	2.307	193	200	210	rBV	265128	408042	34.20%	4.577%
5	2.453	222	224	229	rVB2	825	762	0.06%	0.009%
6	2.642	253	255	256	rBV	424	402	0.03%	0.005%
7	2.739	267	271	274	rBV	464	680	0.06%	0.008%
8	2.788	274	279	285	rBV	5197	8910	0.75%	0.100%
9	2.947	296	305	315	rBV2	12728	30470	2.55%	0.342%
10	3.093	327	329	332	rBV	327	359	0.03%	0.004%
11	3.215	347	349	351	rBV2	466	435	0.04%	0.005%
12	3.288	359	361	363	rBV2	561	386	0.03%	0.004%
13	3.422	380	383	384	rBV	339	440	0.04%	0.005%
14	3.538	399	402	405	rBV2	333	500	0.04%	0.006%
15	3.599	409	412	413	rBV2	321	345	0.03%	0.004%
16	3.630	415	417	419	rBV	403	370	0.03%	0.004%
17	4.209	510	512	514	rVB	682	344	0.03%	0.004%
18	4.300	525	527	528	rVB	554	309	0.03%	0.003%
19	4.312	528	529	531	rBV	451	335	0.03%	0.004%
20	4.355	534	536	538	rVB	547	354	0.03%	0.004%
21	4.459	544	553	566	rBV	97542	275142	23.06%	3.086%
22	4.690	589	591	593	rBV2	611	487	0.04%	0.005%
23	4.885	622	623	628	rBV	422	562	0.05%	0.006%
24	4.952	631	634	635	rVV	425	361	0.03%	0.004%
25	5.068	640	653	670	rVV2	150628	483024	40.48%	5.418%
26	5.379	700	704	707	rBV3	1331	1832	0.15%	0.021%
27	5.556	729	733	740	rVB4	1858	3853	0.32%	0.043%
28	5.794	770	772	773	rBV	425	382	0.03%	0.004%
29	5.867	782	784	787	rBV2	586	574	0.05%	0.006%
30	5.977	789	802	816	rBV2	399550	1193202	100.00%	13.385%
31	6.233	842	844	845	rBV2	581	341	0.03%	0.004%
32	6.458	880	881	884	rBV2	449	394	0.03%	0.004%
33	6.519	889	891	892	rBV	339	314	0.03%	0.004%
34	6.580	899	901	904	rBV	374	567	0.05%	0.006%
35	6.659	911	914	916	rBV2	327	338	0.03%	0.004%
36	6.763	922	931	949	rBV	286651	687818	57.64%	7.716%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX081622\
 Data File : VX030650.D
 Acq On : 16 Aug 2022 13:21
 Operator : JC/MD
 Sample : N4220-02
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VHBLK001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML080422WMA.M
 Title : VOC Analysis

37	7.117	982	989	997	rVB4	8417	19931	1.67%	0.224%
38	7.190	999	1001	1003	rBV	349	404	0.03%	0.005%
39	7.312	1012	1021	1039	rVV	245867	543202	45.52%	6.093%
40	7.696	1082	1084	1086	rBV2	401	333	0.03%	0.004%
41	7.934	1117	1123	1126	rBV2	1372	2495	0.21%	0.028%
42	8.074	1145	1146	1148	rVB	641	314	0.03%	0.004%
43	8.281	1177	1180	1181	rBV	339	379	0.03%	0.004%
44	8.330	1181	1188	1197	rBV	160173	269749	22.61%	3.026%
45	8.458	1207	1209	1210	rVV	734	332	0.03%	0.004%
46	8.574	1227	1228	1230	rBV2	527	347	0.03%	0.004%
47	8.653	1234	1241	1252	rVV	601422	935222	78.38%	10.491%
48	8.799	1264	1265	1270	rVB3	449	503	0.04%	0.006%
49	8.952	1284	1290	1301	rBV	120990	176927	14.83%	1.985%
50	9.208	1331	1332	1334	rBV	375	337	0.03%	0.004%
51	9.250	1336	1339	1340	rBV	393	384	0.03%	0.004%
52	9.269	1340	1342	1345	rVB2	720	673	0.06%	0.008%
53	9.385	1356	1361	1374	rBV	425137	615715	51.60%	6.907%
54	9.610	1397	1398	1400	rBV2	528	460	0.04%	0.005%
55	9.702	1409	1413	1419	rVB2	5495	7683	0.64%	0.086%
56	9.848	1435	1437	1440	rBV2	429	416	0.03%	0.005%
57	9.897	1443	1445	1454	rVB3	759	983	0.08%	0.011%
58	9.958	1454	1455	1457	rBV2	425	349	0.03%	0.004%
59	10.055	1465	1471	1481	rBV	615440	812124	68.06%	9.110%
60	10.244	1500	1502	1504	rBV2	469	512	0.04%	0.006%
61	10.555	1549	1553	1554	rBV	414	336	0.03%	0.004%
62	10.836	1596	1599	1600	rBV	460	427	0.04%	0.005%
63	10.921	1611	1613	1616	rBV	319	417	0.03%	0.005%
64	10.945	1616	1617	1620	rVV2	446	384	0.03%	0.004%
65	11.153	1649	1651	1652	rBV2	484	509	0.04%	0.006%
66	11.195	1652	1658	1668	rVB	442523	567207	47.54%	6.363%
67	11.476	1701	1704	1708	rBV2	864	1003	0.08%	0.011%
68	11.524	1710	1712	1715	rBV2	382	420	0.04%	0.005%
69	11.707	1739	1742	1744	rBV	900	1046	0.09%	0.012%
70	12.024	1789	1794	1804	rVB	613263	737758	61.83%	8.276%
71	12.171	1817	1818	1820	rBV	468	328	0.03%	0.004%
72	12.262	1830	1833	1835	rBV2	434	401	0.03%	0.004%
73	12.323	1837	1843	1850	rBV	633766	790675	66.26%	8.869%
74	12.469	1864	1867	1868	rBV3	516	572	0.05%	0.006%
75	12.549	1878	1880	1883	rVB3	372	363	0.03%	0.004%
76	12.658	1895	1898	1899	rBV3	364	377	0.03%	0.004%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX081622\
 Data File : VX030650.D
 Acq On : 16 Aug 2022 13:21
 Operator : JC/MD
 Sample : N4220-02
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VHBLK001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML080422WMA.M
 Title : VOC Analysis

77	12.768	1912	1916	1921	rBV3	959	1121	0.09%	0.013%
78	12.872	1931	1933	1934	rBV	488	309	0.03%	0.003%
79	13.030	1955	1959	1962	rVB2	492	630	0.05%	0.007%
80	13.140	1976	1977	1982	rVB2	748	787	0.07%	0.009%
81	13.183	1982	1984	1986	rBV	679	576	0.05%	0.006%
82	13.274	1997	1999	2000	rBV	480	383	0.03%	0.004%
83	13.530	2040	2041	2042	rBV	648	340	0.03%	0.004%
84	13.597	2050	2052	2054	rBV3	481	390	0.03%	0.004%
85	13.676	2064	2065	2067	rBV	632	603	0.05%	0.007%
86	14.000	2117	2118	2120	rBV	634	395	0.03%	0.004%
87	14.231	2154	2156	2158	rVB	500	373	0.03%	0.004%
88	14.274	2160	2163	2164	rBV2	670	537	0.05%	0.006%
89	14.292	2164	2166	2168	rBV2	725	505	0.04%	0.006%
90	14.378	2178	2180	2182	rVB2	668	518	0.04%	0.006%
91	14.426	2182	2188	2191	rBV3	542	1093	0.09%	0.012%
92	14.487	2197	2198	2202	rBV2	454	534	0.04%	0.006%
93	14.591	2213	2215	2218	rBV3	444	522	0.04%	0.006%
94	14.621	2218	2220	2224	rBV	671	638	0.05%	0.007%
95	14.658	2224	2226	2228	rBV	605	511	0.04%	0.006%
96	15.274	2325	2327	2328	rBV	652	466	0.04%	0.005%
97	15.493	2362	2363	2364	rBV	936	513	0.04%	0.006%
98	16.060	2455	2456	2457	rBV	744	414	0.03%	0.005%
99	16.621	2546	2548	2550	rBV2	637	601	0.05%	0.007%
100	16.773	2572	2573	2575	rBV	506	363	0.03%	0.004%


Sum of corrected areas: 8914701

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX081622\
Data File : VX030650.D
Acq On : 16 Aug 2022 13:21
Operator : JC/MD
Sample : N4220-02
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML080422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

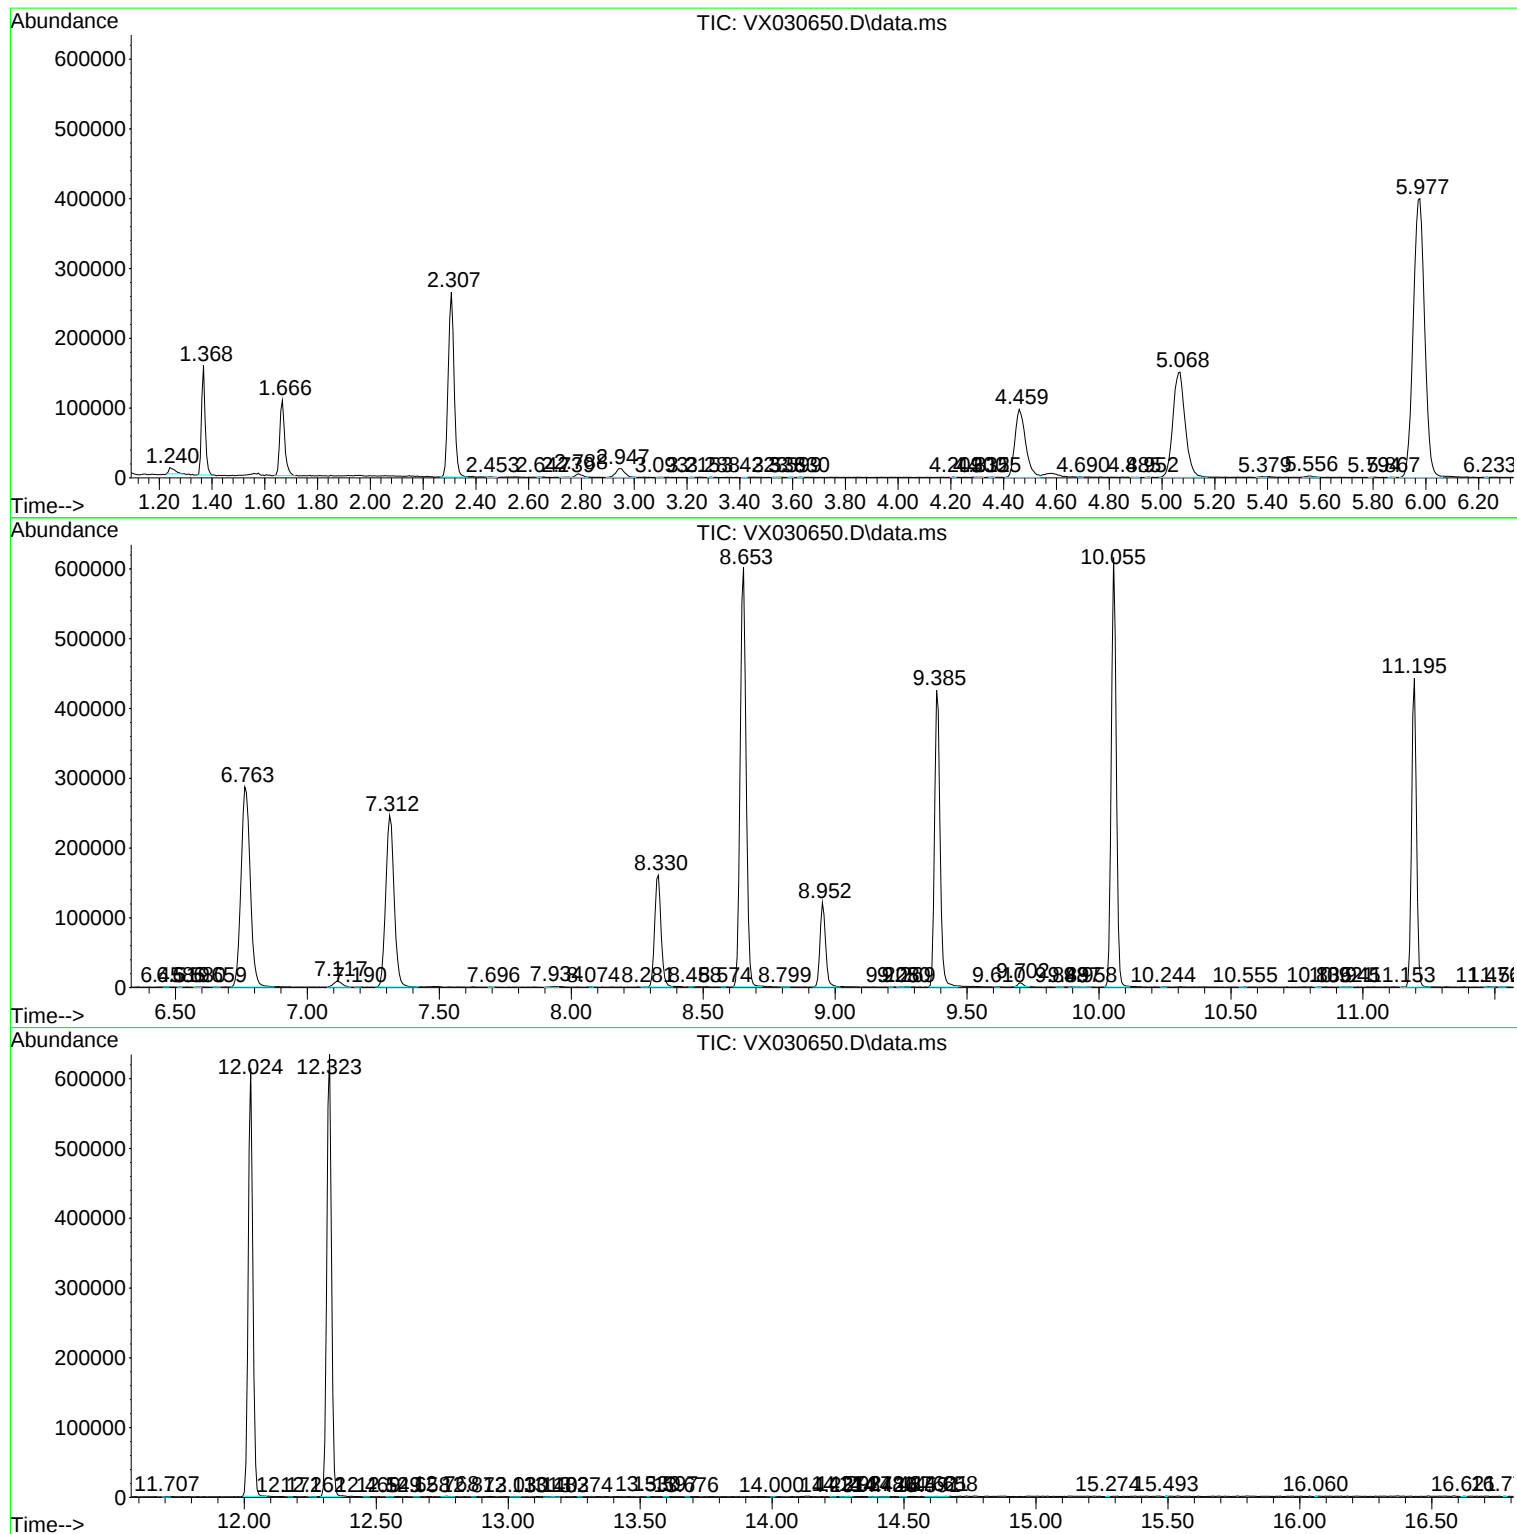

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX081622\
Data File : VX030650.D
Acq On : 16 Aug 2022 13:21
Operator : JC/MD
Sample : N4220-02
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXMLM080422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX081622\
Data File : VX030650.D
Acq On : 16 Aug 2022 13:21
Operator : JC/MD
Sample : N4220-02
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML080422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc