
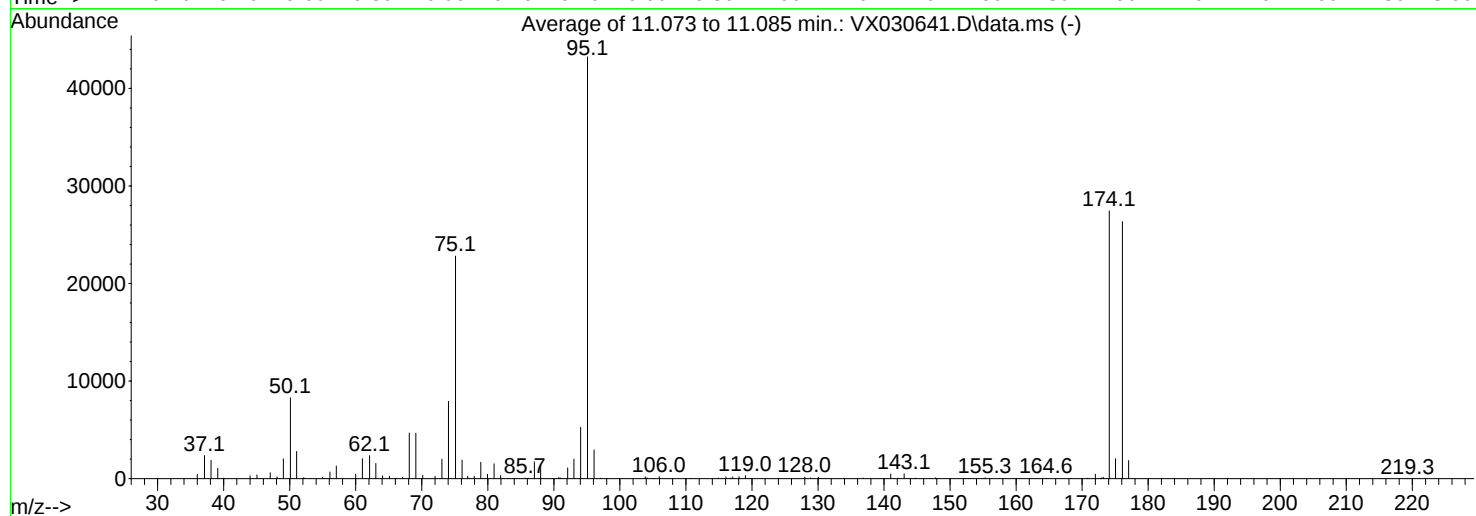


Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX081622\
 Data File : VX030641.D
 Acq On : 16 Aug 2022 08:14
 Operator : JC/MD
 Sample : BFB680
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 BFB680

Integration File: LSCINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM080422WMA.M
 Title : VOC Analysis
 Last Update : Wed Aug 17 02:19:30 2022

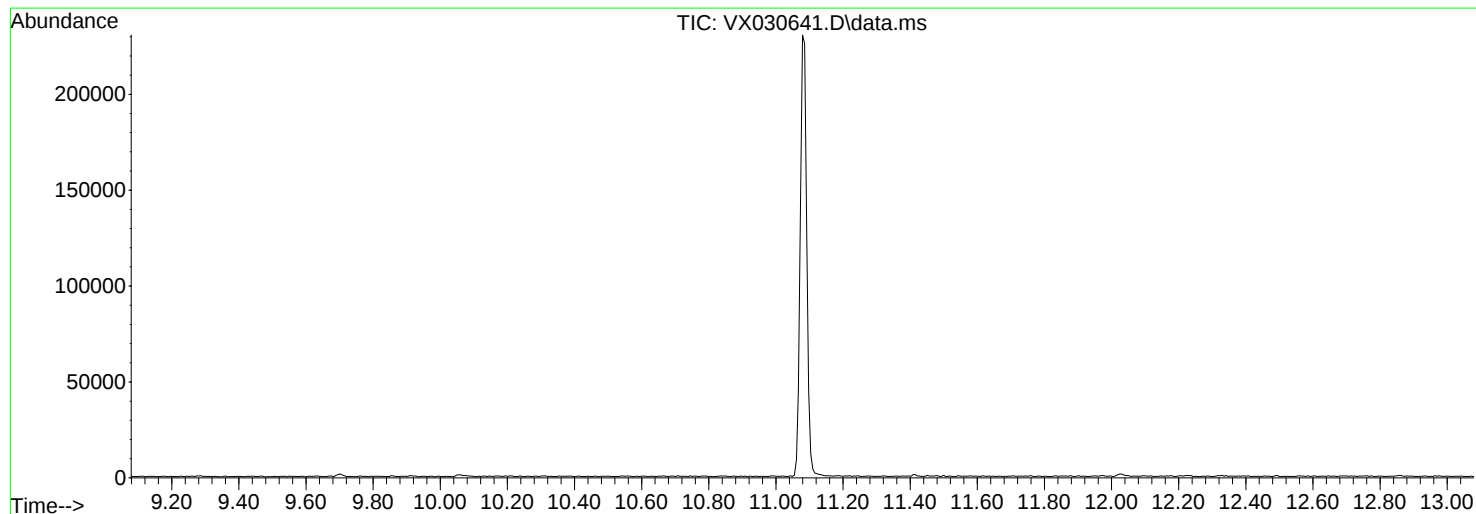

AutoFind: Scans 1638, 1639, 1640; Background Corrected with Scan 1634

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	19.2	8291	PASS
75	95	30	80	52.8	22813	PASS
95	95	100	100	100.0	43232	PASS
96	95	5	9	6.8	2956	PASS
173	174	0.00	2	0.5	124	PASS
174	95	50	120	63.5	27451	PASS
175	174	5	9	7.5	2059	PASS
176	174	95	101	95.9	26333	PASS
177	176	5	9	7.0	1852	PASS

m/z	Abundance
40.00	449.0
44.00	268.0
48.30	59.0

Instrument :
MSVOA_X
ClientSampleId :
BFB680

m/z	Abundance
36.10	291.0
37.10	2001.0
38.10	1893.0
39.10	991.0
40.00	540.0
44.10	571.0
45.10	368.0
47.10	598.0
48.10	323.0
49.00	1520.0
50.10	6312.0
51.10	2404.0
52.20	117.0
54.80	93.0
55.30	69.0
56.10	419.0
57.10	1101.0
60.00	513.0
61.00	2045.0
62.10	1938.0
63.00	1122.0
64.10	203.0
65.20	112.0
65.90	60.0
68.10	3875.0
69.10	3677.0
70.10	297.0
72.00	236.0
73.00	1793.0
74.00	5417.0
75.10	16856.0
76.20	1532.0
76.90	129.0
77.20	128.0
78.00	185.0
78.90	1446.0
80.00	400.0
80.90	1224.0
81.90	200.0
85.60	90.0
87.00	1228.0
88.00	1028.0
90.70	103.0
91.10	69.0
92.00	1024.0
93.00	1276.0
94.00	3837.0
95.10	31672.0
96.10	1987.0
97.10	77.0
103.90	181.0
106.10	104.0
116.10	98.0
116.80	219.0
118.10	255.0
119.00	218.0
127.90	104.0
128.90	58.0
130.10	76.0
136.90	104.0
141.00	401.0
143.10	256.0
147.80	96.0
152.30	51.0
155.40	53.0
172.00	270.0
172.80	119.0
174.10	16346.0
175.10	960.0
176.10	15424.0
177.00	1244.0

Instrument :
MSVOA_X
ClientSampleId :
BFB680

m/z	Abundance
36.00	583.0
37.10	2924.0
38.10	2021.0
39.10	1201.0
40.00	511.0
44.00	614.0
45.00	390.0
47.10	551.0
48.00	287.0
49.10	2773.0
50.10	9884.0
51.10	3153.0
52.10	129.0
53.10	51.0
54.90	116.0
56.10	736.0
57.00	1372.0
59.90	517.0
61.00	2016.0
62.10	2494.0
63.00	1755.0
64.00	348.0
65.10	367.0
66.00	53.0
67.10	138.0
68.10	5250.0
69.10	5589.0
70.10	373.0
72.00	270.0
73.10	2217.0
74.10	8995.0
75.10	27520.0
76.00	2286.0
77.00	357.0
77.90	250.0
79.00	1916.0
79.90	463.0
81.00	1852.0
81.90	344.0
85.70	92.0
86.10	59.0
87.10	1958.0
88.00	2016.0
90.80	280.0
92.10	1041.0
93.00	2635.0
94.10	6031.0
95.10	49160.0
96.10	3567.0
97.00	64.0
103.90	222.0
105.90	313.0
114.90	113.0
116.00	234.0
117.10	259.0
118.00	154.0
119.00	457.0
128.00	232.0
128.90	103.0
130.00	201.0
131.10	67.0
136.80	96.0
141.00	408.0
142.10	65.0
143.00	617.0
144.70	77.0
147.80	148.0
152.80	55.0
155.00	81.0
155.30	72.0
164.50	64.0
170.80	51.0
171.90	488.0
173.00	316.0
174.10	31808.0
175.10	2536.0
176.10	30168.0
177.10	1941.0

Instrument :
MSVOA_X
ClientSampleId :
BFB680

m/z	Abundance
35.90	477.0
37.10	2175.0
38.10	1726.0
39.10	973.0
40.10	443.0
44.10	517.0
45.00	393.0
47.00	692.0
48.20	132.0
49.10	1817.0
50.10	8678.0
51.00	2811.0
52.10	95.0
55.00	260.0
56.10	912.0
57.00	1395.0
60.10	341.0
61.00	2106.0
62.10	2642.0
63.10	1808.0
64.10	355.0
65.10	281.0
66.20	97.0
67.10	230.0
68.10	4909.0
69.10	4713.0
70.20	427.0
72.00	255.0
73.10	1985.0
74.10	9351.0
75.10	24064.0
76.10	1909.0
77.00	269.0
77.90	288.0
79.00	1647.0
80.00	467.0
80.90	1504.0
82.00	381.0
83.00	69.0
86.10	107.0
87.00	1978.0
88.00	1280.0
91.00	129.0
92.20	1213.0
93.10	2113.0
94.10	5923.0
95.10	48864.0
96.10	3315.0
103.80	172.0
104.10	251.0
105.10	64.0
106.00	223.0
110.80	53.0
114.90	80.0
116.00	202.0
117.10	293.0
118.00	186.0
119.00	286.0
128.10	181.0
128.90	108.0
130.00	172.0
131.20	55.0
141.00	624.0
142.10	122.0
143.00	591.0
144.00	53.0
144.80	88.0
148.10	52.0
155.20	124.0
164.60	53.0
170.90	94.0
172.10	628.0
173.20	372.0
174.10	34200.0
175.00	2682.0
176.10	33408.0
177.10	2372.0
219.30	58.0

Instrument :
MSVOA_X
ClientSampleId :
BFB680