

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX081623\
 Data File : VX037040.D
 Acq On : 17 Aug 2023 05:36
 Operator : JC/MD
 Sample : 03958-04 10X
 Misc : 6.55g/5mL/100uL/5.00mL/MSVOA_X/MEOH
 ALS Vial : 43 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 NEVINS-SB02-Z46-47DL

Quant Time: Aug 17 07:12:53 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X072123W.M
 Quant Title : SW846 8260
 QLast Update : Fri Jul 21 12:14:12 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) Pentafluorobenzene	5.550	168	132824	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	6.763	114	244620	50.000	ug/l	0.00
63) Chlorobenzene-d5	10.055	117	243557	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	12.024	152	119810	50.000	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	5.958	65	94204	47.933	ug/l	0.00
Spiked Amount 50.000	Range 78 - 117		Recovery =	95.860%		
35) Dibromofluoromethane	5.385	113	77552	46.124	ug/l	0.00
Spiked Amount 50.000	Range 75 - 124		Recovery =	92.240%		
50) Toluene-d8	8.647	98	297310	49.863	ug/l	0.00
Spiked Amount 50.000	Range 92 - 112		Recovery =	99.720%		
62) 4-Bromofluorobenzene	11.079	95	124110	55.171	ug/l	0.00
Spiked Amount 50.000	Range 83 - 123		Recovery =	110.340%		
Target Compounds						
					Qvalue	
5) Bromomethane	1.605	94	251	0.259	ug/l #	74
11) Tert butyl alcohol	2.940	59	788	1.694	ug/l #	78
13) Acrolein	2.233	56	76	0.286	ug/l #	14
16) Acetone	2.386	43	748	0.917	ug/l #	84
20) Methylene Chloride	2.794	84	672	0.371	ug/l #	60
25) 2-Butanone	4.568	43	635	0.480	ug/l #	51
26) 2,2-Dichloropropane	4.574	77	712	0.242	ug/l #	54
31) Cyclohexane	5.556	56	2941	1.081	ug/l #	1
36) 1,1-Dichloropropene	5.550	75	11273	4.498	ug/l #	50
38) Carbon Tetrachloride	5.550	117	14605	5.482	ug/l #	16
39) Methylcyclohexane	7.385	83	824	0.264	ug/l #	82
40) Benzene	6.037	78	12166	1.669	ug/l	99
51) 4-Methyl-2-Pentanone	8.647	43	1241	0.459	ug/l #	1
67) Ethyl Benzene	10.195	91	155359	15.841	ug/l	99
68) m/p-Xylenes	10.305	106	5449	1.489	ug/l	90
69) o-Xylene	10.640	106	17965	4.918	ug/l	100
73) Isopropylbenzene	10.963	105	18813	1.897	ug/l	98
76) 1,2,3-Trichloropropane	11.079	75	65046	23.082	ug/l #	39
78) n-propylbenzene	11.305	91	10981	0.958	ug/l	99
79) 2-Chlorotoluene	11.402	91	5736	0.825	ug/l #	44
80) 1,3,5-Trimethylbenzene	11.451	105	25744	3.104	ug/l	98
81) trans-1,4-Dichloro-2-b...	11.079	75	65046	52.316	ug/l #	5
82) 4-Chlorotoluene	11.451	91	3251	0.411	ug/l #	46
83) tert-Butylbenzene	11.750	119	11086	1.360	ug/l #	50
84) 1,2,4-Trimethylbenzene	11.750	105	91266	11.002	ug/l	98
85) sec-Butylbenzene	11.750	105	91266	8.981	ug/l #	57
86) p-Isopropyltoluene	12.006	119	11489	1.374	ug/l	91
89) n-Butylbenzene	12.317	91	20002	2.672	ug/l #	1
90) Hexachloroethane	12.695	117	48242	28.458	ug/l #	17
95) Naphthalene	13.774	128	3594315	414.821	ug/l	98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX081623\
Data File : VX037040.D
Acq On : 17 Aug 2023 05:36
Operator : JC/MD
Sample : 03958-04 10X
Misc : 6.55g/5mL/100uL/5.00mL/MSVOA_X/MEOH
ALS Vial : 43 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
NEVINS-SB02-Z46-47DL

Quant Time: Aug 17 07:12:53 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X072123W.M
Quant Title : SW846 8260
QLast Update : Fri Jul 21 12:14:12 2023
Response via : Initial Calibration




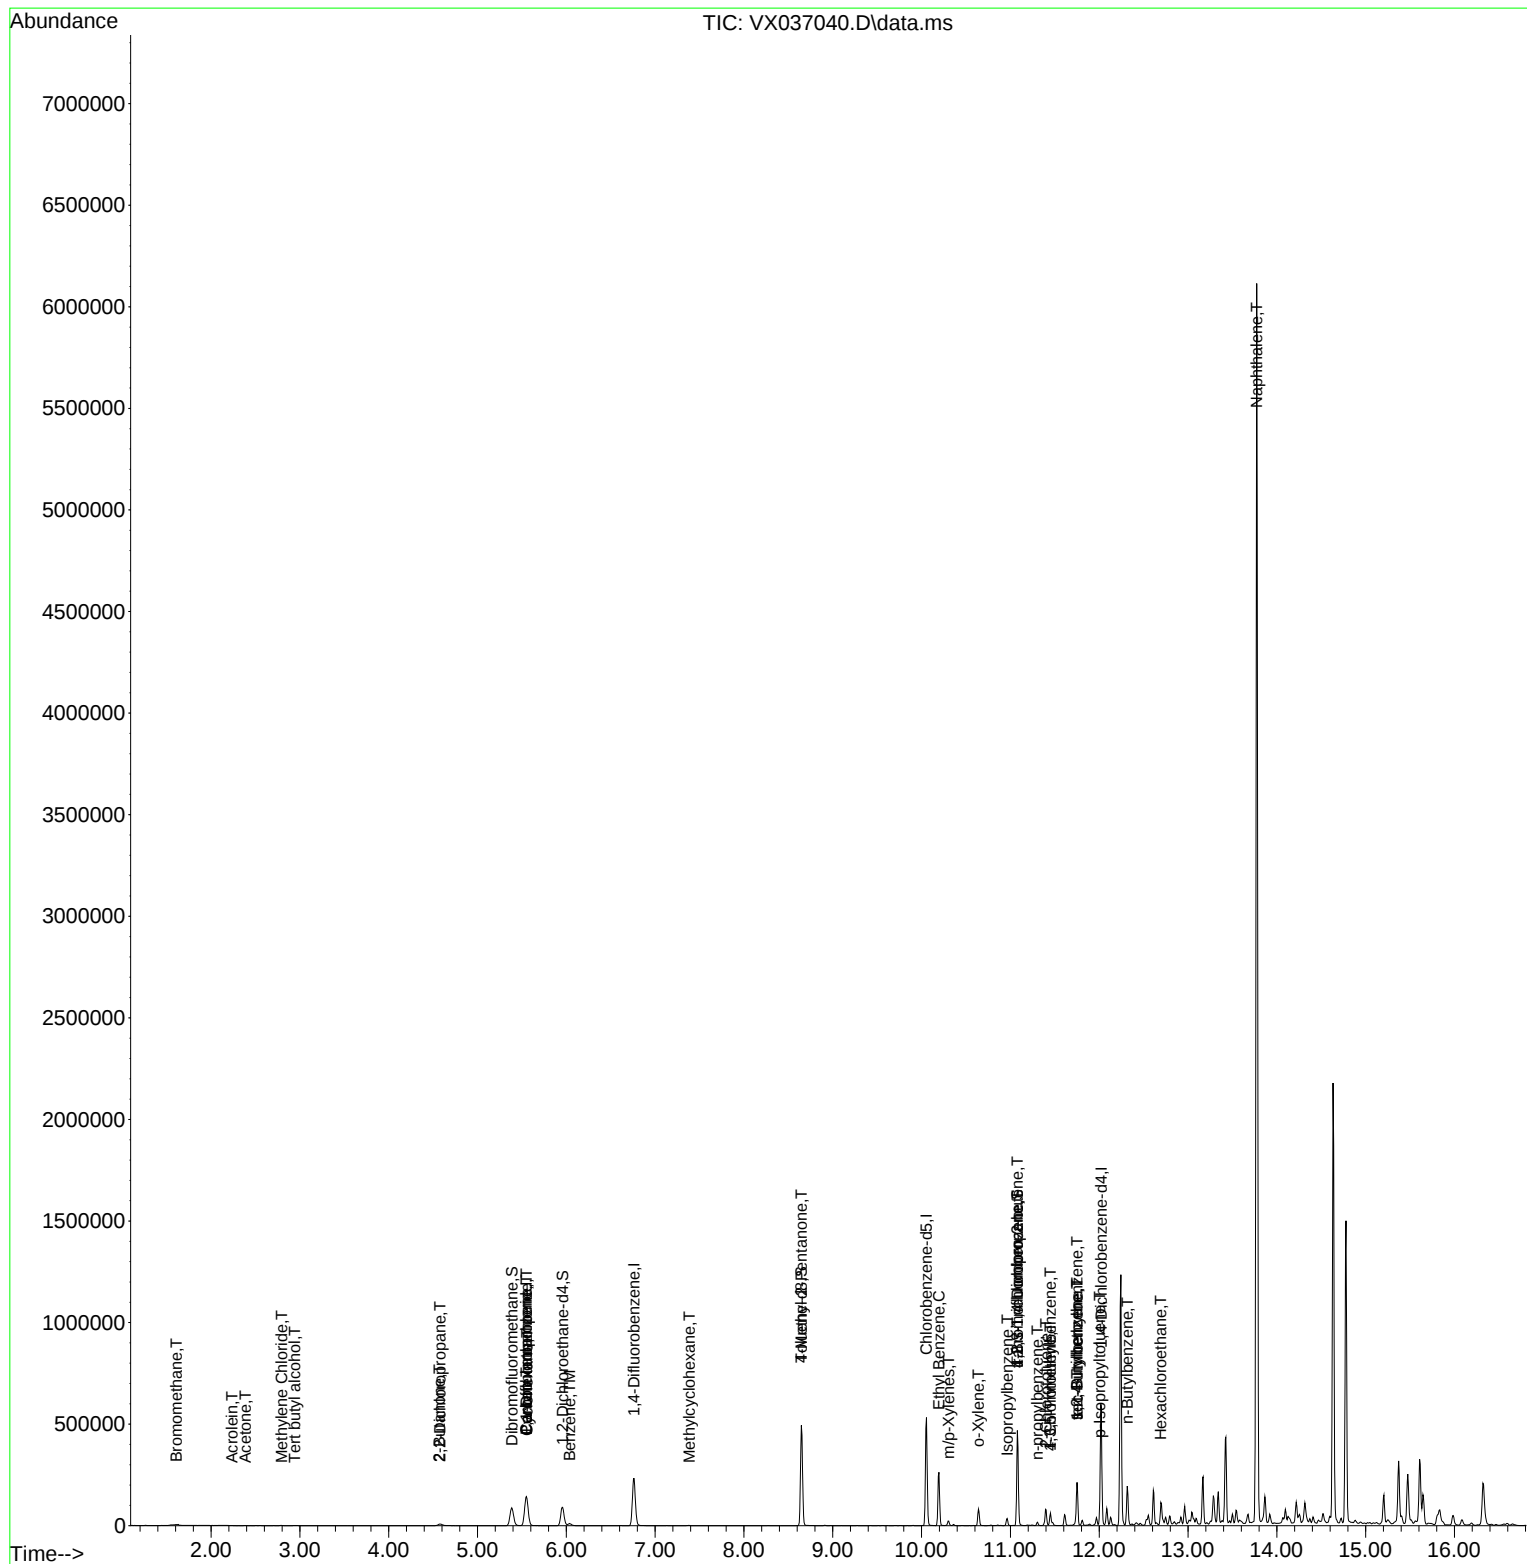


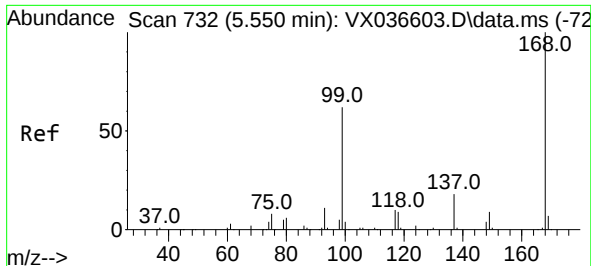

#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 5.550 min Scan# 71
Delta R.T. -0.000 min
Lab File: VX037040.D
Acq: 17 Aug 2023 05:36




Instrument :
MSVOA_X
ClientSampleId :
NEVINS-SB02-Z46-47DL


Tgt Ion:168 Resp: 132824
Ion Ratio Lower Upper
168 100
99 64.3 56.6 85.0

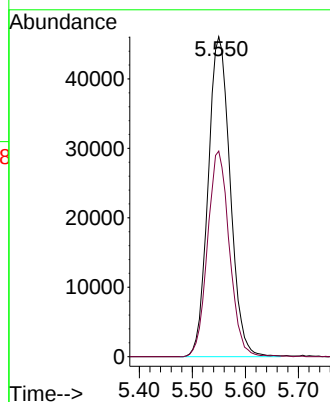

#5
Bromomethane
Concen: 0.259 ug/l
RT: 1.605 min Scan# 85
Delta R.T. -0.012 min
Lab File: VX037040.D
Acq: 17 Aug 2023 05:36

Tgt Ion: 94 Resp: 251
Ion Ratio Lower Upper
94 100
96 68.0 74.6 111.8#

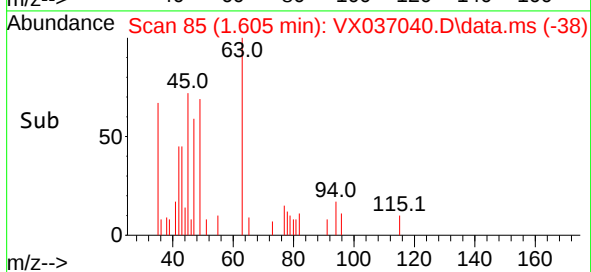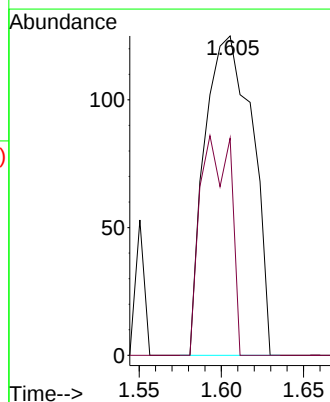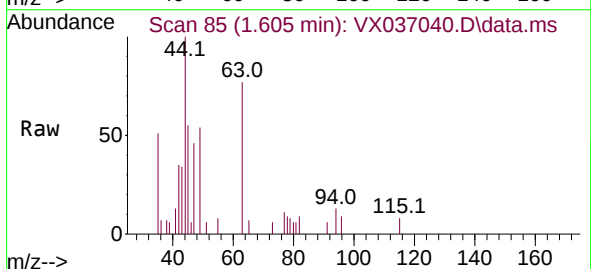

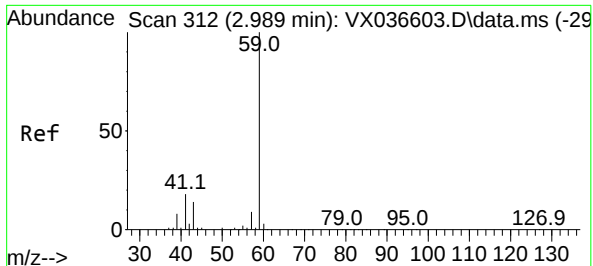

#11

Tert butyl alcohol

Concen: 1.694 ug/l

RT: 2.940 min Scan# 304

Delta R.T. -0.049 min

Lab File: VX037040.D

Acq: 17 Aug 2023 05:36

Instrument :

MSVOA_X

ClientSampleId :





NEVINS-SB02-Z46-47DL

Tgt Ion: 59 Resp: 788

Ion Ratio Lower Upper

59 100

57 0.0 6.0 9.0#

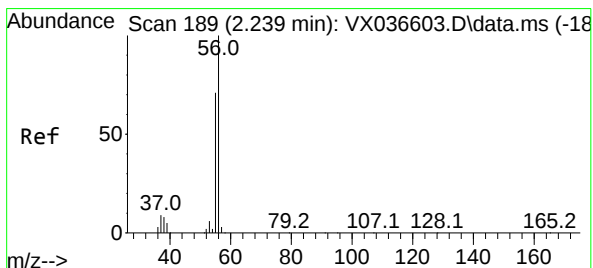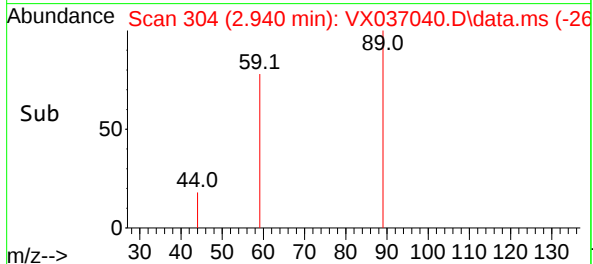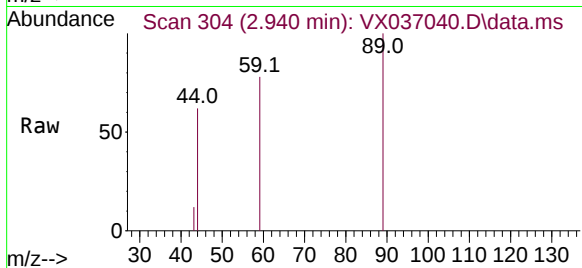

#13

Acrolein

Concen: 0.286 ug/l

RT: 2.233 min Scan# 188

Delta R.T. -0.006 min

Lab File: VX037040.D




Acq: 17 Aug 2023 05:36


Tgt Ion: 56 Resp: 76

Ion Ratio Lower Upper

56 100

55 0.0 57.1 85.7#

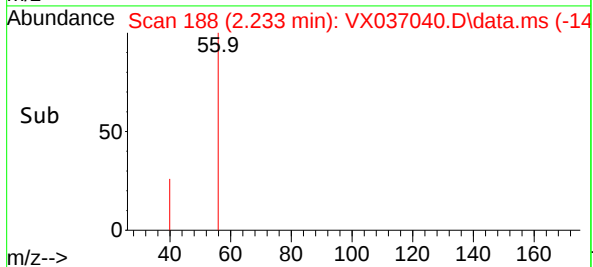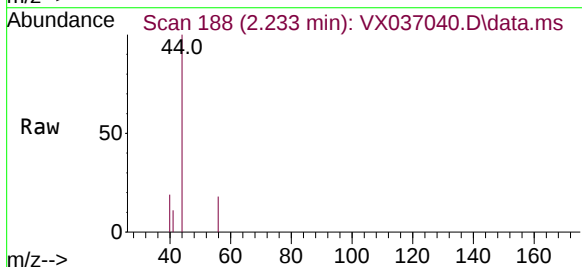



#16

Acetone

Concen: 0.917 ug/l

RT: 2.386 min Scan# 21

Delta R.T. -0.006 min

Lab File: VX037040.D

Acq: 17 Aug 2023 05:36

Instrument :

MSVOA_X

ClientSampleId :





NEVINS-SB02-Z46-47DL

Tgt Ion: 43 Resp: 748

Ion Ratio Lower Upper

43 100

58 35.8 21.9 32.9#

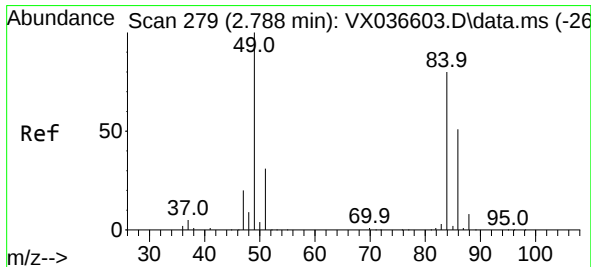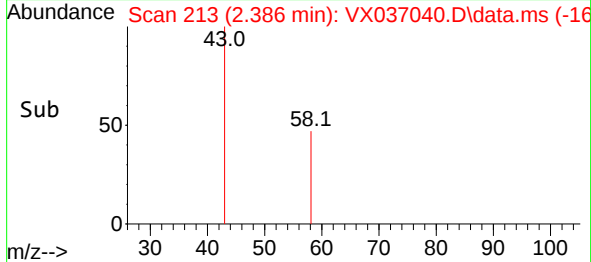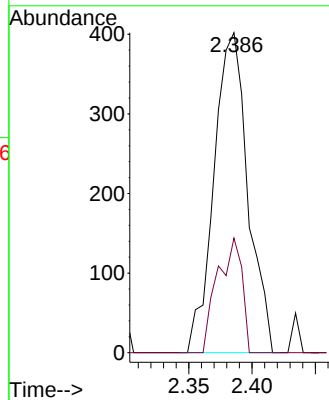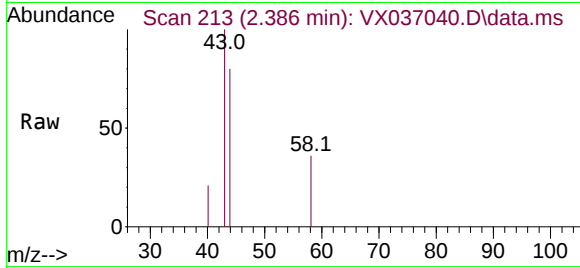

#20

Methylene Chloride

Concen: 0.371 ug/l

RT: 2.794 min Scan# 280

Delta R.T. 0.006 min

Lab File: VX037040.D

Acq: 17 Aug 2023 05:36

Tgt Ion: 84 Resp: 672




Ion Ratio Lower Upper


84 100

49 71.3 103.6 155.4#

51 21.4 33.8 50.6#

86 44.6 49.4 74.0#


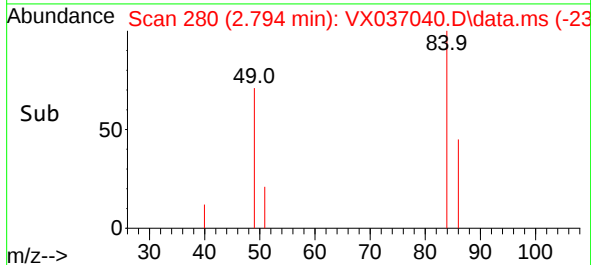
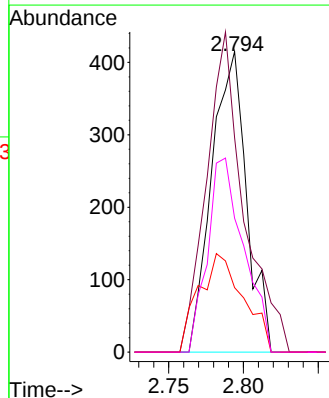
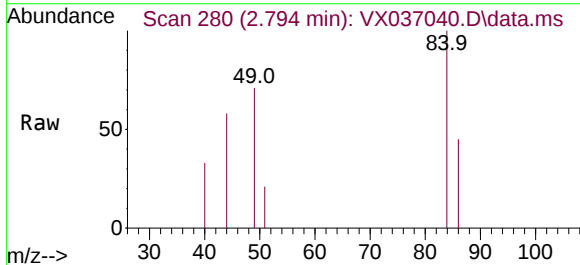




#25
2-Butanone
Concen: 0.480 ug/l
RT: 4.568 min Scan# 51
Delta R.T. 0.006 min
Lab File: VX037040.D
Acq: 17 Aug 2023 05:36




Instrument :
MSVOA_X
ClientSampleId :
NEVINS-SB02-Z46-47DL


Tgt Ion: 43 Resp: 635
Ion Ratio Lower Upper
43 100
72 0.0 19.4 29.2#



#26
2,2-Dichloropropane
Concen: 0.242 ug/l
RT: 4.574 min Scan# 572
Delta R.T. 0.097 min
Lab File: VX037040.D
Acq: 17 Aug 2023 05:36

Tgt Ion: 77 Resp: 712
Ion Ratio Lower Upper
77 100
97 0.0 10.8 32.3#


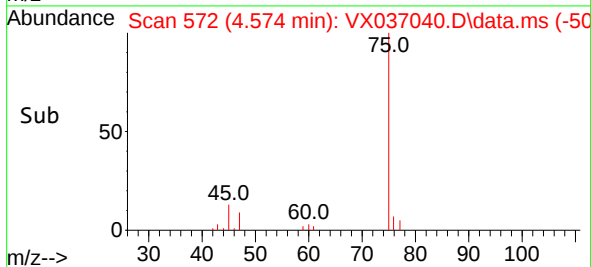

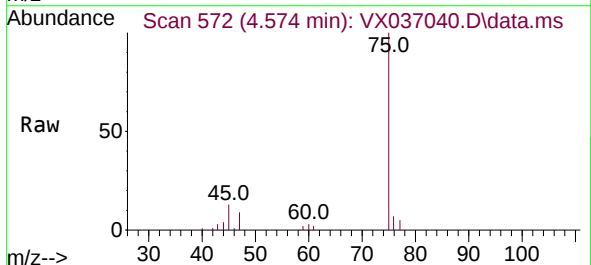




#31
Cyclohexane
Concen: 1.081 ug/l
RT: 5.556 min Scan# 719
Delta R.T. 0.085 min
Lab File: VX037040.D
Acq: 17 Aug 2023 05:36




Instrument :
MSVOA_X
ClientSampleId :
NEVINS-SB02-Z46-47DL


Tgt Ion: 56 Resp: 2941
Ion Ratio Lower Upper
56 100
69 186.7 23.4 35.2#
84 123.2 65.9 98.9#

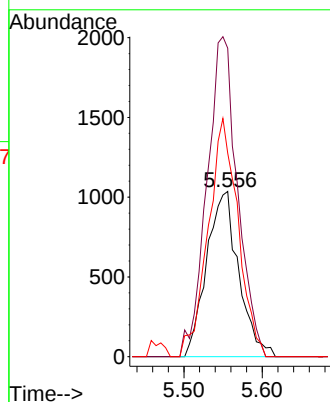

#33
1,2-Dichloroethane-d4
Concen: 47.933 ug/l
RT: 5.958 min Scan# 799
Delta R.T. 0.006 min
Lab File: VX037040.D
Acq: 17 Aug 2023 05:36

Tgt Ion: 65 Resp: 94204
Ion Ratio Lower Upper
65 100
67 49.9 0.0 100.2



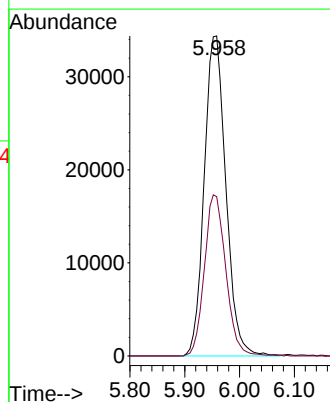
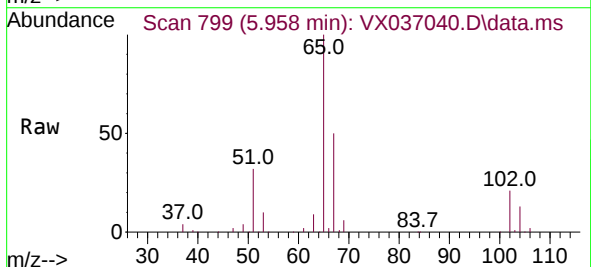


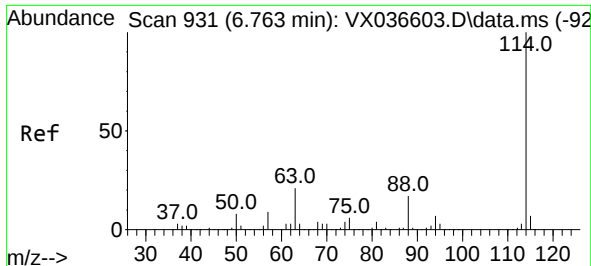

#34
1,4-Difluorobenzene
Concen: 50.000 ug/l
RT: 6.763 min Scan# 911
Delta R.T. -0.000 min
Lab File: VX037040.D
Acq: 17 Aug 2023 05:36




Instrument :
MSVOA_X
ClientSampleId :
NEVINS-SB02-Z46-47DL


Tgt Ion:114 Resp: 244620
Ion Ratio Lower Upper
114 100
63 20.1 0.0 45.0
88 16.7 0.0 36.6

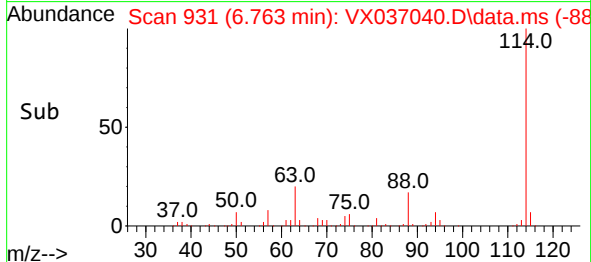

#35
Dibromofluoromethane
Concen: 46.124 ug/l
RT: 5.385 min Scan# 705
Delta R.T. -0.000 min
Lab File: VX037040.D
Acq: 17 Aug 2023 05:36

Tgt Ion:113 Resp: 77552
Ion Ratio Lower Upper
113 100
111 103.2 82.9 124.3
192 18.6 13.3 19.9


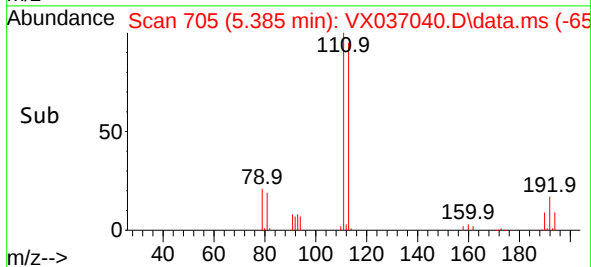

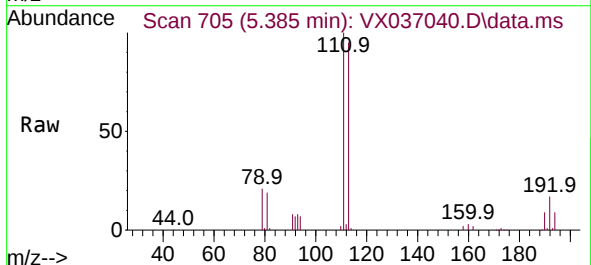


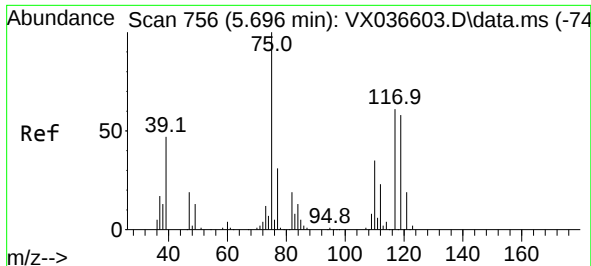

#36
1,1-Dichloropropene
Concen: 4.498 ug/l
RT: 5.550 min Scan# 712
Delta R.T. -0.146 min
Lab File: VX037040.D
Acq: 17 Aug 2023 05:36




Instrument :
MSVOA_X
ClientSampleId :
NEVINS-SB02-Z46-47DL


Tgt Ion: 75 Resp: 11273
Ion Ratio Lower Upper
75 100
110 8.8 17.0 50.9#
77 0.0 24.7 37.1#



#38
Carbon Tetrachloride
Concen: 5.482 ug/l
RT: 5.550 min Scan# 732
Delta R.T. -0.128 min
Lab File: VX037040.D
Acq: 17 Aug 2023 05:36

Tgt Ion: 117 Resp: 14605
Ion Ratio Lower Upper
117 100
119 5.6 78.2 117.2#
121 0.0 24.4 36.6#

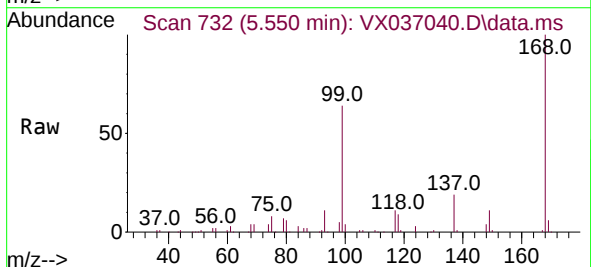

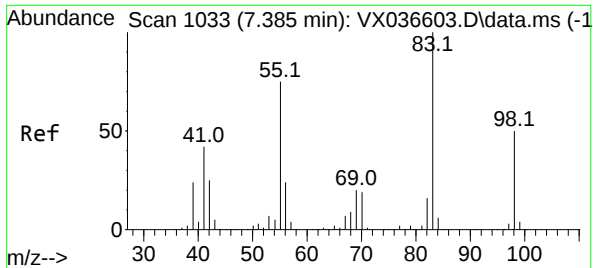

#39

Methylcyclohexane

Concen: 0.264 ug/l

RT: 7.385 min Scan# 1033

Delta R.T. -0.000 min

Lab File: VX037040.D

Acq: 17 Aug 2023 05:36

Instrument :

MSVOA_X

ClientSampleId :

NEVINS-SB02-Z46-47DL





Tgt Ion: 83 Resp: 824

Ion Ratio Lower Upper

83 100

55 60.1 64.6 97.0#

98 40.9 36.7 55.1

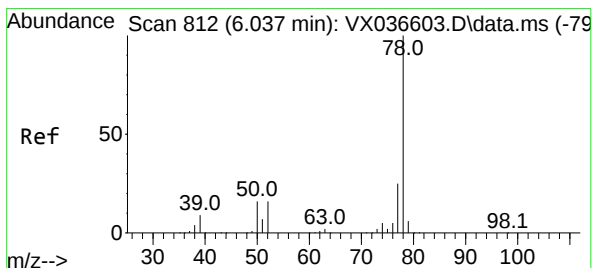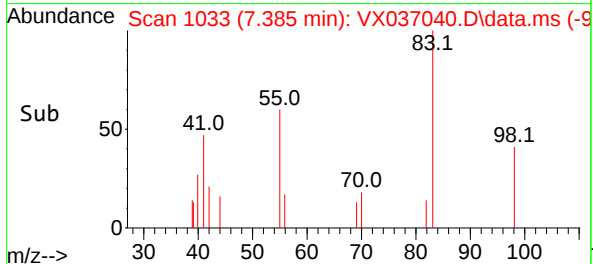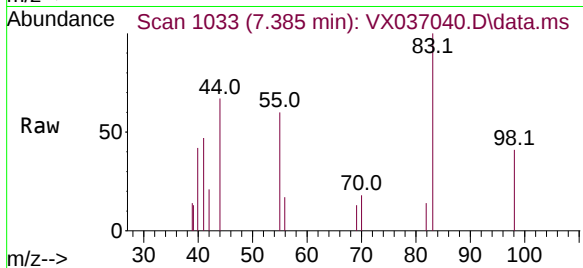

#40

Benzene

Concen: 1.669 ug/l

RT: 6.037 min Scan# 812

Delta R.T. -0.000 min

Lab File: VX037040.D




Acq: 17 Aug 2023 05:36


Tgt Ion: 78 Resp: 12166

Ion Ratio Lower Upper

78 100

77 24.6 19.3 28.9


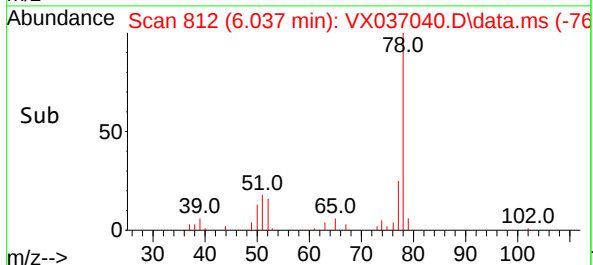

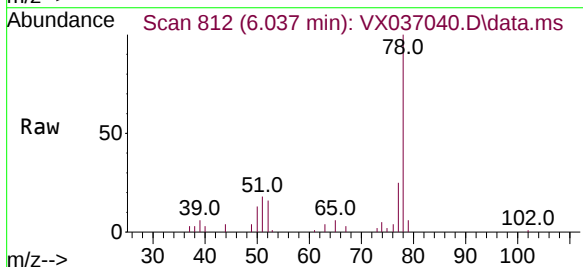


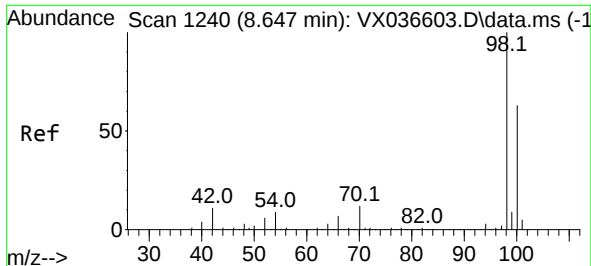

#50
Toluene-d8
Concen: 49.863 ug/l
RT: 8.647 min Scan# 1240
Delta R.T. -0.000 min
Lab File: VX037040.D
Acq: 17 Aug 2023 05:36




Instrument :
MSVOA_X
ClientSampleId :
NEVINS-SB02-Z46-47DL


Tgt Ion: 98 Resp: 297310
Ion Ratio Lower Upper
98 100
100 66.0 53.1 79.7



#51
4-Methyl-2-Pentanone
Concen: 0.459 ug/l
RT: 8.647 min Scan# 1240
Delta R.T. 0.073 min
Lab File: VX037040.D
Acq: 17 Aug 2023 05:36

Tgt Ion: 43 Resp: 1241
Ion Ratio Lower Upper
43 100
58 191.5 30.4 45.6#




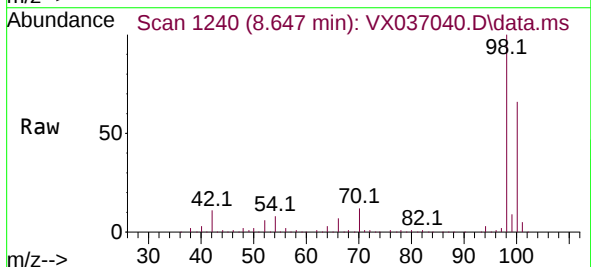




#62
4-Bromofluorobenzene
Concen: 55.171 ug/l
RT: 11.079 min Scan# 1639
Delta R.T. -0.000 min
Lab File: VX037040.D
Acq: 17 Aug 2023 05:36




Instrument :
MSVOA_X
ClientSampleId :
NEVINS-SB02-Z46-47DL


Tgt Ion: 95 Resp: 124110
Ion Ratio Lower Upper
95 100
174 73.0 0.0 135.6
176 71.1 0.0 131.0

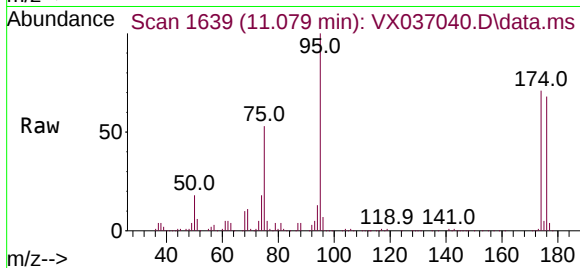

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 10.055 min Scan# 1471
Delta R.T. -0.000 min
Lab File: VX037040.D
Acq: 17 Aug 2023 05:36

Tgt Ion: 117 Resp: 243557
Ion Ratio Lower Upper
117 100
82 55.8 46.2 69.4
119 32.2 25.5 38.3


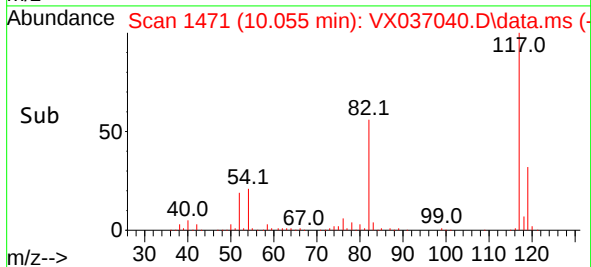

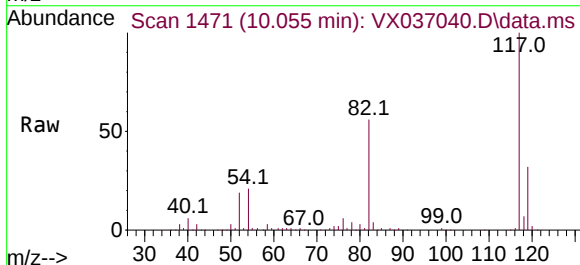


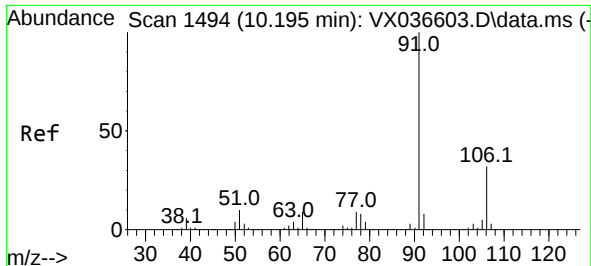

#67
Ethyl Benzene
Concen: 15.841 ug/l
RT: 10.195 min Scan# 1494
Delta R.T. -0.000 min
Lab File: VX037040.D
Acq: 17 Aug 2023 05:36




Instrument :
MSVOA_X
ClientSampleId :
NEVINS-SB02-Z46-47DL


Tgt Ion: 91 Resp: 155359
Ion Ratio Lower Upper
91 100
106 30.6 24.9 37.3

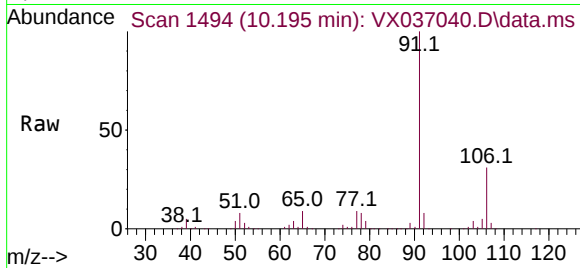

#68
m/p-Xylenes
Concen: 1.489 ug/l
RT: 10.305 min Scan# 1512
Delta R.T. 0.006 min
Lab File: VX037040.D
Acq: 17 Aug 2023 05:36

Tgt Ion: 106 Resp: 5449
Ion Ratio Lower Upper
106 100
91 222.6 165.5 248.3

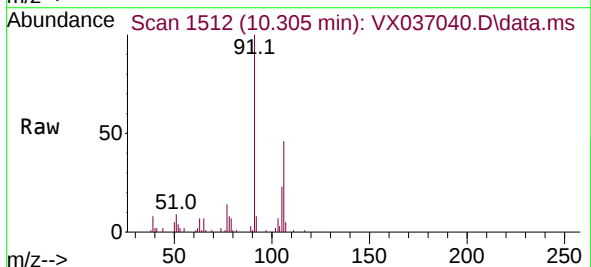



#69

o-Xylene

Concen: 4.918 ug/l

RT: 10.640 min Scan# 11

Delta R.T. -0.000 min

Lab File: VX037040.D

Acq: 17 Aug 2023 05:36

Instrument :

MSVOA_X

ClientSampleId :





NEVINS-SB02-Z46-47DL

Tgt Ion:106 Resp: 17965

Ion Ratio Lower Upper

106 100

91 218.1 108.9 326.8

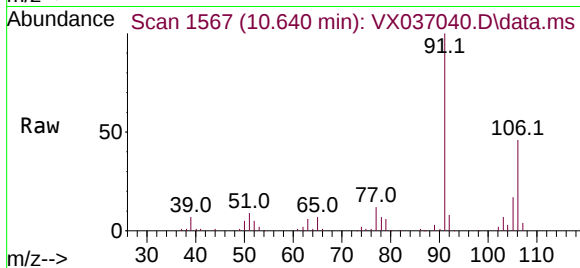

#72

1,4-Dichlorobenzene-d4

Concen: 50.000 ug/l

RT: 12.024 min Scan# 1794

Delta R.T. -0.000 min

Lab File: VX037040.D

Acq: 17 Aug 2023 05:36




Tgt Ion:152 Resp: 119810


Ion Ratio Lower Upper

152 100

115 63.2 43.3 129.9

150 156.7 0.0 345.0




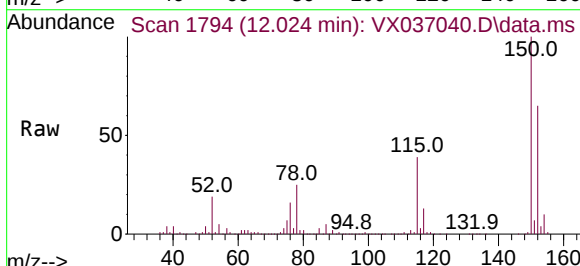




#73
Isopropylbenzene
Concen: 1.897 ug/l
RT: 10.963 min Scan# 1620
Delta R.T. -0.000 min
Lab File: VX037040.D
Acq: 17 Aug 2023 05:36




Instrument :
MSVOA_X
ClientSampleId :
NEVINS-SB02-Z46-47DL


Tgt Ion:105 Resp: 18813
Ion Ratio Lower Upper
105 100
120 26.8 12.9 38.6

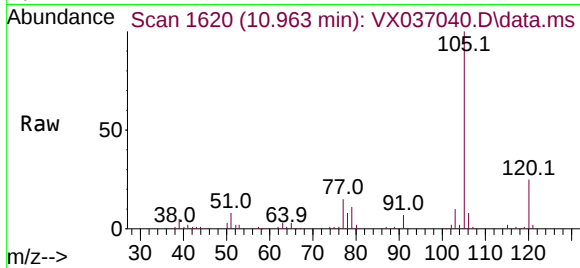

#76
1,2,3-Trichloropropane
Concen: 23.082 ug/l
RT: 11.079 min Scan# 1639
Delta R.T. -0.159 min
Lab File: VX037040.D
Acq: 17 Aug 2023 05:36

Tgt Ion: 75 Resp: 65046
Ion Ratio Lower Upper
75 100
77 1.2 19.1 57.5#




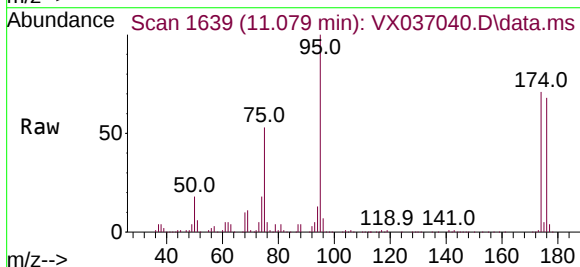


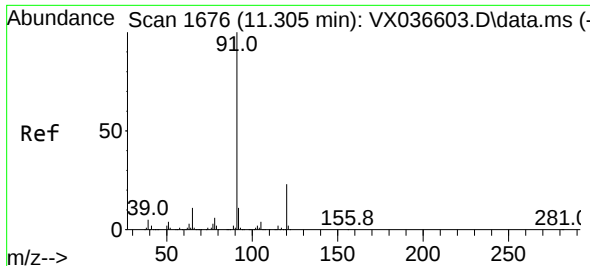

#78
n-propylbenzene
Concen: 0.958 ug/l
RT: 11.305 min Scan# 1676
Delta R.T. -0.000 min
Lab File: VX037040.D
Acq: 17 Aug 2023 05:36




Instrument :
MSVOA_X
ClientSampleId :
NEVINS-SB02-Z46-47DL


Tgt Ion: 91 Resp: 10981
Ion Ratio Lower Upper
91 100
120 22.4 11.5 34.4

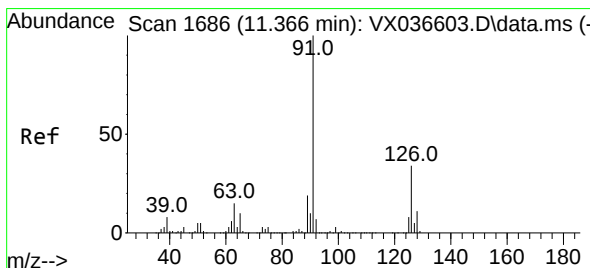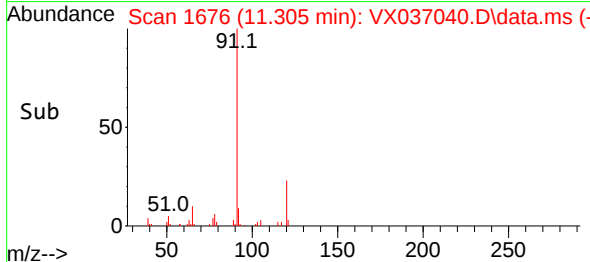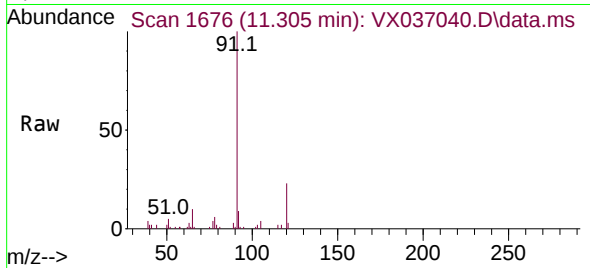

#79
2-Chlorotoluene
Concen: 0.825 ug/l
RT: 11.402 min Scan# 1692
Delta R.T. 0.037 min
Lab File: VX037040.D
Acq: 17 Aug 2023 05:36

Tgt Ion: 91 Resp: 5736
Ion Ratio Lower Upper
91 100
126 0.9 16.3 48.8#


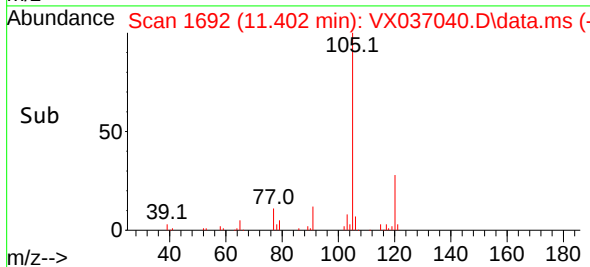

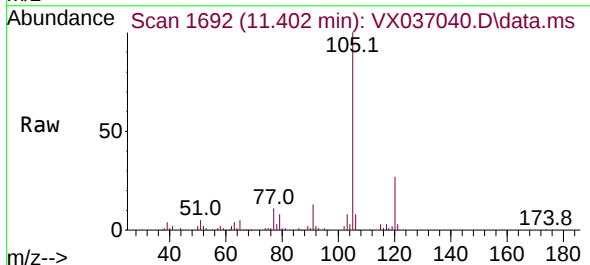


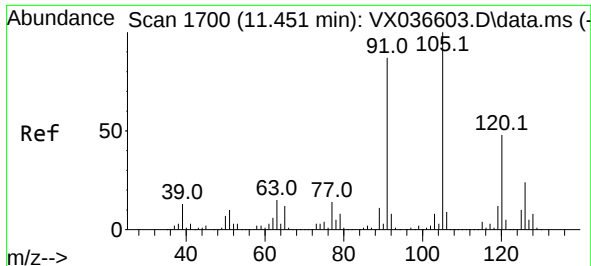

#80
1,3,5-Trimethylbenzene
Concen: 3.104 ug/l
RT: 11.451 min Scan# 11
Delta R.T. -0.000 min
Lab File: VX037040.D
Acq: 17 Aug 2023 05:36




Instrument :
MSVOA_X
ClientSampleId :
NEVINS-SB02-Z46-47DL


Tgt Ion:105 Resp: 25744
Ion Ratio Lower Upper
105 100
120 47.0 24.1 72.3

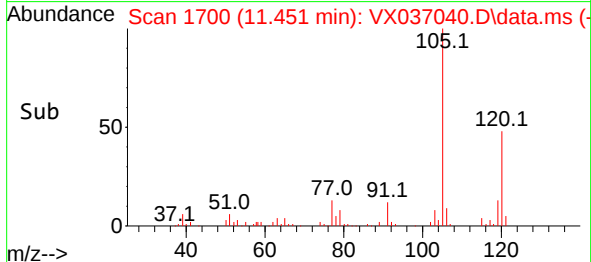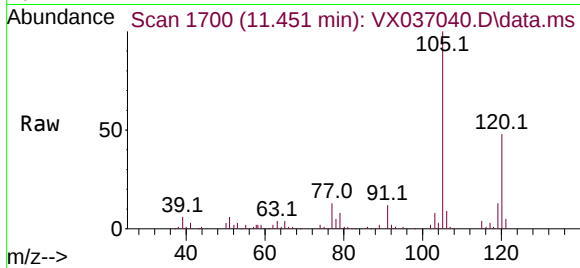

#81
trans-1,4-Dichloro-2-butene
Concen: 52.316 ug/l
RT: 11.079 min Scan# 1639
Delta R.T. 0.061 min
Lab File: VX037040.D
Acq: 17 Aug 2023 05:36

Tgt Ion: 75 Resp: 65046
Ion Ratio Lower Upper
75 100
53 0.0 90.5 135.7#
89 0.0 36.9 55.3#

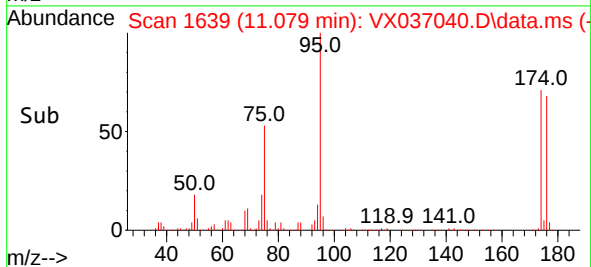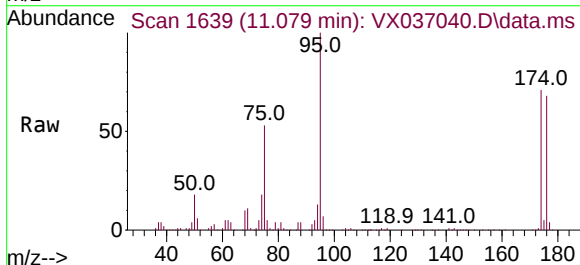



#82

4-Chlorotoluene

Concen: 0.411 ug/l

RT: 11.451 min Scan# 11

Delta R.T. -0.000 min

Lab File: VX037040.D

Acq: 17 Aug 2023 05:36

Instrument :

MSVOA_X

ClientSampleId :





NEVINS-SB02-Z46-47DL

Tgt Ion: 91 Resp: 3251

Ion Ratio Lower Upper

91 100

126 0.0 14.2 42.6#

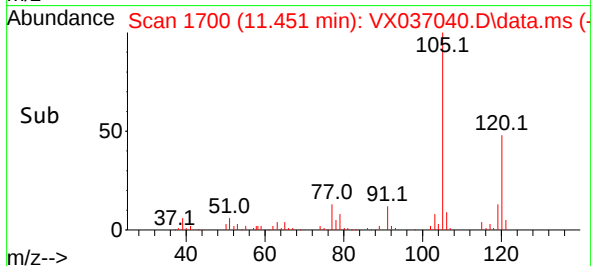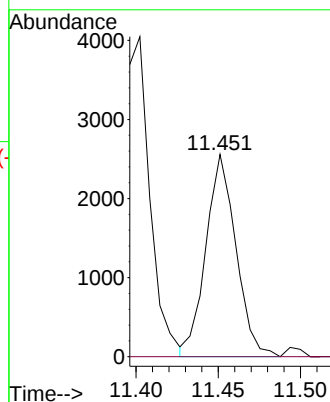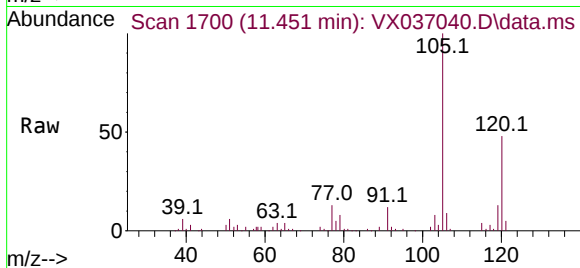

#83

tert-Butylbenzene

Concen: 1.360 ug/l

RT: 11.750 min Scan# 1749

Delta R.T. 0.037 min

Lab File: VX037040.D

Acq: 17 Aug 2023 05:36




Tgt Ion: 119 Resp: 11086


Ion Ratio Lower Upper

119 100

91 101.9 31.2 93.6#

134 0.0 11.7 35.0#

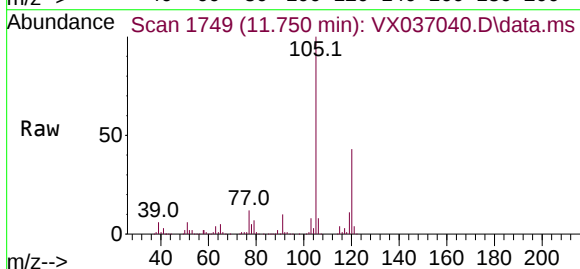



#84

1,2,4-Trimethylbenzene

Concen: 11.002 ug/l

RT: 11.750 min Scan# 1749

Delta R.T. -0.000 min

Lab File: VX037040.D

Acq: 17 Aug 2023 05:36

Instrument :

MSVOA_X

ClientSampleId :





NEVINS-SB02-Z46-47DL

Tgt Ion:105 Resp: 91266

Ion Ratio Lower Upper

105 100

120 43.8 21.2 63.6

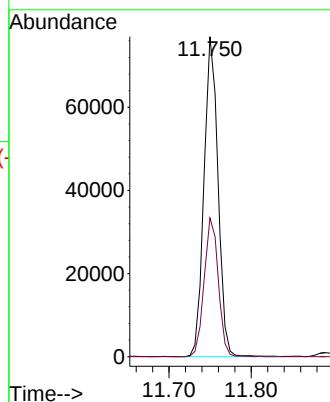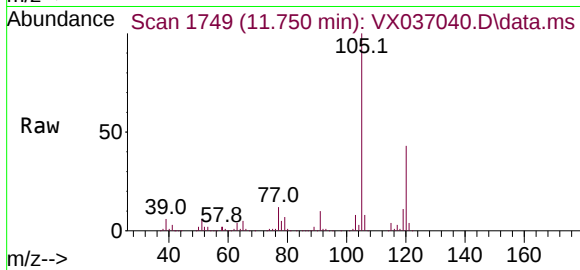

#85

sec-Butylbenzene

Concen: 8.981 ug/l

RT: 11.750 min Scan# 1749

Delta R.T. -0.140 min

Lab File: VX037040.D




Acq: 17 Aug 2023 05:36


Tgt Ion:105 Resp: 91266

Ion Ratio Lower Upper

105 100

134 0.0 9.8 29.4#




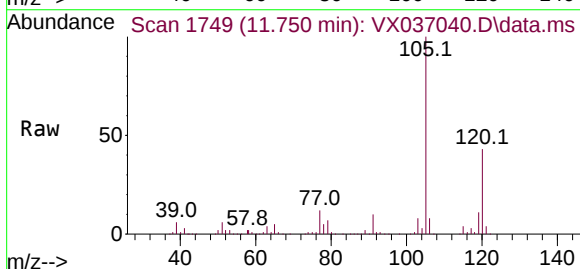




#86
p-Isopropyltoluene
Concen: 1.374 ug/l
RT: 12.006 min Scan# 119
Delta R.T. -0.000 min
Lab File: VX037040.D
Acq: 17 Aug 2023 05:36




Instrument :
MSVOA_X
ClientSampleId :
NEVINS-SB02-Z46-47DL


Tgt Ion:	119	Resp:	11489
Ion	Ratio	Lower	Upper
119	100		
134	26.8	12.8	38.3
91	33.9	13.1	39.3

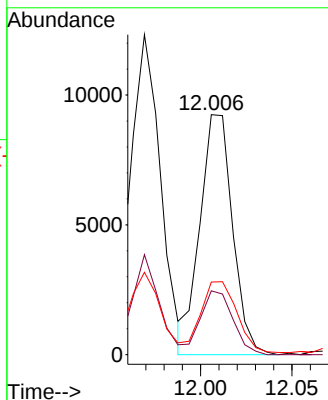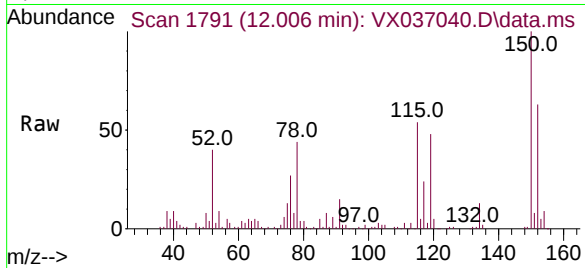

#89
n-Butylbenzene
Concen: 2.672 ug/l
RT: 12.317 min Scan# 1842
Delta R.T. -0.012 min
Lab File: VX037040.D
Acq: 17 Aug 2023 05:36

Tgt Ion:	91	Resp:	20002
Ion	Ratio	Lower	Upper
91	100		
92	19.2	27.4	82.0#
134	133.4	12.6	37.8#



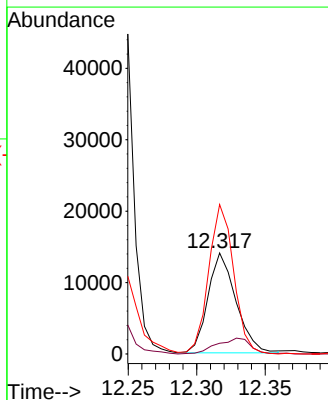
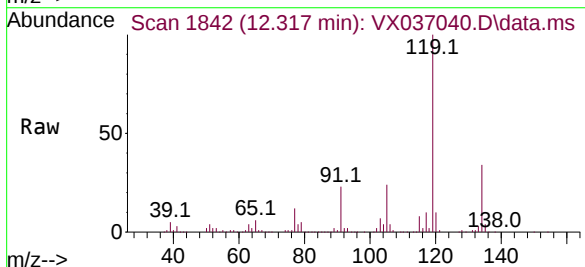


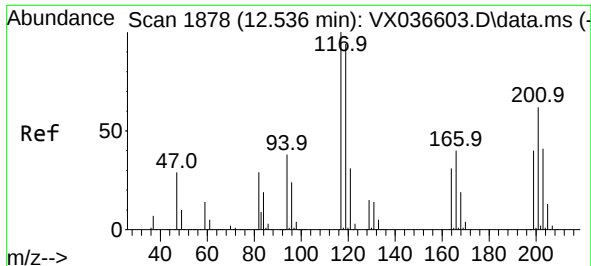

#90
Hexachloroethane
Concen: 28.458 ug/l
RT: 12.695 min Scan# 1904
Delta R.T. 0.158 min
Lab File: VX037040.D
Acq: 17 Aug 2023 05:36

Instrument :
MSVOA_X
ClientSampleId :
NEVINS-SB02-Z46-47DL

Tgt Ion:117 Resp: 48242
Ion Ratio Lower Upper
117 100
201 0.0 32.9 98.6#

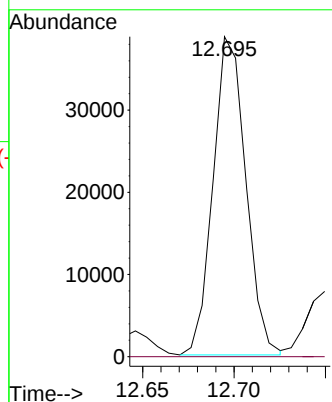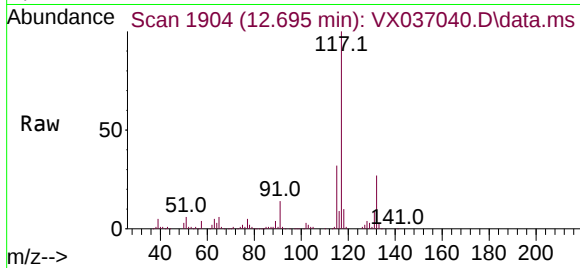

#95
Naphthalene
Concen: 414.821 ug/l
RT: 13.774 min Scan# 2081
Delta R.T. -0.000 min
Lab File: VX037040.D
Acq: 17 Aug 2023 05:36

Tgt Ion:128 Resp: 3594315
Ion Ratio Lower Upper
128 100
127 13.7 10.3 15.5
129 11.9 8.8 13.2

