

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX081623\
 Data File : VX037022.D
 Acq On : 16 Aug 2023 17:00
 Operator : JC/MD
 Sample : 04024-10
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 RE114D2-20230815

Integration Parameters: RTEINT.P

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X072123W.M
 Title : SW846 8260

Signal : TIC: VX037022.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	2.325	197	203	211	rBV2	23548	44621	6.27%	0.995%
2	4.489	551	558	569	rBV2	3517	9629	1.35%	0.215%
3	5.385	694	705	722	rBV2	81703	237847	33.44%	5.301%
4	5.550	722	732	747	rVB	132276	373428	52.50%	8.323%
5	5.958	788	799	812	rBV	85682	225915	31.76%	5.035%
6	6.763	921	931	948	rBV	222197	522759	73.49%	11.651%
7	7.129	982	991	1011	rBV	250379	548077	77.05%	12.216%
8	8.647	1234	1240	1256	rBV	445697	711356	100.00%	15.855%
9	10.055	1465	1471	1488	rBV	498120	659348	92.69%	14.696%
10	11.079	1634	1639	1650	rBV	406903	518250	72.85%	11.551%
11	12.024	1788	1794	1803	rBV	490292	635472	89.33%	14.163%




Sum of corrected areas: 4486702

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX081623\
Data File : VX037022.D
Acq On : 16 Aug 2023 17:00
Operator : JC/MD
Sample : 04024-10
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 19 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
RE114D2-20230815

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X072123W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

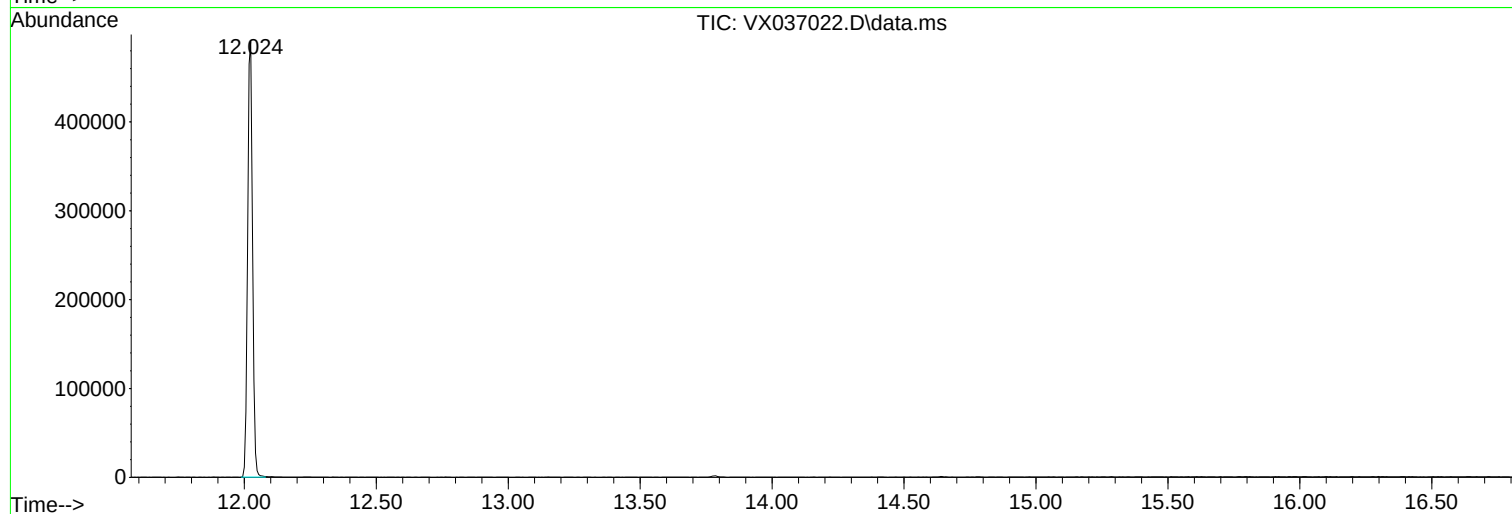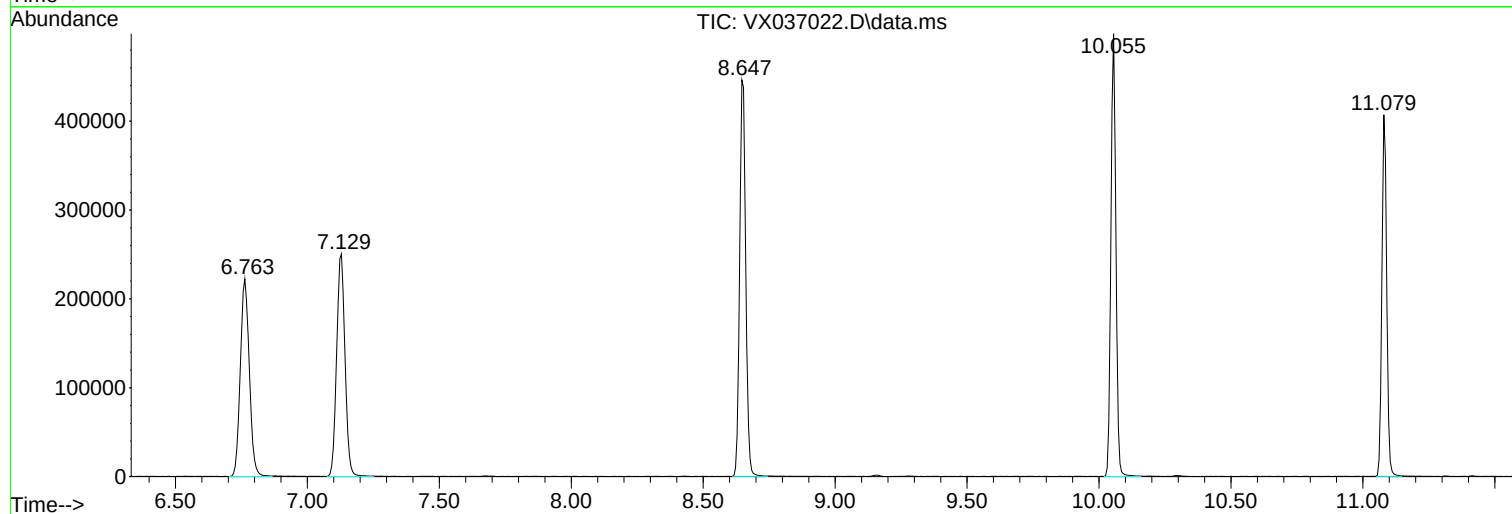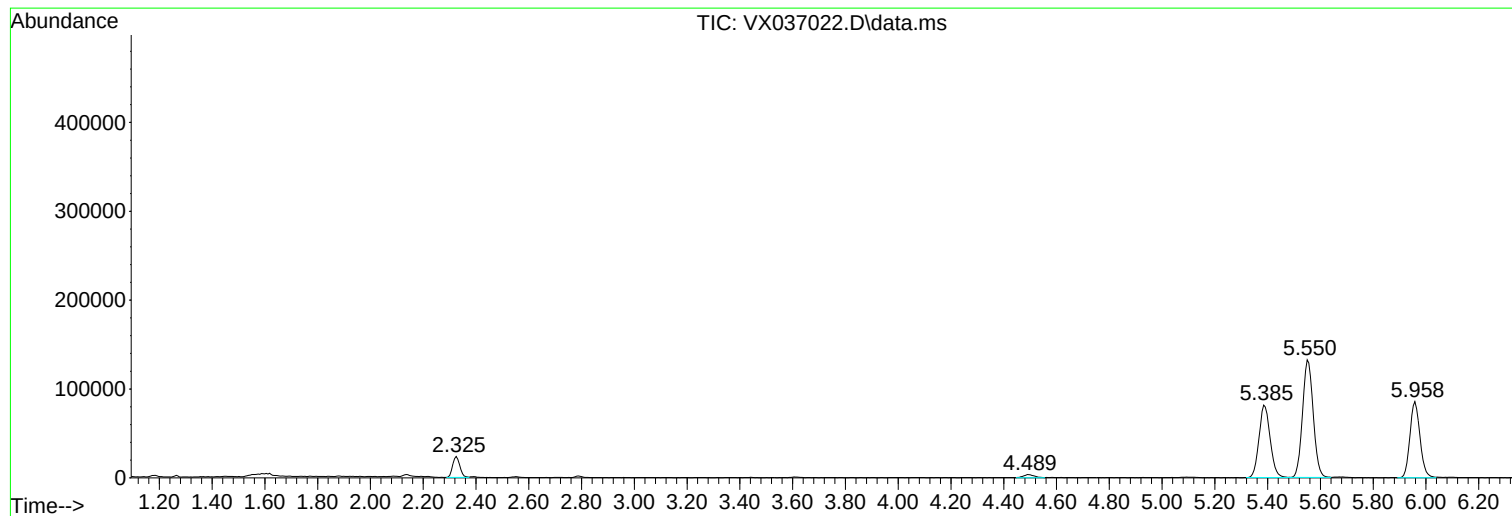

Library Search Compound Report

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX081623\
Data File : VX037022.D
Acq On : 16 Aug 2023 17:00
Operator : JC/MD
Sample : 04024-10
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 19 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
RE114D2-20230815

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X072123W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX081623\
Data File : VX037022.D
Acq On : 16 Aug 2023 17:00
Operator : JC/MD
Sample : 04024-10
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 19 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
RE114D2-20230815

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X072123W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------