

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX081623\
Data File : VX037027.D
Acq On : 16 Aug 2023 19:00
Operator : JC/MD
Sample : 04024-20
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 24 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
RE108D1-20230815

Integration Parameters: RTEINT.P

Integrator: RTE

Smoothing : ON

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 3 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X072123W.M

Title : SW846 8260

Signal : TIC: VX037027.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.575	69	80	84	rBV6	2880	8505	1.12%	0.190%
2	5.385	693	705	722	rBV	88591	256783	33.76%	5.728%
3	5.556	722	733	748	rVB2	139526	401814	52.83%	8.964%
4	5.958	785	799	816	rBV2	91609	247686	32.57%	5.525%
5	6.763	921	931	952	rBV	238186	559546	73.57%	12.482%
6	7.123	982	990	1007	rBV	143319	313119	41.17%	6.985%
7	8.647	1234	1240	1256	rBV	492289	760560	100.00%	16.966%
8	9.275	1337	1343	1349	rBV2	15637	23510	3.09%	0.524%
9	10.055	1465	1471	1489	rBV	508333	697649	91.73%	15.563%
10	11.079	1634	1639	1654	rBV	434580	547246	71.95%	12.208%
11	12.018	1788	1793	1806	rBV	519071	666298	87.61%	14.864%




Sum of corrected areas: 4482716

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX081623\
Data File : VX037027.D
Acq On : 16 Aug 2023 19:00
Operator : JC/MD
Sample : 04024-20
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 24 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
RE108D1-20230815

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X072123W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

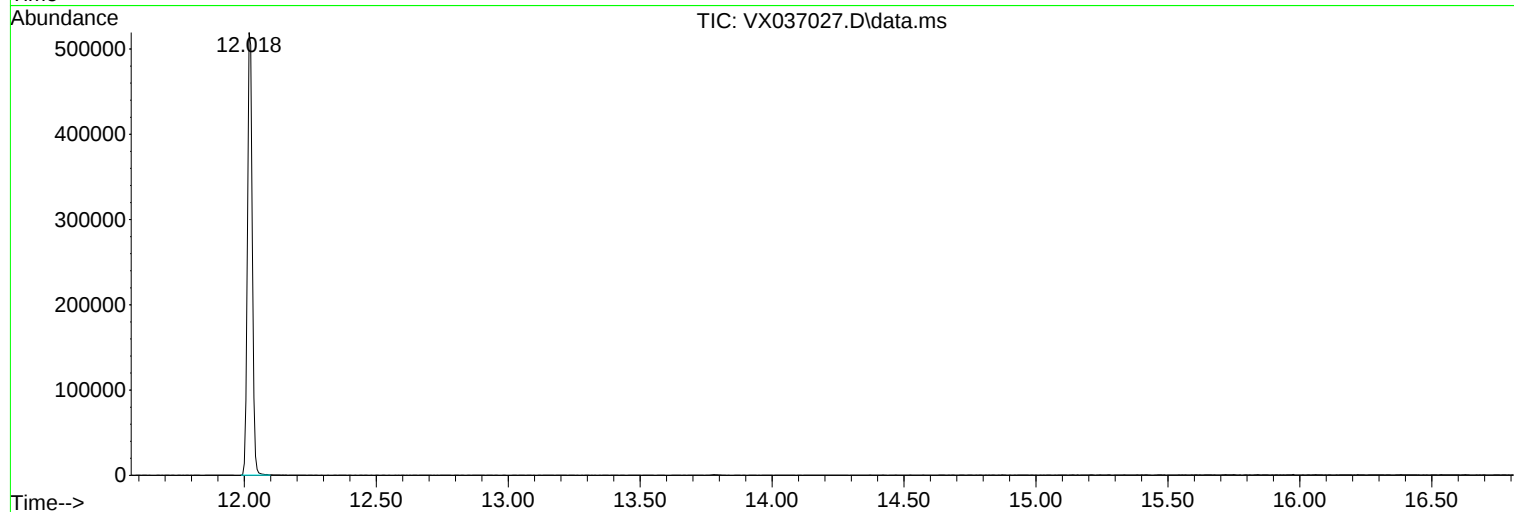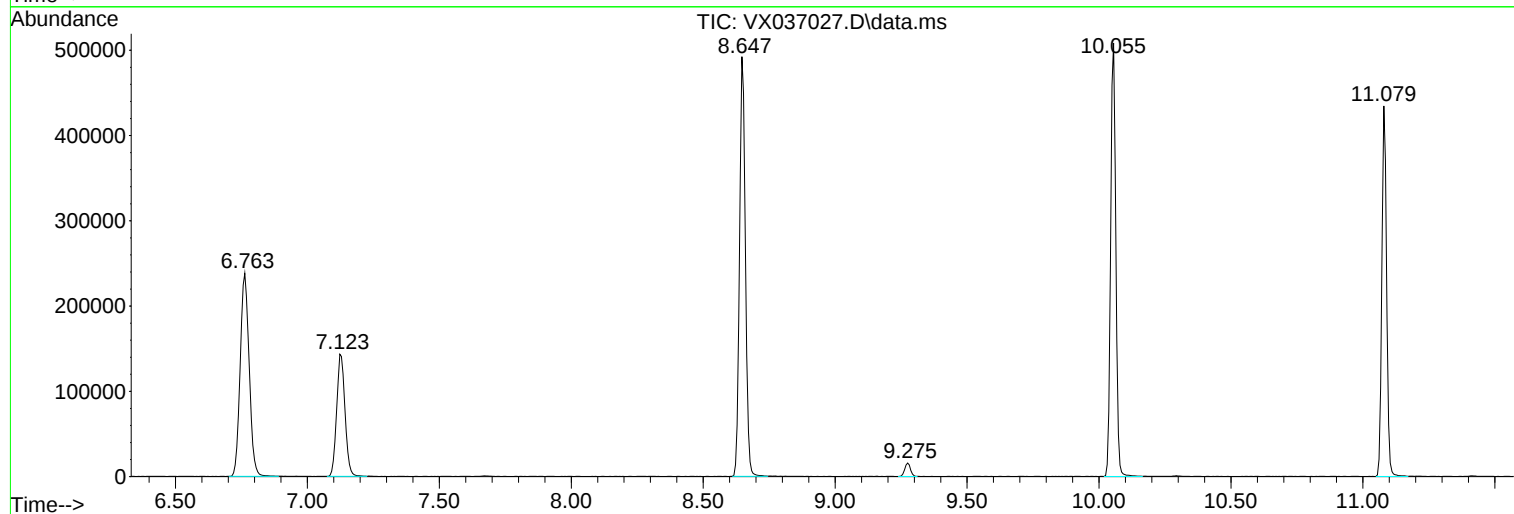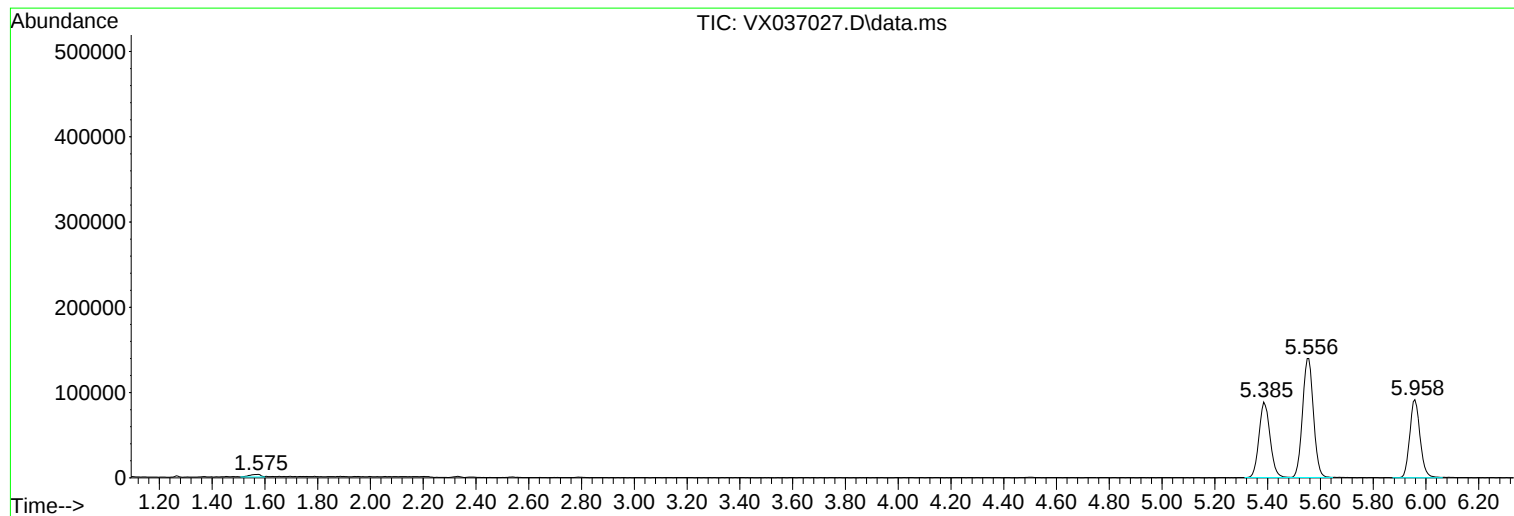

Library Search Compound Report

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX081623\
Data File : VX037027.D
Acq On : 16 Aug 2023 19:00
Operator : JC/MD
Sample : 04024-20
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 24 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
RE108D1-20230815

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X072123W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX081623\
Data File : VX037027.D
Acq On : 16 Aug 2023 19:00
Operator : JC/MD
Sample : 04024-20
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 24 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
RE108D1-20230815

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X072123W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------