


Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX081624\
Data File : VX043060.D
Acq On : 16 Aug 2024 07:51
Operator : JC/MD
Sample : BFB
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
BFB

Integration File: RTEINT3.P

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\624X081324W.M
Title : METHOD 624 VOLATILE ORGANIC ANALYSIS
Last Update : Tue Aug 13 13:22:56 2024

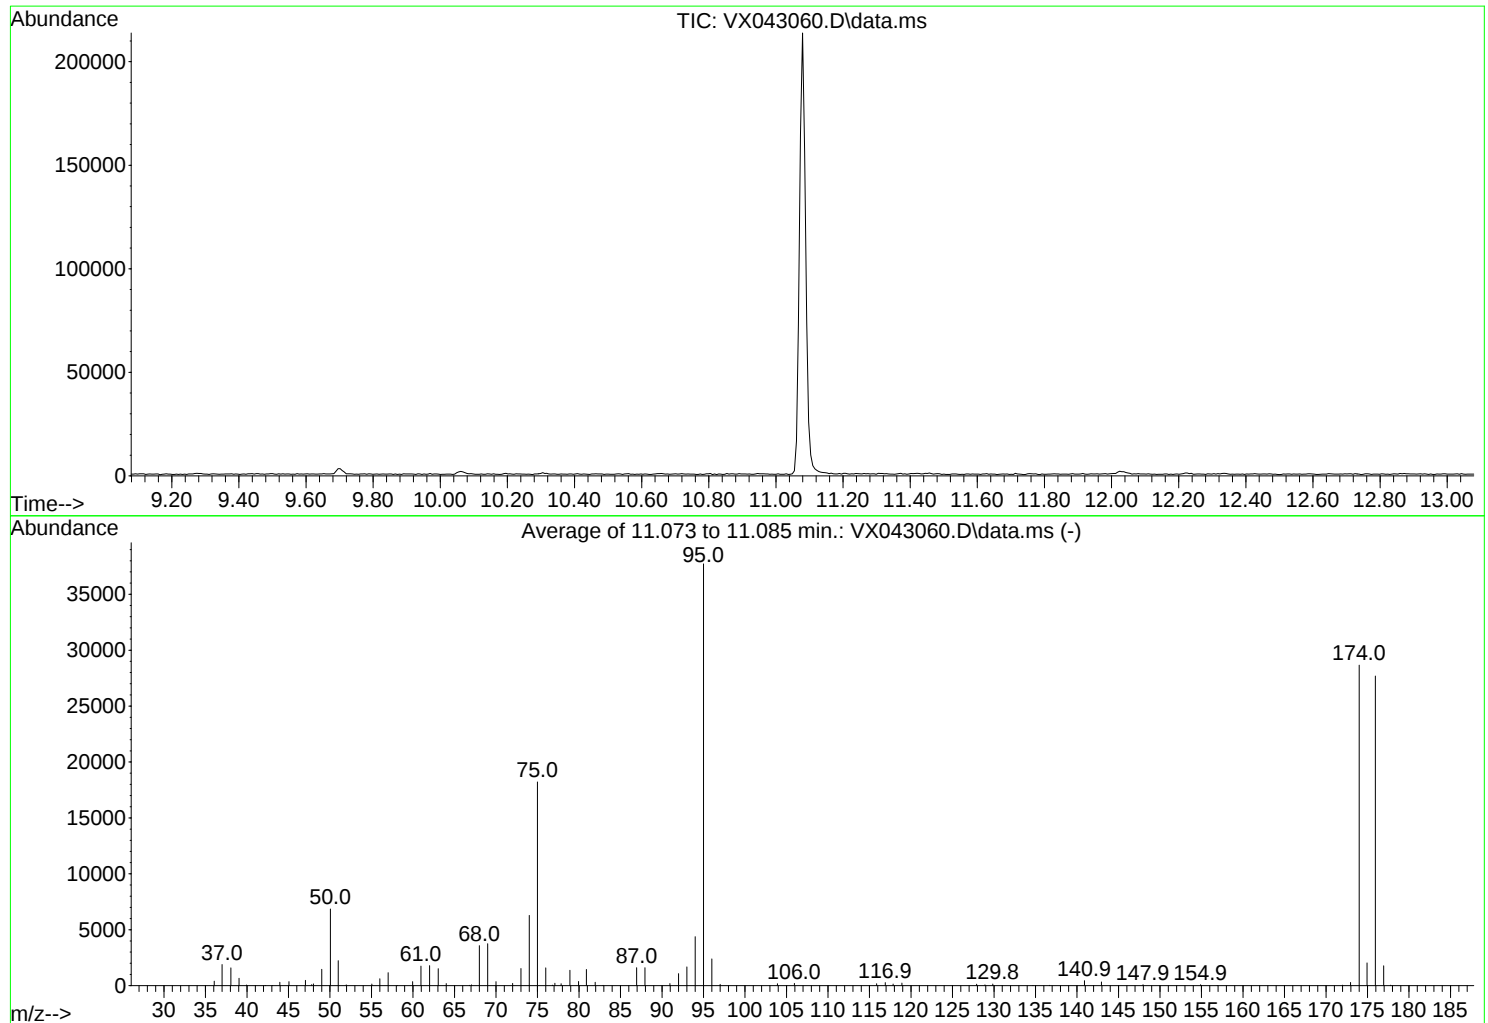

AutoFind: Scans 1638, 1639, 1640; Background Corrected with Scan 1633

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	18.2	6856	PASS
75	95	30	60	48.3	18225	PASS
95	95	100	100	100.0	37725	PASS
96	95	5	9	6.4	2397	PASS
173	174	0.00	2	1.0	292	PASS
174	95	50	100	76.0	28661	PASS
175	174	5	9	7.1	2029	PASS
176	174	95	101	96.6	27691	PASS
177	176	5	9	6.4	1779	PASS