

Data Path : Z:\VOASRV\HPCHEM1\MSVOA X\DATA\VX081718\  
 Data File : VX004122.D  
 Acq On : 17 Aug 2018 10:37  
 Operator : JC/MD  
 Sample : VX0817WBL01  
 Misc : 5.0mL/MSVOA X/WATER  
 ALS Vial : 3 Sample Multiplier: 1

Instrument :  
 MSVOA\_X  
 ClientSampleId :  
 VX0817WBL01

Integration Parameters: RTEINT.P

Integrator: RTE

Smoothing : ON

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 3 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA\_X\METHOD\82X081418W.M

Title : SW846 8260

Signal : TIC

| peak<br># | R.T.<br>min | first<br>scan | max<br>scan | last<br>scan | PK<br>TY | peak<br>height | corr.<br>area | corr.<br>% max. | % of<br>total |
|-----------|-------------|---------------|-------------|--------------|----------|----------------|---------------|-----------------|---------------|
| 1         | 1.075       | 75            | 80          | 108          | rBV      | 1439074        | 1967299       | 100.00%         | 19.589%       |
| 2         | 1.599       | 159           | 166         | 171          | rVB      | 9759           | 20292         | 1.03%           | 0.202%        |
| 3         | 4.727       | 671           | 679         | 690          | rBV      | 5977           | 21423         | 1.09%           | 0.213%        |
| 4         | 5.501       | 792           | 806         | 821          | rBV2     | 203642         | 578313        | 29.40%          | 5.758%        |
| 5         | 5.659       | 821           | 832         | 851          | rVB      | 281386         | 789610        | 40.14%          | 7.862%        |
| 6         | 6.068       | 886           | 899         | 915          | rBV      | 222917         | 579166        | 29.44%          | 5.767%        |
| 7         | 6.860       | 1018          | 1029        | 1045         | rBV      | 431495         | 998659        | 50.76%          | 9.944%        |
| 8         | 8.714       | 1326          | 1333        | 1348         | rBV      | 1052913        | 1628868       | 82.80%          | 16.219%       |
| 9         | 10.116      | 1557          | 1563        | 1578         | rVB      | 873282         | 1210040       | 61.51%          | 12.049%       |
| 10        | 11.140      | 1725          | 1731        | 1743         | rBV      | 812429         | 1000795       | 50.87%          | 9.965%        |
| 11        | 12.079      | 1879          | 1885        | 1895         | rBV      | 1035559        | 1248523       | 63.46%          | 12.432%       |


Sum of corrected areas: 10042988

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA X\DATA\VX081718\  
Data File : VX004122.D  
Acq On : 17 Aug 2018 10:37  
Operator : JC/MD  
Sample : VX0817WBL01  
Misc : 5.0mL/MSVOA X/WATER  
ALS Vial : 3 Sample Multiplier: 1

Instrument :  
MSVOA\_X  
ClientSampleId :  
VX0817WBL01

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA\_X\METHOD\82X081418W.M  
Quant Title : SW846 8260

TIC Library : C:\DATABASE\NIST11.L  
TIC Integration Parameters: LSCINT.P

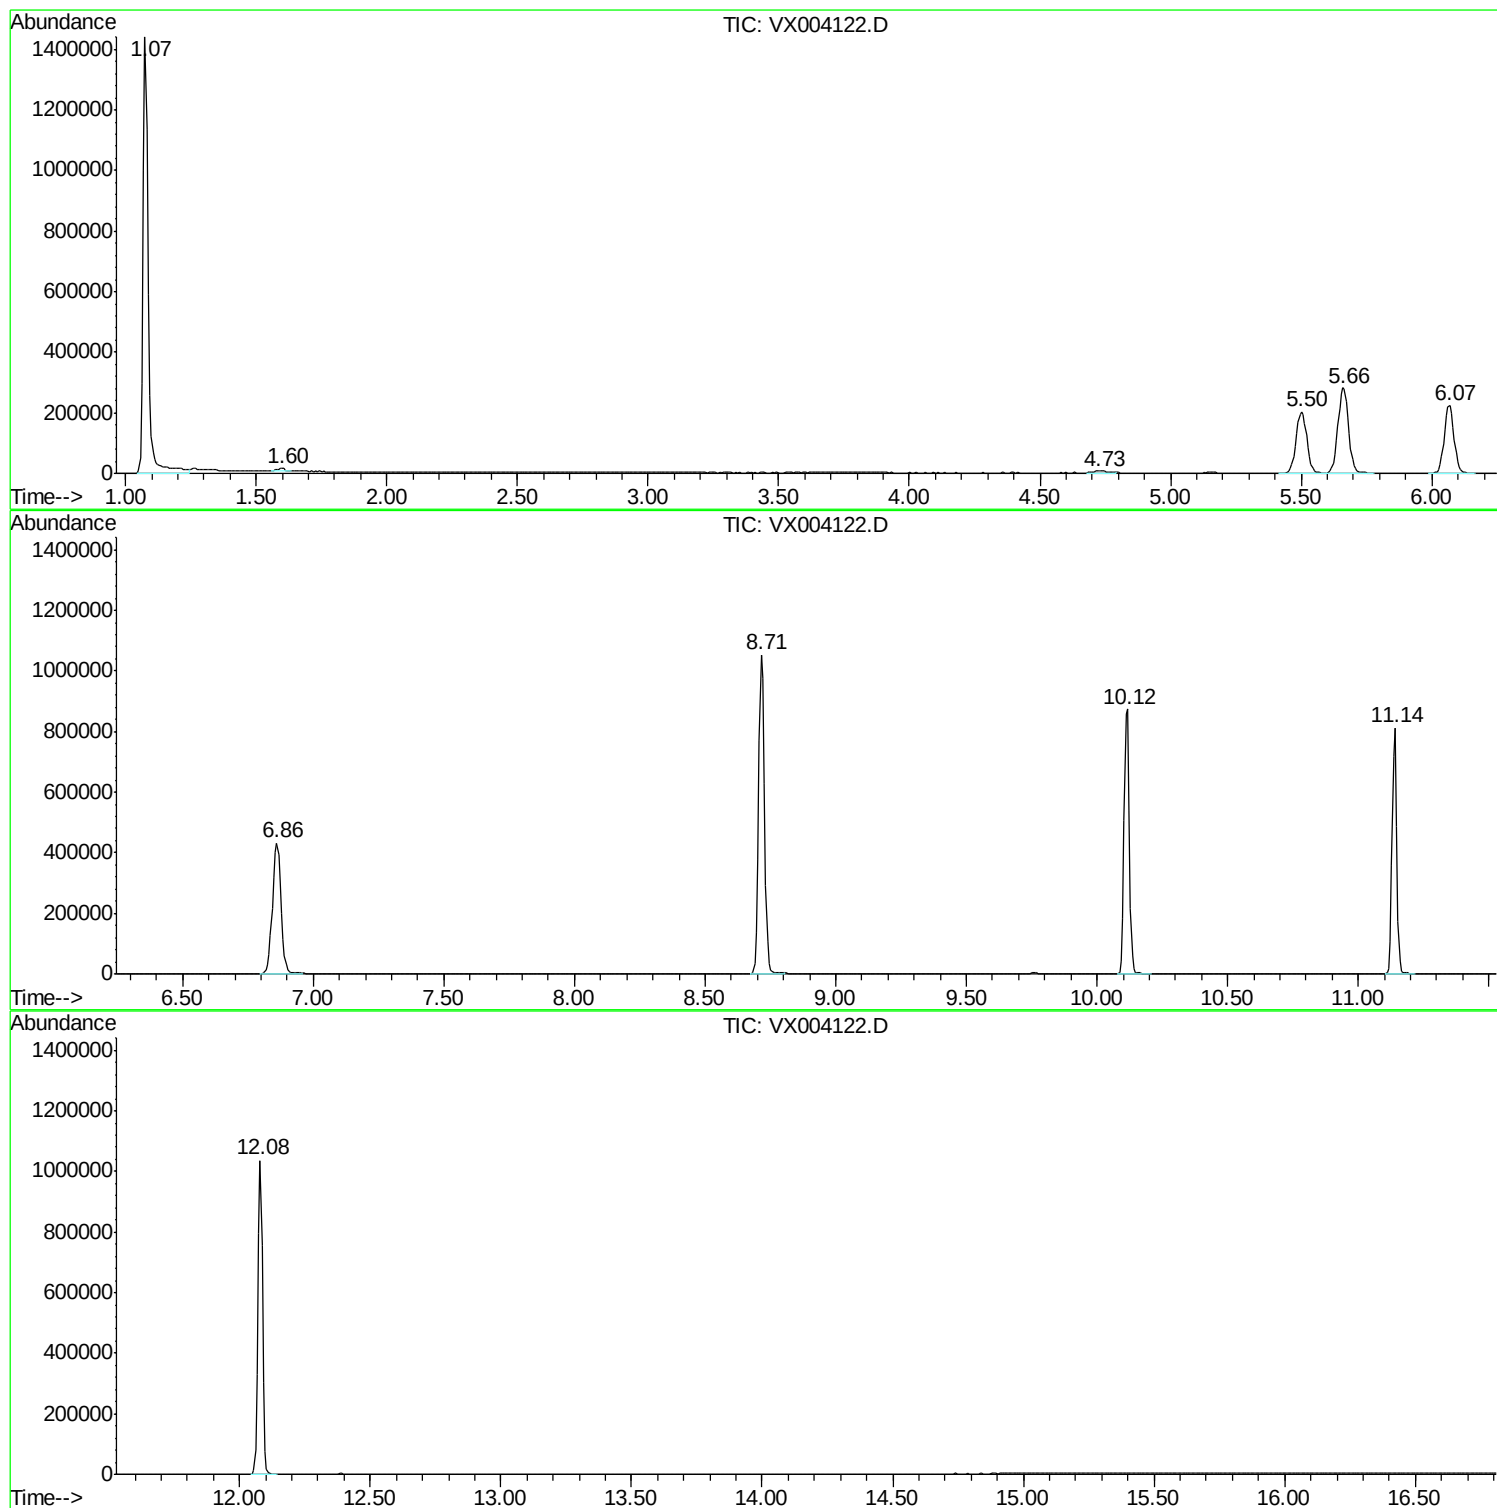

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA\_X\DATA\VX081718\  
Data File : VX004122.D  
Acq On : 17 Aug 2018 10:37  
Operator : JC/MD  
Sample : VX0817WBL01  
Misc : 5.0mL/MSVOA\_X/WATER  
ALS Vial : 3 Sample Multiplier: 1

Instrument :  
MSVOA\_X  
ClientSampleId :  
VX0817WBL01

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA\_X\METHOD\82X081418W.M  
Quant Title : SW846 8260

TIC Library : C:\DATABASE\NIST11.L  
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

\*\*\*\*\*

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA\_X\DATA\VX081718\  
Data File : VX004122.D  
Acq On : 17 Aug 2018 10:37  
Operator : JC/MD  
Sample : VX0817WBL01  
Misc : 5.0mL/MSVOA\_X/WATER  
ALS Vial : 3 Sample Multiplier: 1

Instrument :  
MSVOA\_X  
ClientSampleId :  
VX0817WBL01

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA\_X\METHOD\82X081418W.M  
Quant Title : SW846 8260

TIC Library : C:\DATABASE\NIST11.L  
TIC Integration Parameters: LSCINT.P

| TIC Top Hit name | RT | EstConc | Units | Response | --Internal Standard-- |
|------------------|----|---------|-------|----------|-----------------------|
|                  |    |         |       |          | # RT Resp Conc        |