

Data Path : Z:\VOASRV\HPCHEM1\MSVOA X\DATA\VX081718\
 Data File : VX004130.D
 Acq On : 17 Aug 2018 14:23
 Operator : JC/MD
 Sample : J4522-01
 Misc : 5.0mL/MSVOA X/WATER
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 MW-6

Integration Parameters: RTEINT.P

Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82X081418W.M
 Title : SW846 8260

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.075	75	80	93	rBV	1501967	1971379	100.00%	19.608%
2	1.605	159	167	171	rVB2	9994	20799	1.06%	0.207%
3	2.599	324	330	341	rVB	83851	155309	7.88%	1.545%
4	4.757	673	684	699	rVB2	15507	56021	2.84%	0.557%
5	5.507	794	807	821	rBV	200329	570004	28.91%	5.670%
6	5.666	821	833	850	rVB	270991	747894	37.94%	7.439%
7	6.068	887	899	914	rBV	214783	559089	28.36%	5.561%
8	6.861	1019	1029	1051	rBV	411000	969011	49.15%	9.638%
9	8.720	1326	1334	1348	rBV	1001036	1578989	80.10%	15.705%
10	10.116	1555	1563	1573	rBV	840113	1126831	57.16%	11.208%
11	11.140	1725	1731	1744	rBV	844368	1037587	52.63%	10.320%
12	12.079	1879	1885	1896	rBV	1036822	1260940	63.96%	12.542%


Sum of corrected areas: 10053853

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA X\DATA\VX081718\
Data File : VX004130.D
Acq On : 17 Aug 2018 14:23
Operator : JC/MD
Sample : J4522-01
Misc : 5.0mL/MSVOA X/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
MW-6

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_X\METHOD\82X081418W.M
Quant Title : SW846 8260

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

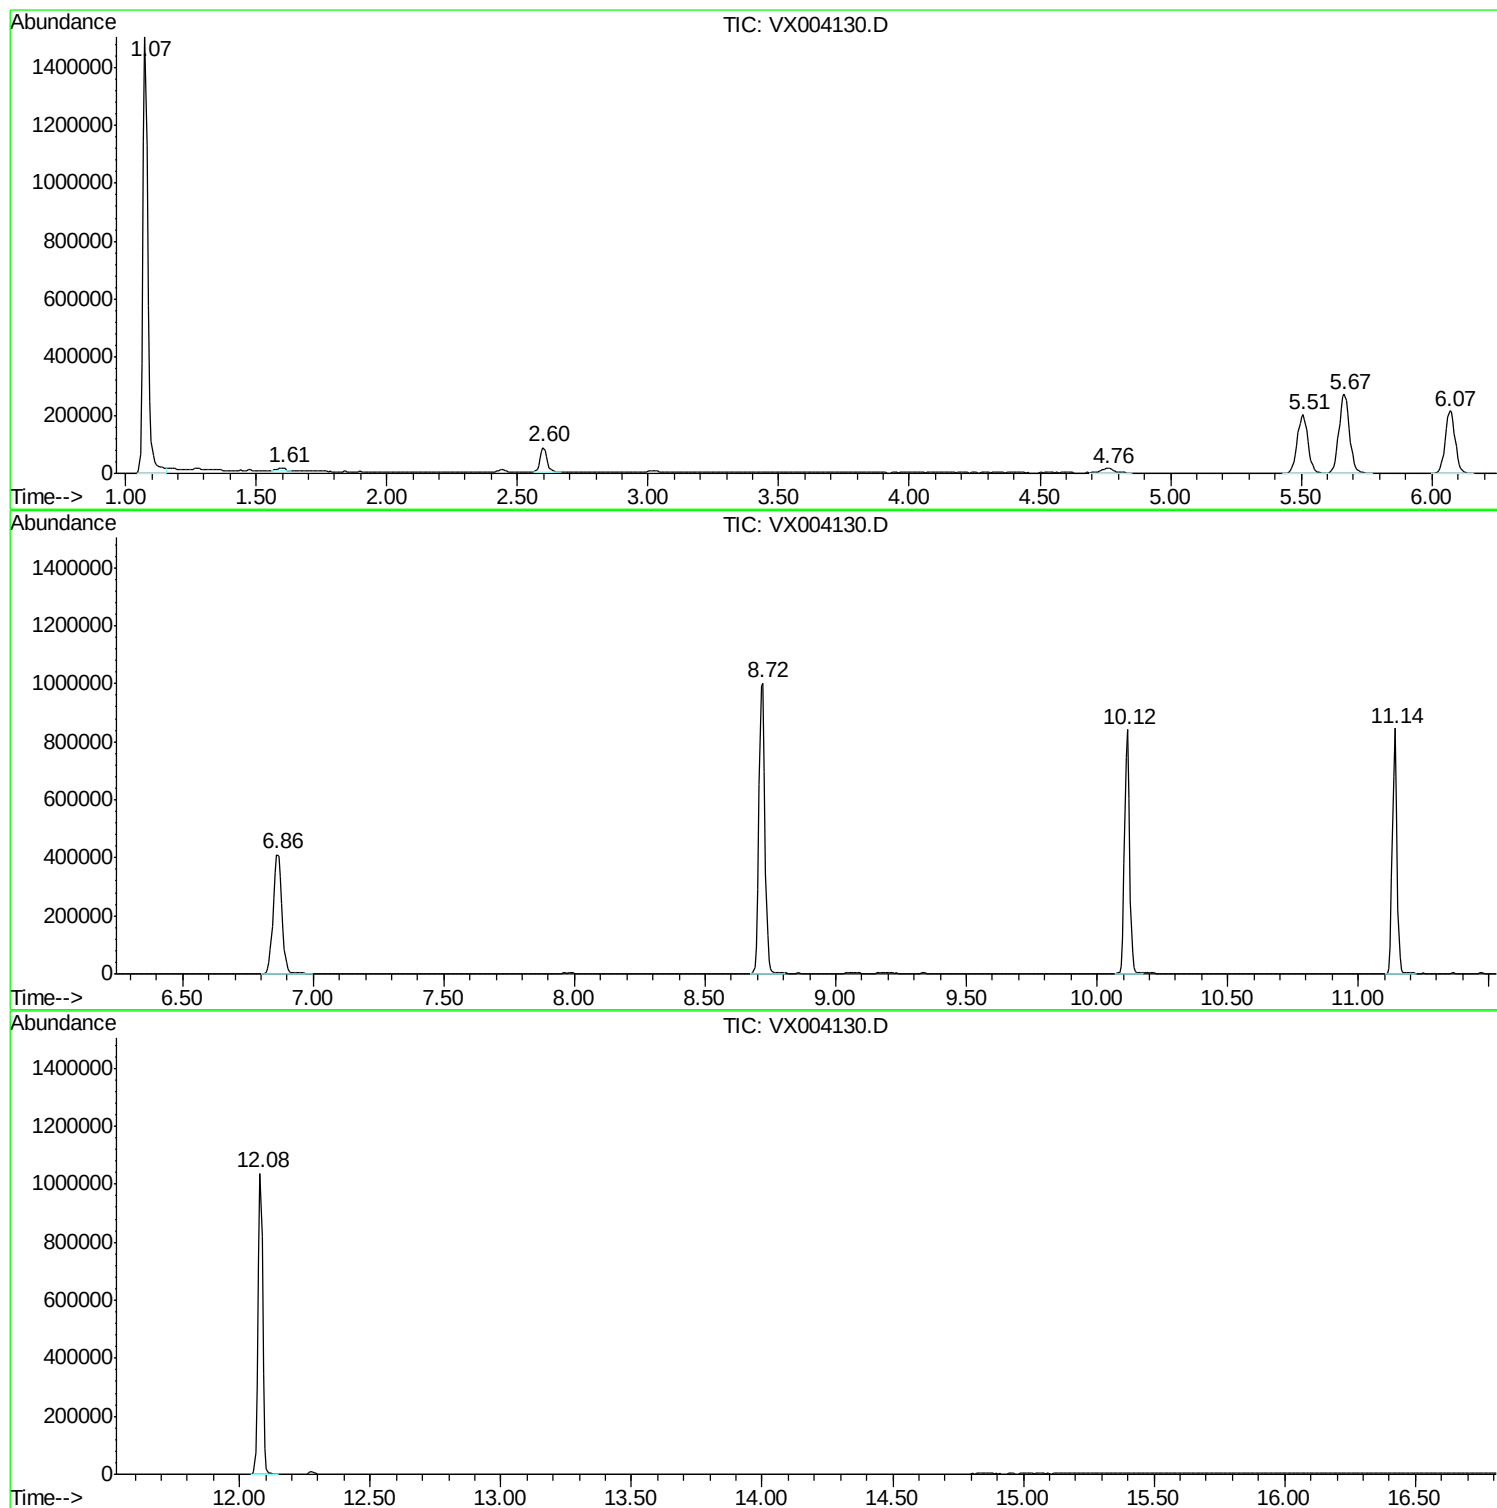

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA X\DATA\VX081718\
Data File : VX004130.D
Acq On : 17 Aug 2018 14:23
Operator : JC/MD
Sample : J4522-01
Misc : 5.0mL/MSVOA X/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
MW-6










Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_X\METHOD\82X081418W.M
Quant Title : SW846 8260

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

Peak Number 2 Isopropyl Alcohol Concentration Rank 2

R.T.	EstConc	Area	Relative to ISTD	R.T.
2.60	10.38 ug/l	155309	Pentafluorobenzene	5.67

Hit#	of	Tentative ID	MW	MolForm	CAS#	Qual
1	5	Isopropyl Alcohol	60	C3H8O	000067-63-0	86
2		Hydrazine, 1,2-dimethyl-	60	C2H8N2	000540-73-8	9
3		4-Penten-2-ol	86	C5H10O	000625-31-0	9
4		Hydrazine, ethyl-	60	C2H8N2	000624-80-6	9
5		Methoxyacetyl chloride	108	C3H5ClO2	038870-89-2	4

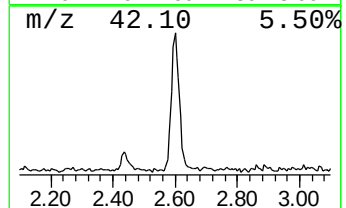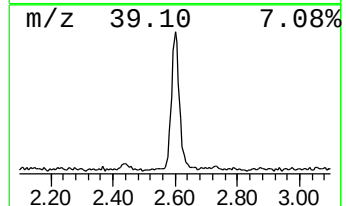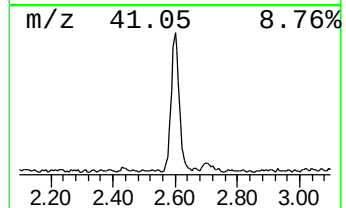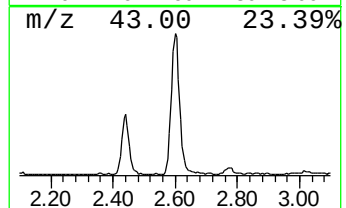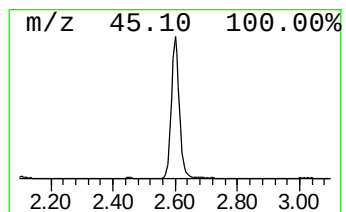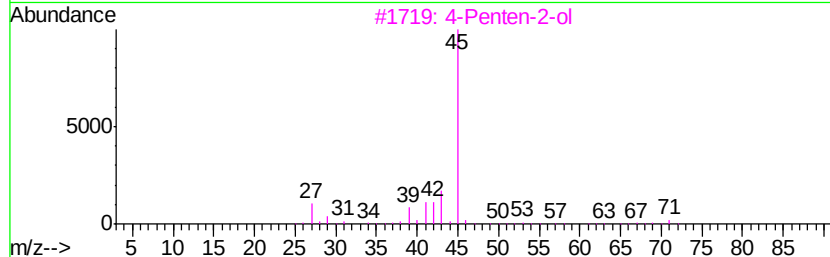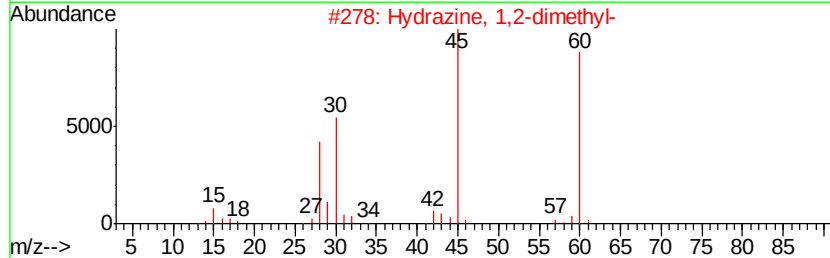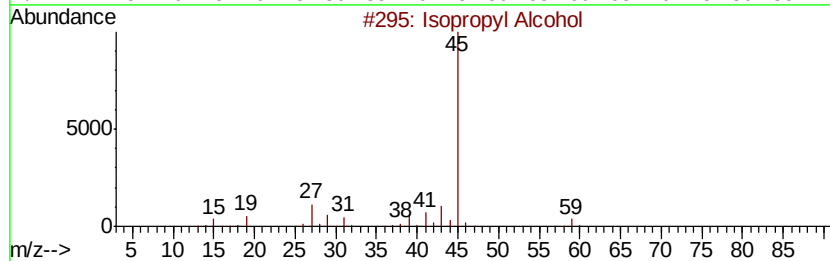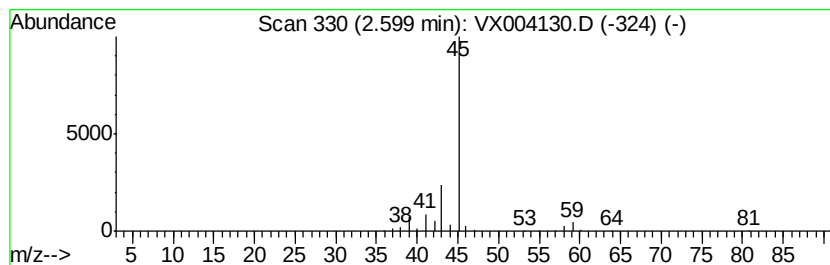

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_X\DATA\VX081718\
Data File : VX004130.D
Acq On : 17 Aug 2018 14:23
Operator : JC/MD
Sample : J4522-01
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
MW-6

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_X\METHOD\82X081418W.M
Quant Title : SW846 8260

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
Isopropyl Alcohol	2.60	10.4	ug/l	155309	1	5.67	747894	50.0