


Data Path : Z:\voasrv\HPCHEM1\MSVOA X\Data\VX081718\
 Data File : VX004120.D
 Acq On : 17 Aug 2018 07:53
 Operator : JC/MD
 Sample : BFB
 Misc : 5.0mL/MSVOA X/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82X081418W.M
 Title : SW846 8260
 Last Update : Tue Aug 14 13:27:25 2018

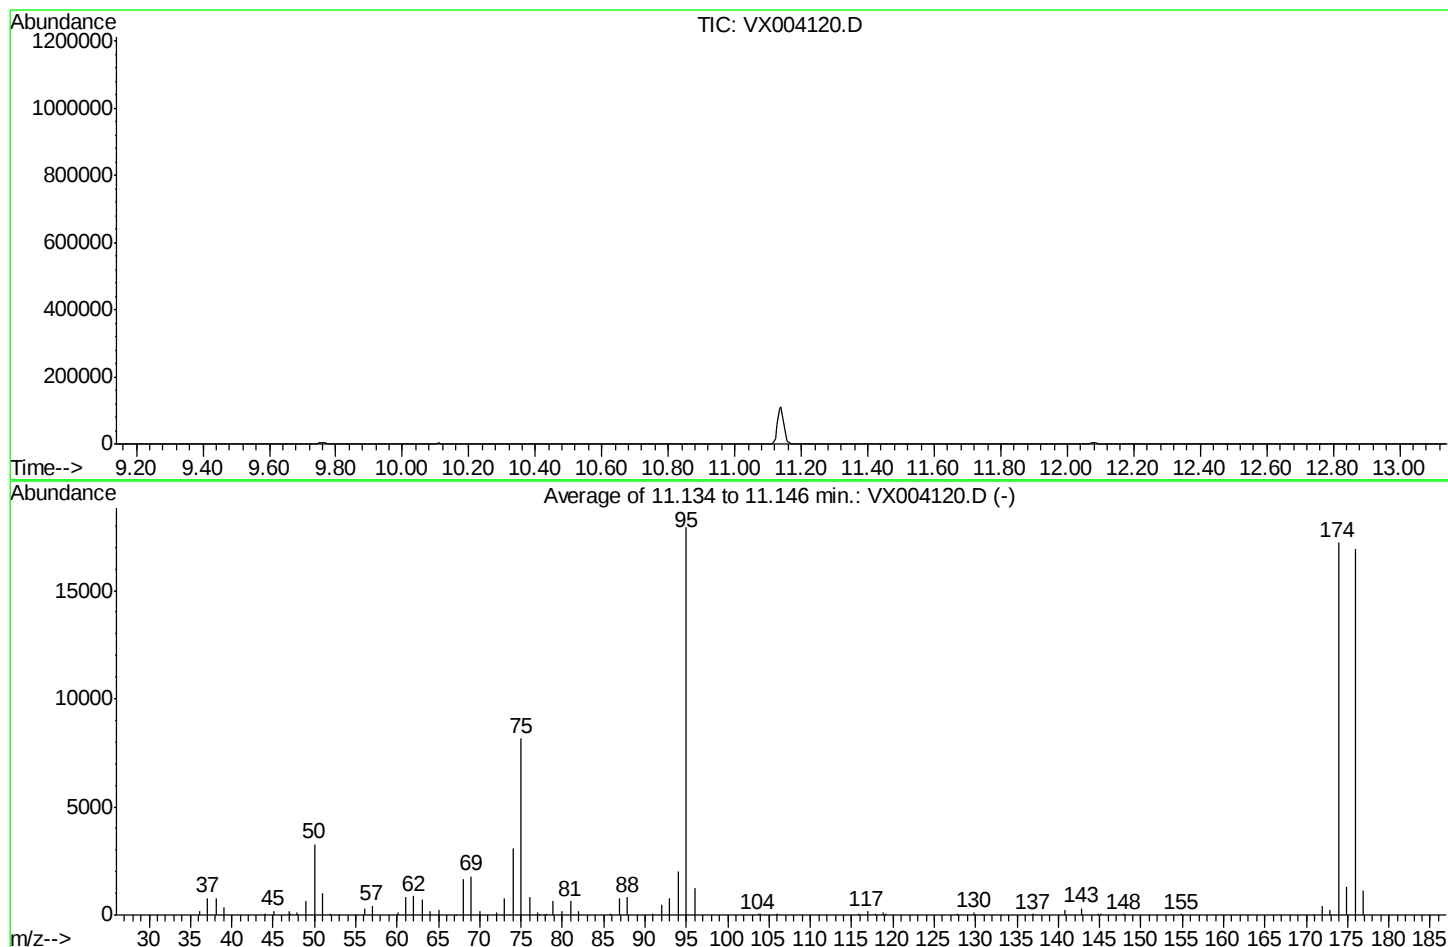

AutoFind: Scans 1730, 1731, 1732; Background Corrected with Scan 1723

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	18.3	3282	PASS
75	95	30	60	45.5	8159	PASS
95	95	100	100	100.0	17922	PASS
96	95	5	9	6.8	1224	PASS
173	174	0.00	2	1.3	226	PASS
174	95	50	100	96.1	17219	PASS
175	174	5	9	7.5	1284	PASS
176	174	95	101	98.4	16951	PASS
177	176	5	9	6.7	1141	PASS