

Data File : VX017936.D
Acq On : 17 Aug 2020 14:09
Operator : JC/SP
Sample : L3701-05
Misc : 25.0mL/MSVOA_X/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
JLTX4

Quant Time: Aug 18 01:31:55 2020
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\SOMXTR080720WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Tue Aug 18 00:59:21 2020
Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	6.83	114	262526	5.00	ug/L	0.00
28) Chlorobenzene-d5	10.10	117	253766	5.00	ug/L	0.00
61) 1,4-Dichlorobenzene-d4	12.06	152	115976	5.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.39	65	78941	4.35	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	87.00%
7) Chloroethane-d5	1.69	69	71745	4.98	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	99.60%
11) 1,1-Dichloroethene-d2	2.34	63	126575	3.39	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	67.80%
20) 2-Butanone-d5	4.53	46	280011	58.12	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	116.24%
24) Chloroform-d	5.14	84	198256	5.38	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	107.60%
26) 1,2-Dichloroethane-d4	6.03	65	112611	5.57	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	111.40%
32) Benzene-d6	6.05	84	354939	5.10	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	102.00%
36) 1,2-Dichloropropane-d6	7.37	67	115854	5.38	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	107.60%
41) Toluene-d8	8.70	98	299321	4.51	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	90.20%
45) trans-1,3-Dichloropropene-	8.99	79	45133	4.84	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	96.80%
48) 2-Hexanone-d5	9.43	63	218378	56.34	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	112.68%
59) 1,1,2,2-Tetrachloroethane-	11.23	84	90758	5.54	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	110.80%
65) 1,2-Dichlorobenzene-d4	12.36	152	131273	5.88	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	117.60%


Target Compounds					Qvalue
13) Acetone	2.42	43	13162	3.739 ug/L	92


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data File : VX017936.D
Acq On : 17 Aug 2020 14:09
Operator : JC/SP
Sample : L3701-05
Misc : 25.0mL/MSVOA_X/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
JLTX4

Quant Time: Aug 18 01:31:55 2020
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\SOMXTR080720WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Tue Aug 18 00:59:21 2020
Response via : Initial Calibration

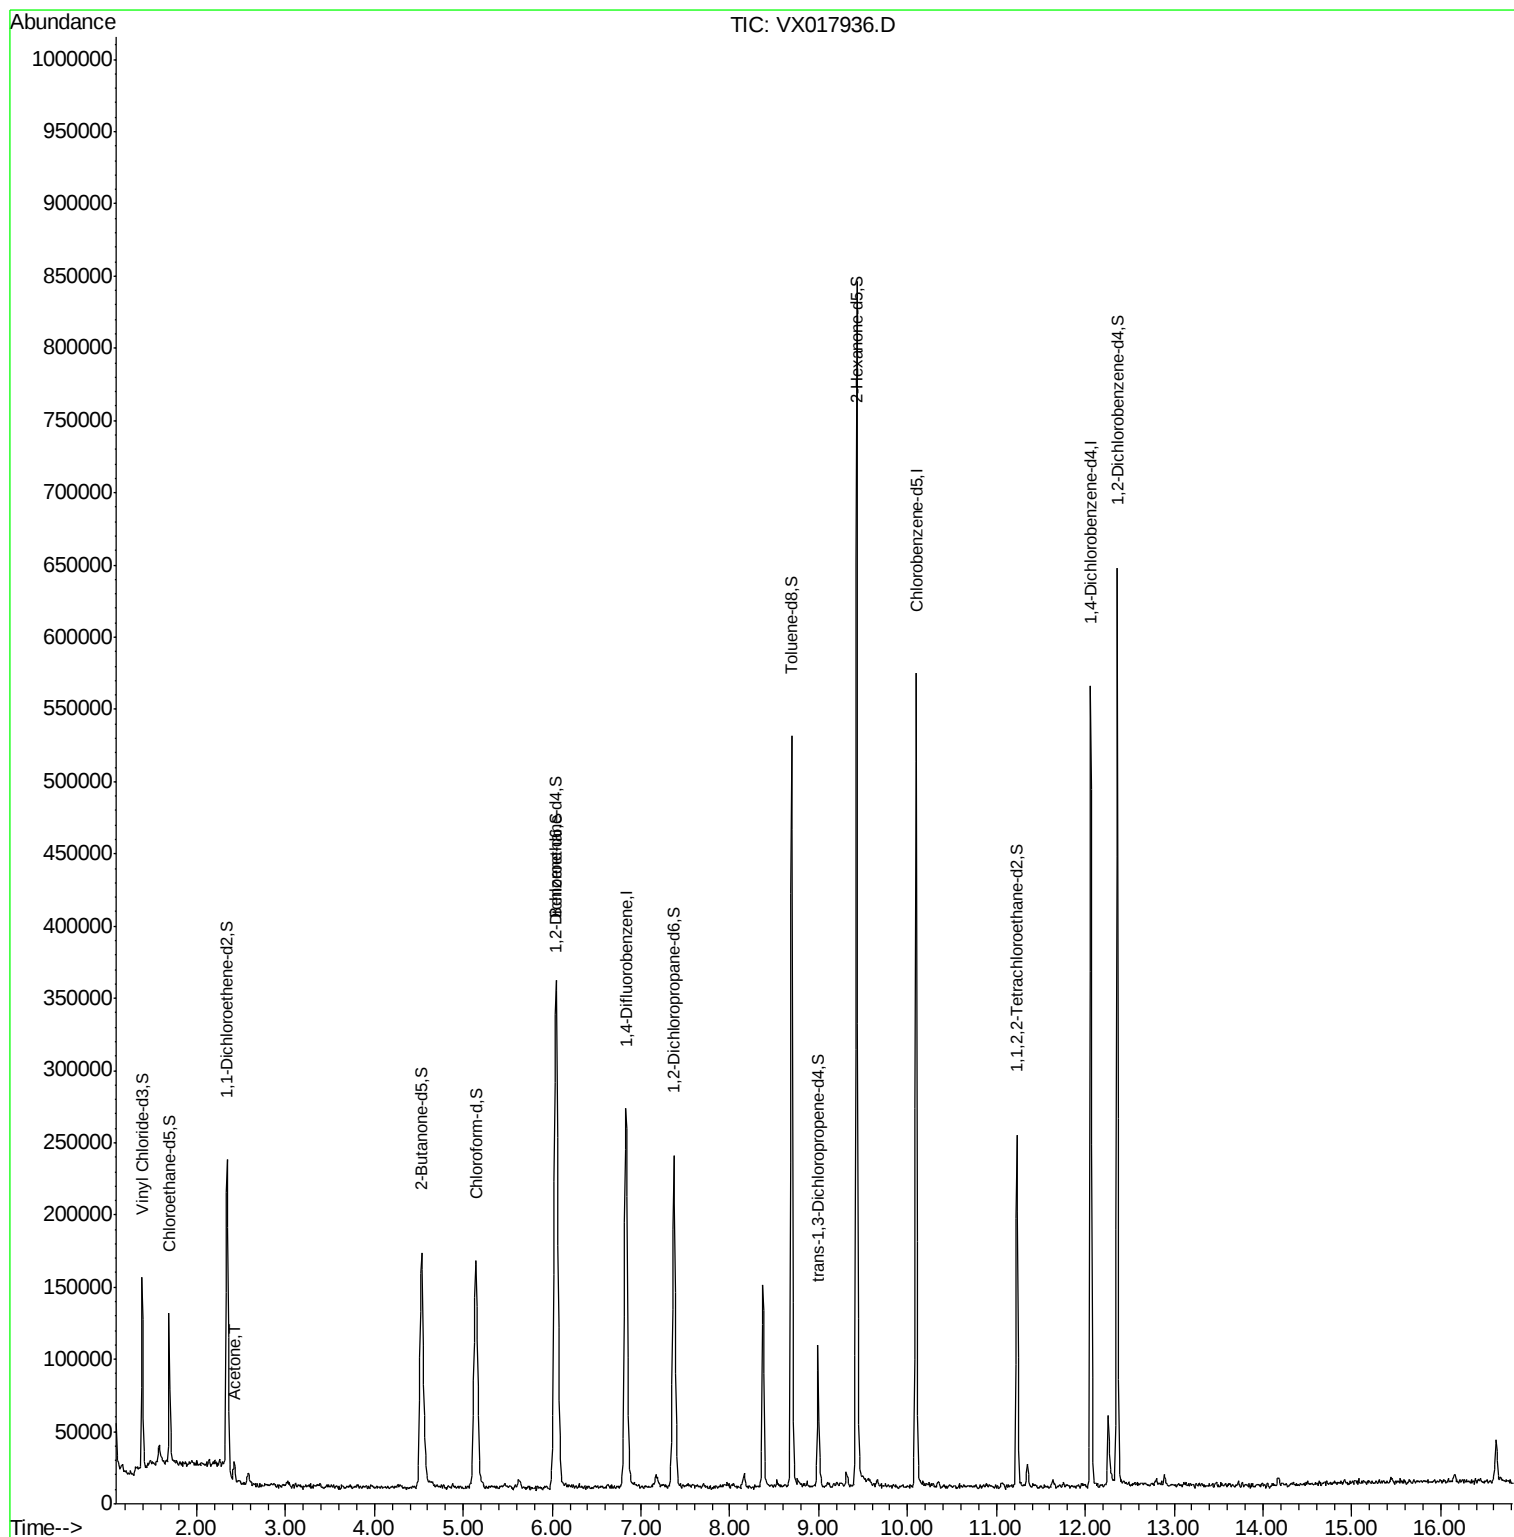

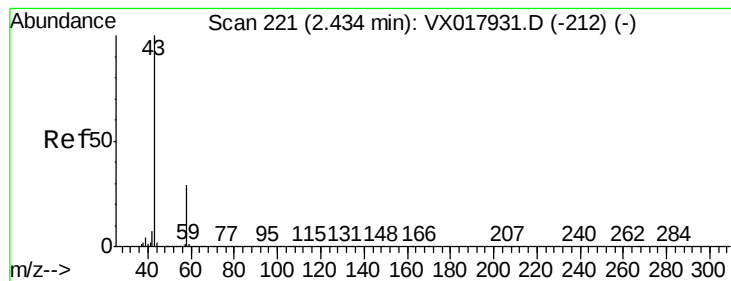

#13
 Acetone
 Concen: 3.739 ug/L
 RT: 2.42 min Scan# 219
 Delta R.T. -0.01 min
 Lab File: VX017936.D
 Acq: 17 Aug 2020 14:09

Instrument :
 MSVOA_X
 ClientSampleId :
 JLTx4

Tgt Ion: 43 Resp: 13162
 Ion Ratio Lower Upper
 43 100
 58 34.5 0.0 60.8

