

Data File : VX017947.D
Acq On : 17 Aug 2020 19:05
Operator : JC/SP
Sample : L3701-03
Misc : 25.0mL/MSVOA_X/WATER
ALS Vial : 20 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
JLTX2

Quant Time: Aug 18 02:17:13 2020
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\SOMXTR080720WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Tue Aug 18 00:59:21 2020
Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	6.83	114	272230	5.00	ug/L	0.00
28) Chlorobenzene-d5	10.10	117	259558	5.00	ug/L	0.00
61) 1,4-Dichlorobenzene-d4	12.06	152	105992	5.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.39	65	75222	4.00	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	80.00%
7) Chloroethane-d5	1.69	69	68564	4.59	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	91.80%
11) 1,1-Dichloroethene-d2	2.34	63	117694	3.04	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	60.80%
20) 2-Butanone-d5	4.53	46	263070	52.66	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	105.32%
24) Chloroform-d	5.14	84	172882	4.53	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	90.60%
26) 1,2-Dichloroethane-d4	6.03	65	100371	4.79	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	95.80%
32) Benzene-d6	6.05	84	317827	4.46	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	89.20%
36) 1,2-Dichloropropane-d6	7.37	67	112004	5.09	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	101.80%
41) Toluene-d8	8.70	98	263073	3.88	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	77.60%
45) trans-1,3-Dichloropropene-	8.99	79	38340	4.02	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	80.40%
48) 2-Hexanone-d5	9.43	63	182908	46.14	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	92.28%
59) 1,1,2,2-Tetrachloroethane-	11.23	84	77544	4.63	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	92.60%
65) 1,2-Dichlorobenzene-d4	12.36	152	116531	5.71	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	114.20%


Target Compounds					Qvalue
13) Acetone	2.42	43	35046	9.602 ug/L	94


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data File : VX017947.D
Acq On : 17 Aug 2020 19:05
Operator : JC/SP
Sample : L3701-03
Misc : 25.0mL/MSVOA_X/WATER
ALS Vial : 20 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
JLTX2

Quant Time: Aug 18 02:17:13 2020
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\SOMXTR080720WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Tue Aug 18 00:59:21 2020
Response via : Initial Calibration

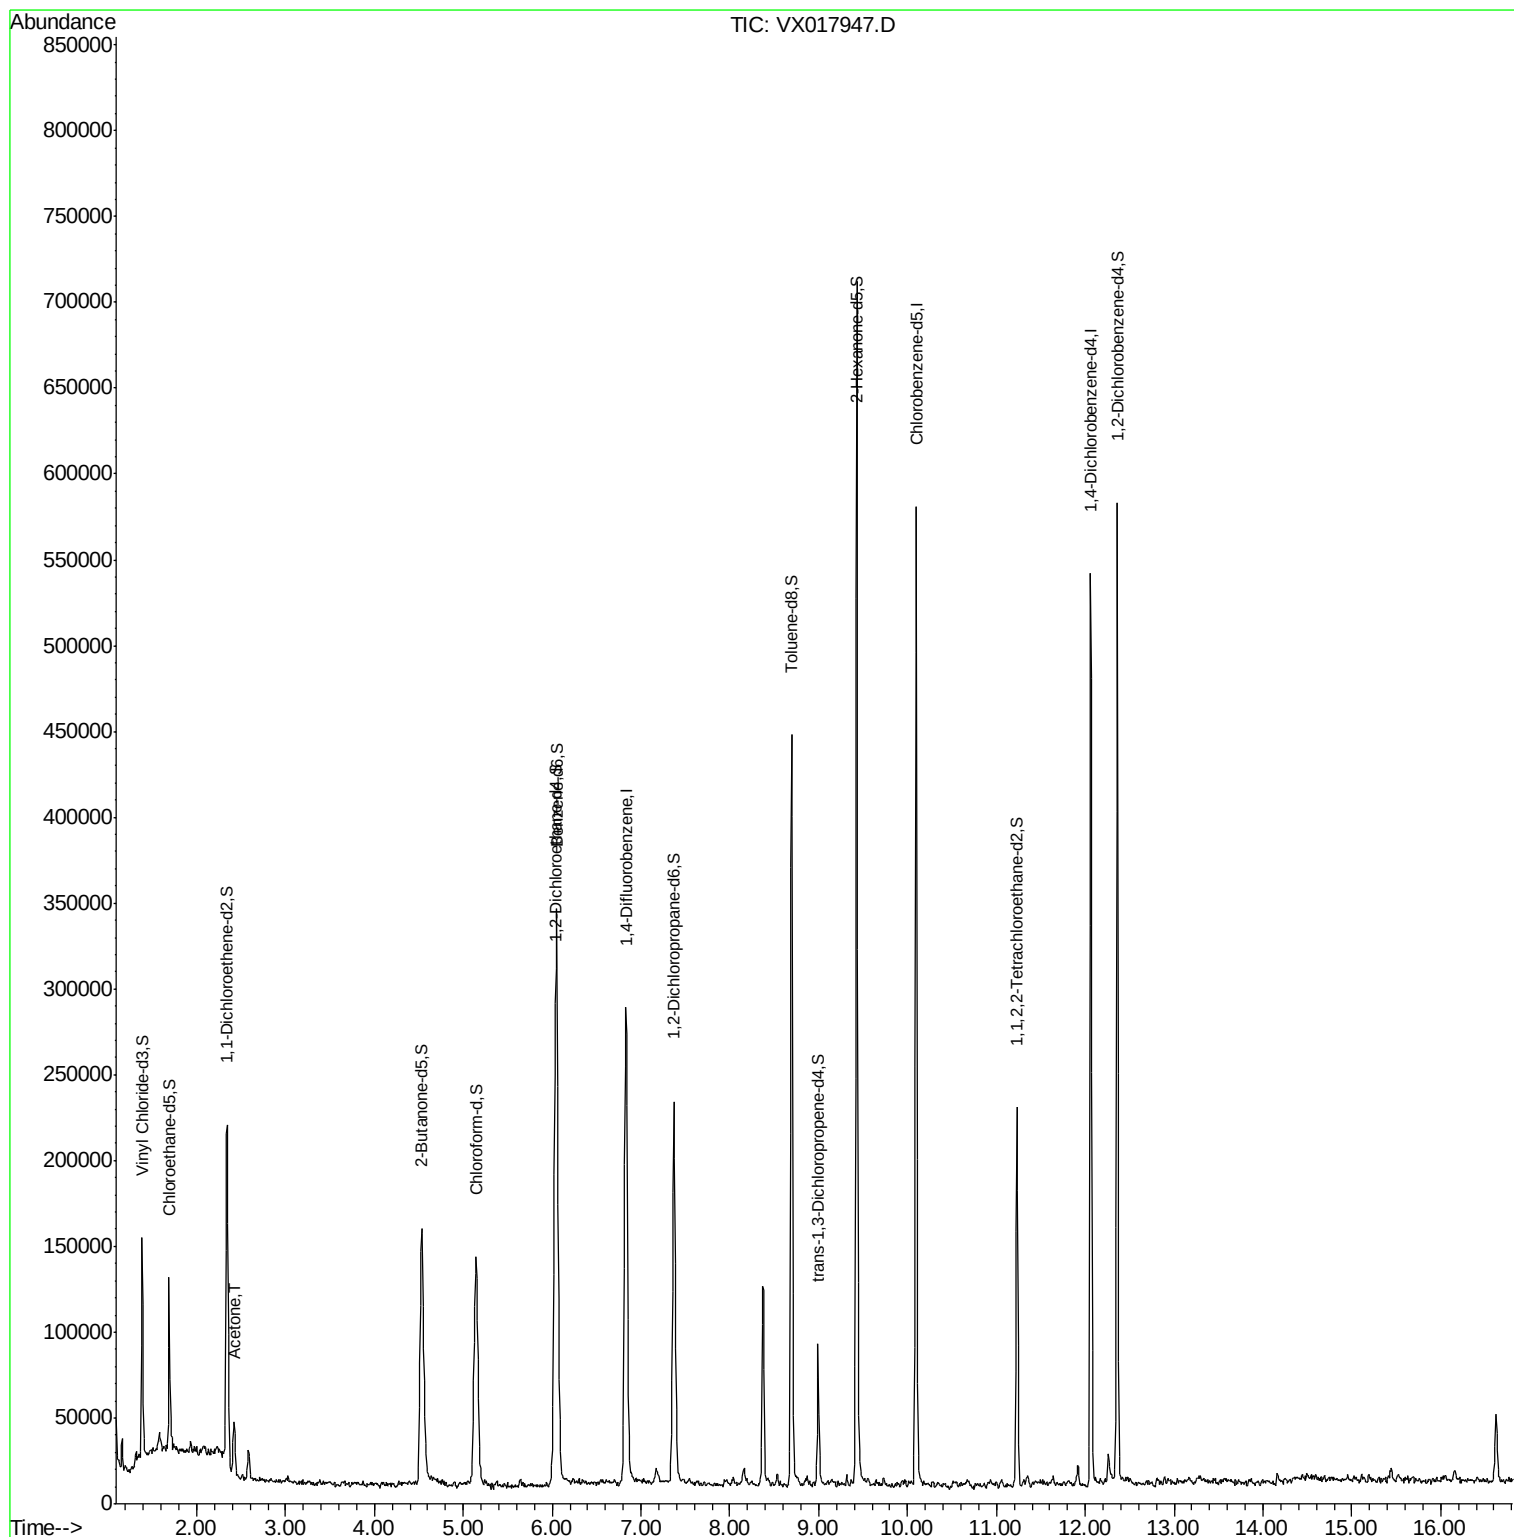

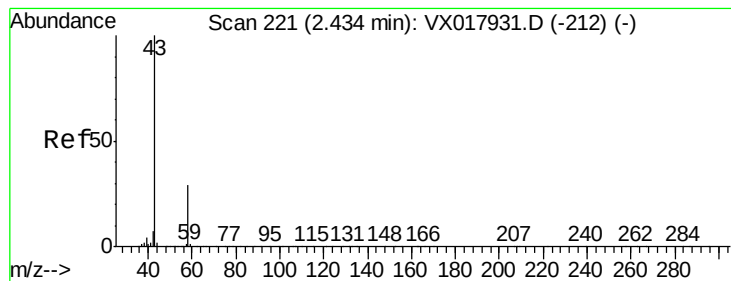

#13
 Acetone
 Concen: 9.602 ug/L
 RT: 2.42 min Scan# 219
 Delta R.T. -0.01 min
 Lab File: VX017947.D
 Acq: 17 Aug 2020 19:05

Instrument :
 MSVOA_X
 ClientSampleId :
 JLTx2

Tgt Ion: 43 Resp: 35046
 Ion Ratio Lower Upper
 43 100
 58 33.9 0.0 60.8

