


Data Path : Z:\voasrv\HPCHEM1\MSVOA X\Data\VX081720\
 Data File : VX017930.D
 Acq On : 17 Aug 2020 09:32
 Operator : JC/SP
 Sample : BFB70
 Misc : 25.0mL/MSVOA X/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 BFB70

Integration File: rteint.p

Method : Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\SOMXTR080720WMA.M
 Title : TRACE VOA SOM01.0
 Last Update : Tue Aug 18 00:59:21 2020

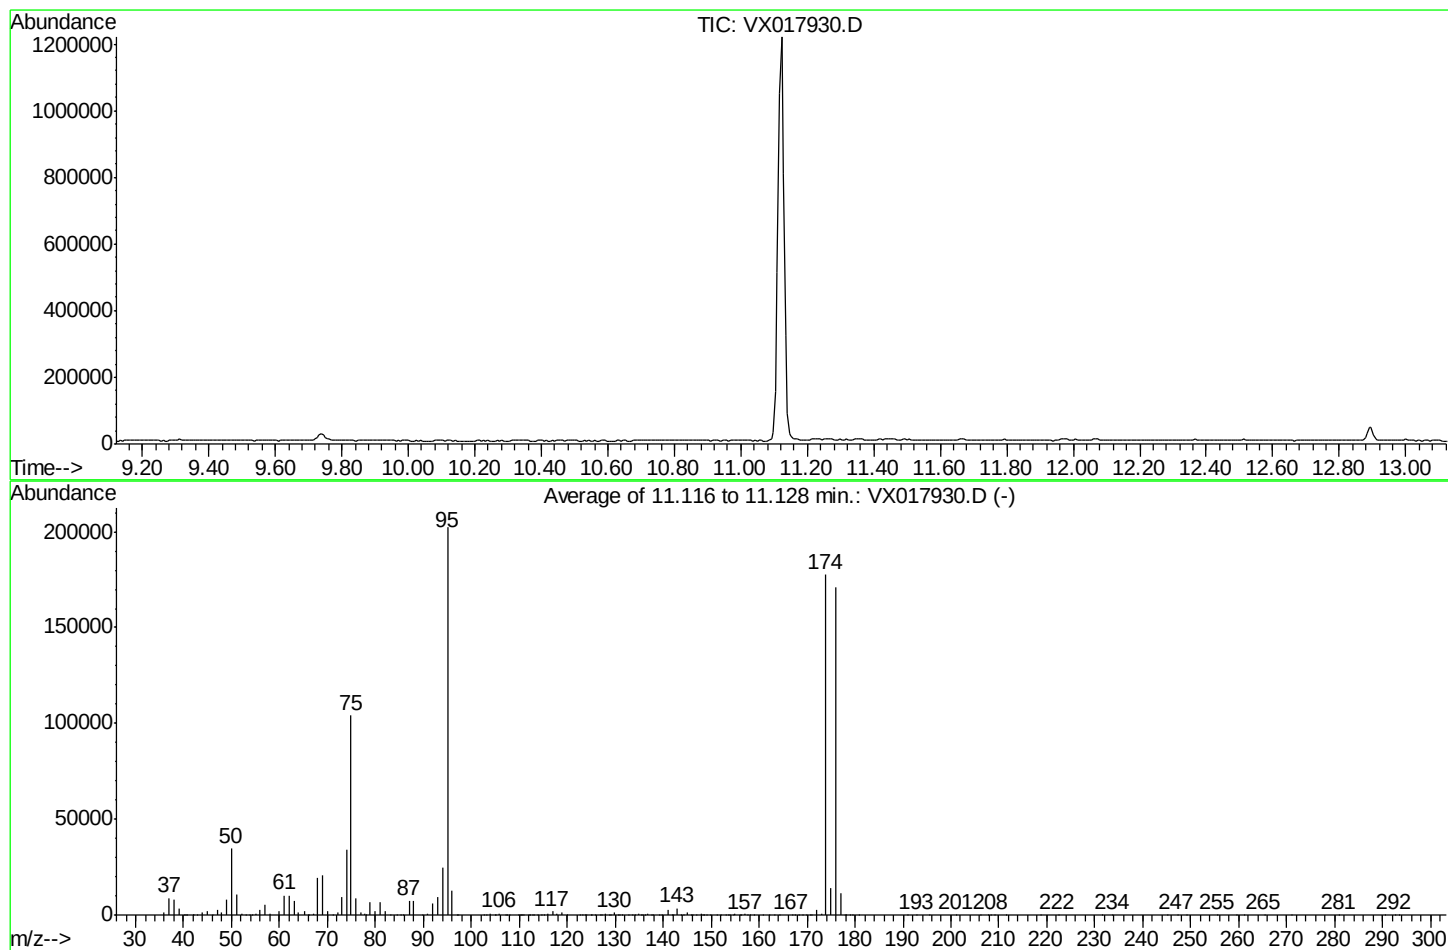

AutoFind: Scans 1645, 1646, 1647; Background Corrected with Scan 1638

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	17.2	34740	PASS
75	95	30	80	51.4	103982	PASS
95	95	100	100	100.0	202325	PASS
96	95	5	9	6.4	12973	PASS
173	174	0.00	2	0.4	698	PASS
174	95	50	120	87.7	177429	PASS
175	174	5	9	7.8	13788	PASS
176	174	95	101	96.5	171306	PASS
177	176	5	9	6.5	11098	PASS

m/z	Abundance
35.20	245.0
36.40	55.0
37.40	75.0
38.00	142.0
38.90	101.0
39.80	460.0
41.10	348.0
41.90	121.0
43.00	169.0
44.00	518.0
45.30	218.0
46.40	136.0
47.10	138.0
48.70	95.0
49.90	190.0
51.00	90.0
52.20	140.0
52.90	165.0
54.00	92.0
55.40	99.0
56.70	144.0
57.60	169.0
58.50	79.0
59.00	86.0
61.50	85.0
62.10	63.0
63.10	51.0
63.80	96.0
65.50	57.0
66.50	121.0
67.00	51.0
69.80	150.0
71.60	96.0
73.00	248.0
73.80	57.0
74.80	108.0
77.80	51.0
78.60	130.0
88.60	81.0
91.10	111.0
94.50	65.0
100.10	77.0
102.60	119.0
103.80	138.0
116.20	85.0
117.40	99.0
120.70	105.0
128.50	73.0
137.90	84.0
138.80	90.0
140.00	101.0
144.20	54.0
147.30	167.0
148.90	61.0
149.40	118.0
154.60	63.0
160.40	122.0
166.90	68.0
179.90	80.0
183.50	63.0
189.90	129.0
191.30	211.0
206.90	408.0
208.10	129.0
224.20	54.0
235.30	55.0
239.70	66.0
244.60	69.0
281.20	165.0
281.90	110.0

Instrument :
MSVOA_X
ClientSampleId :
BFB70

m/z	Abundance
36.00	1546.0
37.00	10051.0
38.00	8742.0
39.00	3287.0
39.80	815.0
40.30	322.0
41.10	248.0
41.90	186.0
42.80	311.0
44.00	1785.0
45.00	1764.0
46.00	288.0
47.00	2946.0
48.00	1570.0
49.00	8941.0
50.00	38800.0
51.00	12472.0
52.00	1065.0
52.80	294.0
53.80	130.0
55.00	607.0
56.00	3573.0
57.00	5645.0
58.00	494.0
60.00	2301.0
61.00	11896.0
62.00	11935.0
63.00	8713.0
64.00	1416.0
65.20	2075.0
65.90	196.0
67.10	778.0
68.00	20680.0
69.00	22720.0
70.00	2250.0
71.00	63.0
72.10	1113.0
73.00	9900.0
74.00	37376.0
75.00	114736.0
76.00	9578.0
77.10	864.0
79.00	8270.0
79.90	2041.0
80.90	7728.0
81.90	1782.0
83.10	96.0
85.20	115.0
85.70	287.0
87.00	8545.0
88.00	7966.0
89.80	61.0
90.80	745.0
92.00	7295.0
93.00	9478.0
94.00	25776.0
95.00	214976.0
96.00	14209.0
96.90	270.0
97.30	229.0
102.80	71.0
103.80	1022.0
104.90	351.0
105.80	932.0
107.00	275.0
107.90	167.0
110.00	225.0
111.00	316.0
111.80	197.0
112.70	211.0
113.10	147.0
113.80	52.0
114.70	269.0
115.90	839.0
116.90	1959.0
117.90	1165.0
118.90	1970.0
119.80	158.0
123.10	68.0
123.90	191.0
124.90	167.0
125.80	299.0
127.00	121.0
127.90	756.0
128.90	289.0
129.90	863.0
131.00	415.0
134.00	116.0
134.80	503.0
135.70	165.0
136.80	721.0
137.50	112.0

Instrument :
MSVOA_X
ClientSampleId :
BFB70

131.30	198.0
134.90	749.0
136.10	101.0
136.90	401.0
137.70	221.0
139.00	245.0
139.60	141.0
140.90	3627.0
142.10	401.0
142.90	3623.0
144.10	345.0
144.90	1146.0
146.20	565.0
147.90	904.0
148.60	284.0
149.80	395.0
151.20	122.0
151.90	147.0
152.90	160.0
153.60	176.0
155.00	769.0
155.90	147.0
157.10	596.0
158.80	563.0
160.80	233.0
162.20	92.0
164.20	76.0
166.80	118.0
169.20	119.0
169.70	209.0
170.60	429.0
171.90	3458.0
174.00	214976.0
175.00	17280.0
176.00	204864.0
176.90	13768.0
178.10	285.0
192.90	95.0
195.60	59.0
206.30	85.0
207.10	320.0
208.30	267.0
208.90	109.0
211.50	67.0
222.40	77.0
247.20	66.0
259.40	61.0
261.00	62.0
265.40	90.0
280.90	161.0
281.90	50.0
292.50	83.0

Instrument :
MSVOA_X
ClientSampleId :
BFB70

m/z	Abundance
35.30	92.0
36.00	2157.0
37.00	10606.0
38.00	10943.0
39.00	4451.0
40.00	434.0
40.70	297.0
41.90	240.0
42.90	225.0
44.00	1500.0
45.00	2078.0
45.90	373.0
46.90	2802.0
48.00	1829.0
49.00	9010.0
50.00	42344.0
51.00	12720.0
52.10	595.0
53.00	328.0
53.70	208.0
54.20	139.0
54.90	720.0
56.00	3166.0
57.00	5925.0
58.10	500.0
59.00	68.0
59.90	2100.0
61.00	11404.0
62.00	10863.0
63.00	8725.0
64.00	1387.0
65.00	2694.0
66.10	383.0
67.10	700.0
68.00	22984.0
69.00	25048.0
69.90	1975.0
71.00	115.0
72.10	1442.0
73.00	11423.0
74.00	41440.0
75.00	120936.0
76.00	9827.0
76.90	1357.0
77.10	1365.0
77.80	835.0
78.10	674.0
78.90	7810.0
79.90	2201.0
80.90	7585.0
81.90	2296.0
83.10	173.0
84.50	64.0
85.20	79.0
85.80	320.0
87.10	7527.0
87.90	7614.0
90.90	1355.0
91.90	6604.0
93.00	11769.0
94.00	28704.0
95.00	239936.0
96.00	15807.0
97.10	491.0
102.60	137.0
103.90	1415.0
105.10	442.0
105.90	1256.0
107.10	414.0
107.90	172.0
109.70	218.0
110.20	177.0
110.80	217.0
111.90	184.0
113.00	344.0
113.90	136.0
115.10	279.0
115.90	984.0
117.00	2446.0
117.90	971.0
118.90	1290.0
119.90	90.0
122.70	119.0
123.20	170.0
123.70	320.0
125.10	228.0
125.80	77.0
126.80	164.0
127.90	1349.0
129.10	598.0
129.80	1400.0
130.70	464.0

Instrument :
MSVOA_X
ClientSampleId :
BFB70

138.70	171.0
139.60	173.0
141.00	2484.0
141.80	373.0
142.90	4047.0
144.20	53.0
144.90	1368.0
145.90	519.0
147.20	289.0
147.80	469.0
149.00	191.0
149.80	301.0
151.10	80.0
151.90	96.0
152.80	243.0
153.60	151.0
155.00	635.0
156.30	56.0
157.00	410.0
158.90	189.0
160.90	345.0
162.20	131.0
167.50	95.0
169.10	176.0
169.80	237.0
170.70	526.0
171.90	2511.0
173.00	2096.0
174.00	165888.0
175.00	12593.0
176.00	154944.0
177.00	10058.0
178.00	187.0
180.70	55.0
190.90	110.0
191.50	66.0
195.50	68.0
201.20	60.0
207.10	427.0
207.90	147.0
209.00	143.0
218.80	52.0
233.70	60.0
245.00	56.0
247.20	52.0
271.00	68.0
281.00	254.0

Instrument :
MSVOA_X
ClientSampleId :
BFB70

m/z	Abundance
35.10	133.0
36.00	1304.0
37.00	6297.0
38.00	4816.0
39.00	2445.0
40.10	474.0
40.90	135.0
42.10	301.0
42.80	370.0
44.00	1742.0
45.00	1563.0
46.00	269.0
46.90	1787.0
48.00	939.0
49.00	5846.0
50.00	23648.0
51.00	8001.0
51.90	293.0
52.30	283.0
53.00	209.0
53.90	92.0
55.10	554.0
56.00	1747.0
57.00	3816.0
57.90	396.0
59.10	169.0
59.90	1611.0
60.90	7581.0
62.00	6563.0
63.00	4903.0
64.00	746.0
65.00	1463.0
66.00	300.0
66.90	414.0
68.00	15445.0
69.00	14027.0
70.10	1448.0
72.00	882.0
73.00	7008.0
74.00	24144.0
75.00	76600.0
76.10	5845.0
77.00	650.0
77.70	430.0
78.90	4968.0
79.90	1789.0
80.90	4513.0
82.00	1482.0
82.90	104.0
85.10	60.0
85.90	451.0
86.90	5988.0
87.90	5727.0
90.90	637.0
92.00	4723.0
93.00	7035.0
94.00	19368.0
95.00	152064.0
96.00	8903.0
96.90	151.0
102.70	188.0
103.10	178.0
103.80	764.0
104.90	259.0
105.80	734.0
107.00	178.0
107.50	99.0
109.90	206.0
110.60	235.0
110.90	240.0
112.10	267.0
113.00	247.0
114.90	395.0
115.80	643.0
117.00	1393.0
117.80	783.0
118.80	1196.0
124.00	164.0
125.20	59.0
125.80	99.0
127.10	207.0
127.90	678.0
128.70	388.0
129.80	859.0
130.90	376.0
132.80	91.0
133.60	138.0
134.70	341.0
135.30	271.0
136.80	416.0
137.60	73.0
139.10	131.0

Instrument :
MSVOA_X
ClientSampleId :
BFB70

139.70	70.0
140.90	2033.0
141.90	329.0
143.00	2390.0
143.70	166.0
144.20	248.0
144.90	828.0
145.90	437.0
146.80	227.0
148.10	553.0
149.00	192.0
149.90	269.0
152.00	88.0
153.00	173.0
153.90	128.0
154.70	453.0
156.00	95.0
157.00	450.0
157.60	74.0
158.20	188.0
158.80	273.0
160.90	252.0
163.10	51.0
164.10	93.0
166.80	119.0
168.20	52.0
169.80	144.0
170.90	362.0
172.00	2157.0
173.90	151424.0
175.00	11493.0
176.00	154112.0
177.00	9469.0
177.80	280.0
178.80	98.0
179.40	67.0
192.80	109.0
206.20	112.0
207.10	278.0
207.80	88.0
208.40	121.0
222.40	66.0
231.60	59.0
249.20	110.0
255.60	52.0
281.00	120.0
290.60	53.0
292.50	63.0
293.30	128.0

Instrument :
MSVOA_X
ClientSampleId :
BFB70