



Chloroethane

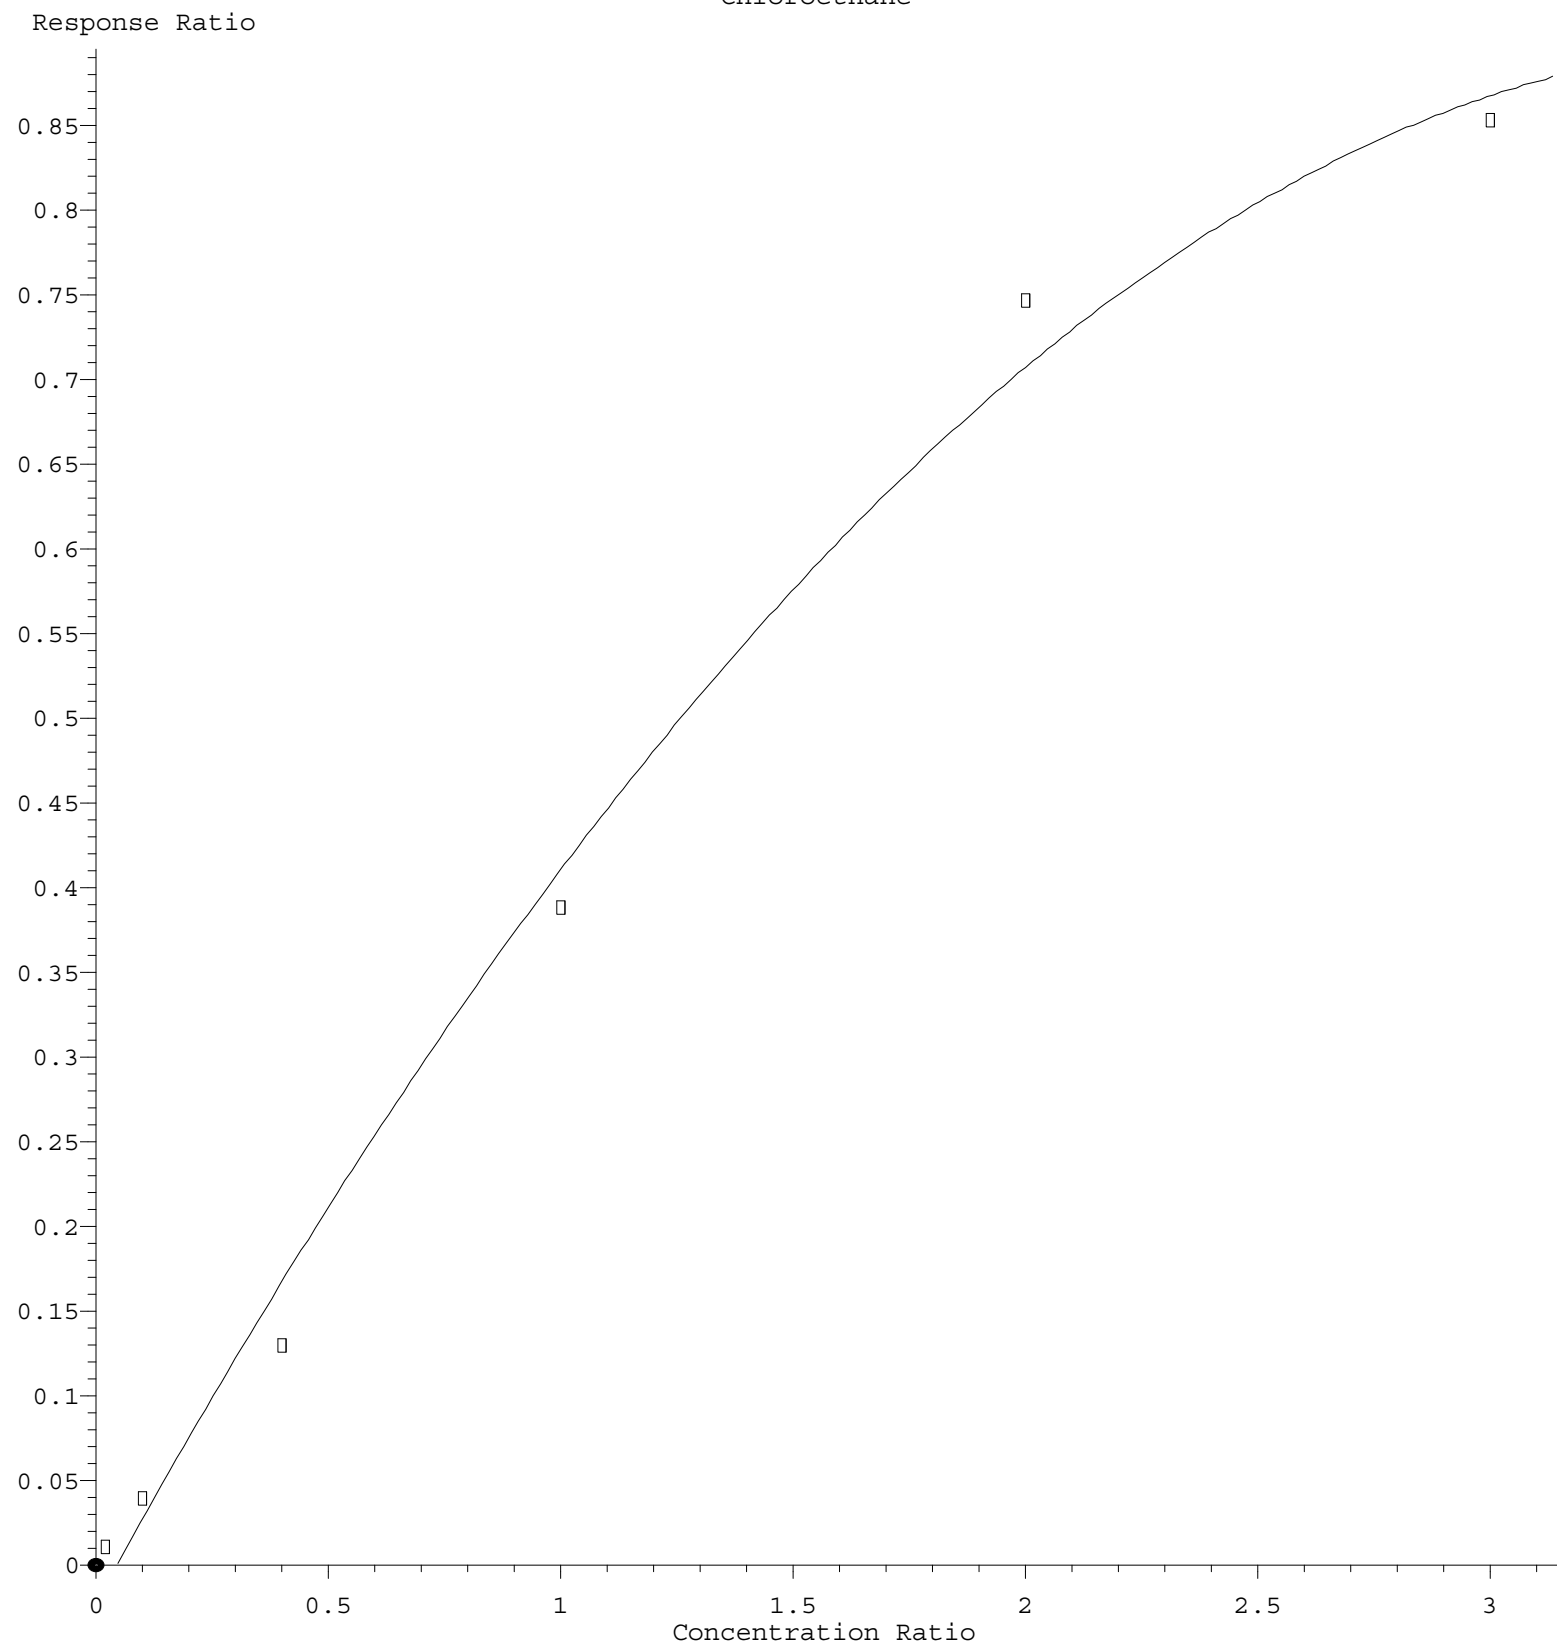

$R = -6.809e-002 A^2 + 5.008e-001 A - 2.208e-002$
 Coef of Det (r^2) = 0.993521 Curve Fit: Quadratic
 Method Name: Z:\voasrv\HPCHEM1\MSVOA X\Method\82X081721W.M
 Calibration Table Last Updated: Tue Aug 17 11:57:51 2021

t-1,3-Dichloropropene

Response Ratio

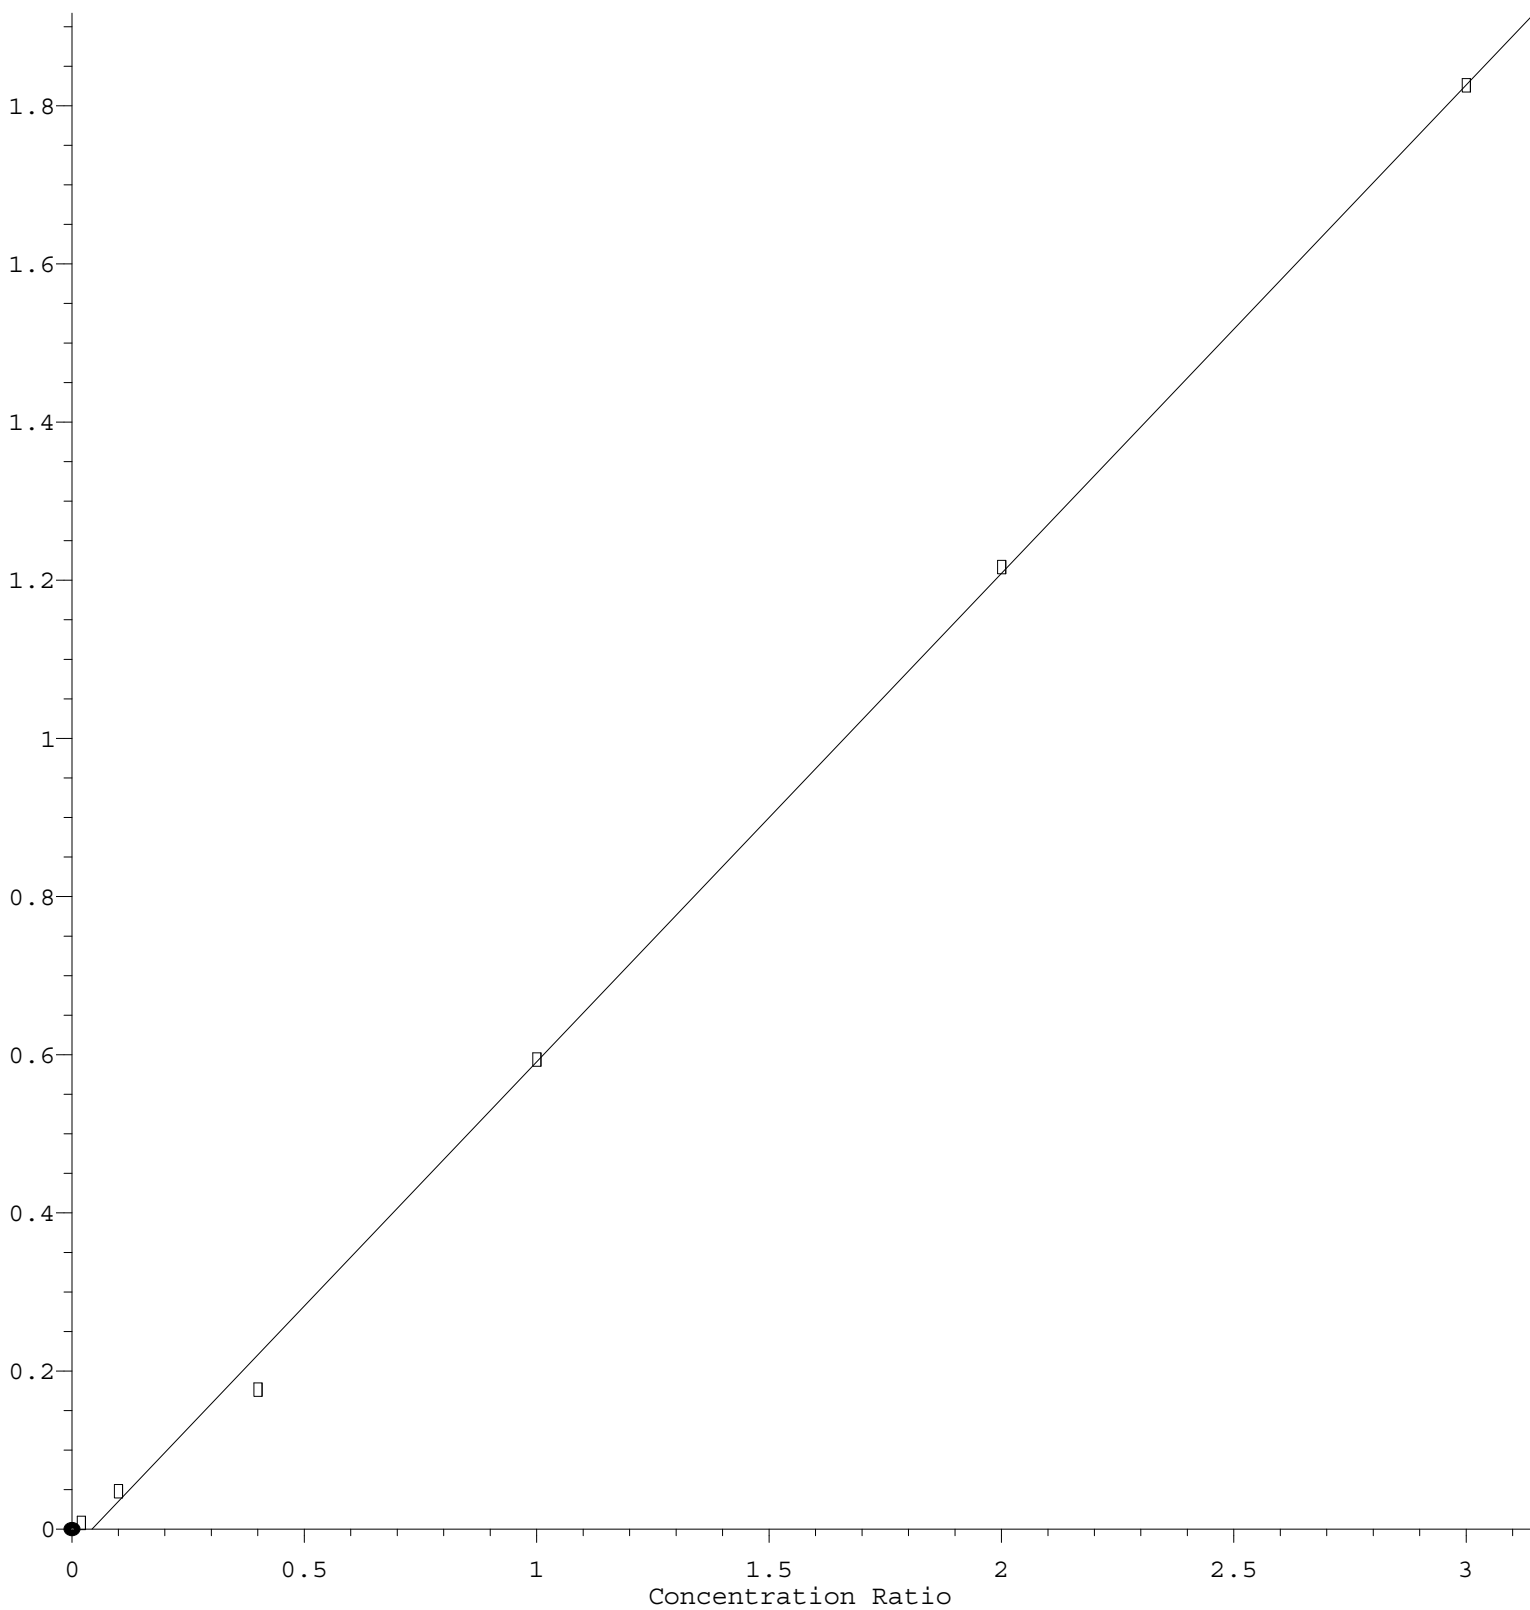

$$\text{Response} = 6.176\text{e-}001 * \text{Amt} - 2.640\text{e-}002$$


Coef of Det (r^2) = 0.999018 Curve Fit: Linear

Method Name: Z:\voasrv\HPCHEM1\MSVOA X\Method\82X081721W.M

Calibration Table Last Updated: Tue Aug 17 11:57:51 2021

Ethyl methacrylate

Response Ratio

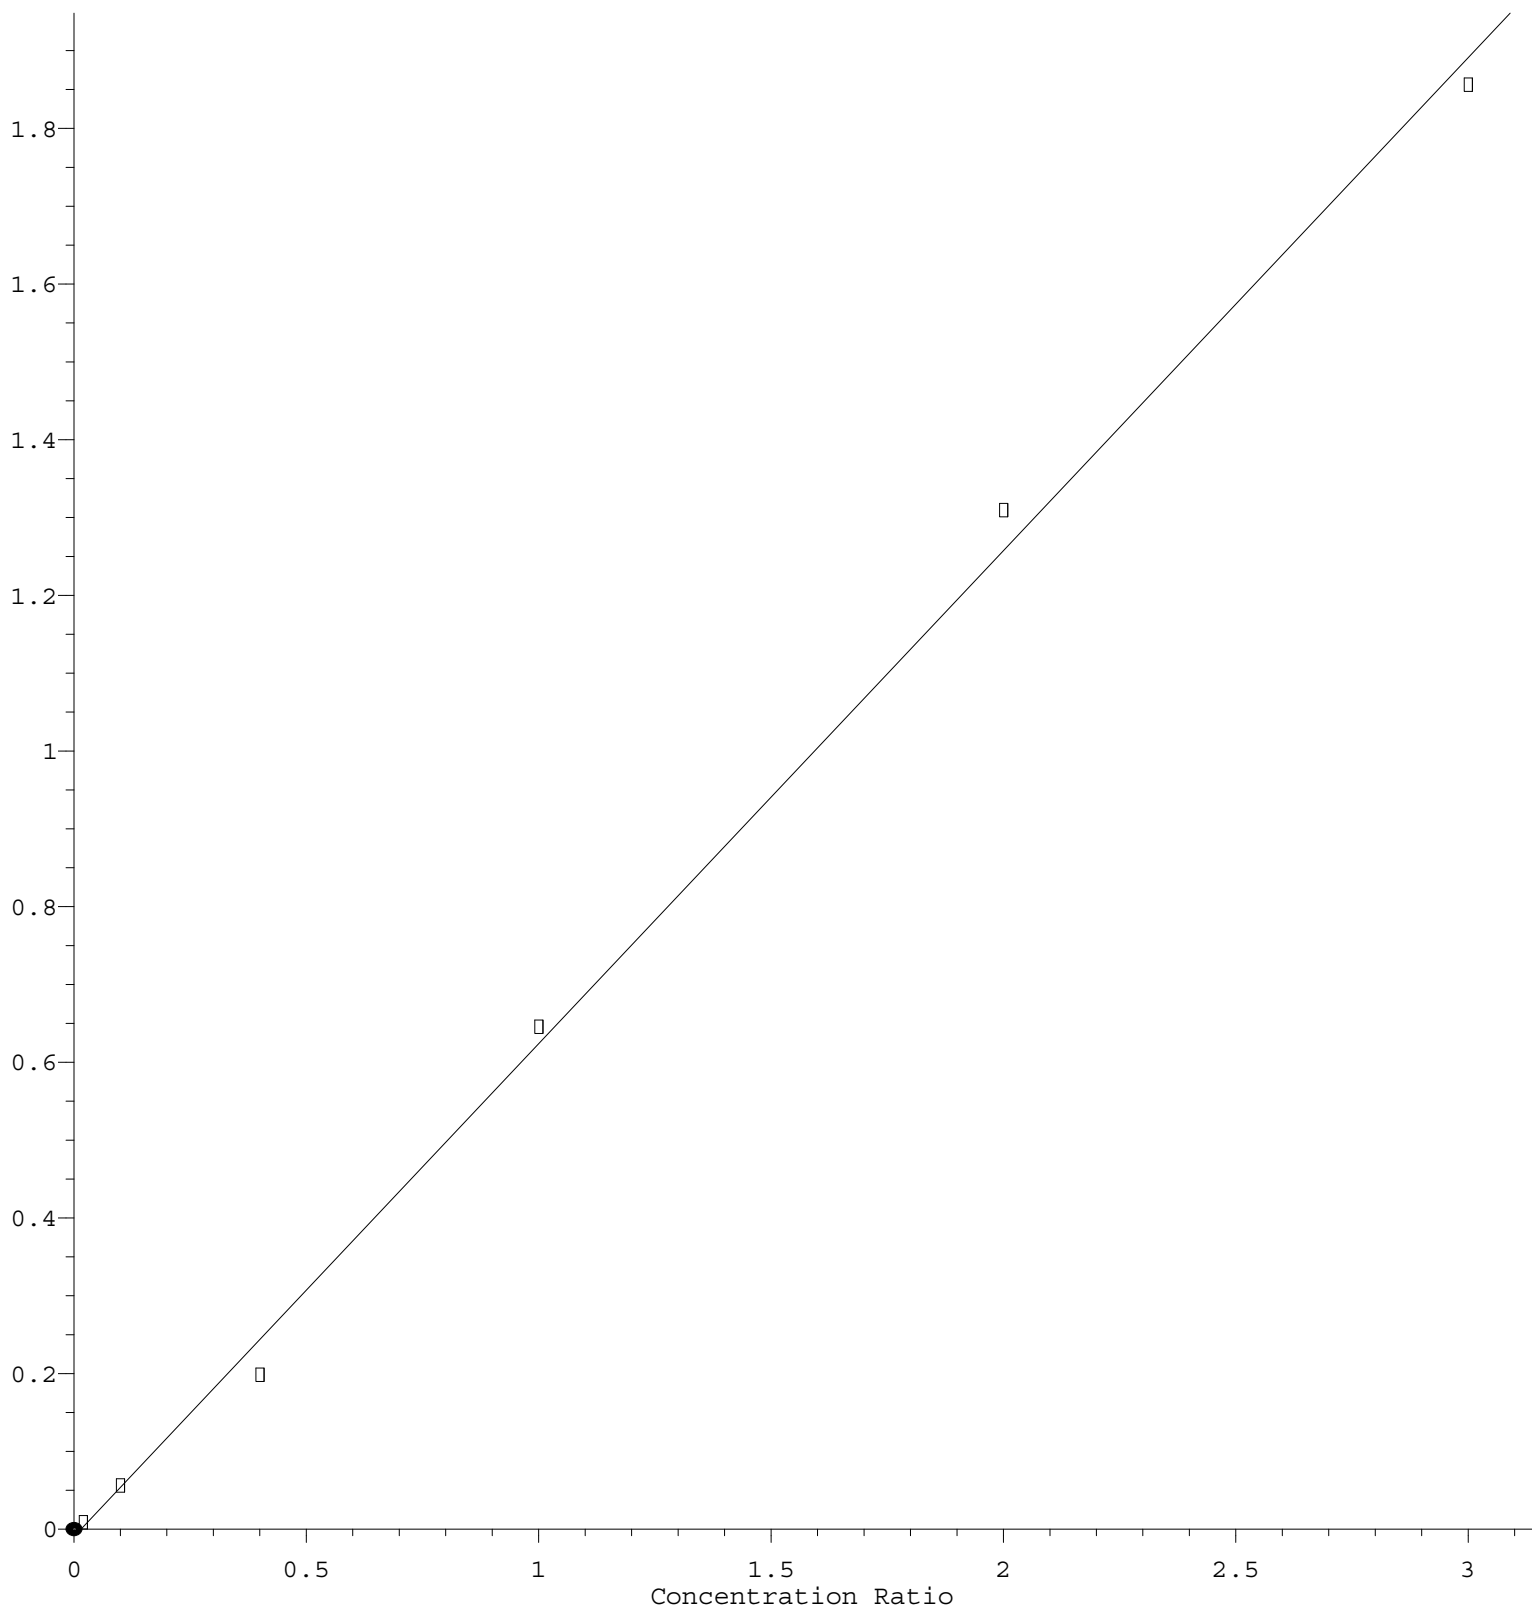

$$\text{Response} = 6.338\text{e-}001 * \text{Amt} - 9.626\text{e-}003$$


Coef of Det (r^2) = 0.997724 Curve Fit: Linear

Method Name: Z:\voasrv\HPCHEM1\MSVOA X\Method\82X081721W.M

Calibration Table Last Updated: Tue Aug 17 11:57:51 2021

Dibromochloromethane


Response Ratio

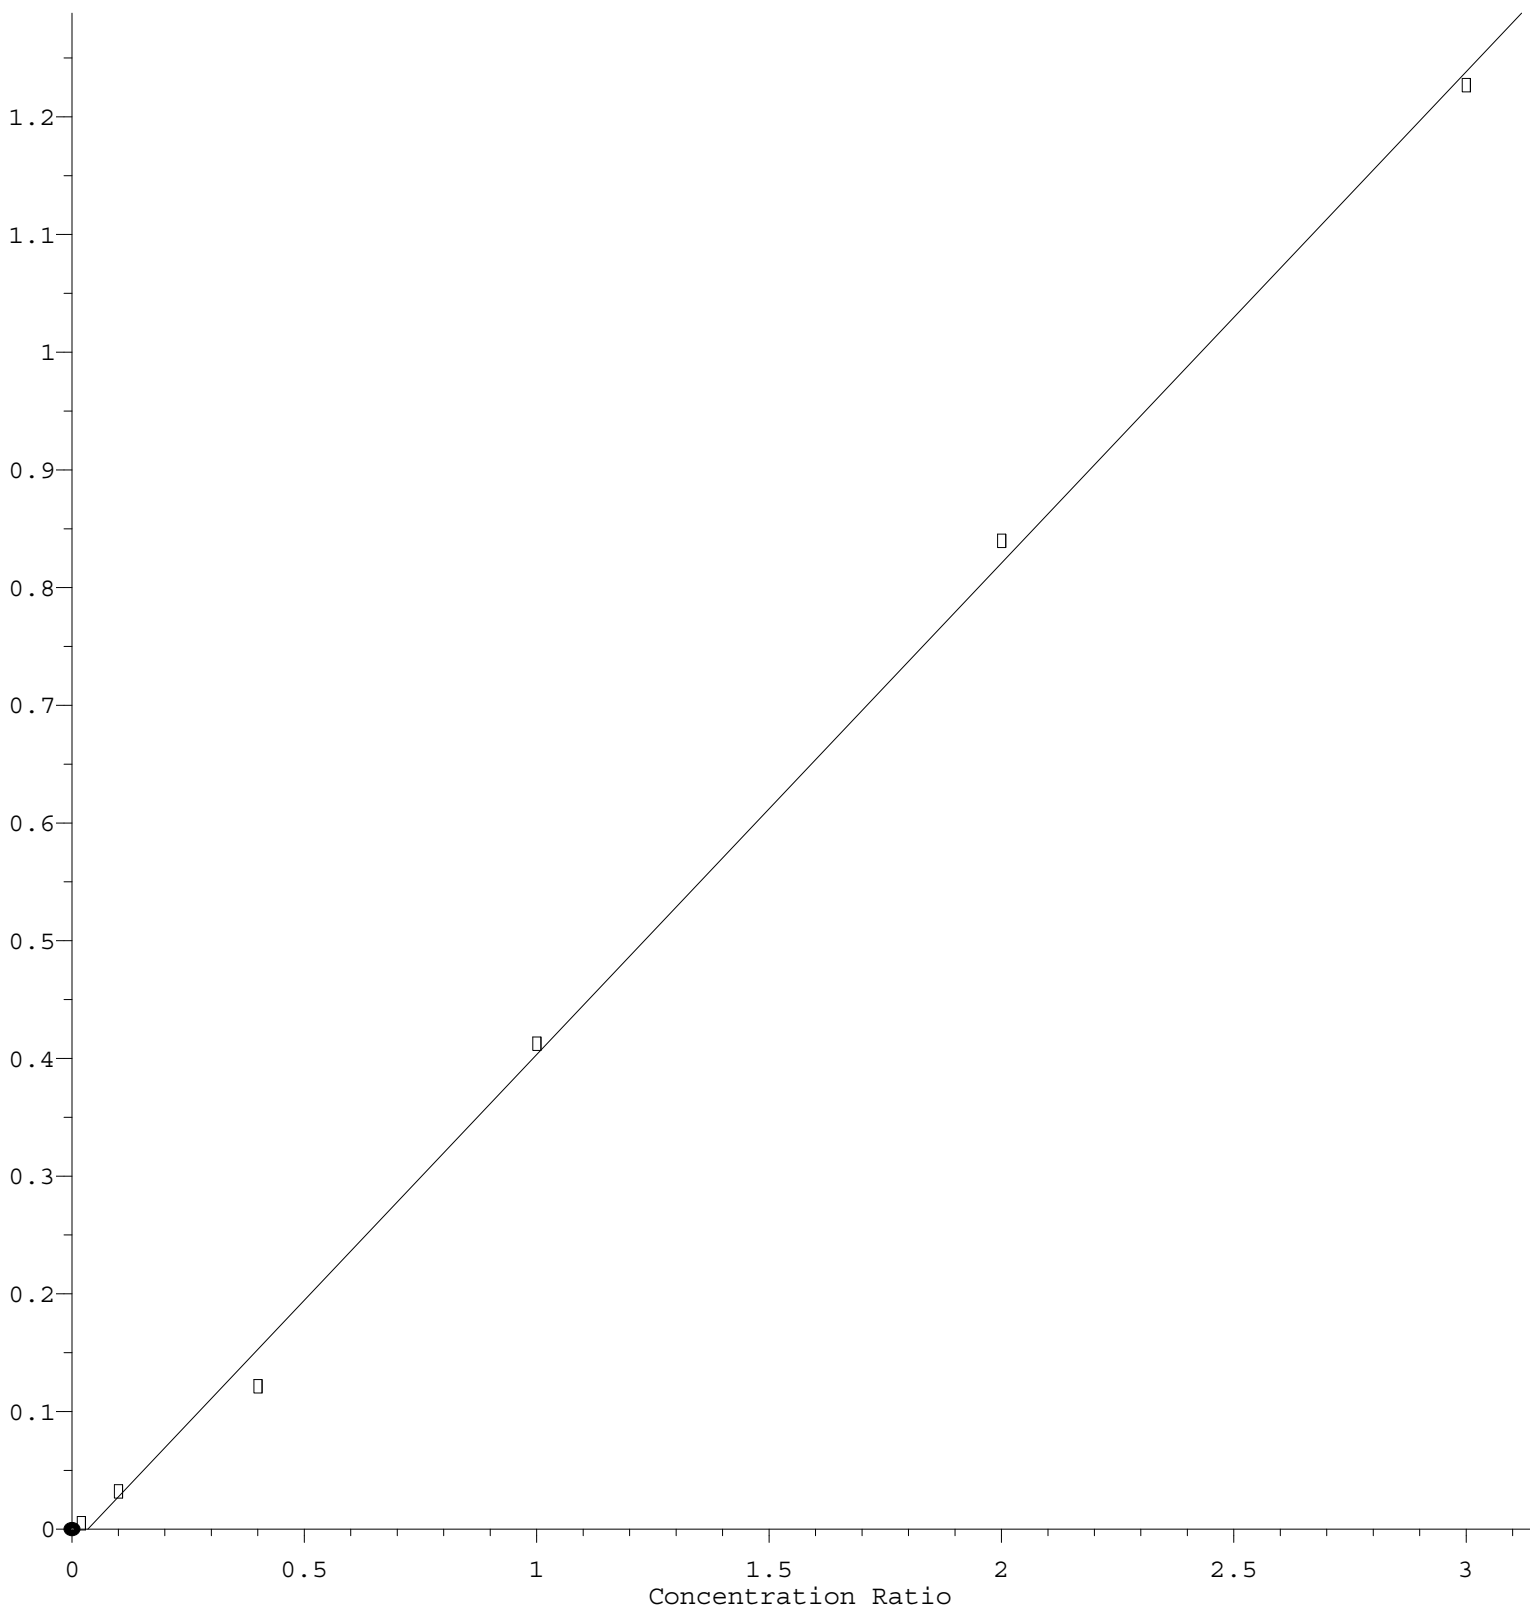

Response = 4.175e-001 * Amt - 1.409e-002
 Coef of Det (r^2) = 0.998629 Curve Fit: Linear
 Method Name: Z:\voasrv\HPCHEM1\MSVOA X\Method\82X081721W.M
 Calibration Table Last Updated: Tue Aug 17 11:57:51 2021

Bromoform

Response Ratio

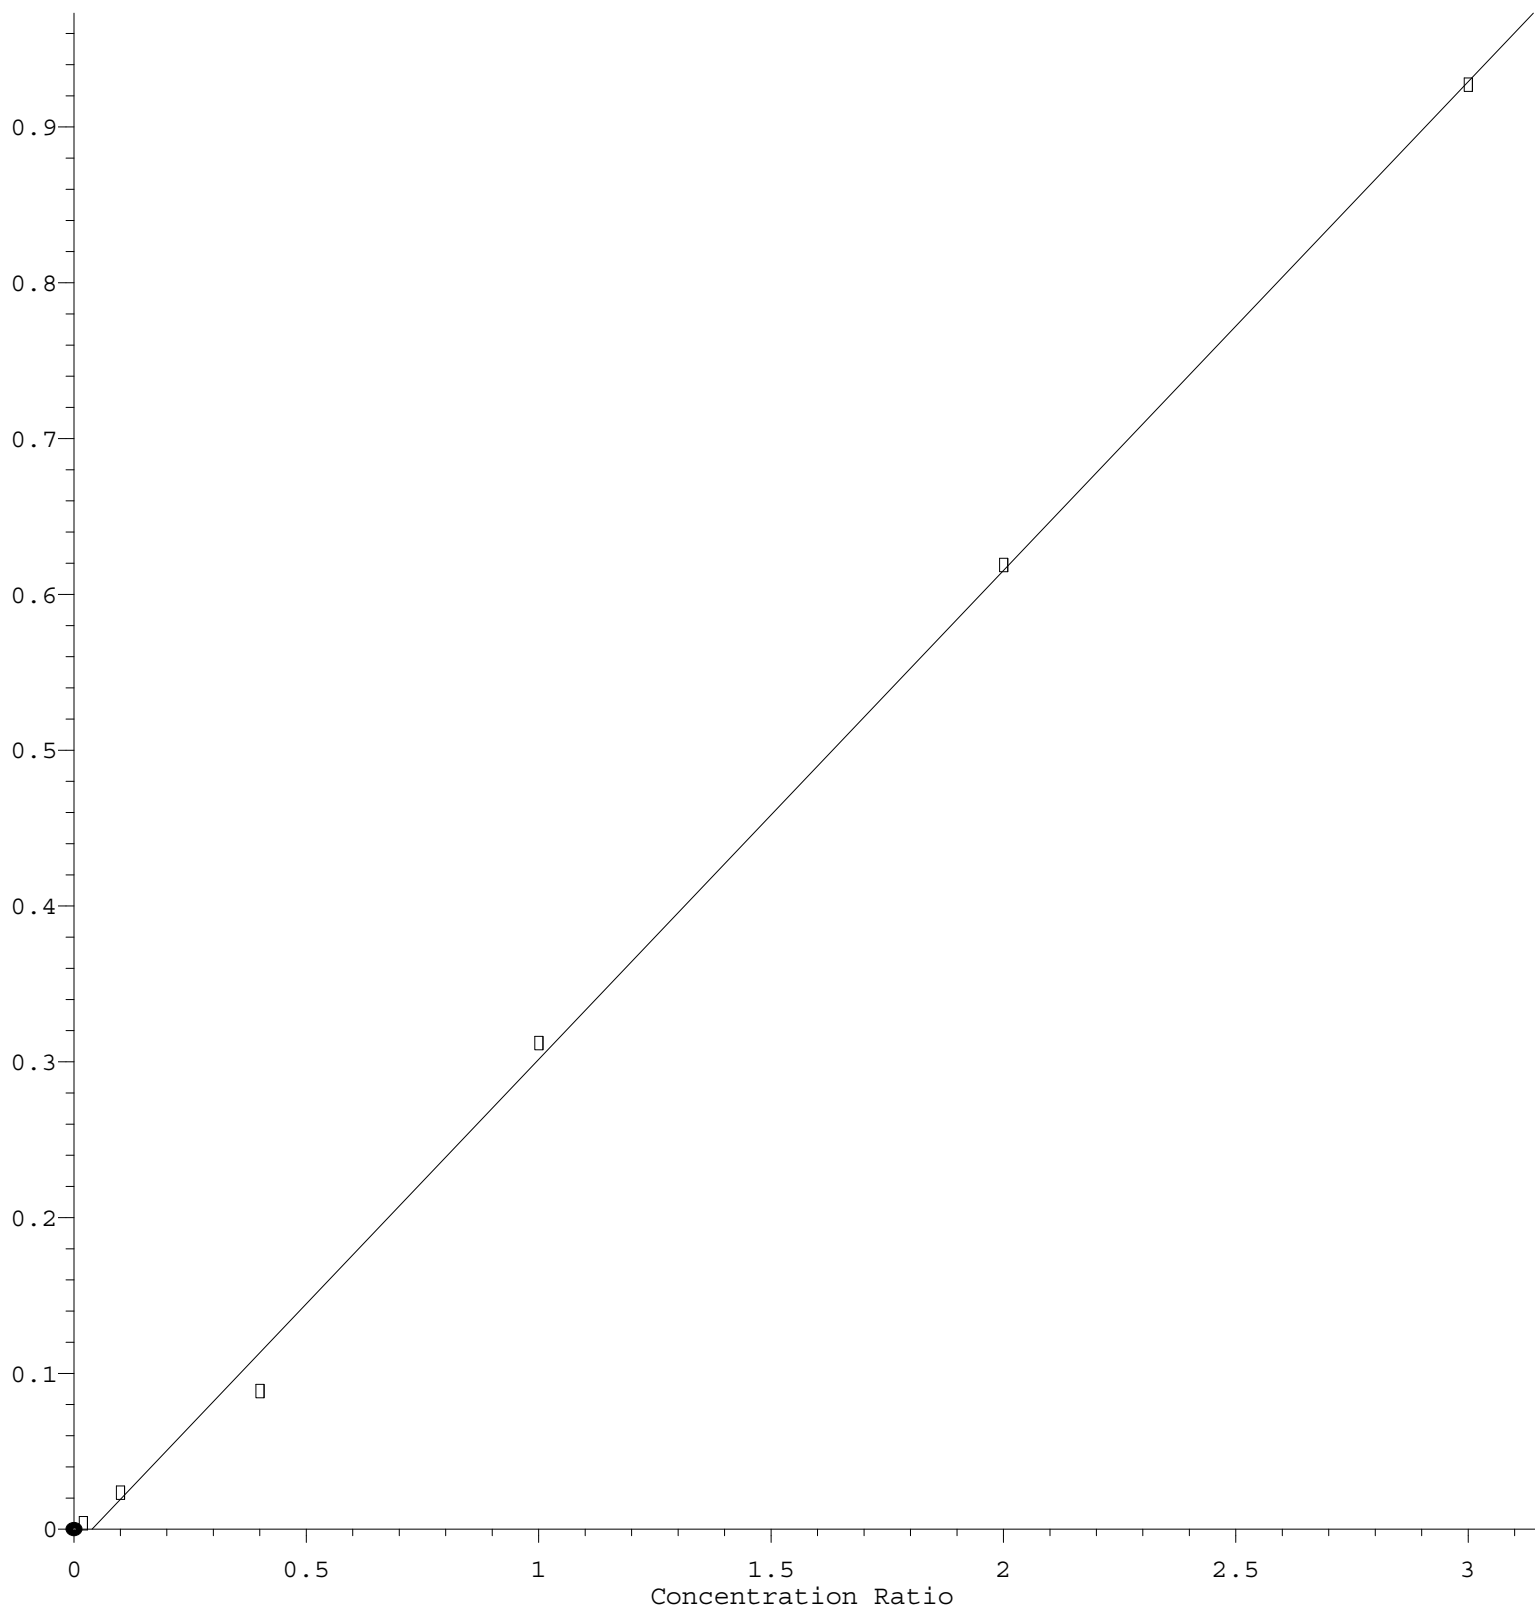

$$\text{Response} = 3.139\text{e-}001 * \text{Amt} - 1.212\text{e-}002$$


Coef of Det (r^2) = 0.998786 Curve Fit: Linear

Method Name: Z:\voasrv\HPCHEM1\MSVOA X\Method\82X081721W.M

Calibration Table Last Updated: Tue Aug 17 11:57:51 2021

Hexachloroethane

Response Ratio

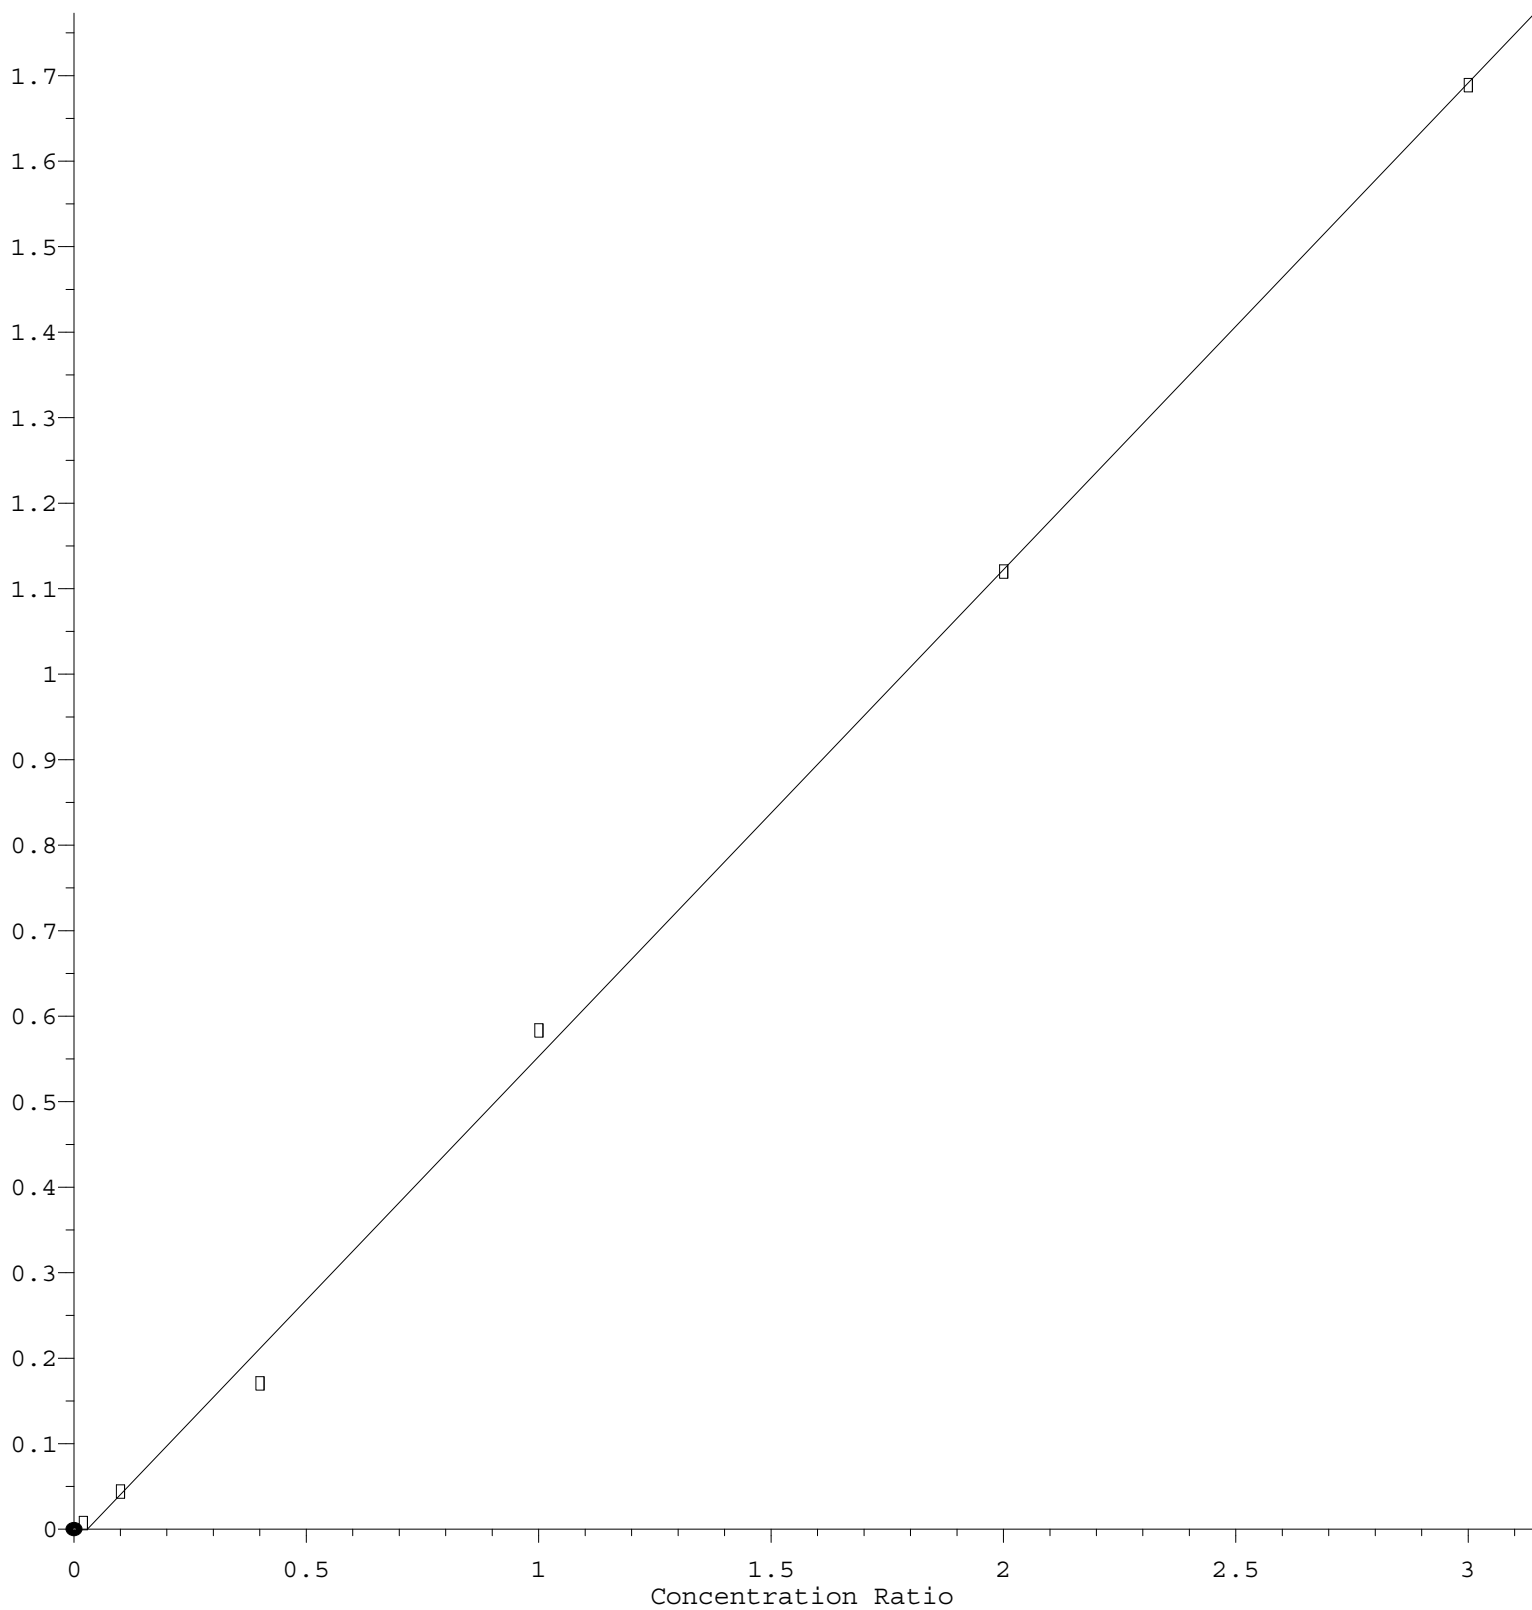

$$\text{Response} = 5.696 \times 10^{-1} \times \text{Amt} - 1.670 \times 10^{-2}$$


Coef of Det (r^2) = 0.998800 Curve Fit: Linear

Method Name: Z:\voasrv\HPCHEM1\MSVOA X\Method\82X081721W.M

Calibration Table Last Updated: Tue Aug 17 11:57:51 2021

1,2-Dibromo-3-Chloropropane

Response Ratio

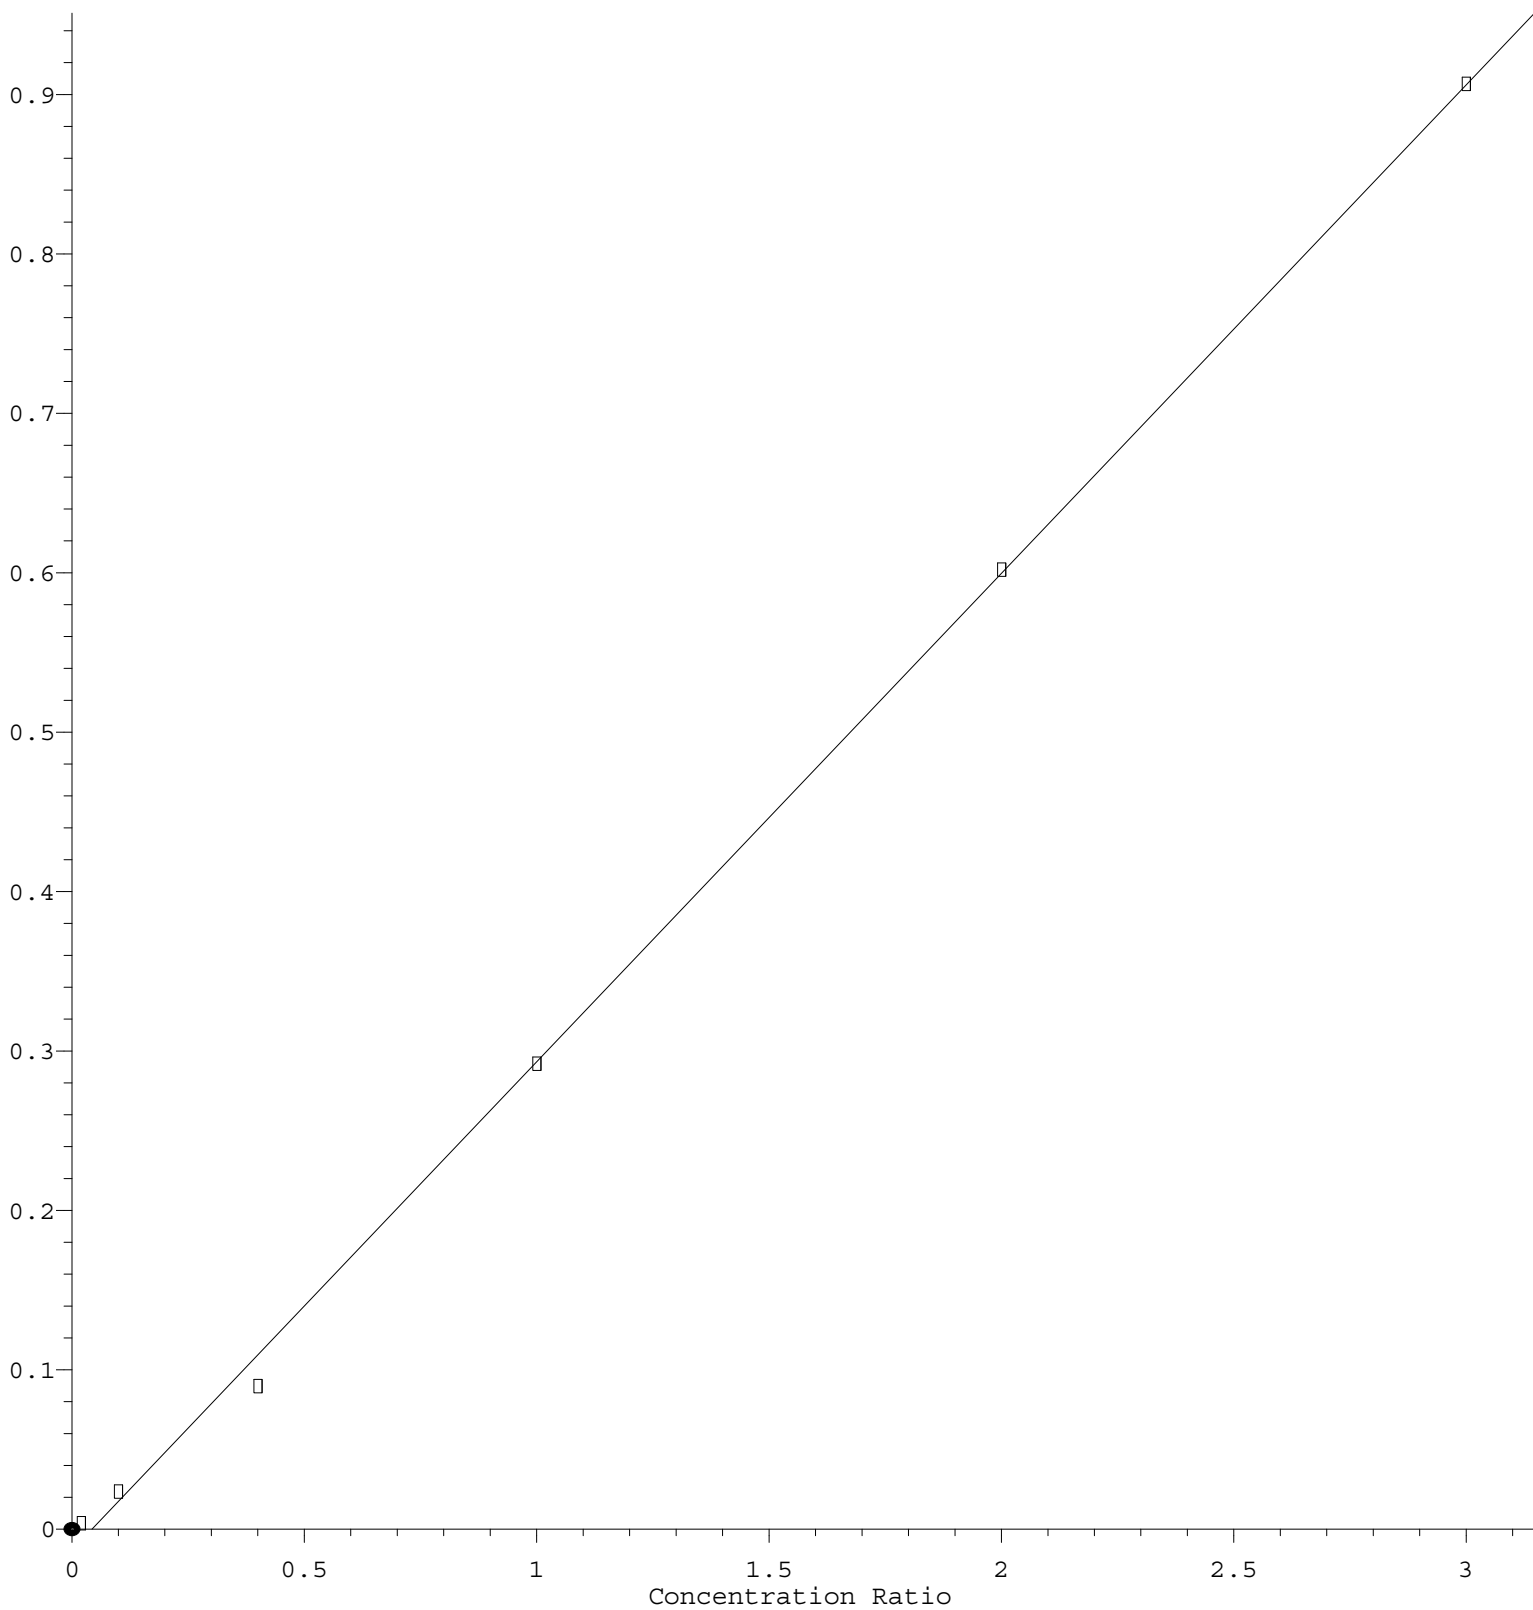

$$\text{Response} = 3.063\text{e-}001 * \text{Amt} - 1.324\text{e-}002$$


Coef of Det (r^2) = 0.999174 Curve Fit: Linear

Method Name: Z:\voasrv\HPCHEM1\MSVOA X\Method\82X081721W.M

Calibration Table Last Updated: Tue Aug 17 11:57:51 2021

Naphthalene

Response Ratio

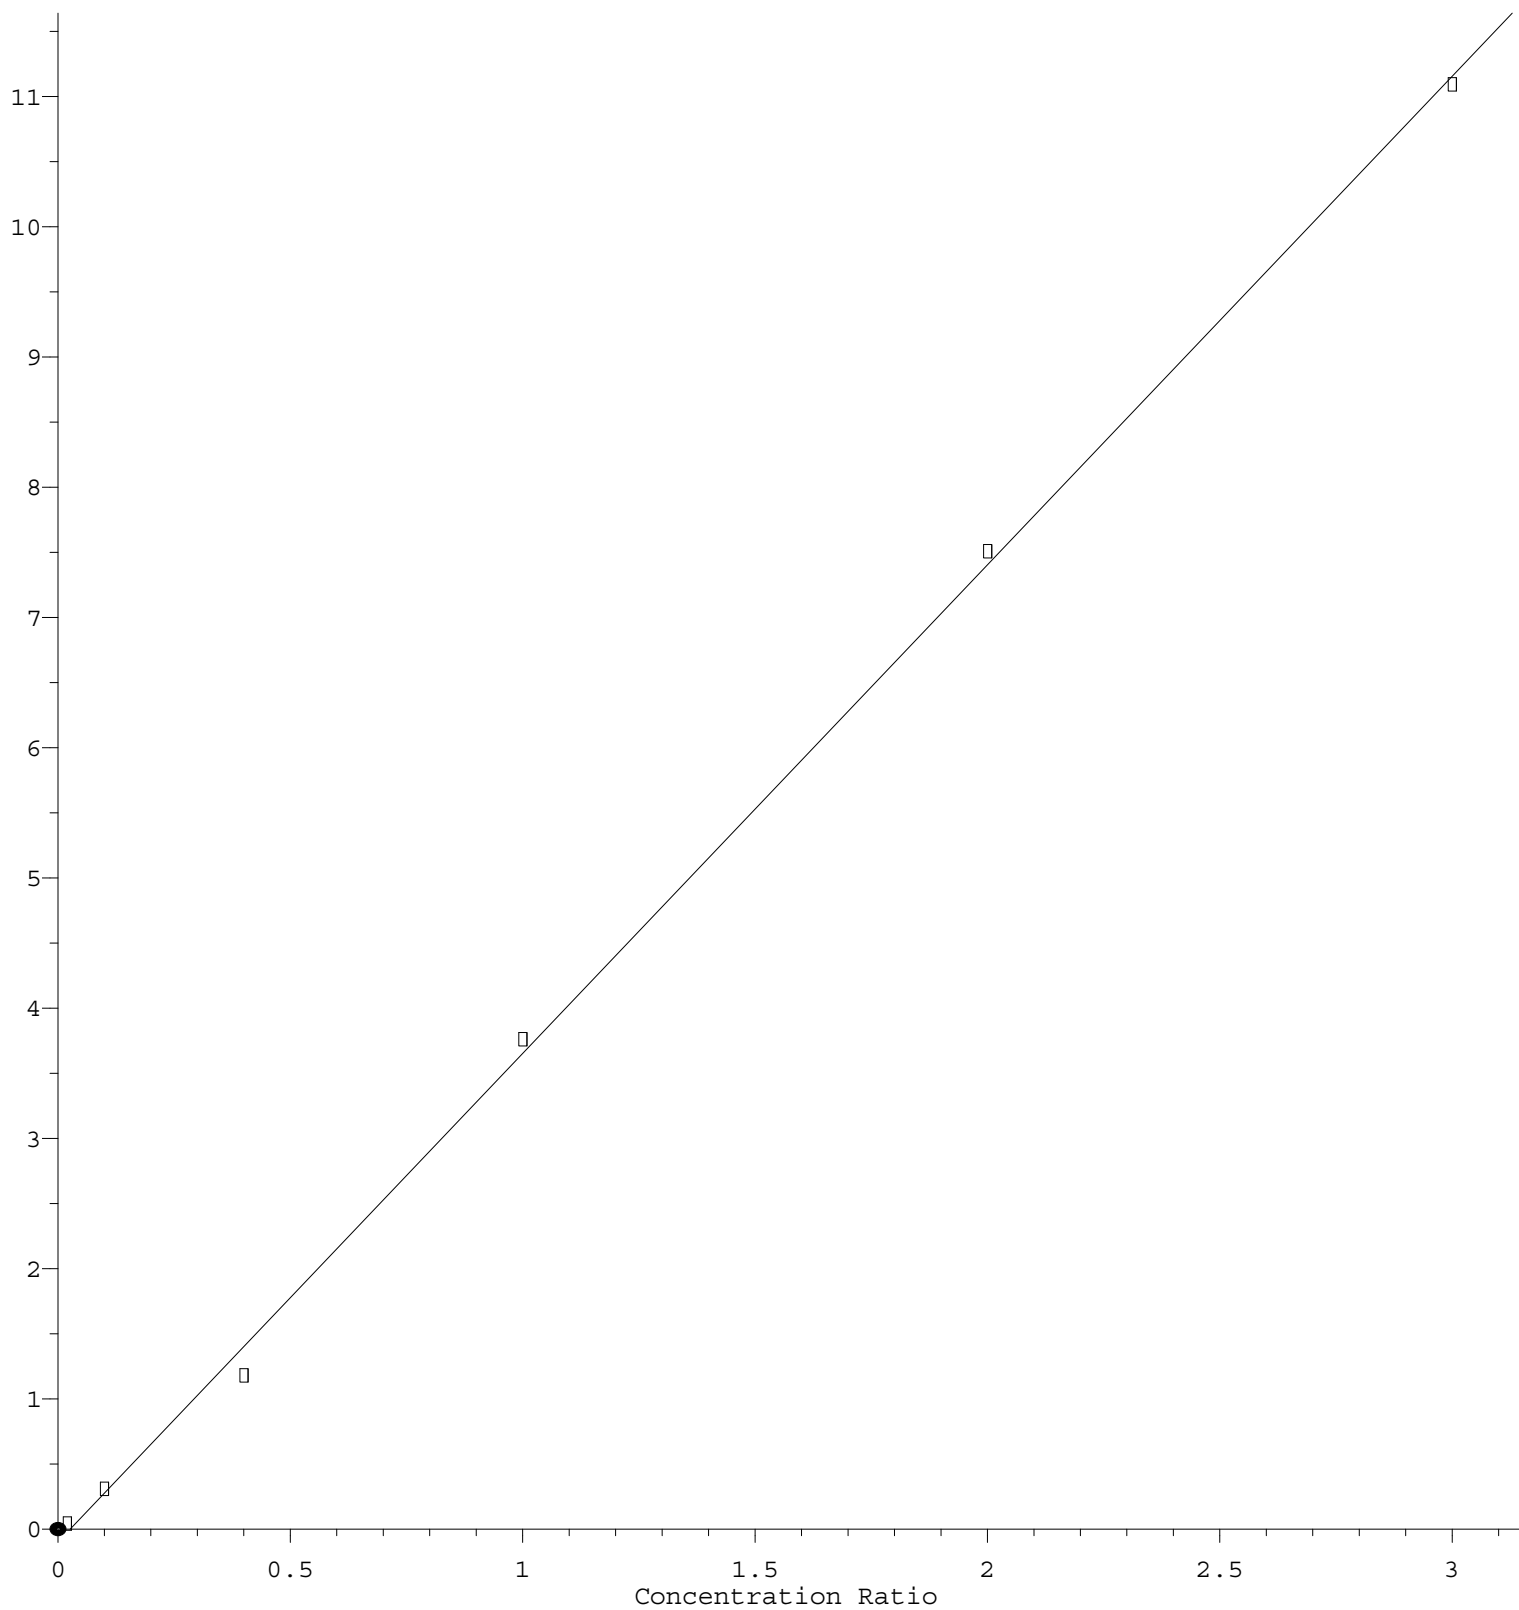

$$\text{Response} = 3.753\text{e}+000 * \text{Amt} - 9.627\text{e}-002$$

Coef of Det (r^2) = 0.999188 Curve Fit: Linear

Method Name: Z:\voasrv\HPCHEM1\MSVOA X\Method\82X081721W.M

Calibration Table Last Updated: Tue Aug 17 11:57:51 2021