
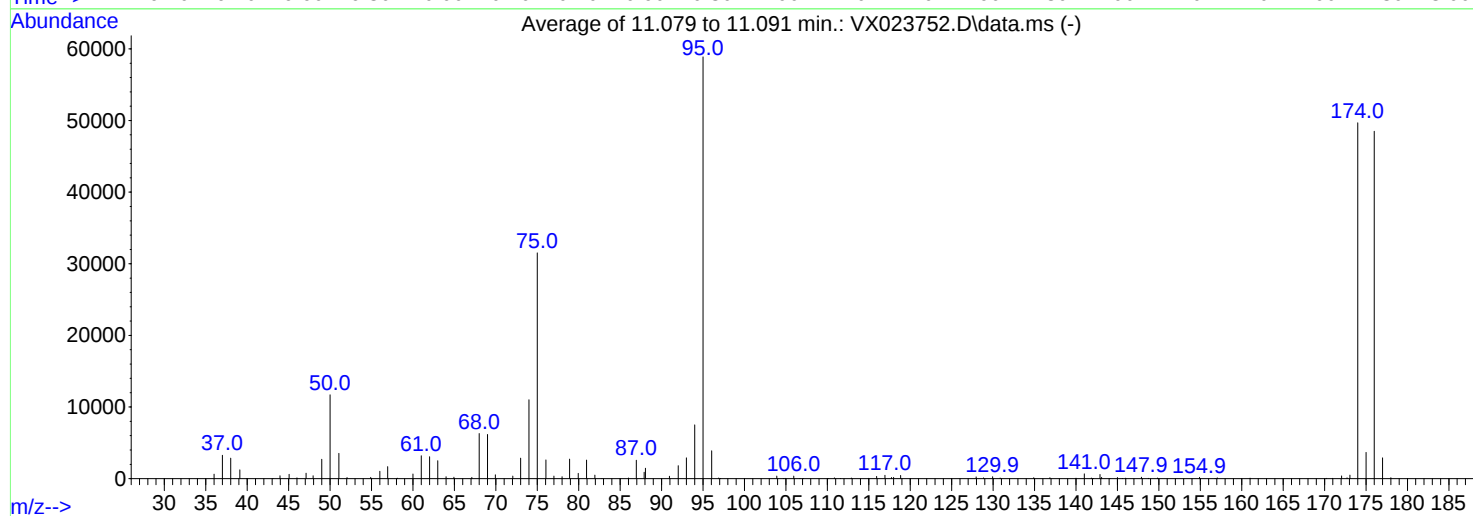


Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX081721\
Data File : VX023752.D
Acq On : 17 Aug 2021 09:02
Operator : JC/MD
Sample : BFB
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X081721W.M
Title : SW846 8260
Last Update : Tue Aug 17 11:57:51 2021

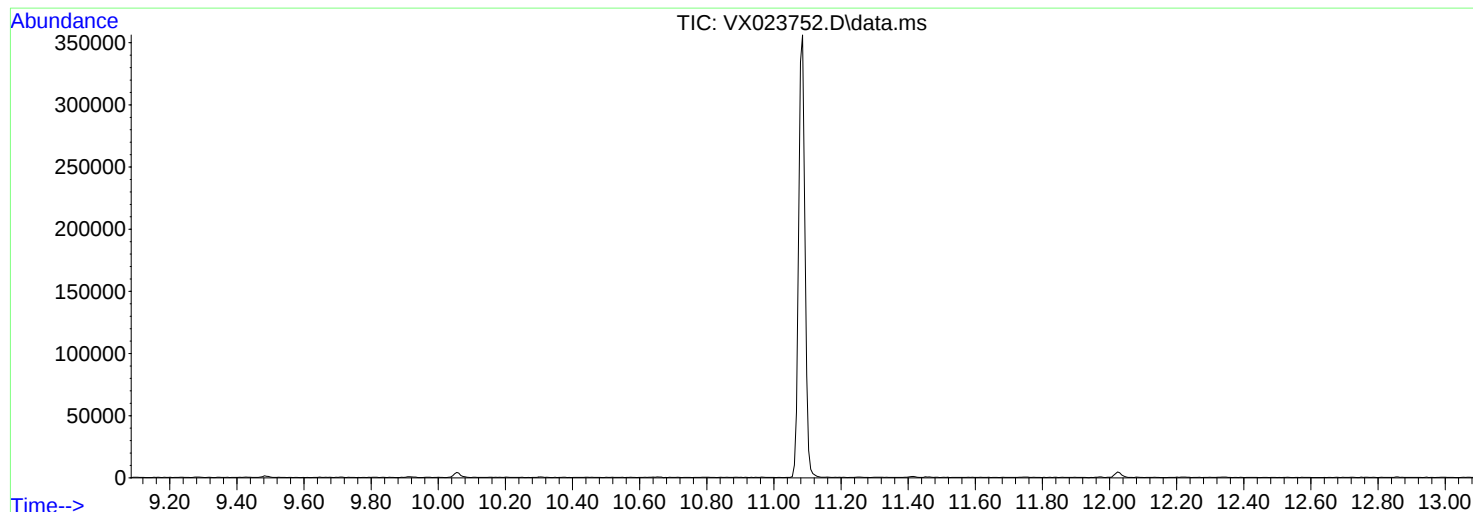

AutoFind: Scans 1639, 1640, 1641; Background Corrected with Scan 1632

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	19.9	11714	PASS
75	95	30	60	53.5	31512	PASS
95	95	100	100	100.0	58891	PASS
96	95	5	9	6.6	3897	PASS
173	174	0.00	2	1.0	491	PASS
174	95	50	100	84.4	49675	PASS
175	174	5	9	7.4	3672	PASS
176	174	95	101	97.6	48496	PASS
177	176	5	9	6.0	2894	PASS