
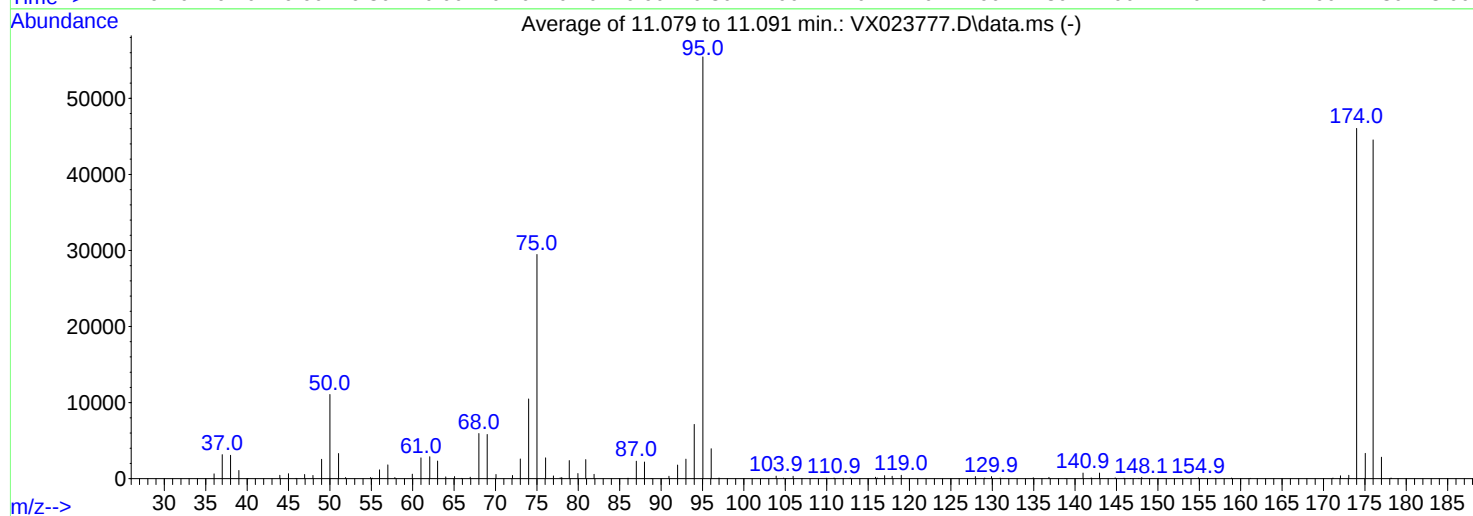


Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX081721\
 Data File : VX023777.D
 Acq On : 17 Aug 2021 21:12
 Operator : JC/MD
 Sample : BFB
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 27 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X081721W.M
 Title : SW846 8260
 Last Update : Tue Aug 17 11:57:51 2021

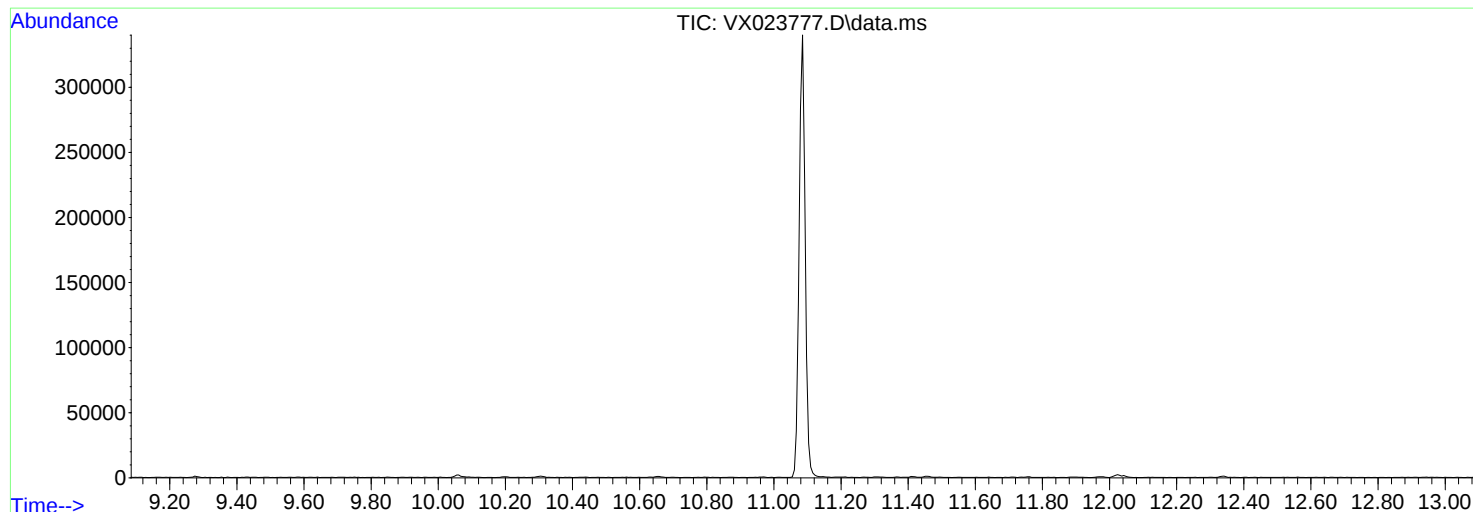

AutoFind: Scans 1639, 1640, 1641; Background Corrected with Scan 1632

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	20.0	11064	PASS
75	95	30	60	53.1	29472	PASS
95	95	100	100	100.0	55456	PASS
96	95	5	9	7.1	3944	PASS
173	174	0.00	2	1.0	442	PASS
174	95	50	100	83.0	46053	PASS
175	174	5	9	7.2	3318	PASS
176	174	95	101	96.7	44536	PASS
177	176	5	9	6.4	2829	PASS