

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX081722\
 Data File : VX030654.D
 Acq On : 17 Aug 2022 12:21
 Operator : JC/MD
 Sample : VX0817MBL01
 Misc : 5.00g/5mL/100uL/5.00mL/MSVOA_X/MEOH
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :

Quant Time: Aug 18 04:21:33 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML080422WMA.M
 Quant Title : VOC Analysis
 QLast Update : Thu Aug 18 04:21:09 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	6.763	114	303009	50.000	ug/L	0.00
28) Chlorobenzene-d5	10.055	117	274264	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	12.024	152	126139	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.367	65	102372	52.610	ug/L	0.00
Spiked Amount 50.000	Range 60 - 135		Recovery = 105.220%			
7) Chloroethane-d5	1.666	69	76819	56.001	ug/L	0.00
Spiked Amount 50.000	Range 70 - 130		Recovery = 112.000%			
11) 1,1-Dichloroethene-d2	2.306	63	162959	44.273	ug/L	0.00
Spiked Amount 50.000	Range 60 - 125		Recovery = 88.540%			
21) 2-Butanone-d5	4.464	46	196189	108.816	ug/L	0.00
Spiked Amount 100.000	Range 40 - 130		Recovery = 108.820%			
24) Chloroform-d	5.062	84	217894	54.397	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery = 108.800%			
26) 1,2-Dichloroethane-d4	5.958	65	143808	52.874	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery = 105.740%			
32) Benzene-d6	5.976	84	442354	56.306	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery = 112.620%			
36) 1,2-Dichloropropane-d6	7.312	67	148856	58.400	ug/L	0.00
Spiked Amount 50.000	Range 70 - 120		Recovery = 116.800%			
41) Toluene-d8	8.653	98	400069	54.024	ug/L	0.00
Spiked Amount 50.000	Range 80 - 120		Recovery = 108.040%			
43) trans-1,3-Dichloroprop...	8.951	79	64774	51.082	ug/L	0.00
Spiked Amount 50.000	Range 60 - 125		Recovery = 102.160%			
47) 2-Hexanone-d5	9.384	63	141737	109.094	ug/L	0.00
Spiked Amount 100.000	Range 45 - 130		Recovery = 109.090%			
56) 1,1,2,2-Tetrachloroeth...	11.195	84	195056	58.253	ug/L	0.00
Spiked Amount 50.000	Range 65 - 120		Recovery = 116.500%			
66) 1,2-Dichlorobenzene-d4	12.323	152	140332	57.358	ug/L	0.00
Spiked Amount 50.000	Range 80 - 120		Recovery = 114.720%			
Target Compounds						Qvalue
44) trans-1,3-Dichloropropene	8.945	75	2692	0.789	ug/L	96


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX081722\
Data File : VX030654.D
Acq On : 17 Aug 2022 12:21
Operator : JC/MD
Sample : VX0817MBL01
Misc : 5.00g/5mL/100uL/5.00mL/MSVOA_X/MEOH
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :


Quant Time: Aug 18 04:21:33 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM080422WMA.M
Quant Title : VOC Analysis
QLast Update : Thu Aug 18 04:21:09 2022
Response via : Initial Calibration

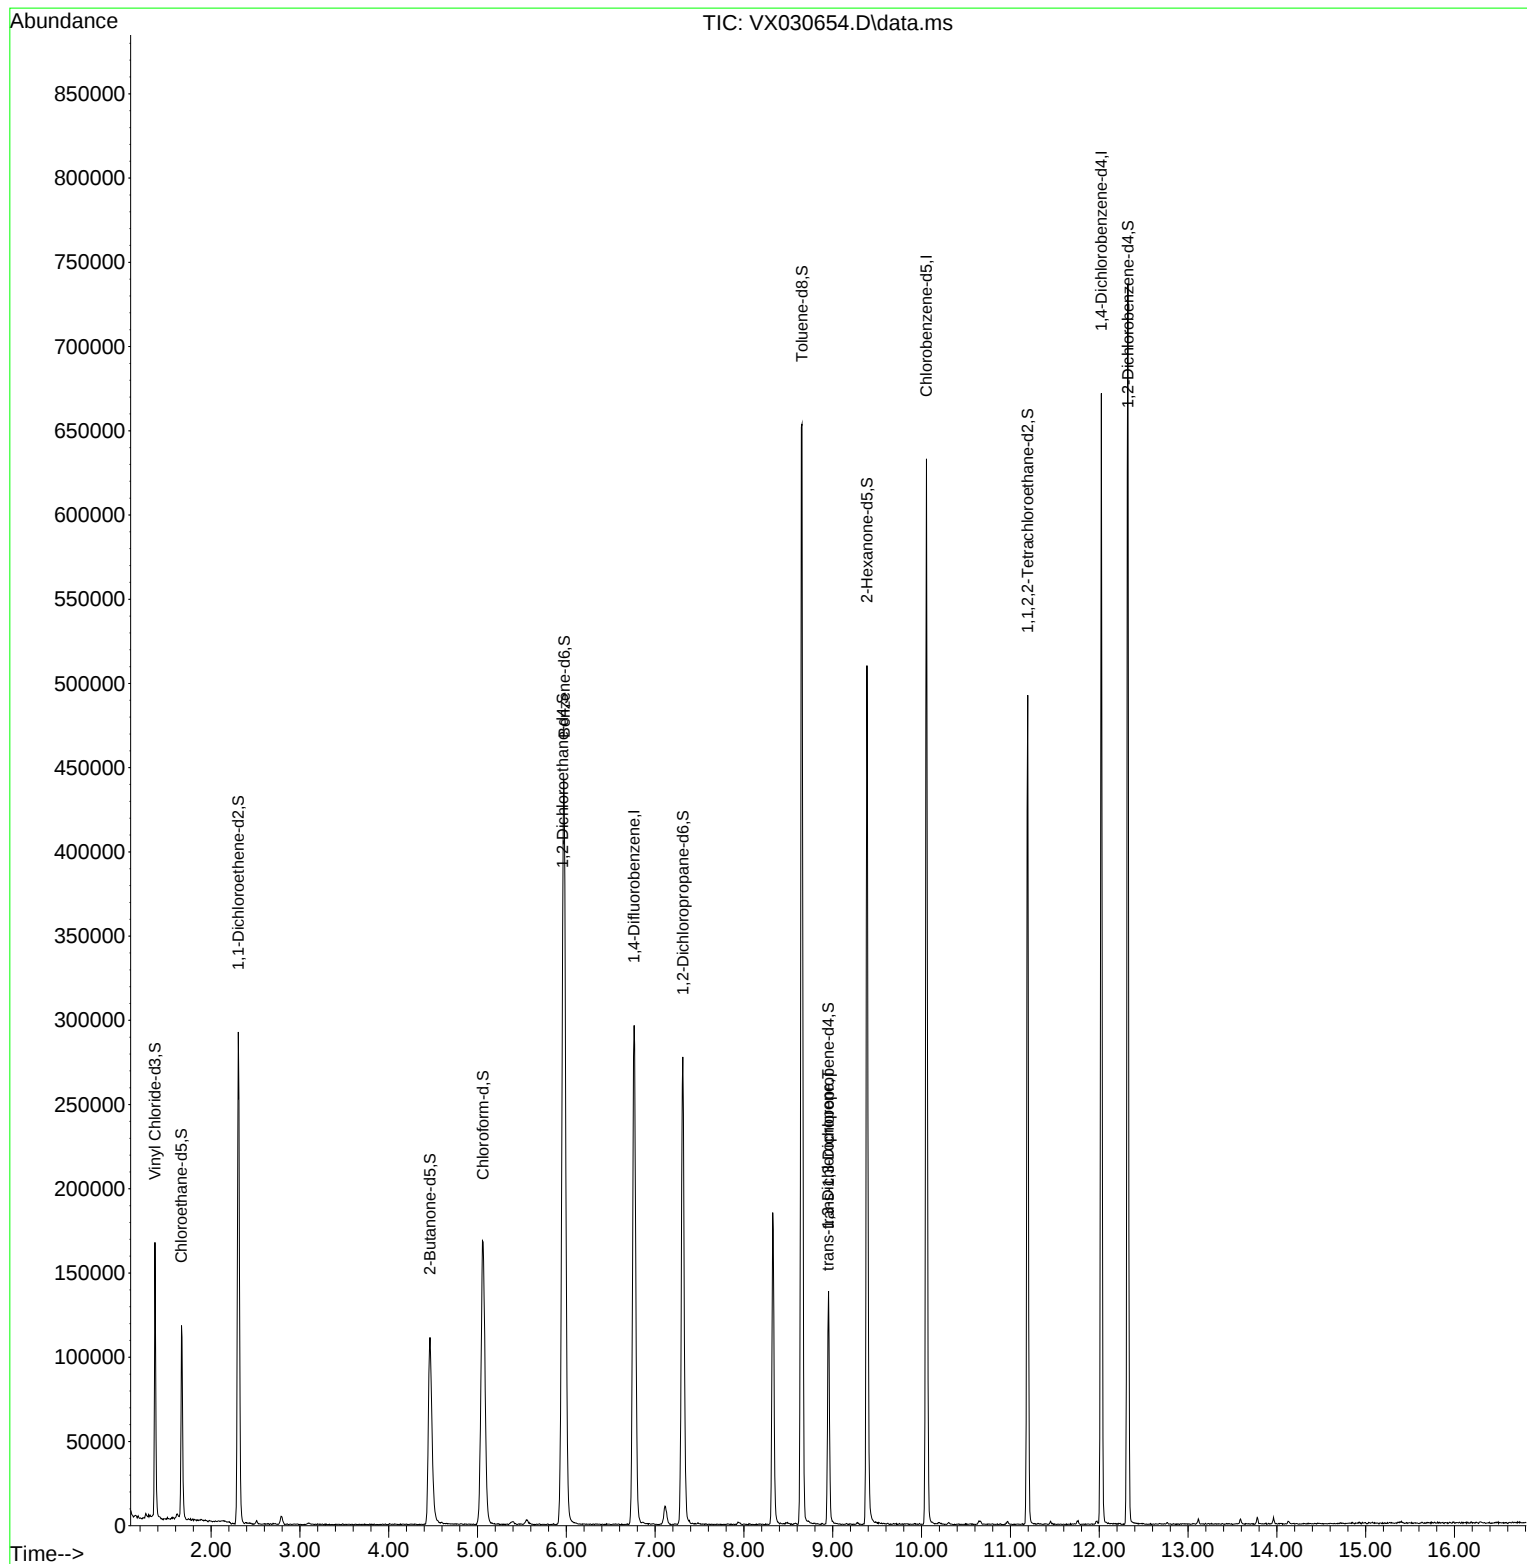

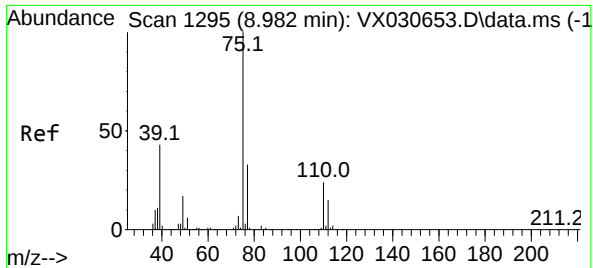

#44
 trans-1,3-Dichloropropene
 Concen: 0.789 ug/L
 RT: 8.945 min Scan# 11
 Delta R.T. -0.037 min
 Lab File: VX030654.D
 Acq: 17 Aug 2022 12:21

Instrument :
 MSVOA_X
 ClientSampleId :

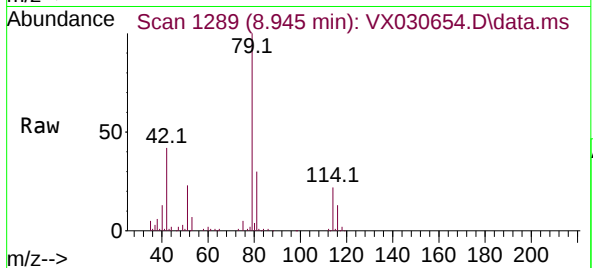

Tgt Ion: 75 Resp: 2692
 Ion Ratio Lower Upper
 75 100
 77 29.9 22.5 41.7

