

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX081722\
 Data File : VX030655.D
 Acq On : 17 Aug 2022 12:47
 Operator : JC/MD
 Sample : VX0817WBL01
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :

Quant Time: Aug 18 04:21:45 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML080422WMA.M
 Quant Title : VOC Analysis
 QLast Update : Thu Aug 18 04:21:09 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	6.769	114	278915	50.000	ug/L	0.00
28) Chlorobenzene-d5	10.055	117	254095	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	12.024	152	115872	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.368	65	95157	53.126	ug/L	0.00
Spiked Amount	50.000	Range 60 - 135	Recovery	=	106.260%	
7) Chloroethane-d5	1.666	69	70451	55.795	ug/L	0.00
Spiked Amount	50.000	Range 70 - 130	Recovery	=	111.600%	
11) 1,1-Dichloroethene-d2	2.306	63	148775	43.911	ug/L	0.00
Spiked Amount	50.000	Range 60 - 125	Recovery	=	87.820%	
21) 2-Butanone-d5	4.465	46	189042	113.909	ug/L	0.00
Spiked Amount	100.000	Range 40 - 130	Recovery	=	113.910%	
24) Chloroform-d	5.062	84	205788	55.813	ug/L	0.00
Spiked Amount	50.000	Range 70 - 125	Recovery	=	111.620%	
26) 1,2-Dichloroethane-d4	5.958	65	136057	54.345	ug/L	0.00
Spiked Amount	50.000	Range 70 - 125	Recovery	=	108.700%	
32) Benzene-d6	5.976	84	412226	56.636	ug/L	0.00
Spiked Amount	50.000	Range 70 - 125	Recovery	=	113.280%	
36) 1,2-Dichloropropane-d6	7.312	67	137243	58.118	ug/L	0.00
Spiked Amount	50.000	Range 70 - 120	Recovery	=	116.240%	
41) Toluene-d8	8.653	98	370674	54.028	ug/L	0.00
Spiked Amount	50.000	Range 80 - 120	Recovery	=	108.060%	
43) trans-1,3-Dichloroprop...	8.952	79	61910	52.699	ug/L	0.00
Spiked Amount	50.000	Range 60 - 125	Recovery	=	105.400%	
47) 2-Hexanone-d5	9.384	63	137721	114.417	ug/L	0.00
Spiked Amount	100.000	Range 45 - 130	Recovery	=	114.420%	
56) 1,1,2,2-Tetrachloroeth...	11.195	84	182649	58.878	ug/L	0.00
Spiked Amount	50.000	Range 65 - 120	Recovery	=	117.760%	
66) 1,2-Dichlorobenzene-d4	12.323	152	124880	55.565	ug/L	0.00
Spiked Amount	50.000	Range 80 - 120	Recovery	=	111.120%	
Target Compounds						Qvalue
10) 1,1,2-Trichloro-1,2,2-...	2.312	101	1582	0.934	ug/L	# 22


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX081722\
Data File : VX030655.D
Acq On : 17 Aug 2022 12:47
Operator : JC/MD
Sample : VX0817WBL01
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :

Quant Time: Aug 18 04:21:45 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML080422WMA.M
Quant Title : VOC Analysis
QLast Update : Thu Aug 18 04:21:09 2022
Response via : Initial Calibration

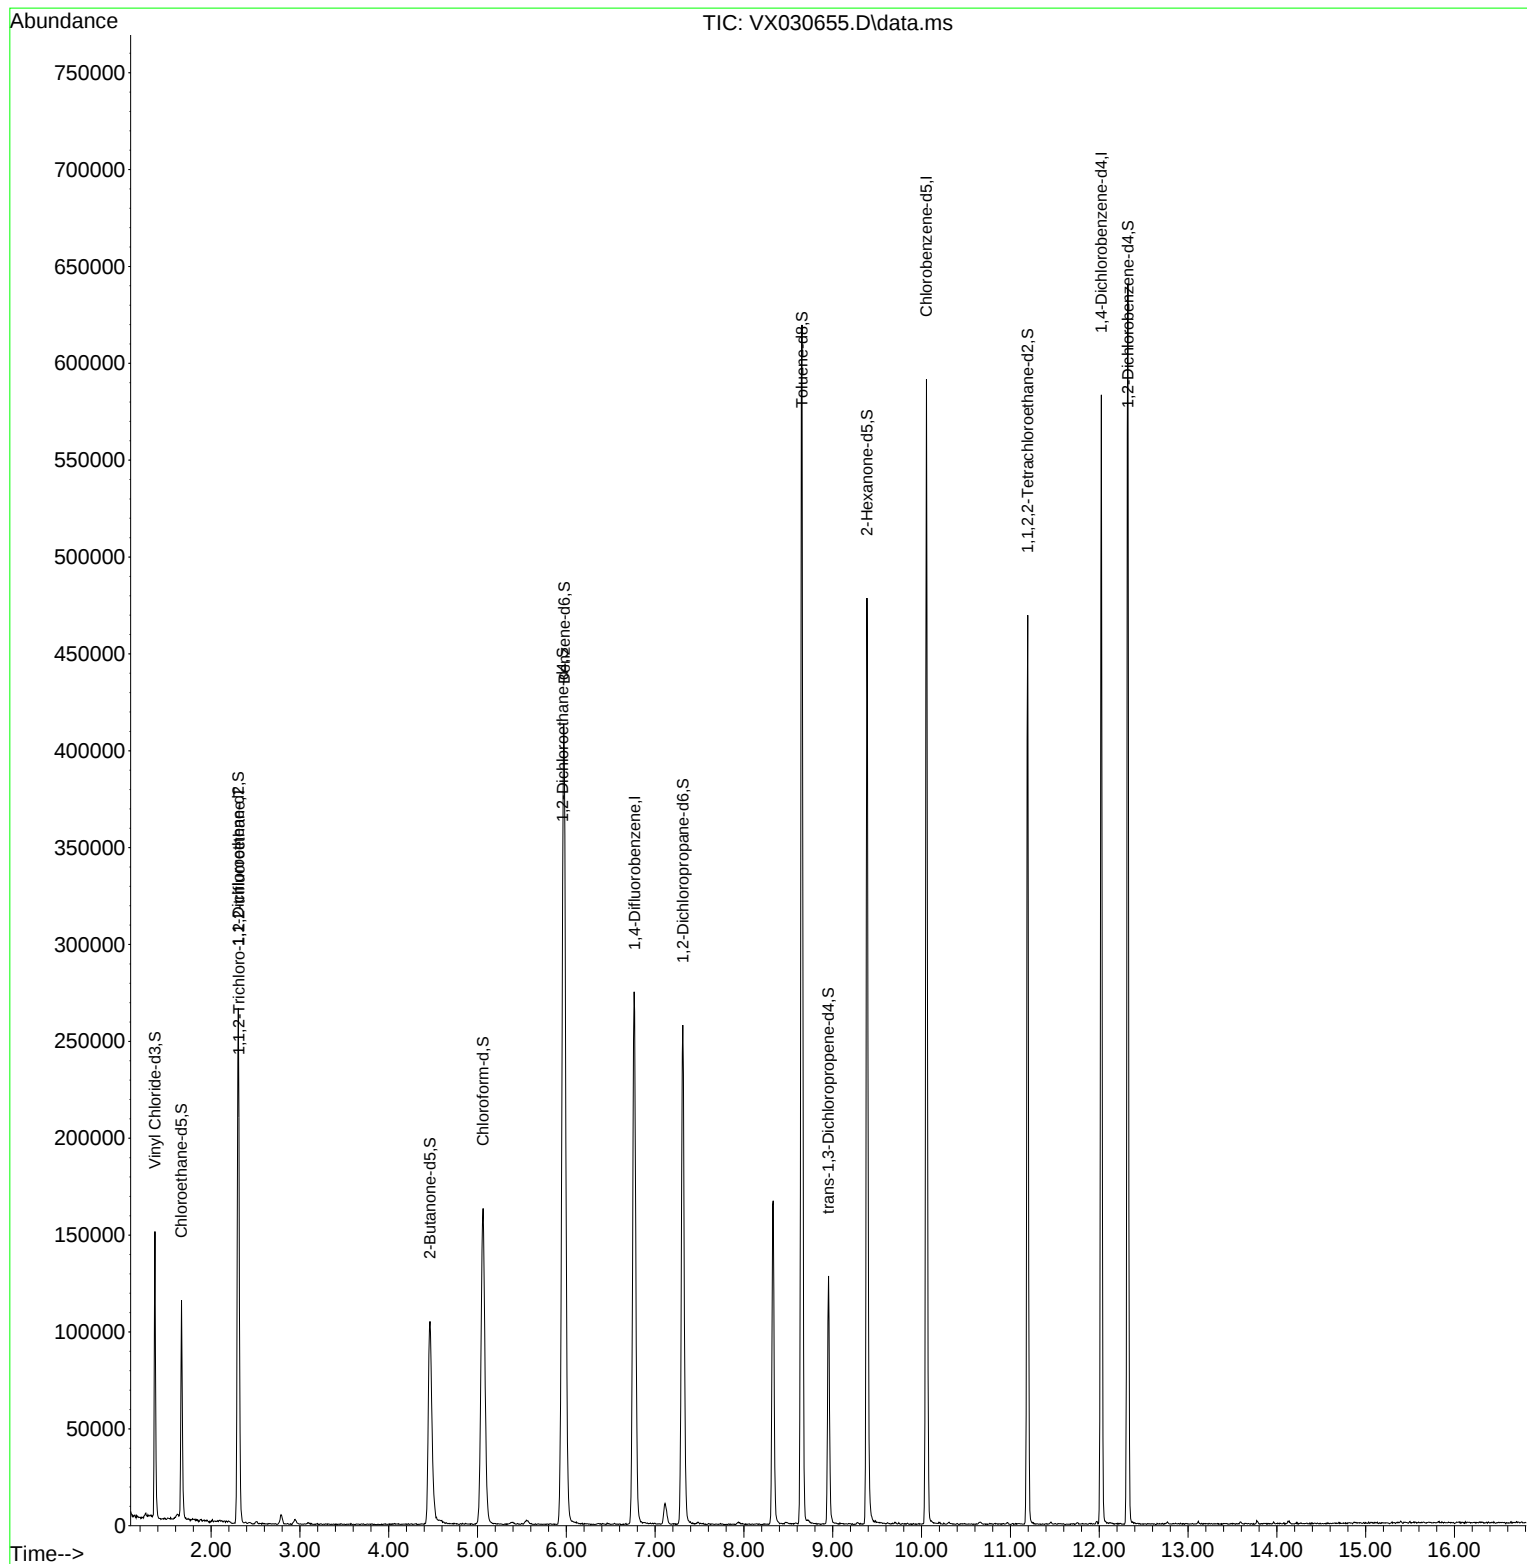

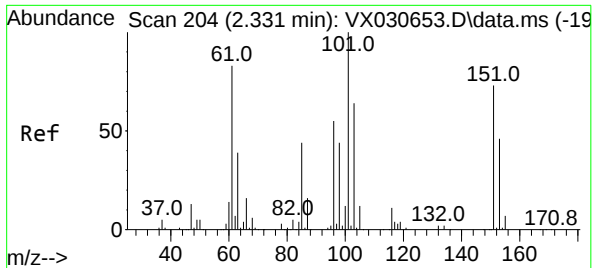

#10
1,1,2-Trichloro-1,2,2-trifluoroethane
Concen: 0.934 ug/L
RT: 2.312 min Scan# 20
Delta R.T. -0.018 min
Lab File: VX030655.D
Acq: 17 Aug 2022 12:47

Instrument :
MSVOA_X
ClientSampleId :

Tgt Ion:101 Resp: 1582
Ion Ratio Lower Upper
101 100
85 2.5 35.3 52.9#
151 0.0 58.3 87.5#

