

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX081722\
 Data File : VX030657.D
 Acq On : 17 Aug 2022 14:05
 Operator : JC/MD
 Sample : N4221-20
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 C0KP6

Quant Time: Aug 18 04:22:13 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML080422WMA.M
 Quant Title : VOC Analysis
 QLast Update : Thu Aug 18 04:21:09 2022
 Response via : Initial Calibration

Compound	R.T. QIon		Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	6.763	114	300480	50.000	ug/L	0.00
28) Chlorobenzene-d5	10.055	117	284940	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	12.024	152	127105	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.368	65	117265	60.771	ug/L	0.00
Spiked Amount	50.000	Range 60 - 135	Recovery	= 121.540%		
7) Chloroethane-d5	1.666	69	86564	63.636	ug/L	0.00
Spiked Amount	50.000	Range 70 - 130	Recovery	= 127.280%		
11) 1,1-Dichloroethene-d2	2.306	63	177585	48.652	ug/L	0.00
Spiked Amount	50.000	Range 60 - 125	Recovery	= 97.300%		
21) 2-Butanone-d5	4.465	46	187049	104.619	ug/L	0.00
Spiked Amount	100.000	Range 40 - 130	Recovery	= 104.620%		
24) Chloroform-d	5.062	84	216898	54.604	ug/L	0.00
Spiked Amount	50.000	Range 70 - 125	Recovery	= 109.200%		
26) 1,2-Dichloroethane-d4	5.964	65	143912	53.357	ug/L	0.00
Spiked Amount	50.000	Range 70 - 125	Recovery	= 106.720%		
32) Benzene-d6	5.976	84	457558	56.060	ug/L	0.00
Spiked Amount	50.000	Range 70 - 125	Recovery	= 112.120%		
36) 1,2-Dichloropropane-d6	7.312	67	146949	55.492	ug/L	0.00
Spiked Amount	50.000	Range 70 - 120	Recovery	= 110.980%		
41) Toluene-d8	8.653	98	407934	53.022	ug/L	0.00
Spiked Amount	50.000	Range 80 - 120	Recovery	= 106.040%		
43) trans-1,3-Dichloroprop...	8.952	79	63510	48.209	ug/L	0.00
Spiked Amount	50.000	Range 60 - 125	Recovery	= 96.420%		
47) 2-Hexanone-d5	9.384	63	133816	99.138	ug/L	0.00
Spiked Amount	100.000	Range 45 - 130	Recovery	= 99.140%		
56) 1,1,2,2-Tetrachloroeth...	11.195	84	187802	53.985	ug/L	0.00
Spiked Amount	50.000	Range 65 - 120	Recovery	= 107.980%		
66) 1,2-Dichlorobenzene-d4	12.323	152	135582	54.995	ug/L	0.00
Spiked Amount	50.000	Range 80 - 120	Recovery	= 110.000%		
Target Compounds						
13) Acetone	2.392	43	4798	3.662	ug/L	Qvalue 98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX081722\
Data File : VX030657.D
Acq On : 17 Aug 2022 14:05
Operator : JC/MD
Sample : N4221-20
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
C0KP6


Quant Time: Aug 18 04:22:13 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM080422WMA.M
Quant Title : VOC Analysis
QLast Update : Thu Aug 18 04:21:09 2022
Response via : Initial Calibration

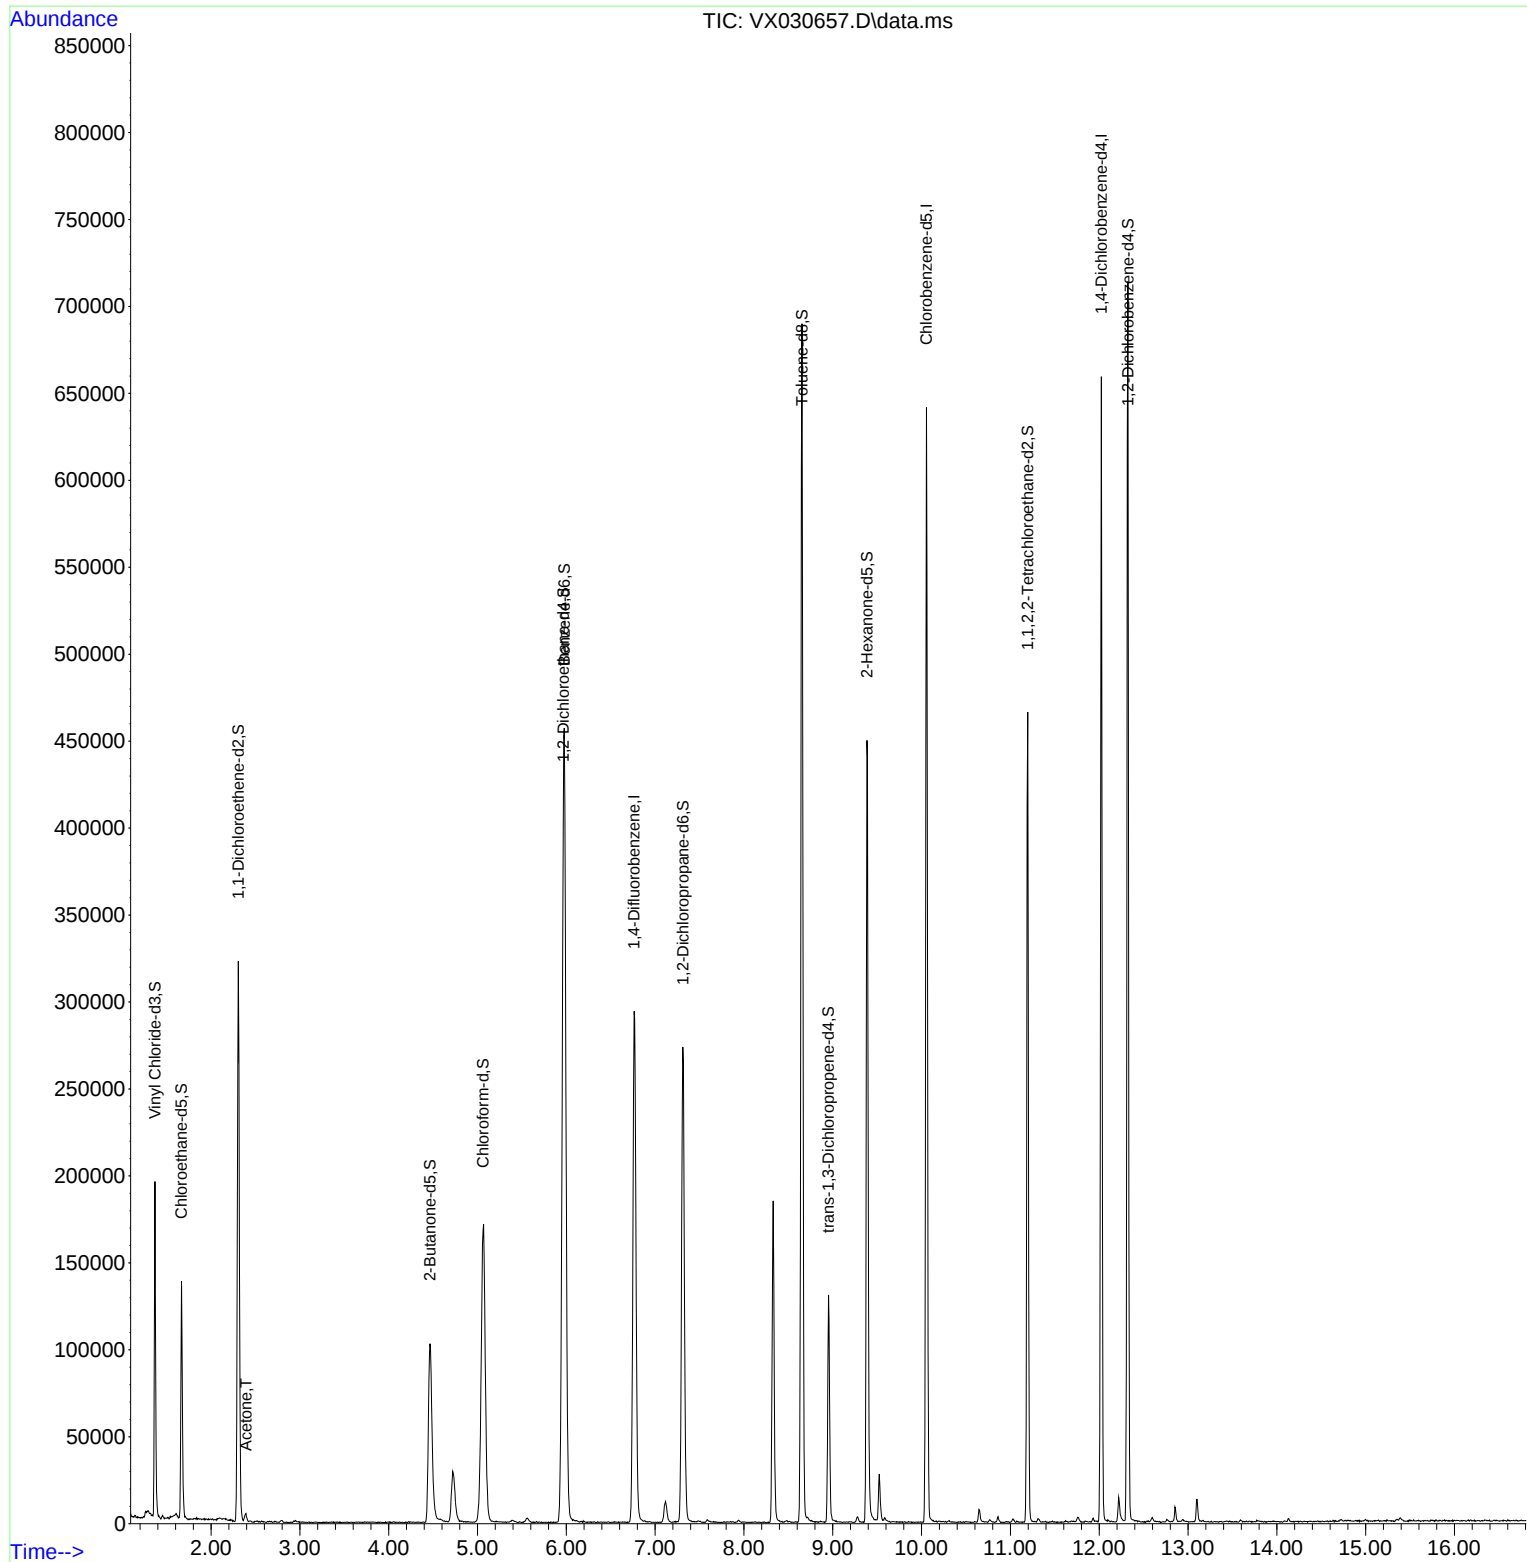

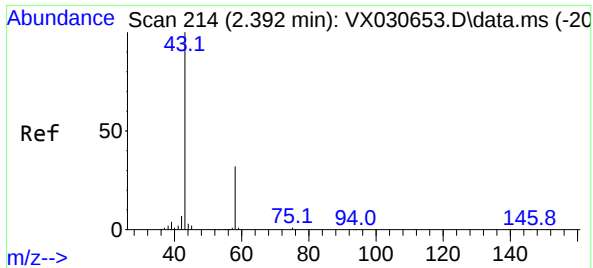

#13
 Acetone
 Concen: 3.662 ug/L
 RT: 2.392 min Scan# 214
 Delta R.T. 0.000 min
 Lab File: VX030657.D
 Acq: 17 Aug 2022 14:05

Instrument :
 MSVOA_X
 ClientSampleId :
 C0KP6

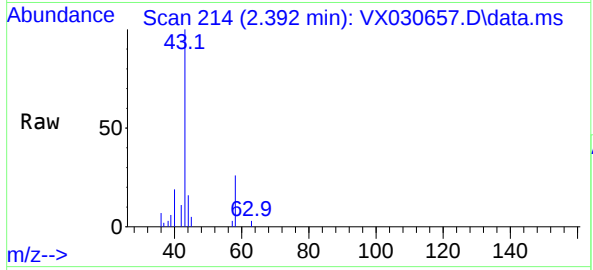

Tgt Ion: 43 Resp: 4798

Ion	Ratio	Lower	Upper
43	100		
58	30.1	0.0	57.8

