

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX081722\
 Data File : VX030658.D
 Acq On : 17 Aug 2022 14:28
 Operator : JC/MD
 Sample : N4231-03
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 C0KQ4

Quant Time: Aug 18 04:22:25 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML080422WMA.M
 Quant Title : VOC Analysis
 QLast Update : Thu Aug 18 04:21:09 2022
 Response via : Initial Calibration

Compound	R.T. QIon		Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	6.769	114	293256	50.000	ug/L	0.00
28) Chlorobenzene-d5	10.055	117	268132	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	12.024	152	120563	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.368	65	118950	63.162	ug/L	0.00
Spiked Amount 50.000	Range 60	- 135	Recovery	=	126.320%	
7) Chloroethane-d5	1.666	69	86975	65.514	ug/L	0.00
Spiked Amount 50.000	Range 70	- 130	Recovery	=	131.020%#	
11) 1,1-Dichloroethene-d2	2.306	63	178259	50.040	ug/L	0.00
Spiked Amount 50.000	Range 60	- 125	Recovery	=	100.080%	
21) 2-Butanone-d5	4.465	46	189988	108.881	ug/L	0.00
Spiked Amount 100.000	Range 40	- 130	Recovery	=	108.880%	
24) Chloroform-d	5.068	84	221069	57.025	ug/L	0.00
Spiked Amount 50.000	Range 70	- 125	Recovery	=	114.040%	
26) 1,2-Dichloroethane-d4	5.958	65	144149	54.762	ug/L	0.00
Spiked Amount 50.000	Range 70	- 125	Recovery	=	109.520%	
32) Benzene-d6	5.983	84	457489	59.565	ug/L	0.00
Spiked Amount 50.000	Range 70	- 125	Recovery	=	119.120%	
36) 1,2-Dichloropropane-d6	7.312	67	146840	58.927	ug/L	0.00
Spiked Amount 50.000	Range 70	- 120	Recovery	=	117.860%	
41) Toluene-d8	8.653	98	409514	56.564	ug/L	0.00
Spiked Amount 50.000	Range 80	- 120	Recovery	=	113.120%	
43) trans-1,3-Dichloroprop...	8.952	79	63681	51.369	ug/L	0.00
Spiked Amount 50.000	Range 60	- 125	Recovery	=	102.740%	
47) 2-Hexanone-d5	9.384	63	138367	108.936	ug/L	0.00
Spiked Amount 100.000	Range 45	- 130	Recovery	=	108.940%	
56) 1,1,2,2-Tetrachloroeth...	11.195	84	182953	55.888	ug/L	0.00
Spiked Amount 50.000	Range 65	- 120	Recovery	=	111.780%	
66) 1,2-Dichlorobenzene-d4	12.323	152	138686	59.307	ug/L	0.00
Spiked Amount 50.000	Range 80	- 120	Recovery	=	118.620%	
Target Compounds						
13) Acetone	2.386	43	4575	3.577	ug/L	Qvalue 93


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX081722\
Data File : VX030658.D
Acq On : 17 Aug 2022 14:28
Operator : JC/MD
Sample : N4231-03
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
C0KQ4


Quant Time: Aug 18 04:22:25 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML080422WMA.M
Quant Title : VOC Analysis
QLast Update : Thu Aug 18 04:21:09 2022
Response via : Initial Calibration

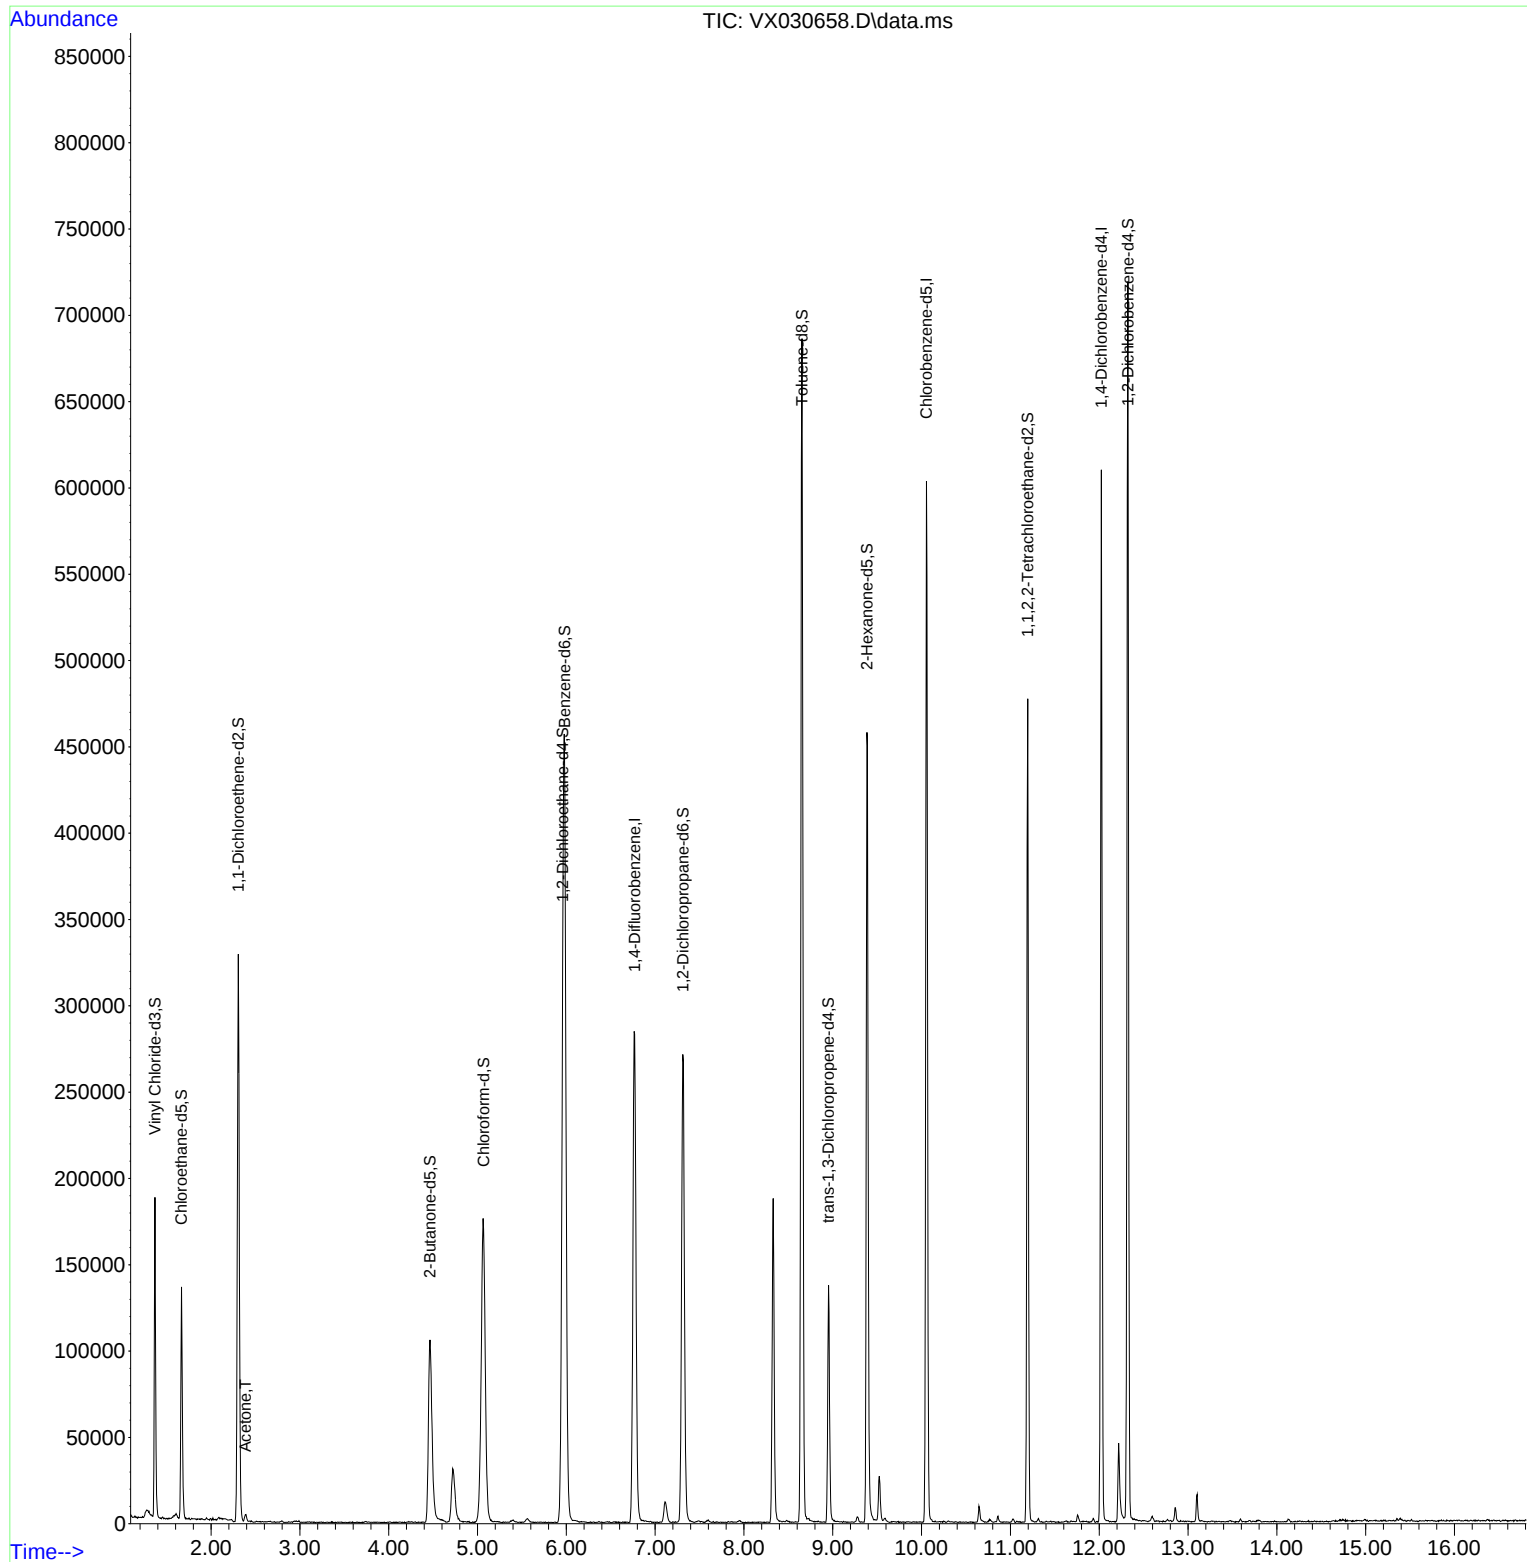

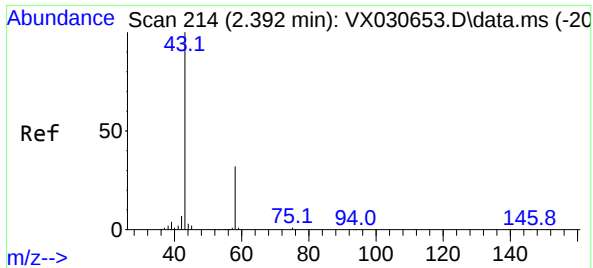

#13
Acetone
Concen: 3.577 ug/L
RT: 2.386 min Scan# 21
Delta R.T. -0.006 min
Lab File: VX030658.D
Acq: 17 Aug 2022 14:28

Instrument :
MSVOA_X
ClientSampleId :
C0KQ4

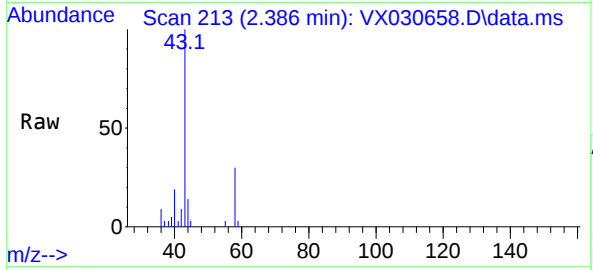

Tgt Ion: 43 Resp: 4575

Ion	Ratio	Lower	Upper
43	100		
58	32.5	0.0	57.8

