

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX081722\
 Data File : VX030671.D
 Acq On : 17 Aug 2022 19:32
 Operator : JC/MD
 Sample : N4221-05ME
 Misc : 5.03g/5mL/100uL/5.00mL/MSVOA_X/MEOH
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 C0KP7ME

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML080422WMA.M
 Title : VOC Analysis

Signal : TIC: VX030671.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.258	25	28	32	rBV2	8575	12995	0.83%	0.112%
2	1.368	42	46	56	rVB	161101	215603	13.74%	1.866%
3	1.654	90	93	99	rVB	55650	68913	4.39%	0.596%
4	2.276	189	195	207	rBV	351327	557578	35.53%	4.826%
5	2.642	253	255	256	rBV2	788	394	0.03%	0.003%
6	2.782	273	278	284	rVB2	5769	10850	0.69%	0.094%
7	2.953	298	306	312	rBV2	12231	33231	2.12%	0.288%
8	3.245	352	354	358	rBV2	349	521	0.03%	0.005%
9	3.422	381	383	388	rVB3	945	1302	0.08%	0.011%
10	3.513	397	398	400	rVB	537	355	0.02%	0.003%
11	3.648	417	420	423	rVB2	552	725	0.05%	0.006%
12	3.678	423	425	426	rBV	413	405	0.03%	0.004%
13	3.794	442	444	446	rVB2	505	323	0.02%	0.003%
14	3.995	475	477	480	rVV2	440	508	0.03%	0.004%
15	4.056	485	487	489	rBV	359	319	0.02%	0.003%
16	4.495	549	559	585	rBV	76563	334271	21.30%	2.893%
17	4.794	606	608	613	rVB2	1124	1058	0.07%	0.009%
18	5.062	641	652	669	rVB	197646	617649	39.35%	5.346%
19	5.263	683	685	687	rBV2	398	359	0.02%	0.003%
20	5.440	712	714	717	rBV2	312	421	0.03%	0.004%
21	5.611	740	742	745	rVB2	802	703	0.04%	0.006%
22	5.647	745	748	749	rBV	367	391	0.02%	0.003%
23	5.855	780	782	784	rVB	675	477	0.03%	0.004%
24	5.970	787	801	816	rBV3	561929	1569483	100.00%	13.585%
25	6.367	857	866	879	rBV3	8038	25038	1.60%	0.217%
26	6.476	882	884	887	rVB3	788	782	0.05%	0.007%
27	6.568	897	899	902	rBV3	542	562	0.04%	0.005%
28	6.763	921	931	948	rBV	359862	874919	55.75%	7.573%
29	7.123	981	990	1000	rBV4	51382	130420	8.31%	1.129%
30	7.312	1013	1021	1033	rVB	313578	688626	43.88%	5.960%
31	7.446	1041	1043	1045	rBV	550	665	0.04%	0.006%
32	7.562	1060	1062	1063	rVB2	555	338	0.02%	0.003%
33	7.610	1066	1070	1075	rBV	551	819	0.05%	0.007%
34	7.842	1107	1108	1111	rVB	545	448	0.03%	0.004%
35	7.866	1111	1112	1115	rBV2	307	372	0.02%	0.003%
36	7.964	1119	1128	1136	rBV7	5180	13368	0.85%	0.116%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX081722\
 Data File : VX030671.D
 Acq On : 17 Aug 2022 19:32
 Operator : JC/MD
 Sample : N4221-05ME
 Misc : 5.03g/5mL/100uL/5.00mL/MSVOA_X/MEOH
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 C0KP7ME

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML080422WMA.M
 Title : VOC Analysis

37	8.043	1139	1141	1142	rBV	874	683	0.04%	0.006%
38	8.183	1162	1164	1165	rBV	467	321	0.02%	0.003%
39	8.202	1165	1167	1168	rVB	492	355	0.02%	0.003%
40	8.330	1181	1188	1200	rBV	197801	326827	20.82%	2.829%
41	8.446	1205	1207	1209	rBV	548	508	0.03%	0.004%
42	8.476	1210	1212	1217	rBV6	1025	1434	0.09%	0.012%
43	8.586	1228	1230	1232	rBV2	537	472	0.03%	0.004%
44	8.653	1234	1241	1254	rVV	808096	1290785	82.24%	11.172%
45	8.756	1254	1258	1272	rVB3	6638	17047	1.09%	0.148%
46	8.915	1280	1284	1285	rBV2	700	673	0.04%	0.006%
47	8.952	1285	1290	1300	rVV	134371	211527	13.48%	1.831%
48	9.043	1304	1305	1310	rVB3	834	626	0.04%	0.005%
49	9.110	1314	1316	1320	rVB4	1829	2250	0.14%	0.019%
50	9.275	1337	1343	1351	rVB2	43436	67729	4.32%	0.586%
51	9.348	1351	1355	1356	rBV2	562	713	0.05%	0.006%
52	9.403	1357	1364	1379	rVV	353209	711665	45.34%	6.160%
53	9.537	1383	1386	1393	rVB2	5460	8819	0.56%	0.076%
54	9.726	1411	1417	1423	rBV4	5564	11752	0.75%	0.102%
55	10.055	1465	1471	1480	rBV	730011	1000920	63.77%	8.663%
56	10.214	1496	1497	1501	rBV3	899	945	0.06%	0.008%
57	10.281	1507	1508	1510	rBV	463	455	0.03%	0.004%
58	10.366	1517	1522	1524	rBV2	573	1018	0.06%	0.009%
59	10.640	1564	1567	1568	rBV	463	501	0.03%	0.004%
60	11.000	1625	1626	1628	rBV2	378	331	0.02%	0.003%
61	11.085	1635	1640	1641	rBV2	1634	1999	0.13%	0.017%
62	11.195	1651	1658	1665	rBV	488802	680666	43.37%	5.892%
63	11.311	1674	1677	1681	rVB2	1027	1541	0.10%	0.013%
64	11.402	1690	1692	1693	rBV	473	340	0.02%	0.003%
65	11.439	1697	1698	1701	rVV2	818	905	0.06%	0.008%
66	11.482	1701	1705	1710	rVB3	4051	5063	0.32%	0.044%
67	11.549	1714	1716	1719	rVB2	498	498	0.03%	0.004%
68	11.591	1719	1723	1727	rBV	402	784	0.05%	0.007%
69	11.634	1727	1730	1735	rBV4	1152	1481	0.09%	0.013%
70	11.677	1735	1737	1740	rVV2	614	582	0.04%	0.005%
71	11.713	1741	1743	1748	rVB4	1433	1420	0.09%	0.012%
72	11.762	1748	1751	1755	rBV2	996	1436	0.09%	0.012%
73	11.939	1777	1780	1781	rBV2	356	405	0.03%	0.004%
74	12.024	1789	1794	1806	rBV	755677	950670	60.57%	8.229%
75	12.250	1827	1831	1834	rBV2	724	1193	0.08%	0.010%
76	12.323	1837	1843	1852	rBV	856049	1067328	68.01%	9.238%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX081722\
 Data File : VX030671.D
 Acq On : 17 Aug 2022 19:32
 Operator : JC/MD
 Sample : N4221-05ME
 Misc : 5.03g/5mL/100uL/5.00mL/MSVOA_X/MEOH
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 C0KP7ME

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML080422WMA.M
 Title : VOC Analysis

77	12.518	1874	1875	1876	rBV	601	316	0.02%	0.003%
78	12.561	1880	1882	1885	rVV3	525	600	0.04%	0.005%
79	12.585	1885	1886	1887	rVV	671	317	0.02%	0.003%
80	12.603	1887	1889	1892	rVB	689	581	0.04%	0.005%
81	12.872	1929	1933	1936	rBV4	841	1063	0.07%	0.009%
82	13.036	1958	1960	1964	rBV2	592	513	0.03%	0.004%
83	13.115	1971	1973	1977	rVB	726	526	0.03%	0.005%
84	13.164	1979	1981	1984	rVB2	596	651	0.04%	0.006%
85	13.213	1986	1989	1991	rBV	564	501	0.03%	0.004%
86	13.311	2002	2005	2006	rVB2	403	345	0.02%	0.003%
87	13.329	2006	2008	2010	rBV2	321	333	0.02%	0.003%
88	13.347	2010	2011	2014	rBV	378	442	0.03%	0.004%
89	13.414	2021	2022	2027	rVB2	656	454	0.03%	0.004%
90	13.756	2076	2078	2081	rBV	460	341	0.02%	0.003%
91	13.792	2081	2084	2085	rBV	486	470	0.03%	0.004%
92	13.908	2101	2103	2105	rBV	478	433	0.03%	0.004%
93	13.951	2108	2110	2112	rBV2	555	534	0.03%	0.005%
94	14.066	2128	2129	2133	rBV2	512	594	0.04%	0.005%
95	14.103	2133	2135	2136	rBV	636	397	0.03%	0.003%
96	14.134	2137	2140	2144	rVB3	1631	2237	0.14%	0.019%
97	14.451	2190	2192	2194	rBV	536	406	0.03%	0.004%
98	14.603	2215	2217	2218	rBV	610	373	0.02%	0.003%
99	14.969	2276	2277	2279	rBV2	1097	544	0.03%	0.005%
100	16.328	2499	2500	2502	rVB2	995	473	0.03%	0.004%




Sum of corrected areas: 11553302

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX081722\
Data File : VX030671.D
Acq On : 17 Aug 2022 19:32
Operator : JC/MD
Sample : N4221-05ME
Misc : 5.03g/5mL/100uL/5.00mL/MSVOA_X/MEOH
ALS Vial : 20 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
C0KP7ME

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML080422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

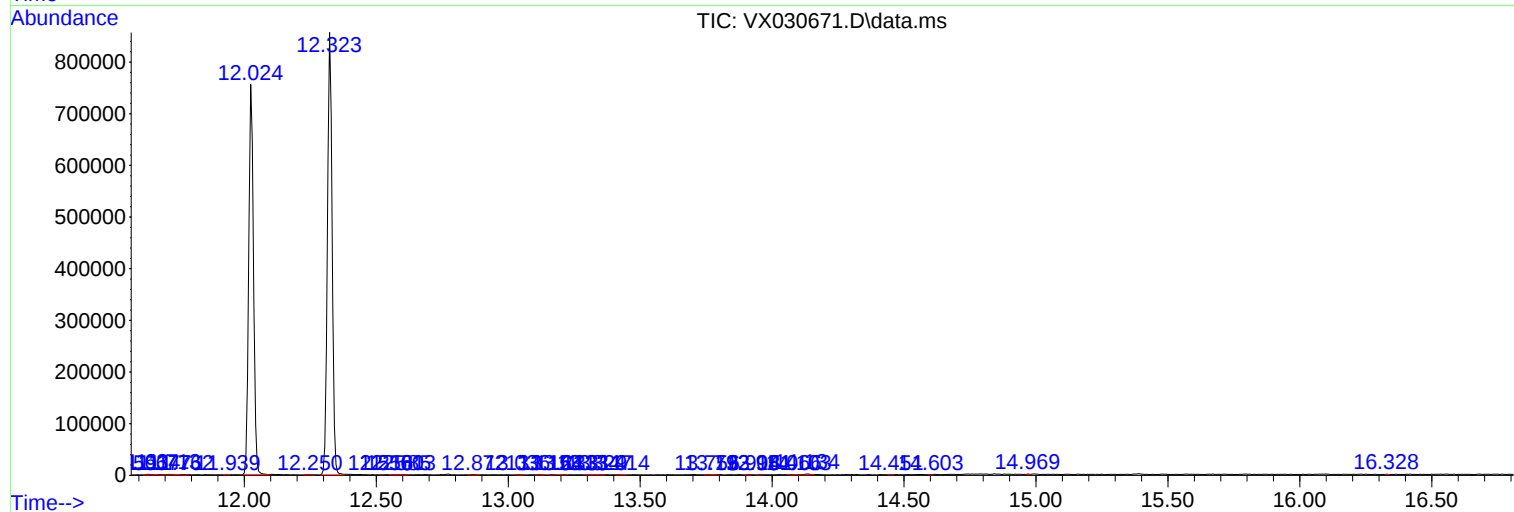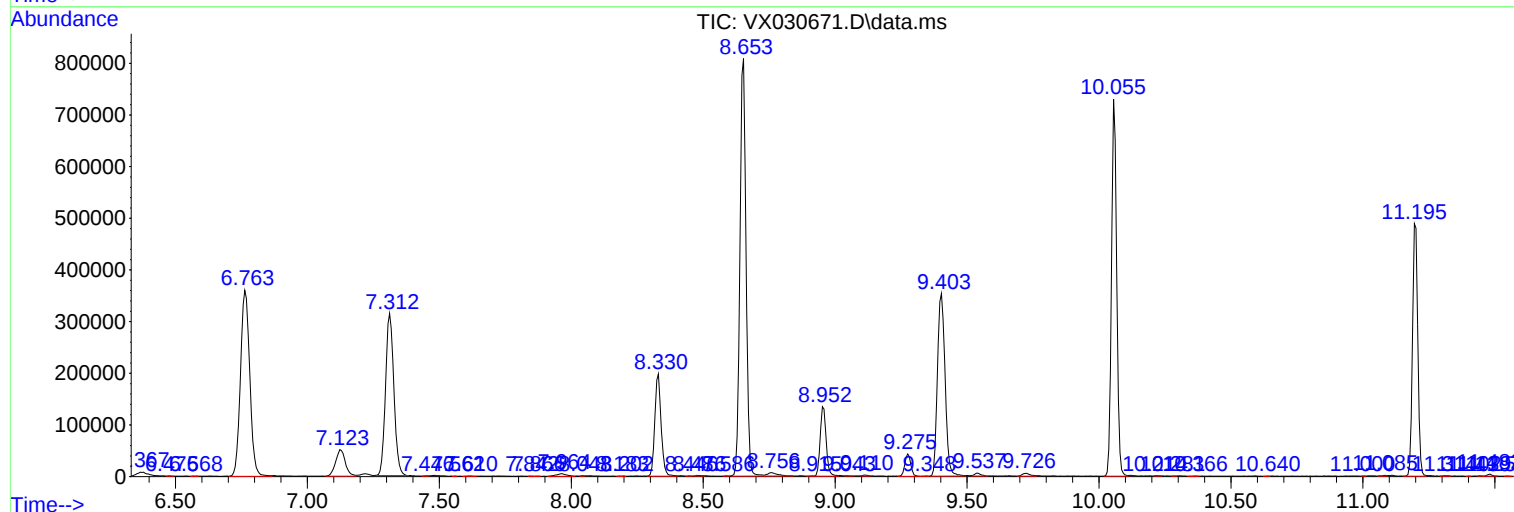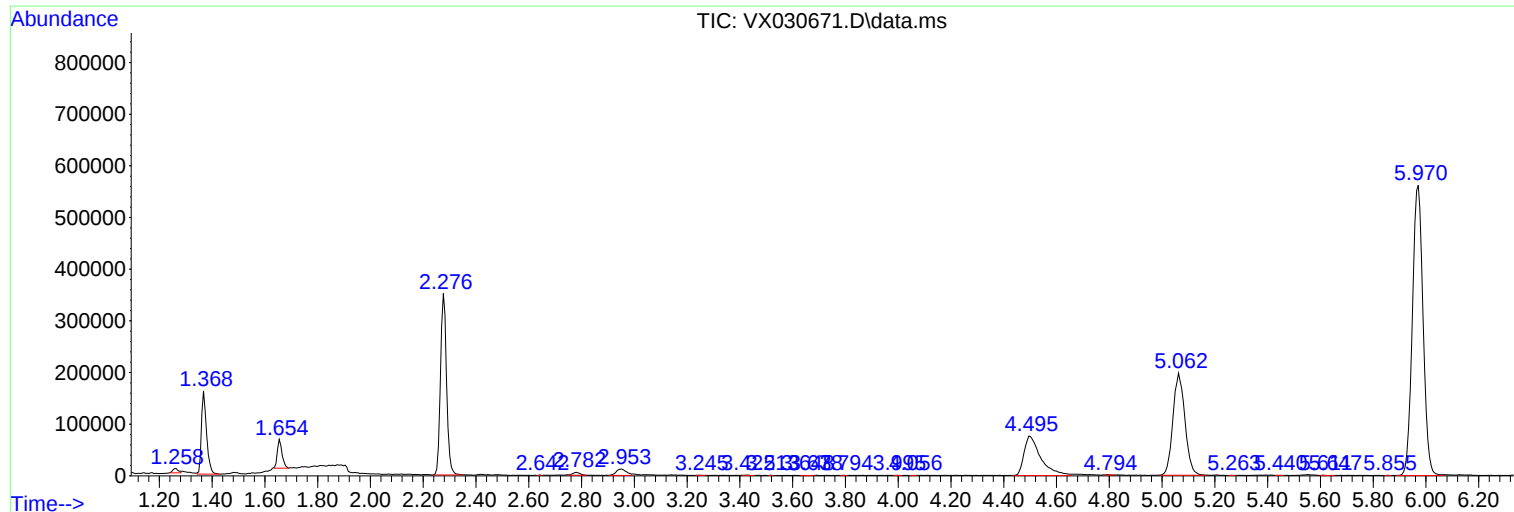

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX081722\
Data File : VX030671.D
Acq On : 17 Aug 2022 19:32
Operator : JC/MD
Sample : N4221-05ME
Misc : 5.03g/5mL/100uL/5.00mL/MSVOA_X/MEOH
ALS Vial : 20 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
C0KP7ME

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML080422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX081722\
Data File : VX030671.D
Acq On : 17 Aug 2022 19:32
Operator : JC/MD
Sample : N4221-05ME
Misc : 5.03g/5mL/100uL/5.00mL/MSVOA_X/MEOH
ALS Vial : 20 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
C0KP7ME

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML080422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc