

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX081722\
 Data File : VX030672.D
 Acq On : 17 Aug 2022 19:56
 Operator : JC/MD
 Sample : N4221-06ME
 Misc : 5.07g/5mL/100uL/5.00mL/MSVOA_X/MEOH
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 C0KP8ME

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML080422WMA.M

Title : VOC Analysis

Signal : TIC: VX030672.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.367	42	46	57	rVB	162052	209023	13.91%	1.920%
2	1.654	90	93	101	rBV	54716	71686	4.77%	0.658%
3	2.276	189	195	209	rVB	339921	536988	35.73%	4.932%
4	2.398	213	215	216	rBV2	824	725	0.05%	0.007%
5	2.776	273	277	286	rVB3	6358	13956	0.93%	0.128%
6	2.953	298	306	317	rBV2	17345	49951	3.32%	0.459%
7	3.324	366	367	369	rBV2	354	299	0.02%	0.003%
8	3.416	379	382	385	rBV2	988	1187	0.08%	0.011%
9	3.641	417	419	421	rBV	308	376	0.03%	0.003%
10	3.715	429	431	435	rVB2	438	519	0.03%	0.005%
11	3.751	435	437	440	rBV2	511	530	0.04%	0.005%
12	3.782	440	442	446	rVB	300	365	0.02%	0.003%
13	3.824	446	449	451	rBV2	421	574	0.04%	0.005%
14	3.879	456	458	461	rBV2	538	816	0.05%	0.007%
15	3.922	463	465	467	rVB	440	357	0.02%	0.003%
16	4.032	481	483	486	rVB2	457	460	0.03%	0.004%
17	4.117	495	497	498	rVB	694	366	0.02%	0.003%
18	4.495	549	559	585	rBV2	70086	314521	20.93%	2.889%
19	5.062	641	652	668	rVB	189520	580991	38.66%	5.336%
20	5.214	675	677	680	rVB2	748	536	0.04%	0.005%
21	5.342	695	698	699	rVB2	383	298	0.02%	0.003%
22	5.476	717	720	723	rBV	462	410	0.03%	0.004%
23	5.525	726	728	729	rBV	1023	941	0.06%	0.009%
24	5.720	758	760	762	rBV	372	238	0.02%	0.002%
25	5.879	785	786	788	rBV	576	554	0.04%	0.005%
26	5.964	788	800	819	rVV2	538425	1502765	100.00%	13.803%
27	6.135	827	828	829	rBV	685	294	0.02%	0.003%
28	6.208	836	840	841	rBV	427	494	0.03%	0.005%
29	6.239	844	845	848	rVB2	436	295	0.02%	0.003%
30	6.373	858	867	879	rBV4	8398	26443	1.76%	0.243%
31	6.598	902	904	906	rBV	461	353	0.02%	0.003%
32	6.677	915	917	919	rBV2	299	363	0.02%	0.003%
33	6.763	921	931	953	rVV	336933	814453	54.20%	7.481%
34	6.964	963	964	966	rBV2	624	310	0.02%	0.003%
35	7.123	980	990	1000	rBV5	42774	108877	7.25%	1.000%
36	7.220	1001	1006	1012	rVV5	4411	10327	0.69%	0.095%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX081722\
 Data File : VX030672.D
 Acq On : 17 Aug 2022 19:56
 Operator : JC/MD
 Sample : N4221-06ME
 Misc : 5.07g/5mL/100uL/5.00mL/MSVOA_X/MEOH
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 C0KP8ME

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML080422WMA.M
 Title : VOC Analysis

37	7.312	1012	1021	1033	rVV	303762	657105	43.73%	6.036%
38	7.476	1045	1048	1050	rBV3	1252	1578	0.11%	0.014%
39	7.525	1054	1056	1059	rVB	810	656	0.04%	0.006%
40	7.866	1109	1112	1113	rBV	545	494	0.03%	0.005%
41	7.964	1119	1128	1139	rVB8	4839	13077	0.87%	0.120%
42	8.037	1139	1140	1141	rBV	867	516	0.03%	0.005%
43	8.244	1171	1174	1177	rBV3	831	1020	0.07%	0.009%
44	8.330	1180	1188	1200	rBV	182841	308209	20.51%	2.831%
45	8.470	1209	1211	1212	rBV2	608	630	0.04%	0.006%
46	8.598	1230	1232	1233	rBV2	492	365	0.02%	0.003%
47	8.653	1234	1241	1253	rVV	778141	1220833	81.24%	11.213%
48	8.756	1255	1258	1272	rVB4	7395	18243	1.21%	0.168%
49	8.915	1282	1284	1285	rBV2	379	361	0.02%	0.003%
50	8.951	1285	1290	1301	rVV	130920	199761	13.29%	1.835%
51	9.110	1313	1316	1323	rVB5	1881	3203	0.21%	0.029%
52	9.275	1338	1343	1351	rBV2	40008	59271	3.94%	0.544%
53	9.403	1357	1364	1376	rBV	324162	661395	44.01%	6.075%
54	9.537	1383	1386	1393	rVB4	5427	7600	0.51%	0.070%
55	9.659	1404	1406	1411	rVB4	747	1088	0.07%	0.010%
56	9.726	1412	1417	1428	rVB5	2975	6358	0.42%	0.058%
57	9.927	1448	1450	1454	rVB	476	477	0.03%	0.004%
58	10.055	1465	1471	1485	rBV	698595	940085	62.56%	8.635%
59	10.299	1508	1511	1517	rBV3	808	1795	0.12%	0.016%
60	10.360	1517	1521	1526	rVV3	534	1112	0.07%	0.010%
61	10.500	1542	1544	1545	rBV2	395	284	0.02%	0.003%
62	10.524	1545	1548	1550	rVV2	533	618	0.04%	0.006%
63	10.567	1553	1555	1556	rVB	436	280	0.02%	0.003%
64	10.646	1566	1568	1570	rBV2	467	456	0.03%	0.004%
65	10.701	1575	1577	1578	rVV	500	359	0.02%	0.003%
66	10.732	1581	1582	1583	rVV	506	239	0.02%	0.002%
67	10.768	1586	1588	1589	rVB2	475	272	0.02%	0.002%
68	10.787	1589	1591	1593	rVB	655	592	0.04%	0.005%
69	10.811	1593	1595	1598	rBV	559	564	0.04%	0.005%
70	10.896	1607	1609	1610	rVB	605	327	0.02%	0.003%
71	10.945	1615	1617	1618	rBV2	370	353	0.02%	0.003%
72	10.994	1623	1625	1626	rVB	372	241	0.02%	0.002%
73	11.030	1628	1631	1634	rBV2	662	792	0.05%	0.007%
74	11.146	1647	1650	1651	rBV2	589	657	0.04%	0.006%
75	11.195	1653	1658	1666	rVB	467447	641882	42.71%	5.896%
76	11.384	1688	1689	1691	rVB2	656	347	0.02%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX081722\
 Data File : VX030672.D
 Acq On : 17 Aug 2022 19:56
 Operator : JC/MD
 Sample : N4221-06ME
 Misc : 5.07g/5mL/100uL/5.00mL/MSVOA_X/MEOH
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 C0KP8ME

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML080422WMA.M
 Title : VOC Analysis

77	11.433	1695	1697	1699	rBV	389	387	0.03%	0.004%
78	11.475	1701	1704	1708	rVB4	2530	3836	0.26%	0.035%
79	11.646	1727	1732	1734	rBV3	992	1340	0.09%	0.012%
80	11.713	1741	1743	1748	rVB4	930	1562	0.10%	0.014%
81	11.756	1748	1750	1752	rBV	698	613	0.04%	0.006%
82	11.884	1769	1771	1773	rBV2	609	574	0.04%	0.005%
83	11.933	1778	1779	1780	rVV	662	296	0.02%	0.003%
84	11.969	1784	1785	1789	rBV2	454	726	0.05%	0.007%
85	12.024	1789	1794	1808	rVB	703066	873278	58.11%	8.021%
86	12.323	1837	1843	1853	rBV	799179	989107	65.82%	9.085%
87	12.573	1882	1884	1887	rBV2	508	612	0.04%	0.006%
88	12.865	1928	1932	1935	rBV2	944	1074	0.07%	0.010%
89	12.957	1943	1947	1948	rBV2	530	534	0.04%	0.005%
90	13.006	1953	1955	1958	rBV2	593	591	0.04%	0.005%
91	13.073	1964	1966	1967	rBV	594	500	0.03%	0.005%
92	13.268	1997	1998	2000	rVB	611	339	0.02%	0.003%
93	13.286	2000	2001	2003	rBV	537	277	0.02%	0.003%
94	13.548	2042	2044	2046	rVB2	512	412	0.03%	0.004%
95	14.091	2131	2133	2135	rBV	579	549	0.04%	0.005%
96	14.127	2135	2139	2144	rVV3	2086	3817	0.25%	0.035%
97	14.213	2152	2153	2155	rBV2	526	304	0.02%	0.003%
98	14.304	2167	2168	2169	rBV	604	320	0.02%	0.003%
99	14.414	2184	2186	2188	rBV2	593	600	0.04%	0.006%
100	14.475	2194	2196	2199	rBV2	452	415	0.03%	0.004%

Sum of corrected areas: 10887199




Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX081722\
Data File : VX030672.D
Acq On : 17 Aug 2022 19:56
Operator : JC/MD
Sample : N4221-06ME
Misc : 5.07g/5mL/100uL/5.00mL/MSVOA_X/MEOH
ALS Vial : 21 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
C0KP8ME

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML080422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L

TIC Integration Parameters: LSCINT.P

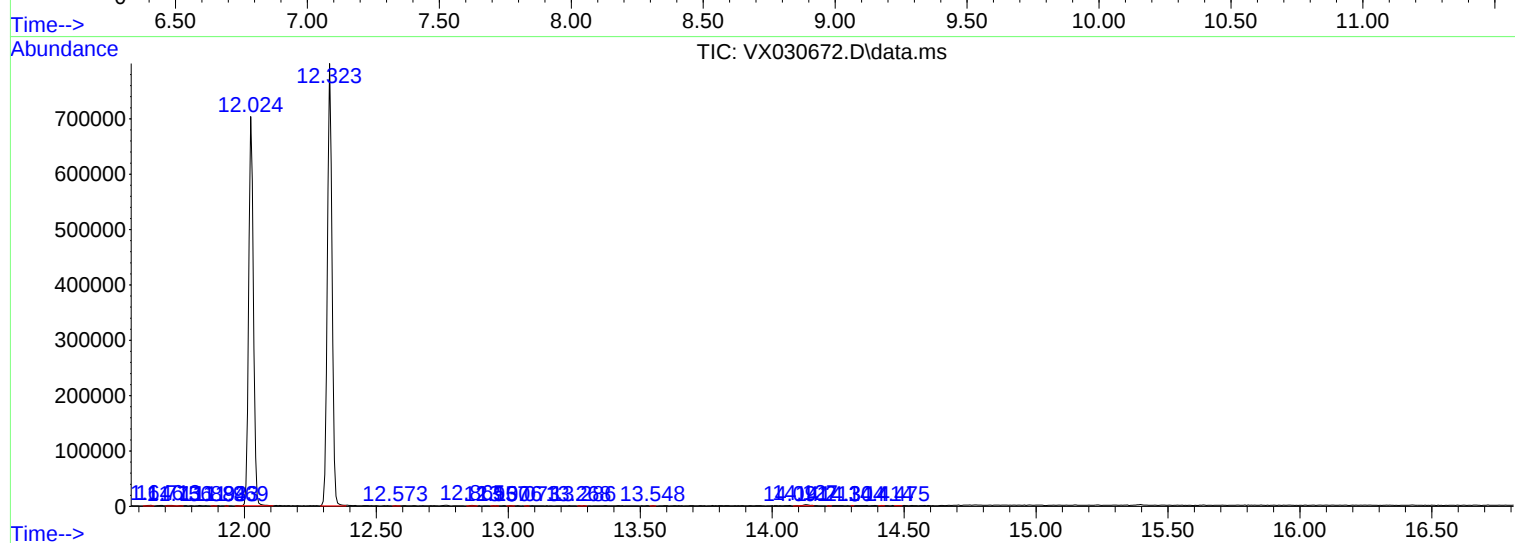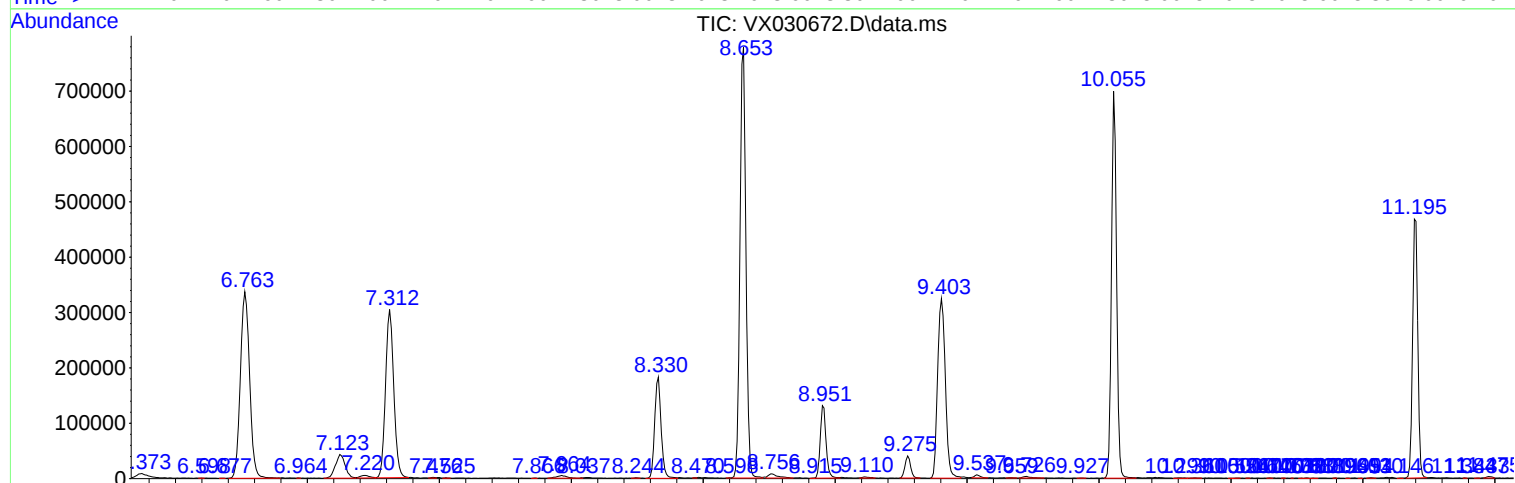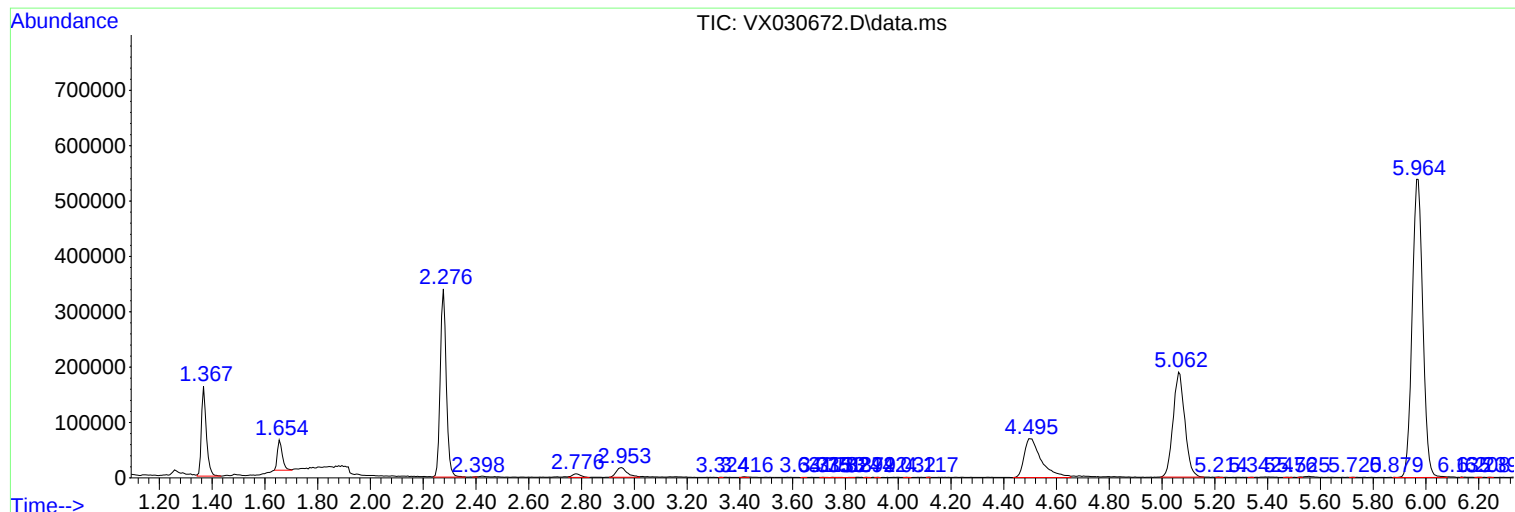

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX081722\
Data File : VX030672.D
Acq On : 17 Aug 2022 19:56
Operator : JC/MD
Sample : N4221-06ME
Misc : 5.07g/5mL/100uL/5.00mL/MSVOA_X/MEOH
ALS Vial : 21 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
C0KP8ME

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML080422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX081722\
Data File : VX030672.D
Acq On : 17 Aug 2022 19:56
Operator : JC/MD
Sample : N4221-06ME
Misc : 5.07g/5mL/100uL/5.00mL/MSVOA_X/MEOH
ALS Vial : 21 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
C0KP8ME

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML080422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc