
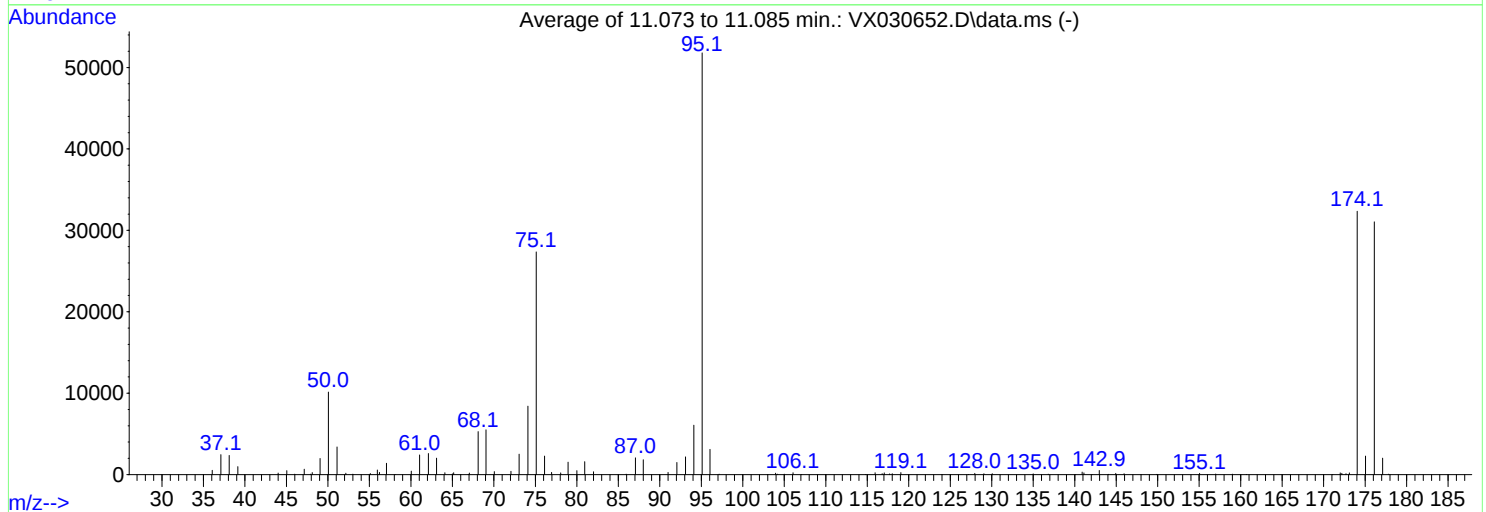


Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX081722\
 Data File : VX030652.D
 Acq On : 17 Aug 2022 10:11
 Operator : JC/MD
 Sample : BFB681
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 BFB681

Integration File: LSCINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM080422WMA.M
 Title : VOC Analysis
 Last Update : Tue Aug 23 02:05:32 2022

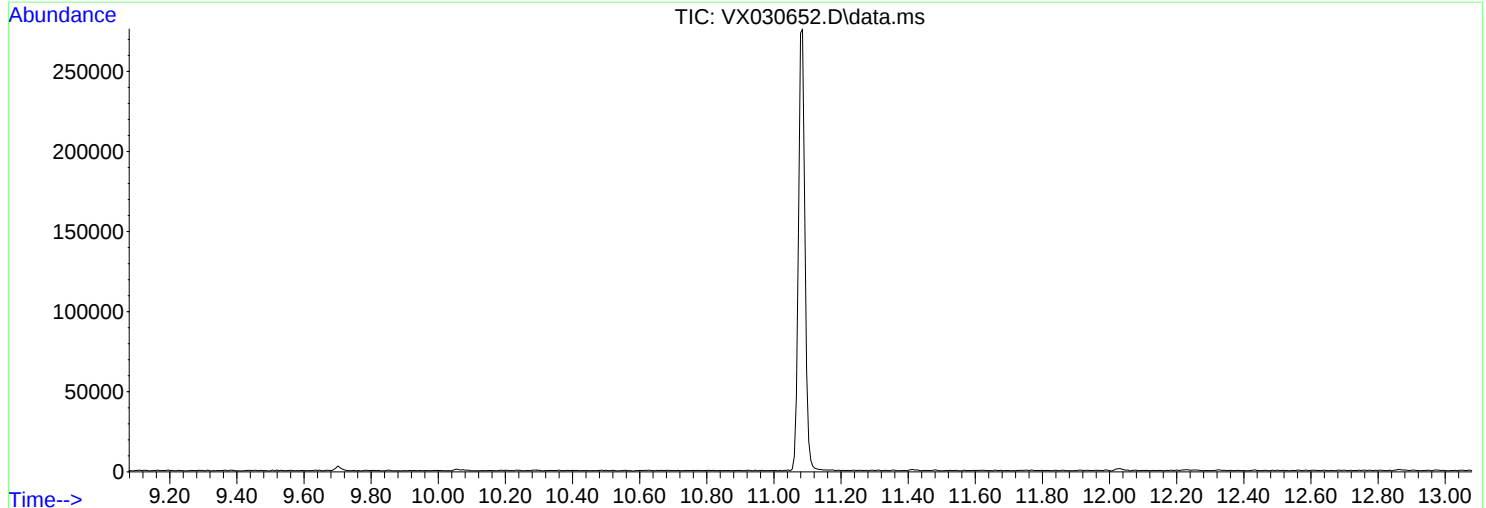

AutoFind: Scans 1638, 1639, 1640; Background Corrected with Scan 1633

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	19.6	10149	PASS
75	95	30	80	52.8	27357	PASS
95	95	100	100	100.0	51803	PASS
96	95	5	9	6.0	3112	PASS
173	174	0.00	2	0.7	220	PASS
174	95	50	120	62.5	32352	PASS
175	174	5	9	7.0	2274	PASS
176	174	95	101	96.0	31050	PASS
177	176	5	9	6.5	2028	PASS

m/z	Abundance
40.10	677.0
43.10	99.0
44.00	398.0

Instrument :
MSVOA_X
ClientSampleId :
BFB681

m/z	Abundance
36.10	438.0
37.10	1733.0
38.10	1684.0
39.20	720.0
40.00	566.0
44.10	459.0
45.00	351.0
46.00	84.0
47.10	685.0
47.90	150.0
49.00	1404.0
50.00	7494.0
51.10	2835.0
52.20	90.0
55.30	109.0
56.20	829.0
57.10	1308.0
60.10	300.0
61.00	1782.0
62.10	1600.0
63.10	1349.0
64.20	136.0
65.00	314.0
66.90	135.0
67.10	129.0
68.10	3884.0
69.00	3657.0
70.00	109.0
72.20	281.0
73.00	1346.0
74.10	5565.0
75.10	19632.0
76.10	1794.0
77.00	176.0
78.10	111.0
79.00	1082.0
80.00	328.0
80.90	1033.0
82.00	274.0
87.10	1367.0
88.00	971.0
91.10	238.0
92.00	958.0
93.10	1350.0
94.10	4045.0
95.10	34360.0
96.10	2138.0
103.90	158.0
106.00	173.0
115.90	143.0
116.80	354.0
118.00	90.0
119.10	105.0
128.00	153.0
130.10	100.0
140.90	290.0
143.00	207.0
144.10	91.0
146.10	60.0
149.90	52.0
155.10	61.0
172.00	232.0
172.70	147.0
174.00	18096.0
175.10	1311.0
176.10	16231.0
177.10	1033.0

Instrument :
MSVOA_X
ClientSampleId :
BFB681

m/z	Abundance
36.00	615.0
37.10	3220.0
38.10	2788.0
39.10	1260.0
40.10	570.0
44.00	714.0
45.10	553.0
46.00	83.0
47.20	803.0
48.10	356.0
49.00	2642.0
50.10	12071.0
51.10	3700.0
52.10	265.0
53.00	85.0
55.10	128.0
55.90	1032.0
57.00	1484.0
58.10	76.0
60.00	588.0
61.10	3119.0
62.10	3125.0
63.10	2306.0
64.20	229.0
65.20	324.0
67.00	193.0
68.10	5968.0
69.10	6891.0
70.10	530.0
72.00	603.0
73.10	3341.0
74.10	10683.0
75.10	32352.0
76.10	2572.0
76.90	327.0
78.00	281.0
79.00	1663.0
80.00	523.0
80.90	1997.0
82.00	440.0
86.00	54.0
87.00	2325.0
88.00	2392.0
90.90	228.0
92.10	1901.0
93.10	2533.0
94.10	7308.0
95.10	62576.0
96.10	3905.0
97.20	52.0
104.20	168.0
105.00	55.0
106.10	264.0
107.10	52.0
115.90	246.0
117.10	257.0
118.00	253.0
119.10	154.0
127.90	150.0
129.00	201.0
130.10	87.0
135.00	121.0
136.80	91.0
140.90	685.0
142.90	685.0
144.00	57.0
145.00	200.0
146.00	194.0
148.00	67.0
149.90	52.0
155.10	144.0
157.00	170.0
159.00	78.0
160.70	59.0
172.00	450.0
172.70	236.0
173.10	237.0
174.10	35632.0
175.00	2565.0
176.10	33968.0
177.10	2505.0
177.90	78.0

Instrument :
MSVOA_X
ClientSampleId :
BFB681

m/z	Abundance
36.00	552.0
37.10	2425.0
38.10	2582.0
39.10	992.0
40.00	573.0
44.00	608.0
45.00	555.0
47.20	537.0
48.10	388.0
49.10	1895.0
50.10	10882.0
51.10	3671.0
52.10	182.0
53.00	79.0
55.00	190.0
56.00	688.0
57.10	1409.0
60.00	433.0
61.00	2341.0
62.10	3038.0
63.10	2401.0
64.00	327.0
65.10	396.0
66.00	75.0
67.00	247.0
68.10	5989.0
69.10	5942.0
70.00	490.0
72.00	335.0
73.00	2844.0
74.10	8978.0
75.10	30088.0
76.10	2478.0
76.90	350.0
78.00	262.0
78.90	1873.0
80.00	630.0
81.00	1751.0
82.00	367.0
85.90	113.0
87.00	2514.0
88.00	2131.0
91.00	340.0
92.10	1636.0
93.10	2673.0
94.10	6892.0
95.10	58472.0
96.00	3292.0
97.10	101.0
103.00	65.0
104.00	354.0
105.00	127.0
106.00	304.0
110.00	92.0
114.80	70.0
116.00	347.0
117.00	384.0
117.70	286.0
119.00	500.0
124.00	51.0
127.20	57.0
127.90	191.0
129.10	144.0
130.00	167.0
135.00	158.0
136.80	92.0
140.10	70.0
141.10	672.0
142.10	80.0
143.00	633.0
144.90	294.0
145.80	76.0
155.00	246.0
157.00	85.0
159.00	75.0
171.10	75.0
172.20	445.0
173.10	423.0
174.10	43328.0
175.10	2946.0
176.10	42952.0
177.10	2547.0
177.80	124.0

Instrument :
MSVOA_X
ClientSampleId :
BFB681