


Data Path : Z:\voasrv\HPCHEM1\MSVOA X\Data\VX081820\
 Data File : VX017952.D
 Acq On : 18 Aug 2020 09:24
 Operator : JC/SP
 Sample : BFB71
 Misc : 25.0mL/MSVOA X/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 BFB71

Integration File: rteint.p

Method : Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\SOMXTR080720WMA.M
 Title : TRACE VOA SOM01.0
 Last Update : Wed Aug 19 03:41:34 2020

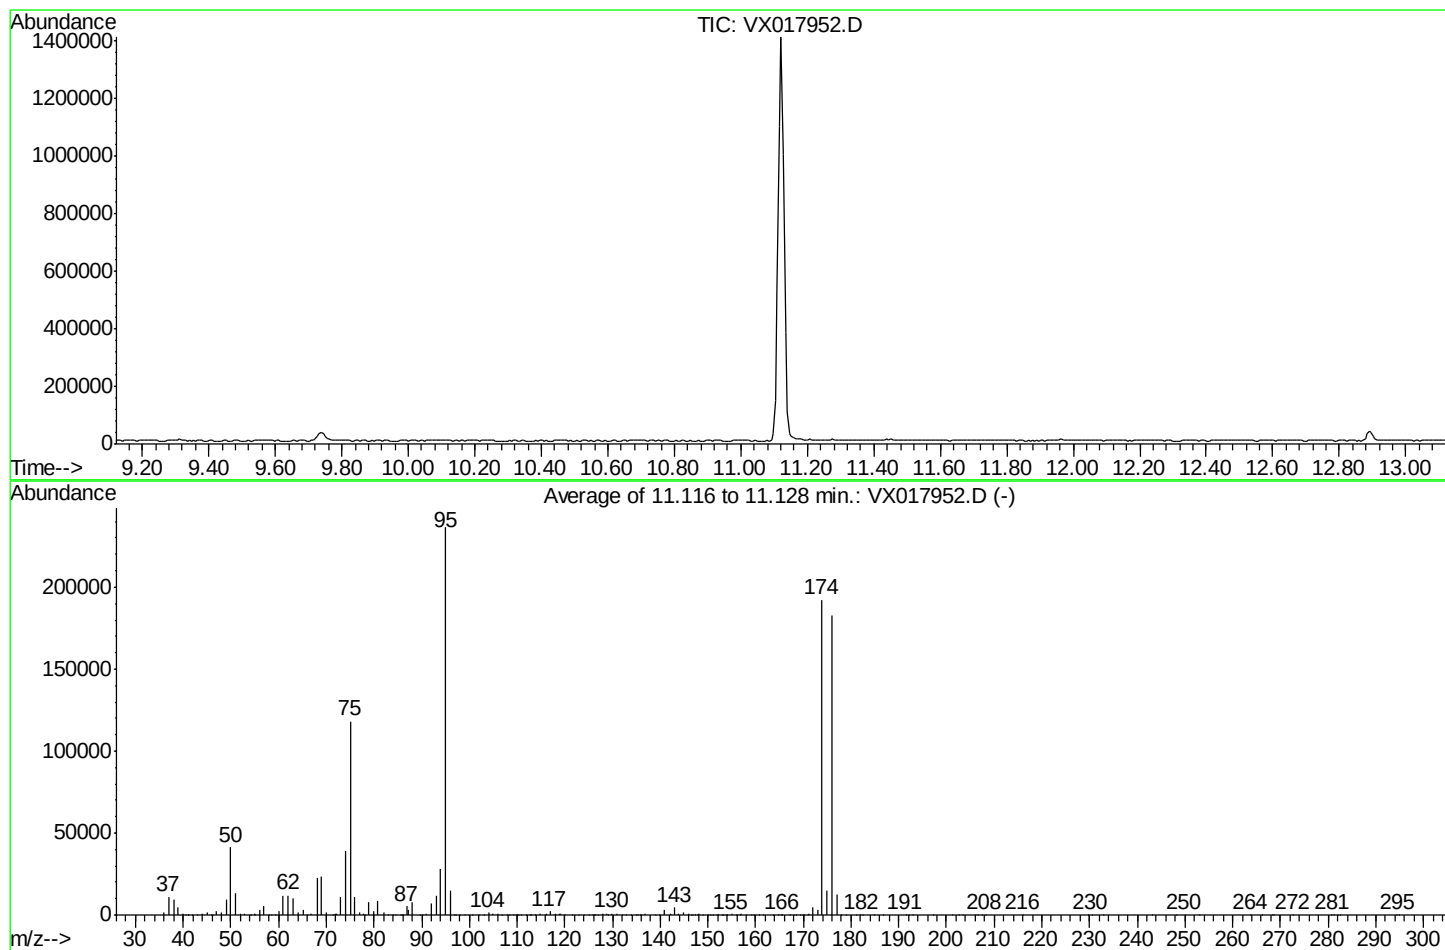

AutoFind: Scans 1645, 1646, 1647; Background Corrected with Scan 1638

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	17.4	41201	PASS
75	95	30	80	49.9	118034	PASS
95	95	100	100	100.0	236501	PASS
96	95	5	9	6.3	14941	PASS
173	174	0.00	2	1.6	3096	PASS
174	95	50	120	81.2	192106	PASS
175	174	5	9	7.6	14677	PASS
176	174	95	101	95.1	182656	PASS
177	176	5	9	6.7	12193	PASS

m/z	Abundance
36.00	2304.0
37.00	12925.0
38.00	11157.0
39.00	5066.0
39.80	594.0
40.30	556.0
41.70	123.0
42.90	310.0
44.00	1811.0
45.10	1896.0
46.20	617.0
47.00	3278.0
47.90	2255.0
49.00	10165.0
50.00	44168.0
51.10	14645.0
52.10	930.0
53.00	792.0
54.10	419.0
54.90	738.0
56.00	3158.0
57.00	6126.0
58.10	296.0
58.80	77.0
59.20	139.0
60.00	2296.0
61.00	12533.0
62.00	13091.0
63.10	9886.0
64.10	1953.0
65.00	3531.0
65.90	374.0
66.80	589.0
68.00	23152.0
69.00	24680.0
70.10	1538.0
71.90	995.0
73.00	12153.0
74.00	40432.0
75.00	121640.0
76.00	10922.0
77.10	1603.0
77.80	845.0
79.00	7862.0
80.00	2962.0
80.90	8036.0
82.00	2245.0
83.00	191.0
84.00	59.0
84.40	87.0
85.60	298.0
86.90	8732.0
88.00	8247.0
89.50	52.0
90.20	118.0
90.90	1241.0
91.90	7369.0
93.00	11986.0
94.00	27848.0
95.00	231744.0
96.00	14403.0
96.90	577.0
97.80	94.0
99.80	89.0
103.00	123.0
103.90	1085.0
104.80	302.0
105.80	1092.0
106.80	253.0
108.30	170.0
109.20	91.0
109.70	157.0
110.20	153.0
110.90	213.0
112.00	360.0
112.60	190.0
113.00	237.0
113.90	159.0
114.90	320.0
115.80	1123.0
116.90	2037.0
118.00	859.0
118.90	1578.0
120.00	196.0
122.80	148.0
123.80	54.0
126.00	147.0
127.90	746.0
128.70	410.0
129.00	388.0
129.80	771.0
130.90	483.0

Instrument :
MSVOA_X
ClientSampleId :
BFB71

132.20	91.0
132.80	182.0
133.40	57.0
134.00	321.0
134.90	595.0
136.00	183.0
136.70	721.0
139.00	108.0
139.70	118.0
140.90	2337.0
142.20	536.0
143.00	4331.0
144.00	592.0
144.90	2092.0
146.50	299.0
146.90	192.0
147.80	461.0
148.20	307.0
148.90	189.0
150.00	309.0
150.90	66.0
152.10	182.0
153.20	188.0
154.00	221.0
155.00	863.0
155.90	133.0
156.80	328.0
157.10	304.0
157.90	70.0
159.00	277.0
160.90	317.0
161.40	96.0
165.70	55.0
167.10	66.0
168.00	67.0
169.80	178.0
171.10	702.0
171.90	3973.0
173.00	2569.0
174.00	148736.0
174.90	12329.0
176.00	145792.0
177.10	11596.0
178.10	470.0
181.20	101.0
184.80	52.0
191.50	70.0
202.60	93.0
206.10	74.0
206.70	126.0
207.20	180.0
208.10	336.0
216.00	61.0
229.70	50.0
243.10	64.0
268.30	52.0
268.70	92.0
272.60	60.0
280.70	262.0
281.30	54.0
282.00	74.0
294.80	90.0

Instrument :
MSVOA_X
ClientSampleId :
BFB71

m/z	Abundance
36.00	2392.0
37.00	13614.0
38.10	11088.0
39.00	5988.0
39.90	471.0
40.20	486.0
40.90	232.0
42.30	99.0
43.00	349.0
44.10	2542.0
45.00	2072.0
45.90	915.0
47.00	3004.0
48.00	1844.0
49.00	11518.0
50.00	50656.0
51.00	16006.0
52.00	634.0
52.80	460.0
54.00	388.0
55.10	753.0
56.00	3745.0
57.00	6499.0
57.90	312.0
59.10	131.0
60.00	3096.0
61.00	13244.0
62.00	14921.0
63.00	12525.0
64.00	2133.0
65.10	3511.0
66.10	467.0
66.80	923.0
68.00	28480.0
69.00	28632.0
70.00	2356.0
71.30	200.0
72.10	1403.0
73.00	11575.0
74.00	46488.0
75.00	138688.0
76.00	12815.0
77.10	1720.0
77.90	1158.0
78.90	9804.0
79.90	2996.0
80.90	10950.0
81.90	2029.0
83.00	296.0
84.00	170.0
85.80	706.0
86.20	849.0
87.10	10240.0
88.00	9439.0
90.00	107.0
90.90	1070.0
92.00	8017.0
93.00	12922.0
94.00	33504.0
95.00	289408.0
96.10	17640.0
97.10	845.0
97.90	71.0
98.90	126.0
100.50	122.0
102.90	203.0
103.90	1666.0
104.90	823.0
105.90	1265.0
106.90	403.0
107.70	136.0
108.30	165.0
109.90	424.0
110.80	280.0
111.90	195.0
112.80	269.0
113.80	56.0
115.00	703.0
116.00	1238.0
117.00	2143.0
118.00	1203.0
119.10	1861.0
120.00	102.0
121.50	111.0
122.80	101.0
123.90	209.0
125.00	91.0
125.70	291.0
126.90	178.0
128.00	1076.0
128.80	499.0
129.90	1102.0

Instrument :
MSVOA_X
ClientSampleId :
BFB71

130.80	436.0
132.00	94.0
132.90	98.0
133.90	249.0
134.90	568.0
135.70	185.0
136.80	507.0
138.90	201.0
139.80	244.0
141.00	3882.0
142.00	637.0
143.00	5923.0
143.90	555.0
144.90	2068.0
145.90	667.0
146.80	232.0
147.30	112.0
148.10	497.0
148.80	162.0
150.00	529.0
151.00	164.0
152.00	149.0
152.90	284.0
153.90	233.0
155.10	760.0
155.90	134.0
157.00	1028.0
158.00	104.0
159.10	548.0
160.70	395.0
163.60	89.0
165.20	68.0
165.60	100.0
167.10	64.0
168.00	105.0
168.40	91.0
169.70	311.0
171.10	812.0
171.90	5809.0
173.10	3996.0
173.90	239232.0
175.00	17784.0
176.00	218240.0
177.00	13564.0
178.00	234.0
179.00	71.0
182.00	62.0
191.50	64.0
193.00	80.0
194.00	74.0
197.30	53.0
202.60	80.0
203.40	90.0
206.10	61.0
207.00	399.0
207.80	116.0
208.20	53.0
232.80	64.0
263.80	54.0
272.60	62.0
281.20	469.0
294.30	56.0

Instrument :
MSVOA_X
ClientSampleId :
BFB71

m/z	Abundance
36.10	1291.0
37.00	7242.0
38.00	6961.0
39.00	3531.0
39.90	452.0
40.60	440.0
41.10	184.0
41.70	182.0
42.80	171.0
43.90	2064.0
45.00	1219.0
46.20	457.0
47.00	1693.0
48.00	1479.0
49.00	6185.0
50.00	29112.0
51.00	10046.0
52.00	560.0
53.00	305.0
53.80	185.0
54.90	837.0
55.90	2803.0
57.00	4798.0
57.90	440.0
58.50	134.0
59.90	2030.0
61.00	8619.0
62.00	8265.0
63.00	7624.0
64.00	1231.0
65.00	2419.0
66.00	326.0
66.80	664.0
68.00	16576.0
69.00	17336.0
70.00	1632.0
71.90	1006.0
72.90	8902.0
74.00	31160.0
75.00	93776.0
76.00	8725.0
77.10	962.0
78.10	917.0
78.90	6396.0
80.10	1764.0
80.90	6679.0
81.90	1364.0
83.00	245.0
84.00	202.0
85.90	343.0
86.90	6937.0
88.00	6595.0
88.80	185.0
89.80	106.0
90.80	860.0
92.10	5742.0
93.00	9413.0
94.00	23328.0
95.00	188352.0
96.00	12780.0
97.00	356.0
97.80	94.0
98.80	59.0
100.50	59.0
101.20	80.0
102.00	177.0
102.90	215.0
104.00	1207.0
104.90	368.0
105.90	932.0
106.90	301.0
108.10	113.0
109.90	137.0
110.30	145.0
110.90	505.0
112.00	162.0
112.90	381.0
114.80	236.0
116.10	842.0
117.00	1871.0
118.00	656.0
119.00	1720.0
119.80	152.0
122.80	185.0
123.80	213.0
124.90	100.0
126.00	124.0
126.40	105.0
126.80	108.0
127.90	818.0
128.80	832.0
130.00	1013.0

Instrument :
MSVOA_X
ClientSampleId :
BFB71

130.70	225.0
131.00	214.0
132.00	127.0
133.20	120.0
133.80	130.0
135.10	429.0
136.10	260.0
136.80	518.0
139.80	227.0
140.90	2753.0
141.90	300.0
143.00	3808.0
143.80	232.0
144.90	1284.0
145.80	762.0
146.70	161.0
148.10	1117.0
148.90	296.0
149.90	315.0
150.60	167.0
151.80	98.0
153.00	363.0
153.70	183.0
154.90	514.0
156.20	61.0
157.00	706.0
158.00	120.0
159.10	416.0
159.70	169.0
160.80	336.0
164.70	71.0
165.30	101.0
165.60	89.0
167.80	105.0
168.40	91.0
169.30	207.0
170.10	101.0
170.80	714.0
172.00	4859.0
173.10	2723.0
174.00	188352.0
175.00	13918.0
176.00	183936.0
177.00	11849.0
177.90	324.0
178.90	106.0
182.40	147.0
186.60	110.0
192.00	52.0
201.10	73.0
203.40	91.0
206.90	310.0
207.50	119.0
230.40	78.0
248.10	73.0
250.00	79.0
253.00	60.0
263.80	131.0
266.20	70.0
281.10	432.0
281.80	72.0
282.40	79.0

Instrument :
MSVOA_X
ClientSampleId :
BFB71

m/z	Abundance
35.30	207.0
36.20	272.0
36.90	129.0
37.90	95.0
39.40	283.0
40.10	440.0
42.10	187.0
42.90	148.0
43.90	975.0
45.70	116.0
46.30	89.0
47.00	206.0
47.60	165.0
50.10	111.0
51.40	356.0
52.20	79.0
52.70	52.0
53.30	123.0
54.80	67.0
55.40	94.0
56.00	89.0
56.90	50.0
58.90	118.0
59.40	103.0
60.10	138.0
61.40	100.0
63.00	139.0
65.30	166.0
65.80	136.0
68.40	115.0
70.00	79.0
70.50	85.0
72.00	59.0
73.30	163.0
74.50	209.0
75.90	107.0
76.70	56.0
77.80	87.0
79.40	101.0
80.80	56.0
81.60	290.0
82.20	117.0
83.50	53.0
84.90	105.0
88.80	227.0
89.70	130.0
90.90	54.0
92.60	85.0
95.80	134.0
98.50	141.0
99.20	97.0
101.20	107.0
106.50	95.0
114.20	51.0
117.70	62.0
125.80	80.0
131.70	57.0
133.10	130.0
134.40	72.0
137.00	100.0
139.10	52.0
145.20	131.0
152.00	109.0
152.50	78.0
163.00	130.0
177.10	143.0
178.50	59.0
194.00	58.0
194.80	69.0
206.90	379.0
207.80	57.0
227.10	53.0
234.50	88.0
239.80	95.0
253.30	129.0
267.20	60.0
271.80	109.0
281.10	227.0
292.10	64.0

Instrument :
MSVOA_X
ClientSampleId :
BFB71