

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX081821\
 Data File : VX023827.D
 Acq On : 18 Aug 2021 19:22
 Operator : JC/MD
 Sample : M3414-02 10X
 Misc : 5.04g/10mL/100uL/5.00mL/MSVOA_X/MEOH
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 B-2

Quant Time: Aug 19 04:21:59 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X081721W.M
 Quant Title : SW846 8260
 QLast Update : Tue Aug 17 11:57:51 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Pentafluorobenzene	5.562	168	138772	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	6.769	114	239179	50.000	ug/l	0.00
63) Chlorobenzene-d5	10.055	117	218887	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	12.024	152	80012	50.000	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	5.964	65	97990	50.593	ug/l	0.00
Spiked Amount	50.000	Range	78 - 117	Recovery	=	101.180%
35) Dibromofluoromethane	5.397	113	75352	47.599	ug/l	0.00
Spiked Amount	50.000	Range	75 - 124	Recovery	=	95.200%
50) Toluene-d8	8.653	98	297401	49.359	ug/l	0.00
Spiked Amount	50.000	Range	92 - 112	Recovery	=	98.720%
62) 4-Bromofluorobenzene	11.085	95	97513	43.963	ug/l	0.00
Spiked Amount	50.000	Range	83 - 123	Recovery	=	87.920%
Target Compounds						
					Qvalue	
5) Bromomethane	1.605	94	818	0.830	ug/l #	64
6) Chloroethane	1.690	64	27	2.237	ug/l #	43
10) Methyl Iodide	2.459	142	834	0.430	ug/l #	89
11) Tert butyl alcohol	2.965	59	94	0.240	ug/l #	73
16) Acetone	2.386	43	909	1.050	ug/l #	65
18) Methyl Acetate	2.709	43	590	0.273	ug/l #	47
20) Methylene Chloride	2.794	84	1227	0.742	ug/l #	76
31) Cyclohexane	5.507	56	1529	0.614	ug/l #	49
36) 1,1-Dichloropropene	5.556	75	10797	4.875	ug/l #	49
38) Carbon Tetrachloride	5.562	117	14745	6.384	ug/l #	15
39) Methylcyclohexane	7.391	83	6055	2.245	ug/l	90
48) Methyl methacrylate	7.659	41	969	0.466	ug/l #	80
51) 4-Methyl-2-Pentanone	8.653	43	2434	0.884	ug/l #	5
56) Ethyl methacrylate	9.104	69	1010	1.093	ug/l #	1
59) 2-Hexanone	9.390	43	2984	1.410	ug/l #	19
60) Dibromochloromethane	9.274	129	92	1.734	ug/l #	11
67) Ethyl Benzene	10.195	91	6793	0.852	ug/l	97
68) m/p-Xylenes	10.311	106	1679	0.553	ug/l	75
73) Isopropylbenzene	10.963	105	7146	1.171	ug/l	93
74) N-amyl acetate	10.853	43	1959	0.710	ug/l #	17
75) 1,1,2,2-Tetrachloroethane	11.195	83	990	0.495	ug/l #	92
76) 1,2,3-Trichloropropane	11.085	75	50839	27.238	ug/l #	40
78) n-propylbenzene	11.305	91	31290	4.483	ug/l	98
79) 2-Chlorotoluene	11.402	91	966	0.229	ug/l #	41
80) 1,3,5-Trimethylbenzene	11.451	105	2597	0.518	ug/l	90
81) trans-1,4-Dichloro-2-b...	11.085	75	50839	80.122	ug/l #	12
82) 4-Chlorotoluene	11.402	91	966	0.202	ug/l #	45
84) 1,2,4-Trimethylbenzene	11.756	105	12642	2.528	ug/l	99
85) sec-Butylbenzene	11.896	105	8195	1.329	ug/l	96
86) p-Isopropyltoluene	12.183	119	1929	0.380	ug/l	87
89) n-Butylbenzene	12.335	91	18918	4.174	ug/l #	83
90) Hexachloroethane	12.615	117	8599	10.900	ug/l #	9
92) 1,2-Dibromo-3-Chloropr...	12.920	75	388	2.953	ug/l #	1
95) Naphthalene	13.780	128	16298	3.996	ug/l #	91

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX081821\
Data File : VX023827.D
Acq On : 18 Aug 2021 19:22
Operator : JC/MD
Sample : M3414-02 10X
Misc : 5.04g/10mL/100uL/5.00mL/MSVOA_X/MEOH
ALS Vial : 25 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
B-2

Quant Time: Aug 19 04:21:59 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X081721W.M
Quant Title : SW846 8260
QLast Update : Tue Aug 17 11:57:51 2021
Response via : Initial Calibration


Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


(#)=qualifier out of range (m)=manual integration (+)=signals summed						

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX081821\
Data File : VX023827.D
Acq On : 18 Aug 2021 19:22
Operator : JC/MD
Sample : M3414-02 10X
Misc : 5.04g/10mL/100uL/5.00mL/MSVOA_X/MEOH
ALS Vial : 25 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
B-2


Quant Time: Aug 19 04:21:59 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X081721W.M
Quant Title : SW846 8260
QLast Update : Tue Aug 17 11:57:51 2021
Response via : Initial Calibration

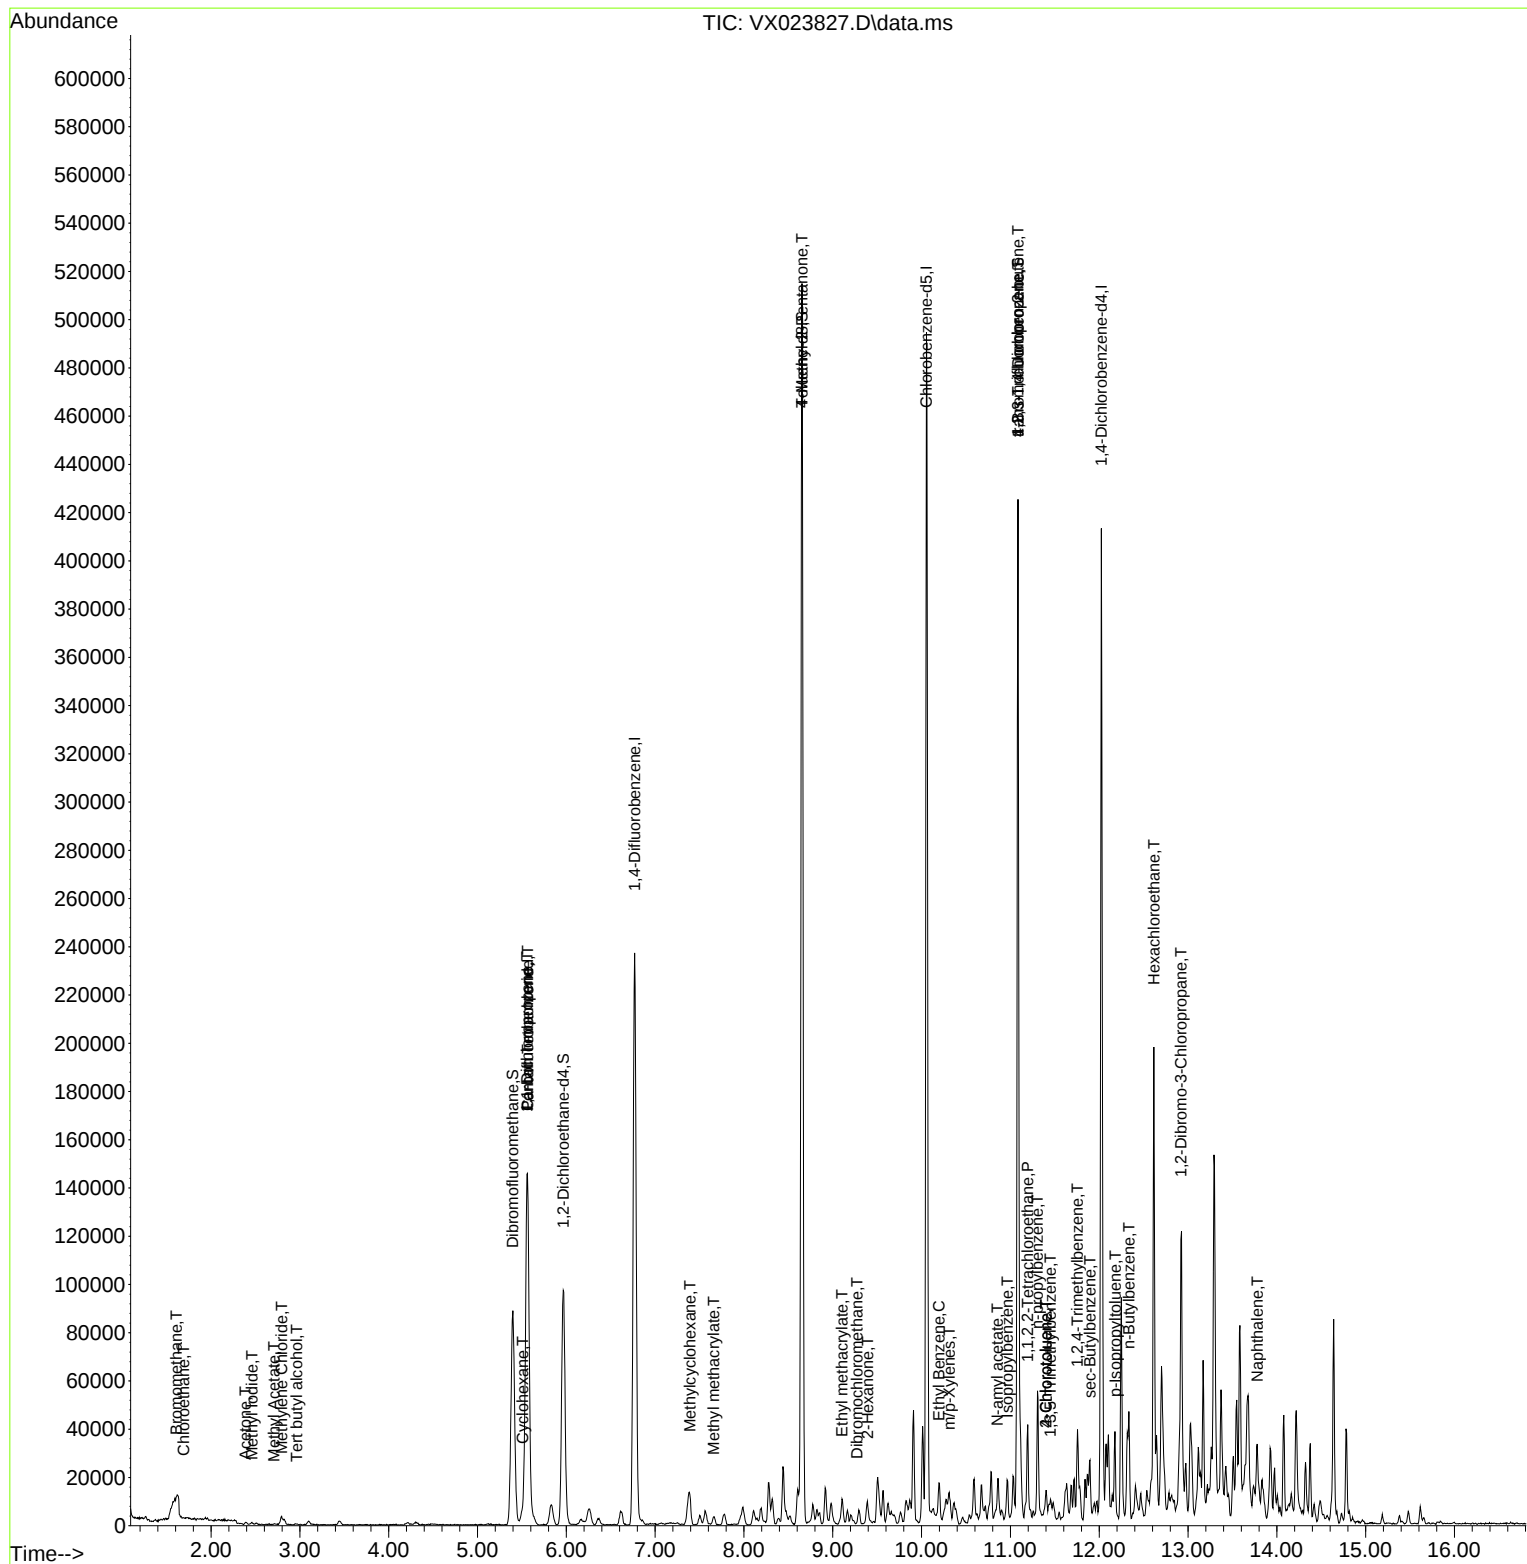



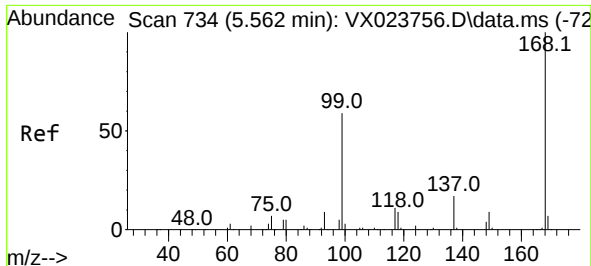


#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 5.562 min Scan# 734
Delta R.T. -0.000 min
Lab File: VX023827.D
Acq: 18 Aug 2021 19:22

Instrument :
MSVOA_X
ClientSampled :
B-2







Tgt Ion:168 Resp: 138772
Ion Ratio Lower Upper
168 100
99 55.8 45.8 68.6

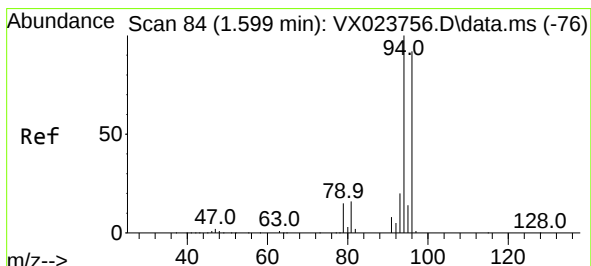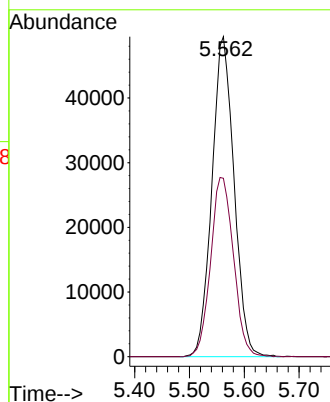

#5
Bromomethane
Concen: 0.830 ug/l
RT: 1.605 min Scan# 85
Delta R.T. 0.006 min
Lab File: VX023827.D
Acq: 18 Aug 2021 19:22

Tgt Ion: 94 Resp: 818
Ion Ratio Lower Upper
94 100
96 60.1 76.4 114.6#







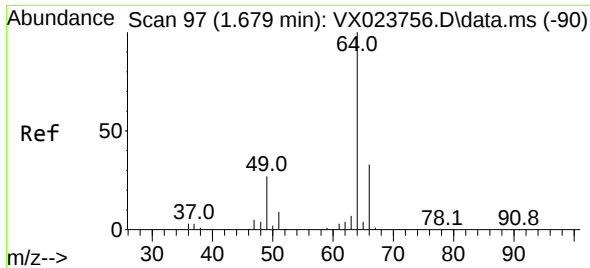

#6
Chloroethane
Concen: 2.237 ug/l
RT: 1.690 min Scan# 99
Delta R.T. 0.011 min
Lab File: VX023827.D
Acq: 18 Aug 2021 19:22




Instrument :
MSVOA_X
ClientSampled :
B-2


Tgt Ion: 64 Resp: 27
Ion Ratio Lower Upper
64 100
66 0.0 25.4 38.0#

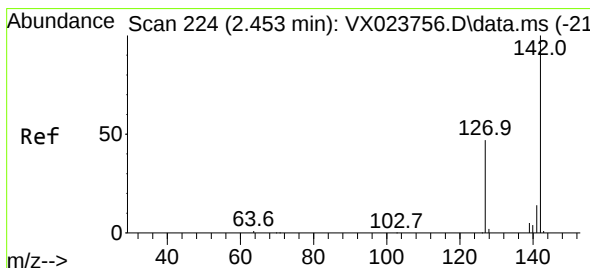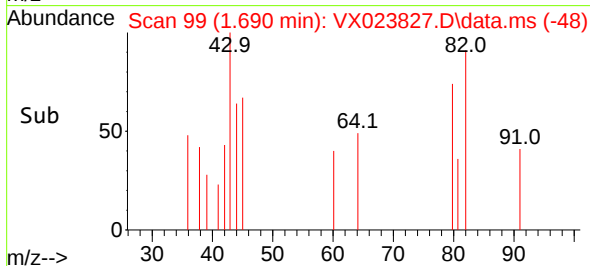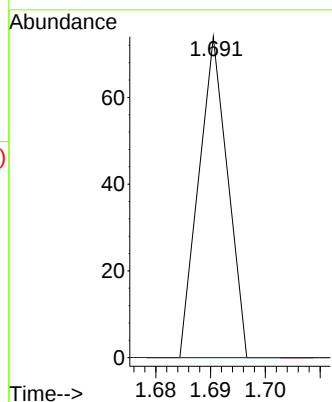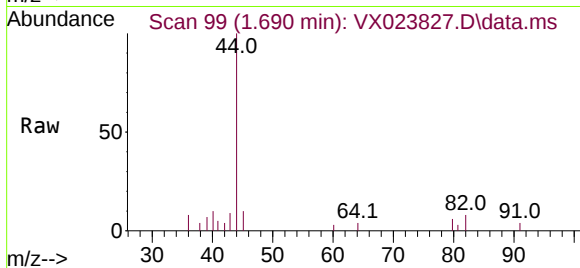

#10
Methyl Iodide
Concen: 0.430 ug/l
RT: 2.459 min Scan# 225
Delta R.T. 0.006 min
Lab File: VX023827.D
Acq: 18 Aug 2021 19:22

Tgt Ion: 142 Resp: 834
Ion Ratio Lower Upper
142 100
127 36.8 33.3 49.9
141 5.0 11.4 17.0#

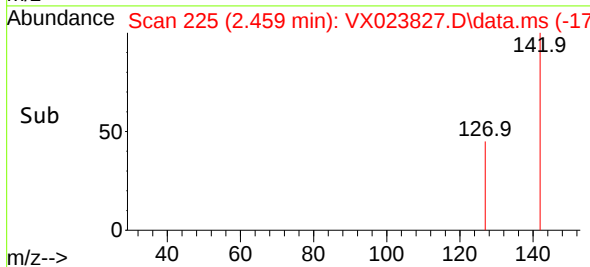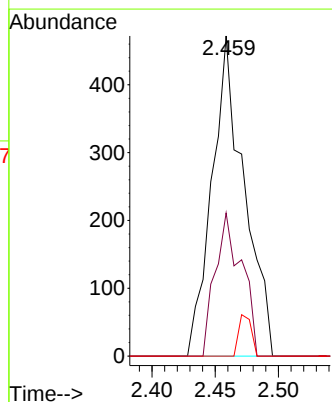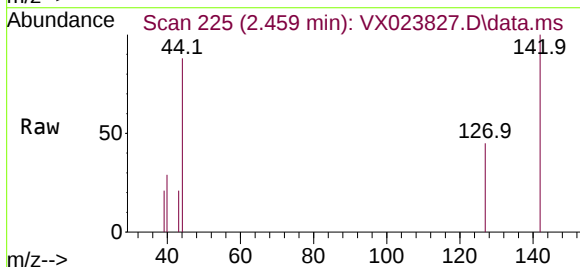







#11

Tert butyl alcohol
Concen: 0.240 ug/l
RT: 2.965 min Scan# 308
Delta R.T. -0.018 min
Lab File: VX023827.D
Acq: 18 Aug 2021 19:22

Instrument :
MSVOA_X
ClientSampled :
B-2




Tgt Ion: 59 Resp: 94
Ion Ratio Lower Upper
59 100
57 0.0 7.8 11.8#

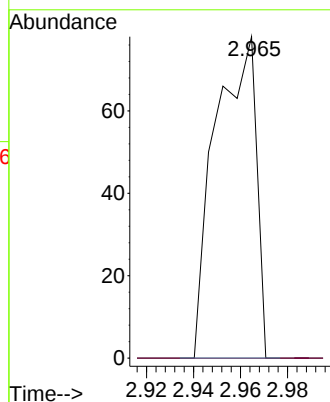


#16

Acetone
Concen: 1.050 ug/l
RT: 2.386 min Scan# 213
Delta R.T. -0.006 min
Lab File: VX023827.D
Acq: 18 Aug 2021 19:22

Tgt Ion: 43 Resp: 909
Ion Ratio Lower Upper
43 100
58 14.3 27.8 41.8#


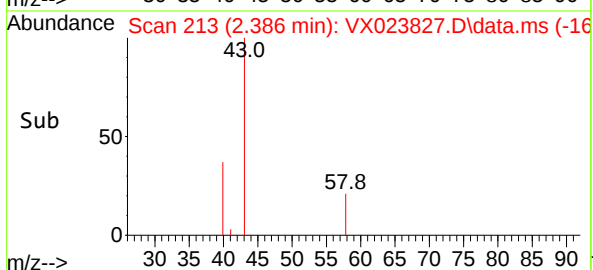






#18
Methyl Acetate
Concen: 0.273 ug/l
RT: 2.709 min Scan# 266
Delta R.T. -0.006 min
Lab File: VX023827.D
Acq: 18 Aug 2021 19:22




Instrument :
MSVOA_X
ClientSampled :
B-2


Tgt Ion: 43 Resp: 590
Ion Ratio Lower Upper
43 100
74 0.0 21.9 32.9#

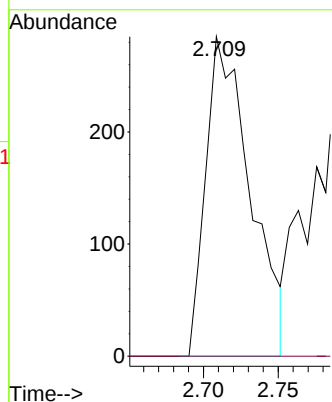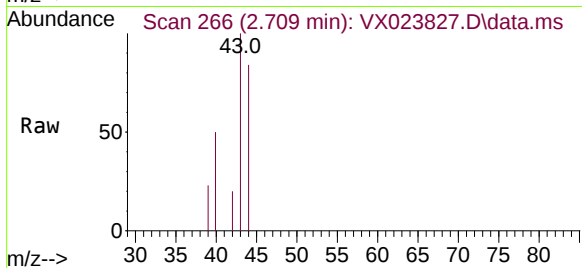

#20
Methylene Chloride
Concen: 0.742 ug/l
RT: 2.794 min Scan# 280
Delta R.T. -0.000 min
Lab File: VX023827.D
Acq: 18 Aug 2021 19:22

Tgt Ion: 84 Resp: 1227
Ion Ratio Lower Upper
84 100
49 116.2 88.6 132.8
51 81.3 27.0 40.6#
86 83.8 50.3 75.5#


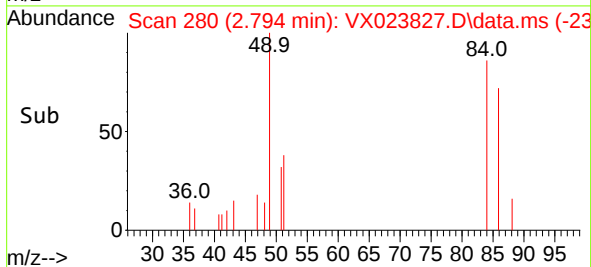

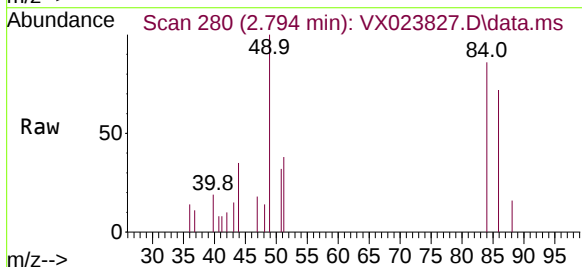




#31
Cyclohexane
Concen: 0.614 ug/l
RT: 5.507 min Scan# 725
Delta R.T. 0.030 min
Lab File: VX023827.D
Acq: 18 Aug 2021 19:22




Instrument :
MSVOA_X
ClientSampled :
B-2


Tgt Ion: 56 Resp: 1529
Ion Ratio Lower Upper
56 100
69 14.5 25.3 37.9#
84 35.0 71.4 107.0#

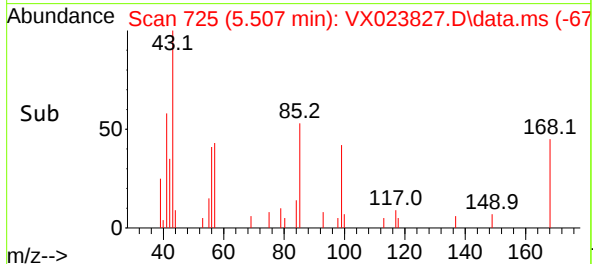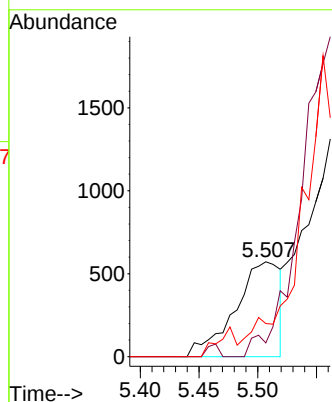

#33
1,2-Dichloroethane-d4
Concen: 50.593 ug/l
RT: 5.964 min Scan# 800
Delta R.T. 0.000 min
Lab File: VX023827.D
Acq: 18 Aug 2021 19:22

Tgt Ion: 65 Resp: 97990
Ion Ratio Lower Upper
65 100
67 50.5 0.0 105.4


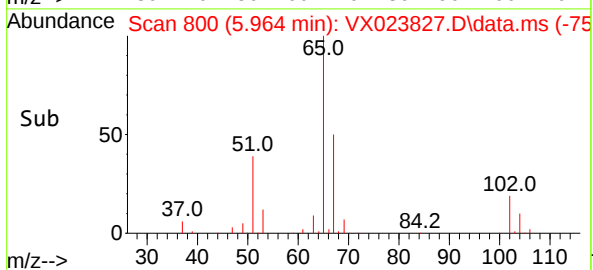
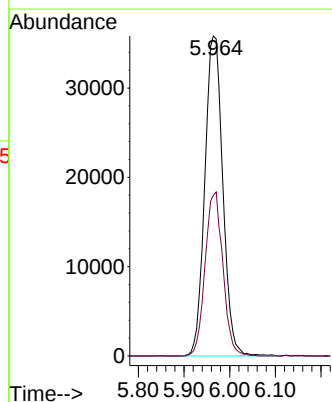
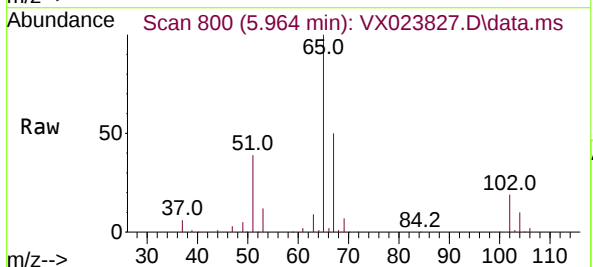


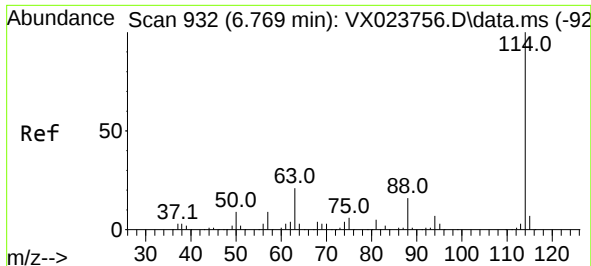

#34
1,4-Difluorobenzene
Concen: 50.000 ug/l
RT: 6.769 min Scan# 932
Delta R.T. -0.000 min
Lab File: VX023827.D
Acq: 18 Aug 2021 19:22




Instrument :
MSVOA_X
ClientSampled :
B-2


Tgt Ion:114 Resp: 239179
Ion Ratio Lower Upper
114 100
63 20.8 0.0 40.8
88 15.9 0.0 32.8



#35
Dibromofluoromethane
Concen: 47.599 ug/l
RT: 5.397 min Scan# 707
Delta R.T. 0.000 min
Lab File: VX023827.D
Acq: 18 Aug 2021 19:22

Tgt Ion:113 Resp: 75352
Ion Ratio Lower Upper
113 100
111 102.7 81.9 122.9
192 19.6 16.7 25.1


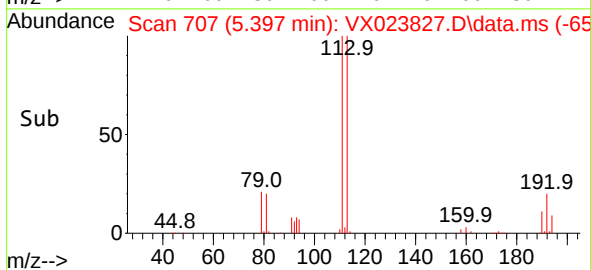

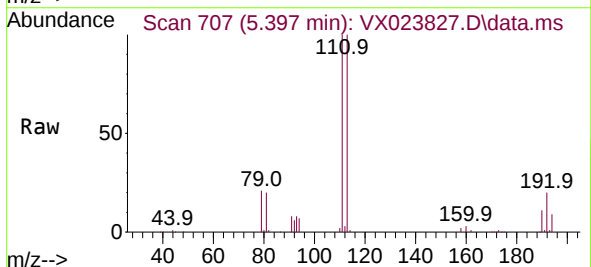




#36
1,1-Dichloropropene
Concen: 4.875 ug/l
RT: 5.556 min Scan# 733
Delta R.T. -0.146 min
Lab File: VX023827.D
Acq: 18 Aug 2021 19:22




Instrument :
MSVOA_X
ClientSampled :
B-2


Tgt Ion: 75 Resp: 10797
Ion Ratio Lower Upper
75 100
110 9.3 18.1 54.4#
77 0.0 25.3 37.9#

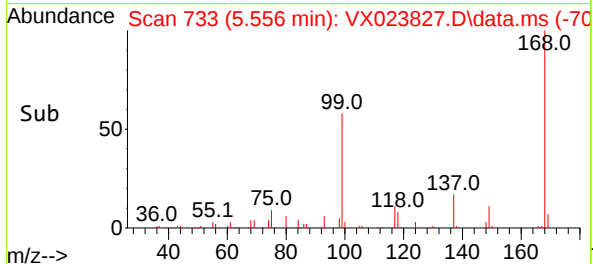

#38
Carbon Tetrachloride
Concen: 6.384 ug/l
RT: 5.562 min Scan# 734
Delta R.T. -0.128 min
Lab File: VX023827.D
Acq: 18 Aug 2021 19:22

Tgt Ion: 117 Resp: 14745
Ion Ratio Lower Upper
117 100
119 3.7 76.2 114.2#
121 0.0 24.8 37.2#

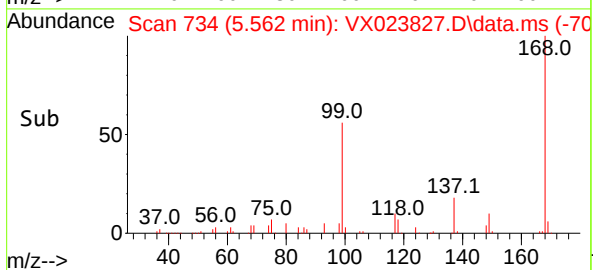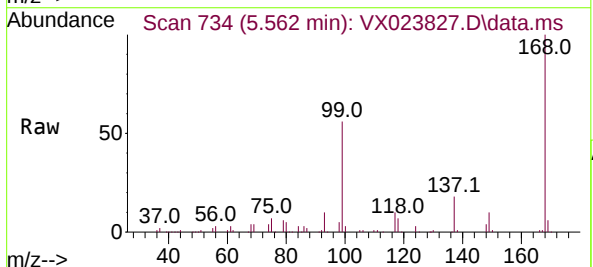



#39

Methylcyclohexane

Concen: 2.245 ug/l

RT: 7.391 min Scan# 1034





Delta R.T. 0.006 min

Lab File: VX023827.D

Acq: 18 Aug 2021 19:22

Tgt Ion: 83 Resp: 6055

Ion	Ratio	Lower	Upper
83	100		
55	64.8	58.9	88.3
98	40.9	38.1	57.1

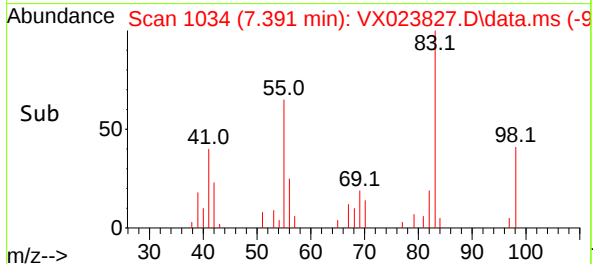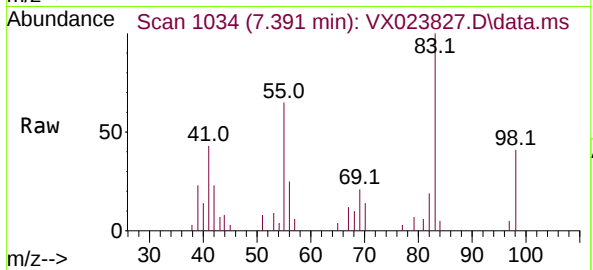

#48

Methyl methacrylate

Concen: 0.466 ug/l

RT: 7.659 min Scan# 1078




Delta R.T. -0.043 min


Lab File: VX023827.D

Acq: 18 Aug 2021 19:22

Tgt Ion: 41 Resp: 969

Ion	Ratio	Lower	Upper
41	100		
69	116.1	76.0	114.0#
39	68.2	44.6	67.0#

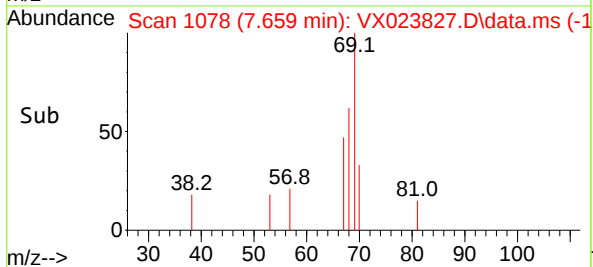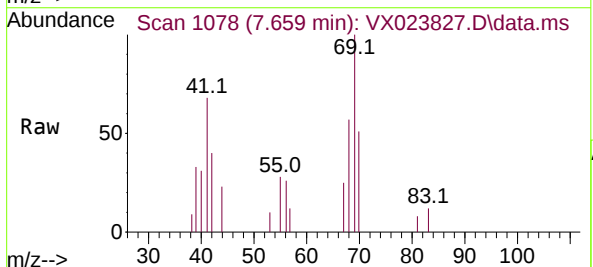



#50

Toluene-d8

Concen: 49.359 ug/l

RT: 8.653 min Scan# 1241

Delta R.T. -0.000 min

Lab File: VX023827.D

Acq: 18 Aug 2021 19:22

Tgt Ion: 98 Resp: 297401

Ion Ratio Lower Upper

98 100





100 63.0 51.9 77.9

Instrument :

MSVOA_X

ClientSampled :

B-2

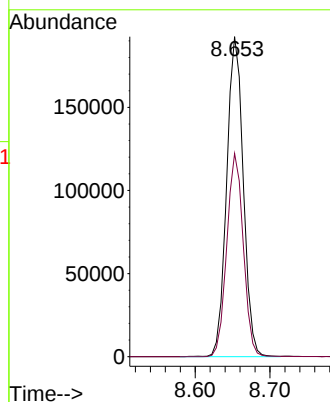

#51

4-Methyl-2-Pentanone

Concen: 0.884 ug/l

RT: 8.653 min Scan# 1241

Delta R.T. 0.073 min

Lab File: VX023827.D




Acq: 18 Aug 2021 19:22


Tgt Ion: 43 Resp: 2434

Ion Ratio Lower Upper

43 100

58 105.8 35.4 53.0#



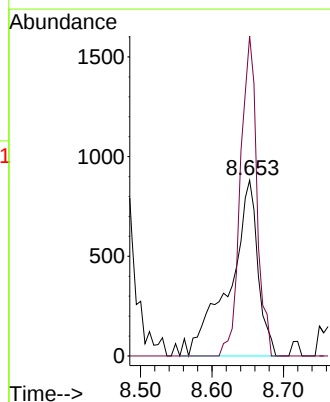
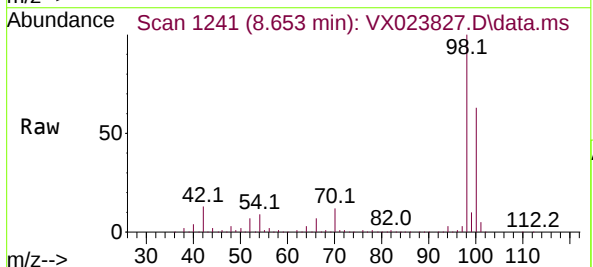




#56
Ethyl methacrylate
Concen: 1.093 ug/l
RT: 9.104 min Scan# 1315
Delta R.T. -0.018 min
Lab File: VX023827.D
Acq: 18 Aug 2021 19:22




Instrument :
MSVOA_X
ClientSampled :
B-2


Tgt Ion: 69 Resp: 1010
Ion Ratio Lower Upper
69 100
41 216.4 46.8 70.2#
39 97.8 24.7 37.1#

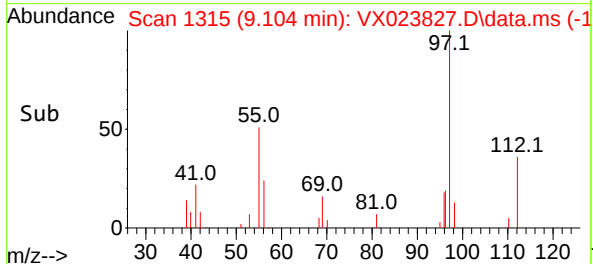

#59
2-Hexanone
Concen: 1.410 ug/l
RT: 9.390 min Scan# 1362
Delta R.T. -0.043 min
Lab File: VX023827.D
Acq: 18 Aug 2021 19:22

Tgt Ion: 43 Resp: 2984
Ion Ratio Lower Upper
43 100
58 0.0 30.9 92.8#


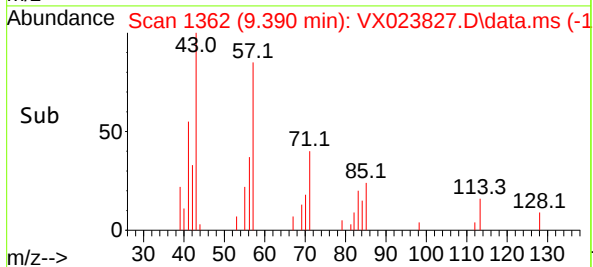

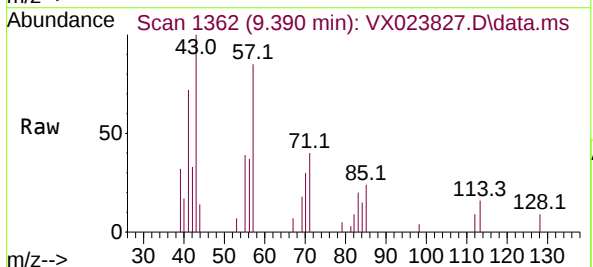




#60
Dibromochloromethane
Concen: 1.734 ug/l
RT: 9.274 min Scan# 1343
Delta R.T. -0.251 min
Lab File: VX023827.D
Acq: 18 Aug 2021 19:22




Instrument :
MSVOA_X
ClientSampled :
B-2


Tgt Ion:129 Resp: 92
Ion Ratio Lower Upper
129 100
127 0.0 38.4 115.2#

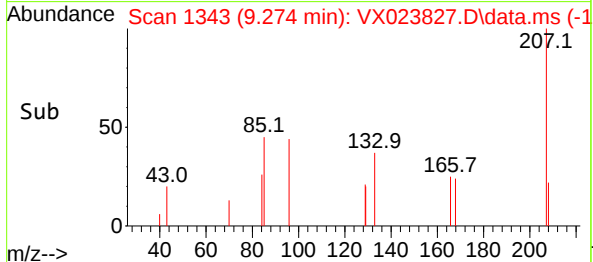

#62
4-Bromofluorobenzene
Concen: 43.963 ug/l
RT: 11.085 min Scan# 1640
Delta R.T. 0.000 min
Lab File: VX023827.D
Acq: 18 Aug 2021 19:22

Tgt Ion: 95 Resp: 97513
Ion Ratio Lower Upper
95 100
174 79.8 0.0 154.6
176 76.8 0.0 155.8


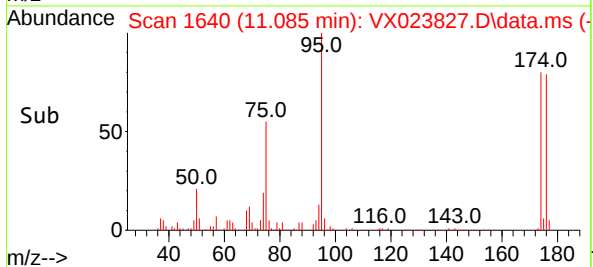

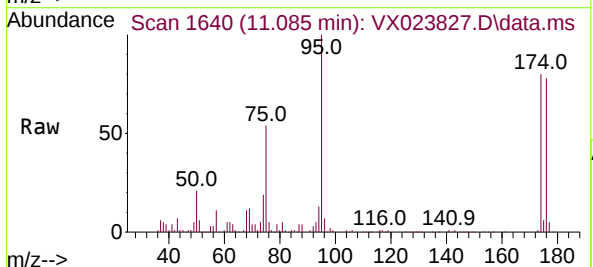




#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 10.055 min Scan# 1471
Delta R.T. -0.006 min
Lab File: VX023827.D
Acq: 18 Aug 2021 19:22




Instrument :
MSVOA_X
ClientSampled :
B-2


Tgt Ion:117 Resp: 218887
Ion Ratio Lower Upper
117 100
82 58.4 47.4 71.2
119 33.2 26.6 39.8



#67
Ethyl Benzene
Concen: 0.852 ug/l
RT: 10.195 min Scan# 1494
Delta R.T. 0.000 min
Lab File: VX023827.D
Acq: 18 Aug 2021 19:22

Tgt Ion: 91 Resp: 6793
Ion Ratio Lower Upper
91 100
106 29.3 24.6 37.0



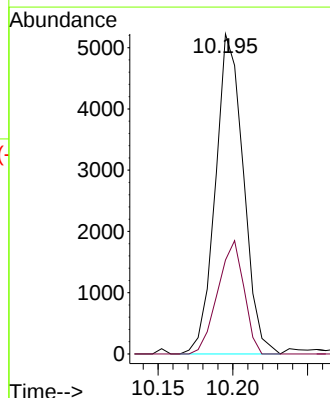
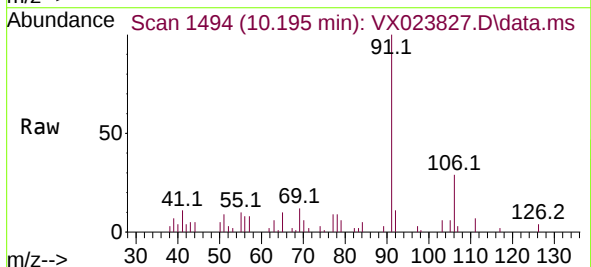


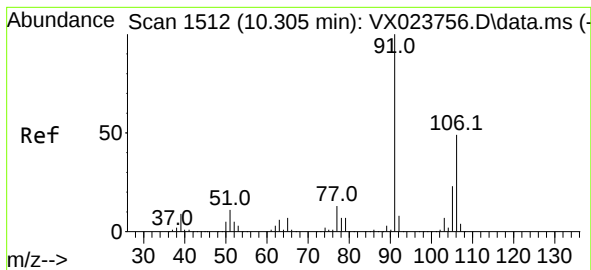

#68
m/p-Xylenes
Concen: 0.553 ug/l
RT: 10.311 min Scan# 1513
Delta R.T. 0.006 min
Lab File: VX023827.D
Acq: 18 Aug 2021 19:22




Instrument :
MSVOA_X
ClientSampled :
B-2


Tgt Ion:106 Resp: 1679
Ion Ratio Lower Upper
106 100
91 242.3 162.8 244.2

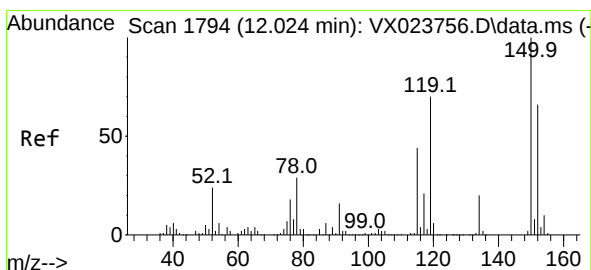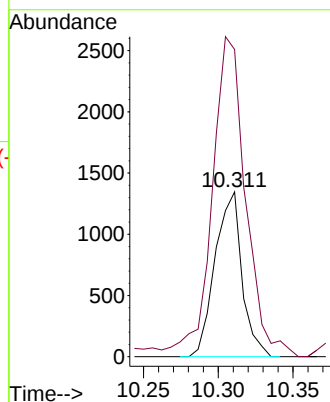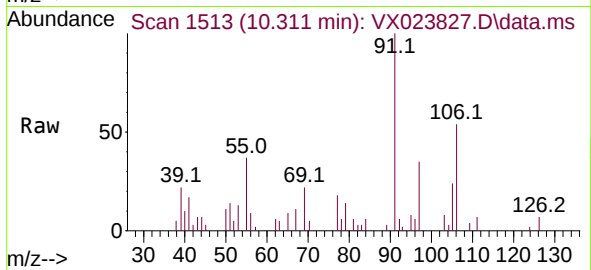

#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 12.024 min Scan# 1794
Delta R.T. 0.000 min
Lab File: VX023827.D
Acq: 18 Aug 2021 19:22

Tgt Ion:152 Resp: 80012
Ion Ratio Lower Upper
152 100
115 59.4 41.1 123.3
150 159.4 0.0 349.0




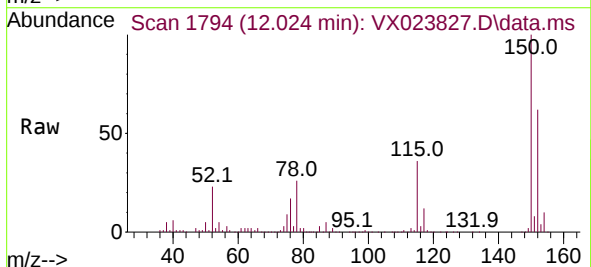




#73
Isopropylbenzene
Concen: 1.171 ug/l
RT: 10.963 min Scan# 1620
Delta R.T. 0.000 min
Lab File: VX023827.D
Acq: 18 Aug 2021 19:22




Instrument :
MSVOA_X
ClientSampled :
B-2


Tgt Ion:105 Resp: 7146
Ion Ratio Lower Upper
105 100
120 30.1 13.2 39.6

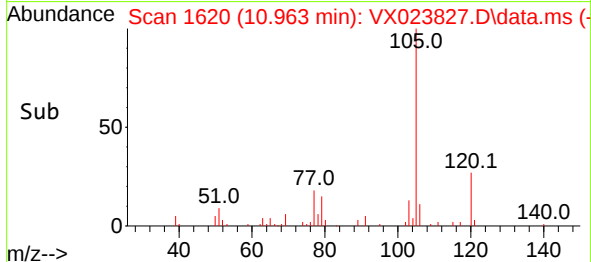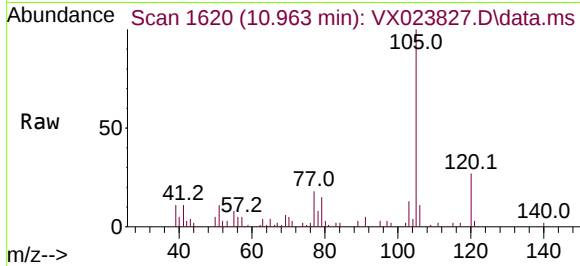

#74
N-ethyl acetate
Concen: 0.710 ug/l
RT: 10.853 min Scan# 1602
Delta R.T. 0.005 min
Lab File: VX023827.D
Acq: 18 Aug 2021 19:22

Tgt Ion: 43 Resp: 1959
Ion Ratio Lower Upper
43 100
70 40.9 39.0 58.6
55 152.4 21.5 32.3#
61 0.0 22.1 33.1#


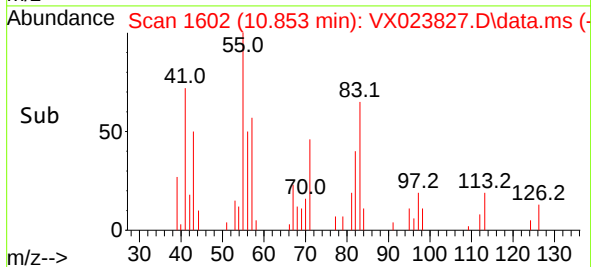
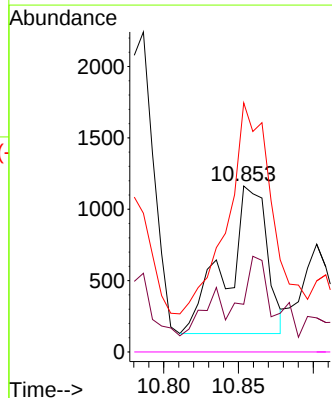
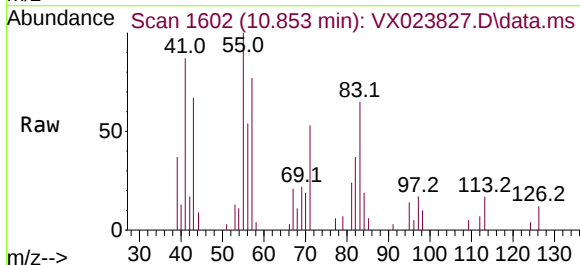




#75
1,1,2,2-Tetrachloroethane
Concen: 0.495 ug/l
RT: 11.195 min Scan# 1658
Delta R.T. -0.018 min
Lab File: VX023827.D
Acq: 18 Aug 2021 19:22




Instrument :
MSVOA_X
ClientSampled :
B-2


Tgt Ion: 83 Resp: 990
Ion Ratio Lower Upper
83 100
131 0.0 5.1 15.2#
85 67.5 31.8 95.4

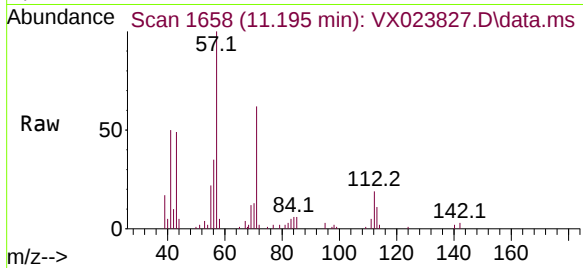

#76
1,2,3-Trichloropropane
Concen: 27.238 ug/l
RT: 11.085 min Scan# 1640
Delta R.T. -0.159 min
Lab File: VX023827.D
Acq: 18 Aug 2021 19:22

Tgt Ion: 75 Resp: 50839
Ion Ratio Lower Upper
75 100
77 1.8 19.1 57.5#


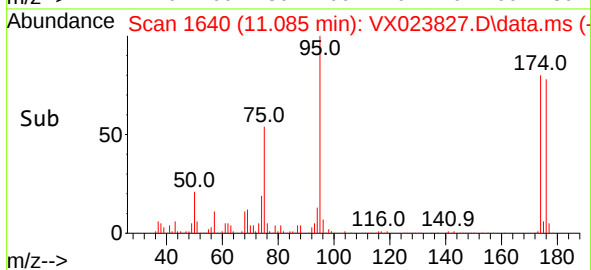

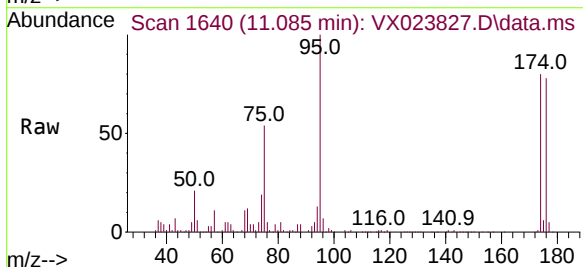




#78
n-propylbenzene
Concen: 4.483 ug/l
RT: 11.305 min Scan# 1676
Delta R.T. -0.000 min
Lab File: VX023827.D
Acq: 18 Aug 2021 19:22




Instrument :
MSVOA_X
ClientSampled :
B-2


Tgt Ion: 91 Resp: 31290
Ion Ratio Lower Upper
91 100
120 24.2 11.5 34.5



#79
2-Chlorotoluene
Concen: 0.229 ug/l
RT: 11.402 min Scan# 1692
Delta R.T. 0.036 min
Lab File: VX023827.D
Acq: 18 Aug 2021 19:22

Tgt Ion: 91 Resp: 966
Ion Ratio Lower Upper
91 100
126 0.0 16.6 49.8#


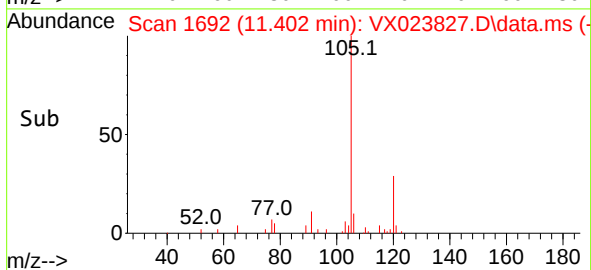

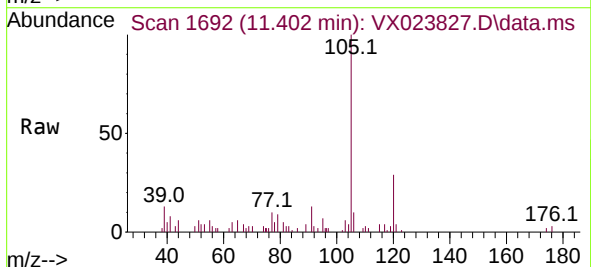


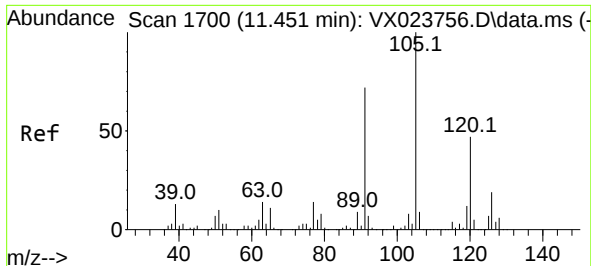

#80
1,3,5-Trimethylbenzene
Concen: 0.518 ug/l
RT: 11.451 min Scan# 1700
Delta R.T. -0.000 min
Lab File: VX023827.D
Acq: 18 Aug 2021 19:22




Instrument :
MSVOA_X
ClientSampled :
B-2


Tgt Ion:105 Resp: 2597
Ion Ratio Lower Upper
105 100
120 54.4 23.8 71.5

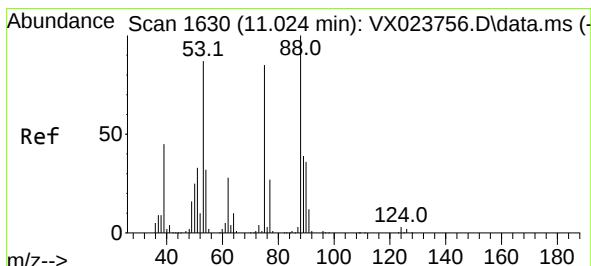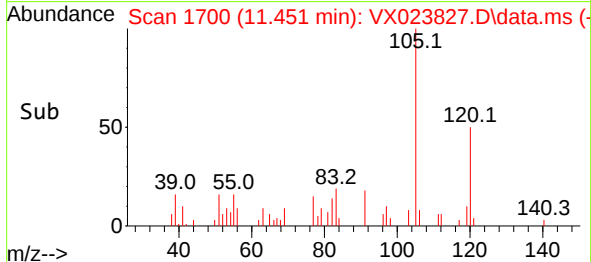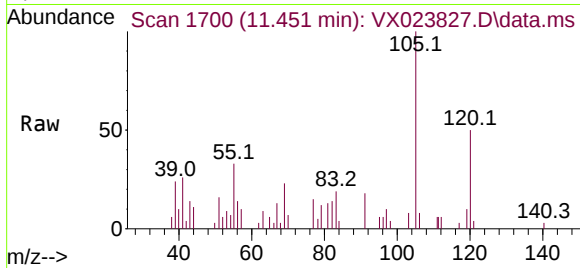

#81
trans-1,4-Dichloro-2-butene
Concen: 80.122 ug/l
RT: 11.085 min Scan# 1640
Delta R.T. 0.061 min
Lab File: VX023827.D
Acq: 18 Aug 2021 19:22

Tgt Ion: 75 Resp: 50839
Ion Ratio Lower Upper
75 100
53 0.3 74.5 111.7#
89 0.0 37.9 56.9#


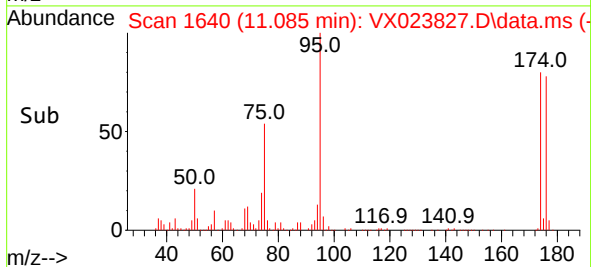

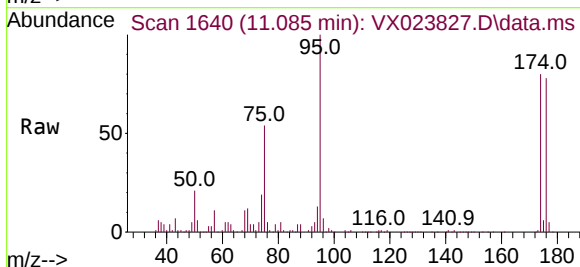




#82
4-Chlorotoluene
Concen: 0.202 ug/l
RT: 11.402 min Scan# 1692
Delta R.T. -0.055 min
Lab File: VX023827.D
Acq: 18 Aug 2021 19:22




Instrument :
MSVOA_X
ClientSampled :
B-2


Tgt Ion: 91 Resp: 966
Ion Ratio Lower Upper
91 100
126 0.0 14.9 44.5#

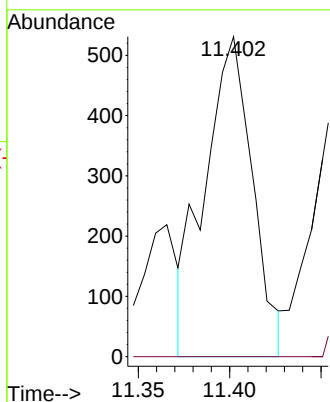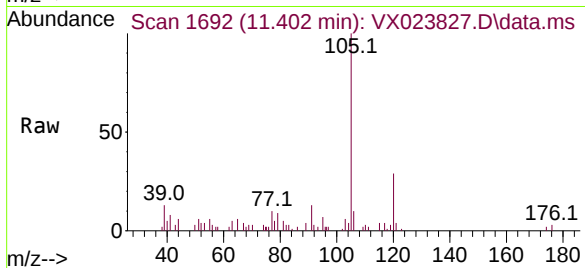

#84
1,2,4-Trimethylbenzene
Concen: 2.528 ug/l
RT: 11.756 min Scan# 1750
Delta R.T. -0.000 min
Lab File: VX023827.D
Acq: 18 Aug 2021 19:22

Tgt Ion: 105 Resp: 12642
Ion Ratio Lower Upper
105 100
120 45.7 22.4 67.3


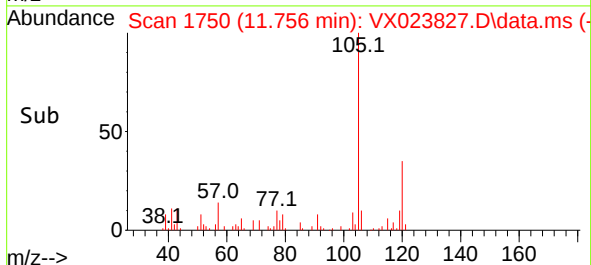

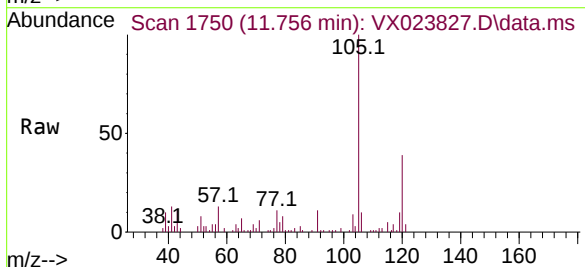


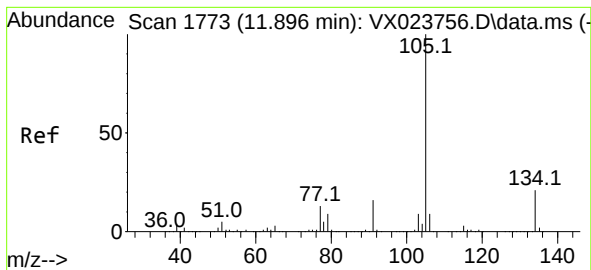

#85
 sec-Butylbenzene
 Concen: 1.329 ug/l
 RT: 11.896 min Scan# 1773
 Delta R.T. -0.000 min
 Lab File: VX023827.D
 Acq: 18 Aug 2021 19:22




Instrument :
 MSVOA_X
 ClientSampled :
 B-2


Tgt Ion:105 Resp: 8195
 Ion Ratio Lower Upper
 105 100
 134 18.1 10.0 29.8

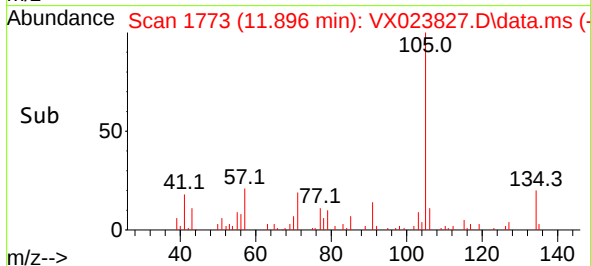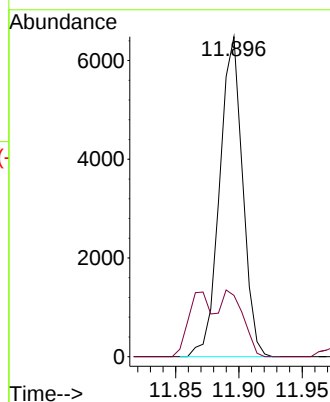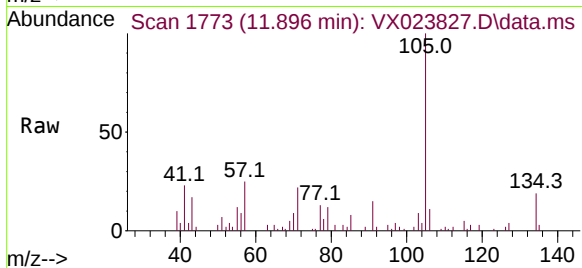

#86
 p-Isopropyltoluene
 Concen: 0.380 ug/l
 RT: 12.183 min Scan# 1820
 Delta R.T. 0.171 min
 Lab File: VX023827.D
 Acq: 18 Aug 2021 19:22

Tgt Ion:119 Resp: 1929
 Ion Ratio Lower Upper
 119 100
 134 24.1 12.9 38.7
 91 34.4 11.7 35.0


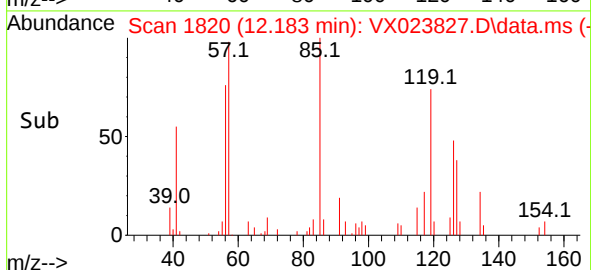

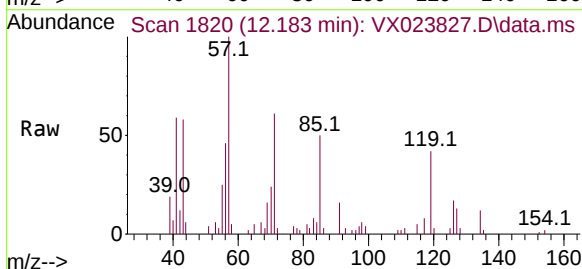


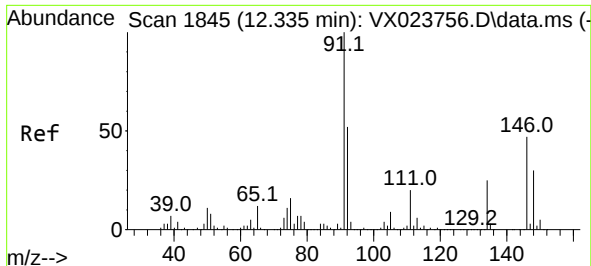

#89
n-Butylbenzene
Concen: 4.174 ug/l
RT: 12.335 min Scan# 1845
Delta R.T. -0.000 min
Lab File: VX023827.D
Acq: 18 Aug 2021 19:22




Instrument :
MSVOA_X
ClientSampled :
B-2


Tgt Ion: 91 Resp: 18918
Ion Ratio Lower Upper
91 100
92 46.5 27.4 82.0
134 40.7 13.2 39.5#

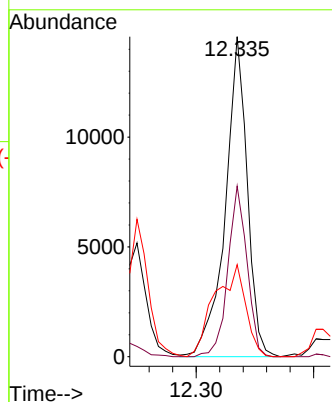

#90
Hexachloroethane
Concen: 10.900 ug/l
RT: 12.615 min Scan# 1891
Delta R.T. 0.073 min
Lab File: VX023827.D
Acq: 18 Aug 2021 19:22

Tgt Ion: 117 Resp: 8599
Ion Ratio Lower Upper
117 100
201 0.0 40.4 121.2#


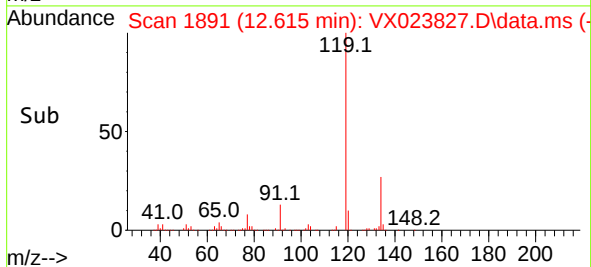
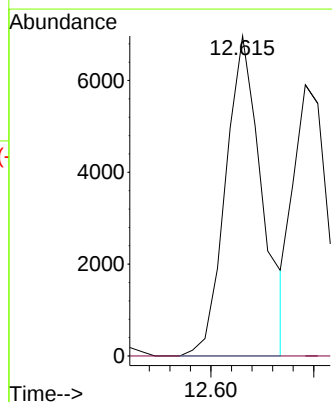
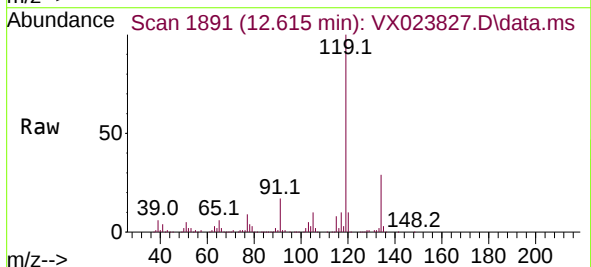


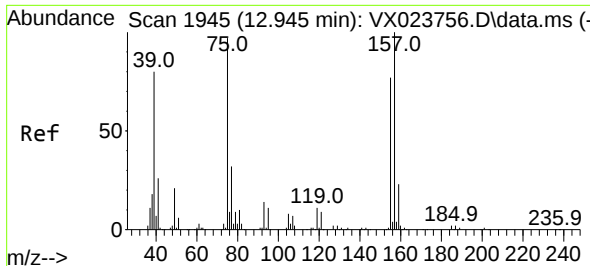

#92
1,2-Dibromo-3-Chloropropane
Concen: 2.953 ug/l
RT: 12.920 min Scan# 1941
Delta R.T. -0.025 min
Lab File: VX023827.D
Acq: 18 Aug 2021 19:22

Instrument :
MSVOA_X
ClientSampleId :
B-2

Tgt Ion: 75 Resp: 388
Ion Ratio Lower Upper
75 100
155 0.0 45.3 135.9#
157 0.0 57.7 173.1#

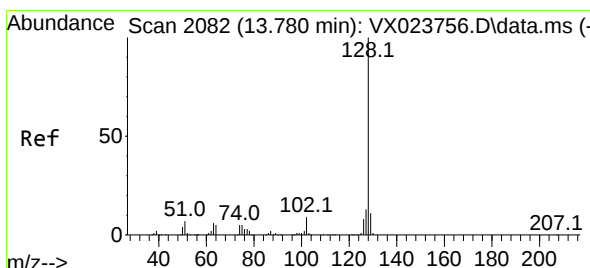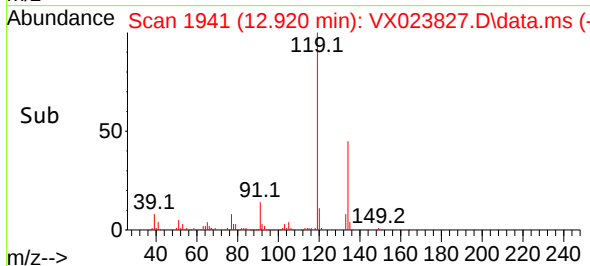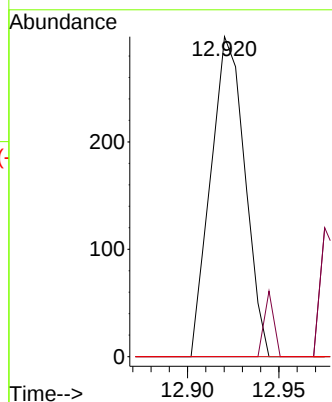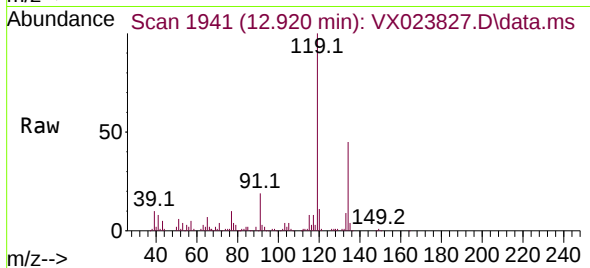

#95
Naphthalene
Concen: 3.996 ug/l
RT: 13.780 min Scan# 2082
Delta R.T. -0.000 min
Lab File: VX023827.D
Acq: 18 Aug 2021 19:22

Tgt Ion: 128 Resp: 16298
Ion Ratio Lower Upper
128 100
127 14.7 10.3 15.5
129 16.0 8.8 13.2#

