

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX081821\
 Data File : VX023828.D
 Acq On : 18 Aug 2021 19:46
 Operator : JC/MD
 Sample : M3414-01 10X
 Misc : 5.02g/10mL/100uL/5.00mL/MSVOA_X/MEOH
 ALS Vial : 26 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 B-1DL

Quant Time: Aug 19 04:22:11 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X081721W.M
 Quant Title : SW846 8260
 QLast Update : Tue Aug 17 11:57:51 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
Internal Standards						
1) Pentafluorobenzene	5.562	168	135935	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	6.769	114	230473	50.000	ug/l	0.00
63) Chlorobenzene-d5	10.055	117	218745	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	12.024	152	87258	50.000	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	5.964	65	95771	50.480	ug/l	0.00
Spiked Amount	50.000	Range	78 - 117	Recovery	= 100.960%	
35) Dibromofluoromethane	5.397	113	73295	48.048	ug/l	0.00
Spiked Amount	50.000	Range	75 - 124	Recovery	= 96.100%	
50) Toluene-d8	8.653	98	288439	49.680	ug/l	0.00
Spiked Amount	50.000	Range	92 - 112	Recovery	= 99.360%	
62) 4-Bromofluorobenzene	11.085	95	100812	47.168	ug/l	0.00
Spiked Amount	50.000	Range	83 - 123	Recovery	= 94.340%	
Target Compounds						
					Qvalue	
5) Bromomethane	1.611	94	627	0.649	ug/l #	37
6) Chloroethane	1.666	64	20	2.233	ug/l #	43
10) Methyl Iodide	2.465	142	801	0.422	ug/l #	93
11) Tert butyl alcohol	2.953	59	79	0.206	ug/l #	73
13) Acrolein	2.233	56	69	0.302	ug/l #	52
16) Acetone	2.392	43	871	1.027	ug/l	92
18) Methyl Acetate	2.715	43	488	0.230	ug/l #	64
20) Methylene Chloride	2.794	84	1344	0.829	ug/l	87
31) Cyclohexane	5.501	56	1646	0.675	ug/l #	38
36) 1,1-Dichloropropene	5.562	75	10576	4.955	ug/l #	51
38) Carbon Tetrachloride	5.562	117	13760	6.182	ug/l #	17
39) Methylcyclohexane	7.385	83	4940	1.901	ug/l	90
48) Methyl methacrylate	7.665	41	870	0.435	ug/l #	68
51) 4-Methyl-2-Pentanone	8.653	43	2404	0.906	ug/l #	1
55) 1,1,2-Trichloroethane	9.104	97	2314	1.374	ug/l #	19
56) Ethyl methacrylate	9.134	69	221	0.835	ug/l #	29
67) Ethyl Benzene	10.195	91	35671	4.475	ug/l	98
68) m/p-Xylenes	10.305	106	46456	15.301	ug/l	96
69) o-Xylene	10.646	106	709	0.238	ug/l	80
73) Isopropylbenzene	10.963	105	9107	1.368	ug/l	98
75) 1,1,2,2-Tetrachloroethane	11.195	83	540	0.248	ug/l #	78
76) 1,2,3-Trichloropropane	11.085	75	53915	26.487	ug/l #	39
78) n-propylbenzene	11.305	91	32915	4.324	ug/l	100
79) 2-Chlorotoluene	11.402	91	8690	1.889	ug/l #	41
80) 1,3,5-Trimethylbenzene	11.457	105	52406	9.581	ug/l	99
81) trans-1,4-Dichloro-2-b...	11.085	75	53915	77.914	ug/l #	12
82) 4-Chlorotoluene	11.451	91	6109	1.170	ug/l #	47
83) tert-Butylbenzene	11.756	119	22822	4.296	ug/l #	50
84) 1,2,4-Trimethylbenzene	11.756	105	188967	34.650	ug/l	100
85) sec-Butylbenzene	11.896	105	6532	0.971	ug/l	90
86) p-Isopropyltoluene	12.012	119	4028	0.728	ug/l	84
89) n-Butylbenzene	12.329	91	24817	5.021	ug/l #	34
90) Hexachloroethane	12.536	117	3771	5.260	ug/l #	9
92) 1,2-Dibromo-3-Chloropr...	12.926	75	310	2.742	ug/l #	1
95) Naphthalene	13.780	128	40533	7.470	ug/l	97

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX081821\
Data File : VX023828.D
Acq On : 18 Aug 2021 19:46
Operator : JC/MD
Sample : M3414-01 10X
Misc : 5.02g/10mL/100uL/5.00mL/MSVOA_X/MEOH
ALS Vial : 26 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
B-1DL

Quant Time: Aug 19 04:22:11 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X081721W.M
Quant Title : SW846 8260
QLast Update : Tue Aug 17 11:57:51 2021
Response via : Initial Calibration


Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
----------	------	------	----------	------	-------	----------


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX081821\
 Data File : VX023828.D
 Acq On : 18 Aug 2021 19:46
 Operator : JC/MD
 Sample : M3414-01 10X
 Misc : 5.02g/10mL/100uL/5.00mL/MSVOA_X/MEOH
 ALS Vial : 26 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 B-1DL


Quant Time: Aug 19 04:22:11 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X081721W.M
 Quant Title : SW846 8260
 QLast Update : Tue Aug 17 11:57:51 2021
 Response via : Initial Calibration

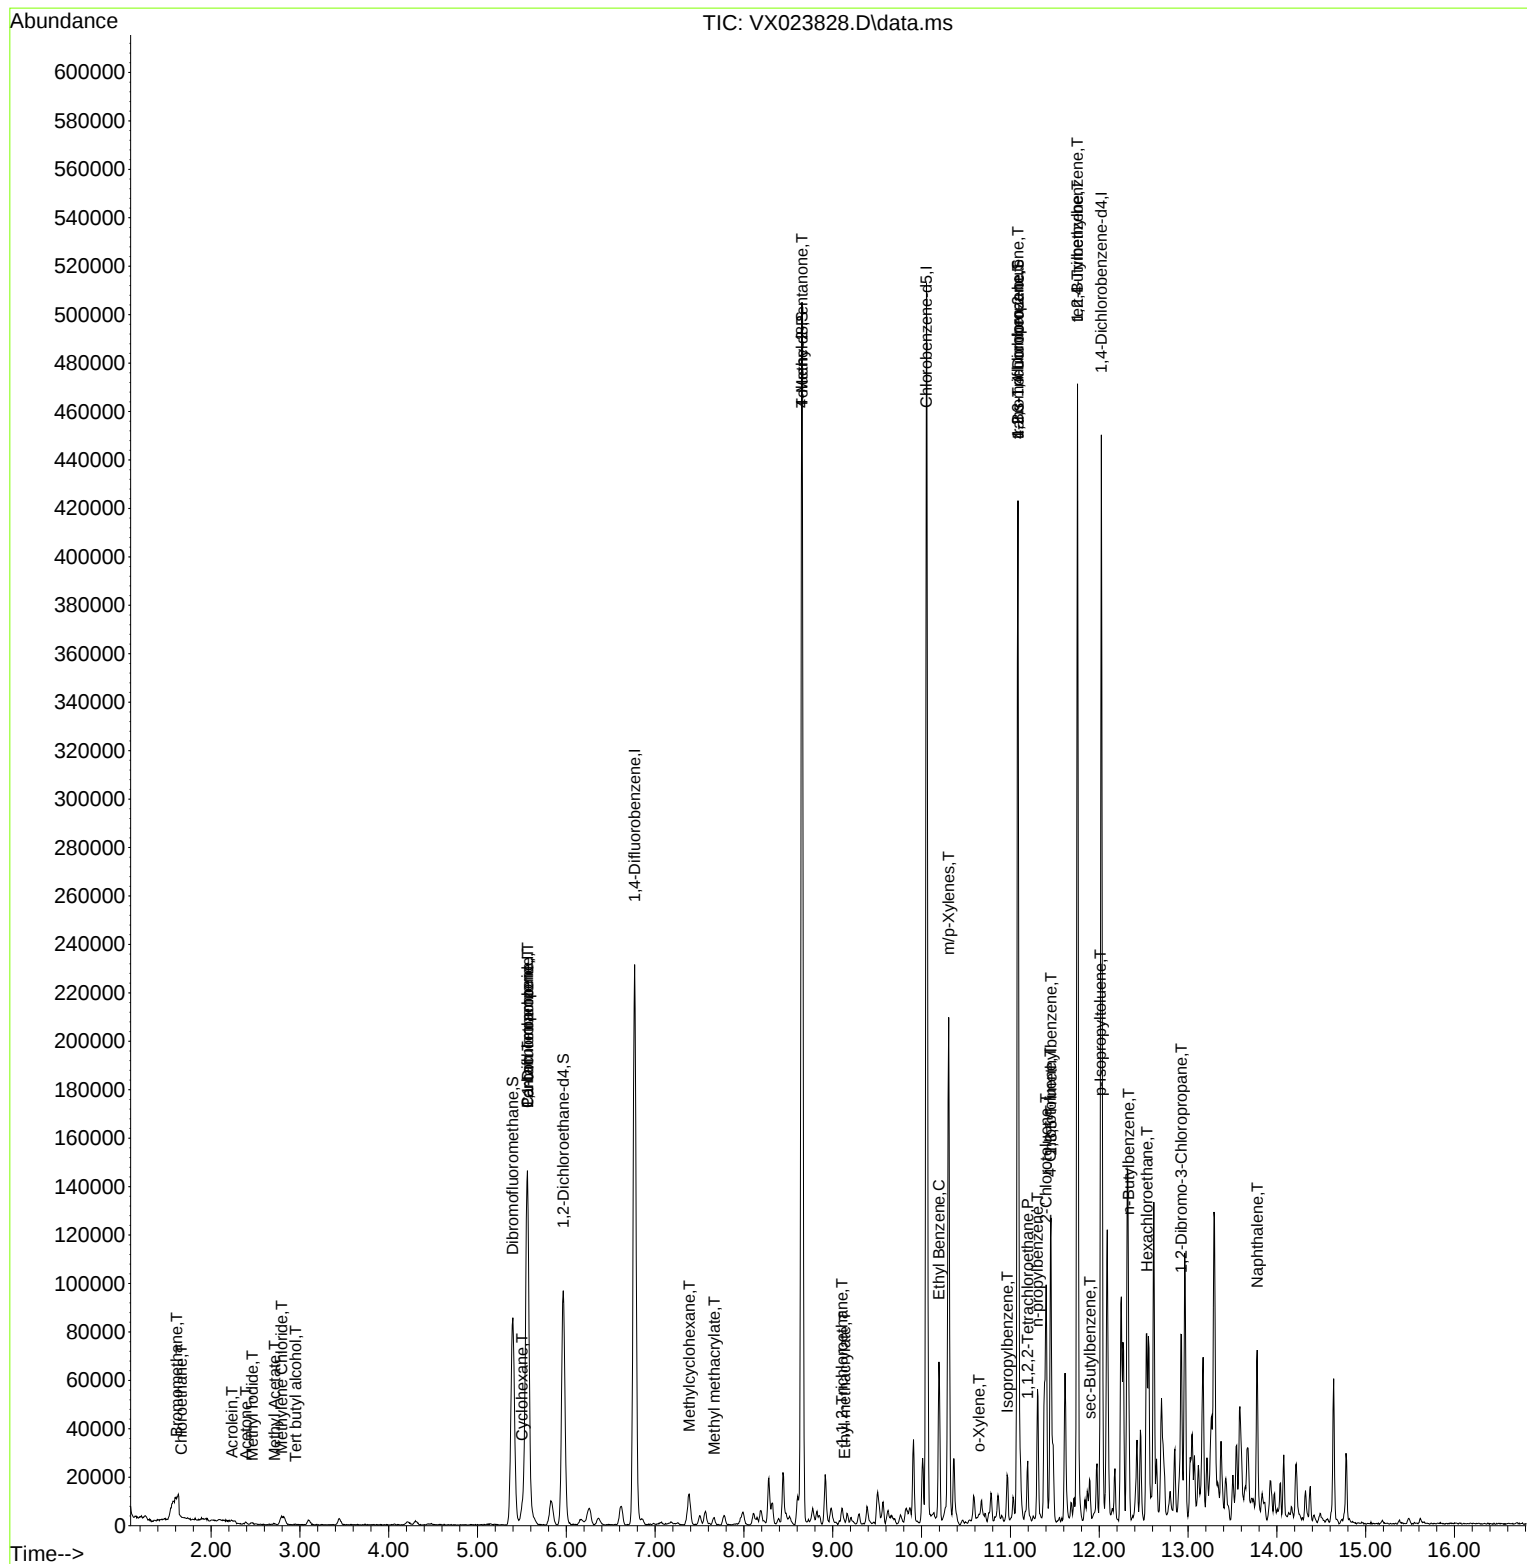






#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 5.562 min Scan# 734
Delta R.T. -0.000 min
Lab File: VX023828.D
Acq: 18 Aug 2021 19:46


Instrument :
MSVOA_X
ClientSampled :
B-1DL





Tgt Ion:168 Resp: 135935
Ion Ratio Lower Upper
168 100
99 55.0 45.8 68.6

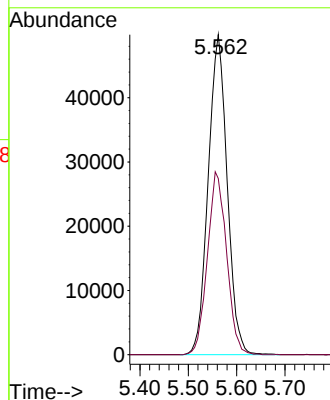


#5
Bromomethane
Concen: 0.649 ug/l
RT: 1.611 min Scan# 86
Delta R.T. 0.012 min
Lab File: VX023828.D
Acq: 18 Aug 2021 19:46

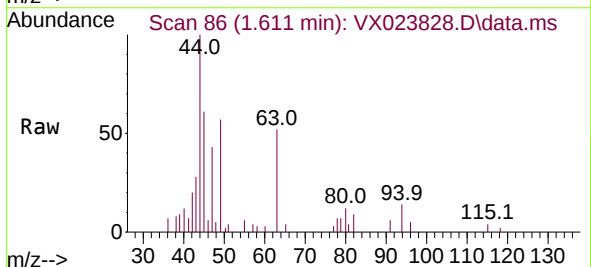

Tgt Ion: 94 Resp: 627
Ion Ratio Lower Upper
94 100
96 34.6 76.4 114.6#



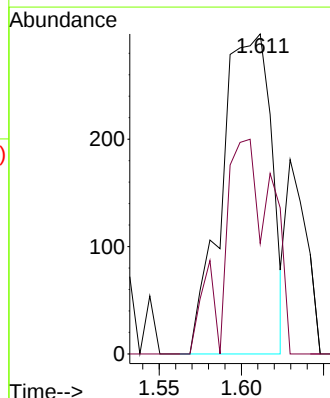



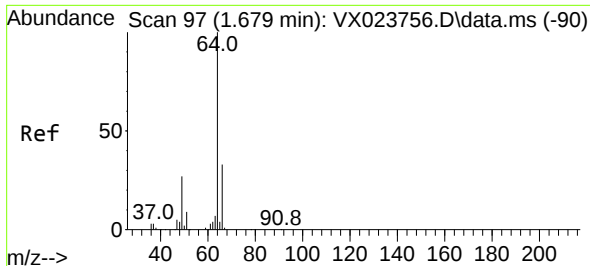

#6
Chloroethane
Concen: 2.233 ug/l
RT: 1.666 min Scan# 95
Delta R.T. -0.013 min
Lab File: VX023828.D
Acq: 18 Aug 2021 19:46




Instrument :
MSVOA_X
ClientSampled :
B-1DL


Tgt Ion: 64 Resp: 20
Ion Ratio Lower Upper
64 100
66 0.0 25.4 38.0#

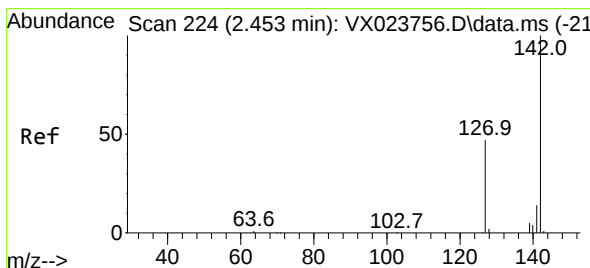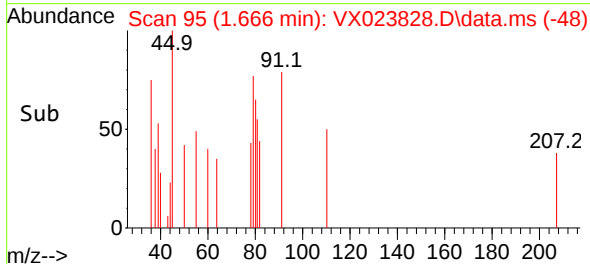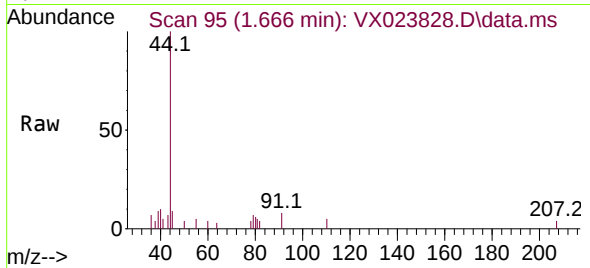

#10
Methyl Iodide
Concen: 0.422 ug/l
RT: 2.465 min Scan# 226
Delta R.T. 0.012 min
Lab File: VX023828.D
Acq: 18 Aug 2021 19:46

Tgt Ion: 142 Resp: 801
Ion Ratio Lower Upper
142 100
127 40.2 33.3 49.9
141 6.0 11.4 17.0#


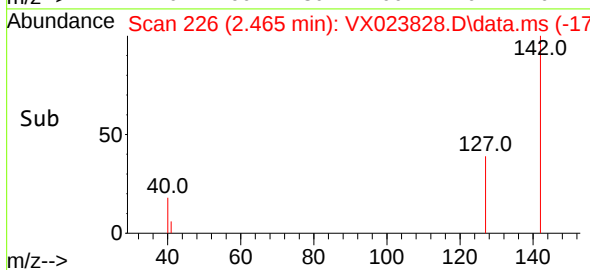

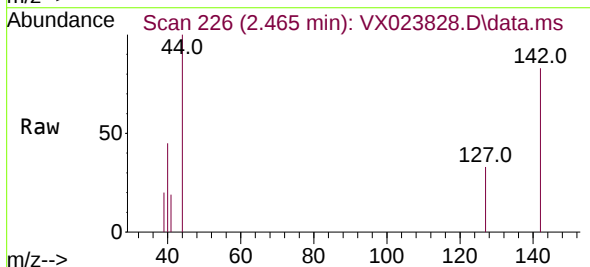




#11
Tert butyl alcohol
Concen: 0.206 ug/l
RT: 2.953 min Scan# 306
Delta R.T. -0.030 min
Lab File: VX023828.D
Acq: 18 Aug 2021 19:46




Instrument :
MSVOA_X
ClientSampled :
B-1DL


Tgt Ion: 59 Resp: 79
Ion Ratio Lower Upper
59 100
57 0.0 7.8 11.8#

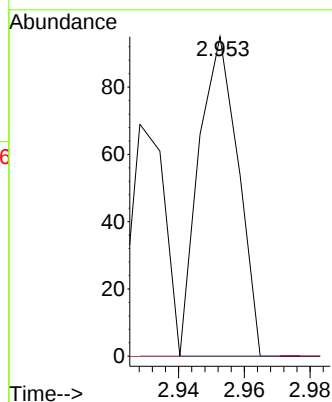

#13
Acrolein
Concen: 0.302 ug/l
RT: 2.233 min Scan# 188
Delta R.T. -0.012 min
Lab File: VX023828.D
Acq: 18 Aug 2021 19:46

Tgt Ion: 56 Resp: 69
Ion Ratio Lower Upper
56 100
55 110.1 56.4 84.6#


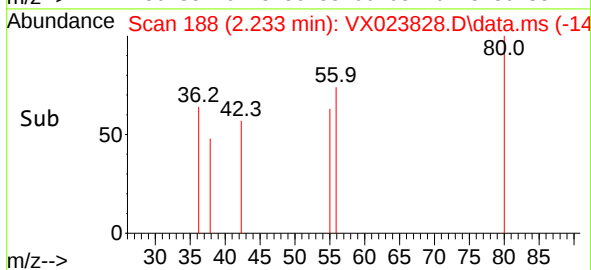
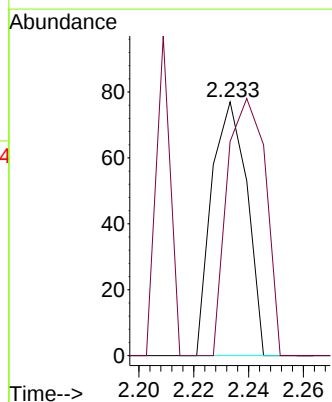



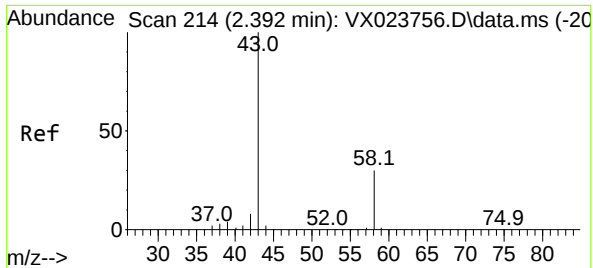

#16
Acetone
Concen: 1.027 ug/l
RT: 2.392 min Scan# 214
Delta R.T. -0.000 min
Lab File: VX023828.D
Acq: 18 Aug 2021 19:46




Instrument :
MSVOA_X
ClientSampled :
B-1DL


Tgt Ion	Ratio	Lower	Upper
43	100		
58	29.9	27.8	41.8

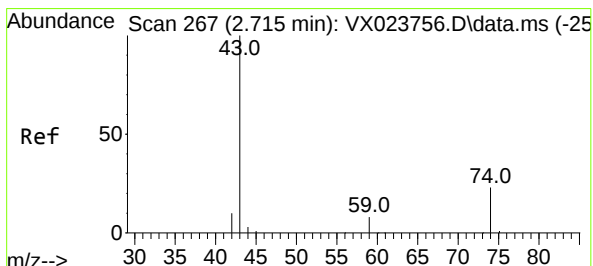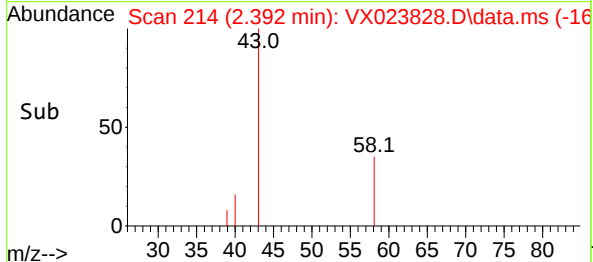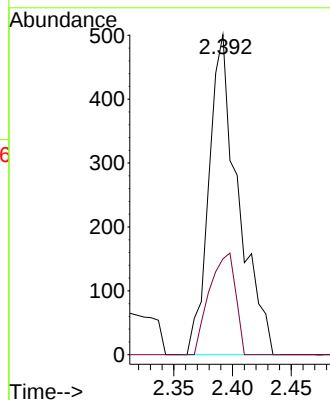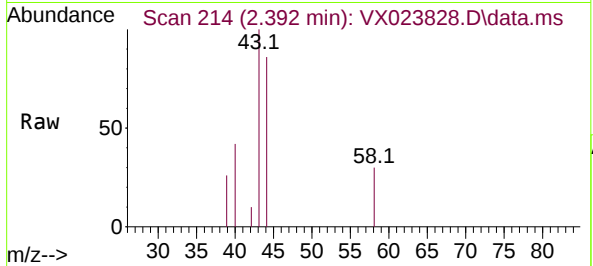

#18
Methyl Acetate
Concen: 0.230 ug/l
RT: 2.715 min Scan# 267
Delta R.T. -0.000 min
Lab File: VX023828.D
Acq: 18 Aug 2021 19:46

Tgt Ion	Ratio	Lower	Upper
43	100		
74	8.8	21.9	32.9#


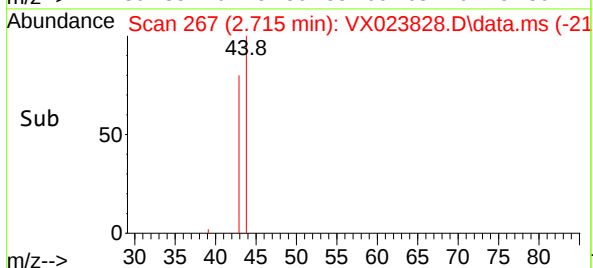
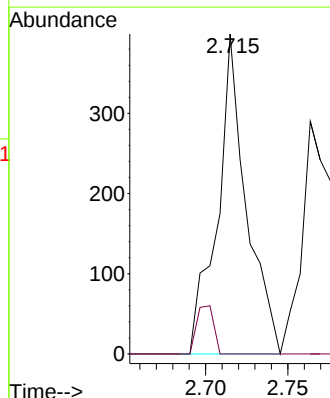
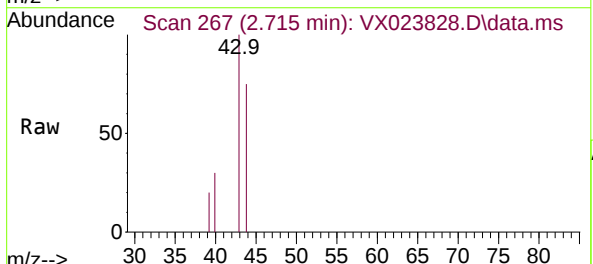




#20
Methylene Chloride
Concen: 0.829 ug/l
RT: 2.794 min Scan# 280
Delta R.T. 0.000 min
Lab File: VX023828.D
Acq: 18 Aug 2021 19:46




Instrument :
MSVOA_X
ClientSampled :
B-1DL


Tgt Ion:	84	Resp:	1344
Ion	Ratio	Lower	Upper
84	100		
49	127.8	88.6	132.8
51	32.3	27.0	40.6
86	72.2	50.3	75.5



#31
Cyclohexane
Concen: 0.675 ug/l
RT: 5.501 min Scan# 724
Delta R.T. 0.024 min
Lab File: VX023828.D
Acq: 18 Aug 2021 19:46

Tgt Ion:	56	Resp:	1646
Ion	Ratio	Lower	Upper
56	100		
69	7.5	25.3	37.9#
84	24.8	71.4	107.0#

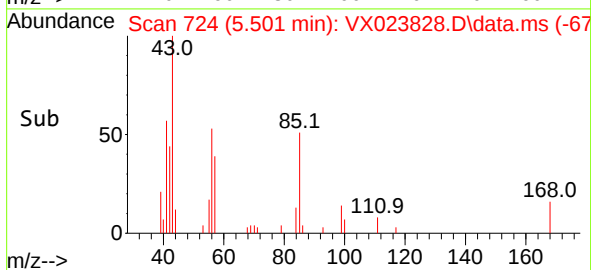



#33

1,2-Dichloroethane-d4

Concen: 50.480 ug/l

RT: 5.964 min Scan# 800

Delta R.T. 0.000 min

Lab File: VX023828.D

Acq: 18 Aug 2021 19:46

Tgt Ion: 65 Resp: 95771

Ion Ratio Lower Upper

65 100





67 50.7 0.0 105.4

Instrument :

MSVOA_X

ClientSampleId :

B-1DL

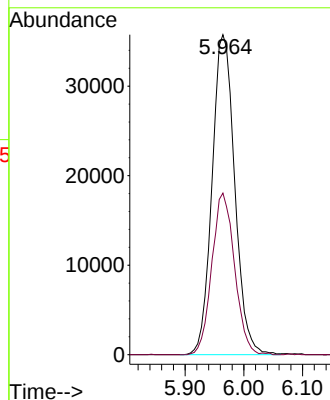

#34

1,4-Difluorobenzene

Concen: 50.000 ug/l

RT: 6.769 min Scan# 932

Delta R.T. -0.000 min

Lab File: VX023828.D

Acq: 18 Aug 2021 19:46




Tgt Ion: 114 Resp: 230473


Ion Ratio Lower Upper

114 100

63 20.5 0.0 40.8

88 16.2 0.0 32.8


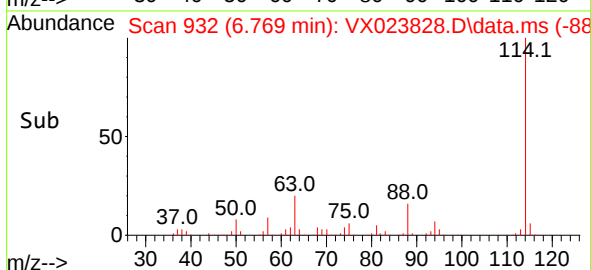
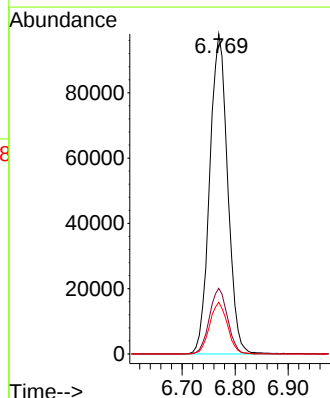



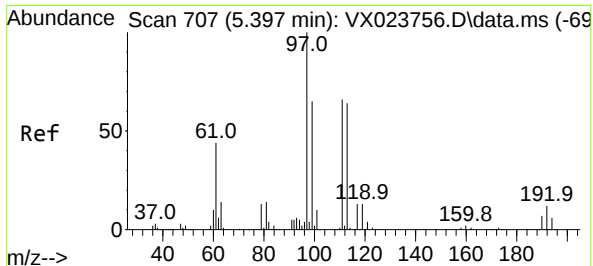

#35
Dibromofluoromethane
Concen: 48.048 ug/l
RT: 5.397 min Scan# 707
Delta R.T. 0.000 min
Lab File: VX023828.D
Acq: 18 Aug 2021 19:46




Instrument :
MSVOA_X
ClientSampled :
B-1DL


Tgt Ion:	113	Resp:	73295
Ion	Ratio	Lower	Upper
113	100		
111	102.2	81.9	122.9
192	19.3	16.7	25.1

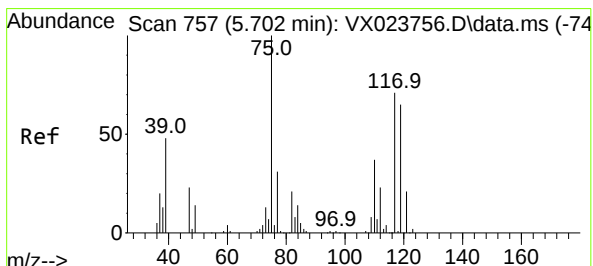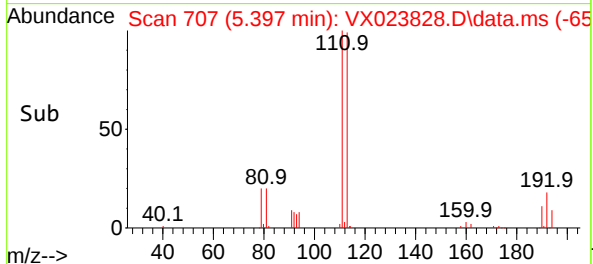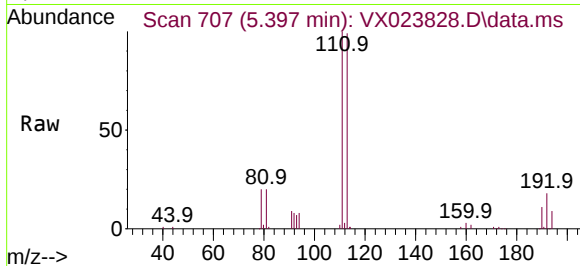

#36
1,1-Dichloropropene
Concen: 4.955 ug/l
RT: 5.562 min Scan# 734
Delta R.T. -0.140 min
Lab File: VX023828.D
Acq: 18 Aug 2021 19:46


Tgt Ion:	75	Resp:	10576
Ion	Ratio	Lower	Upper
75	100		
110	11.3	18.1	54.4#
77	0.0	25.3	37.9#

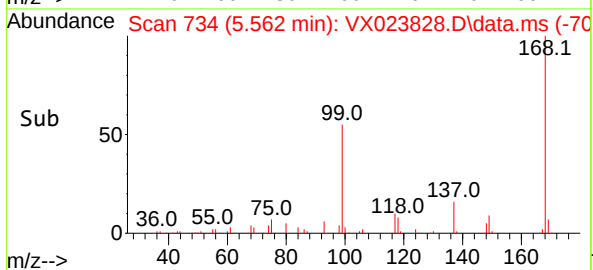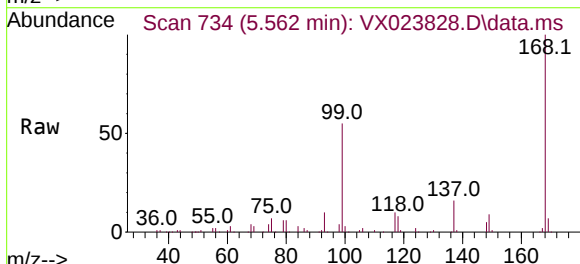



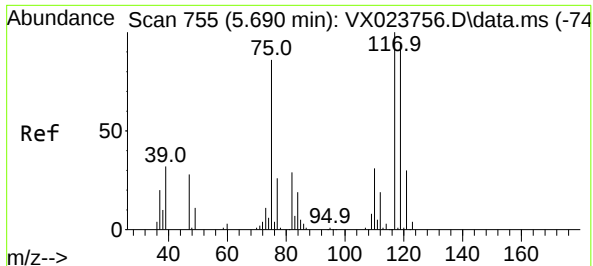


#38
Carbon Tetrachloride
Concen: 6.182 ug/l
RT: 5.562 min Scan# 734
Delta R.T. -0.128 min
Lab File: VX023828.D
Acq: 18 Aug 2021 19:46

Instrument :
MSVOA_X
ClientSampled :
B-1DL



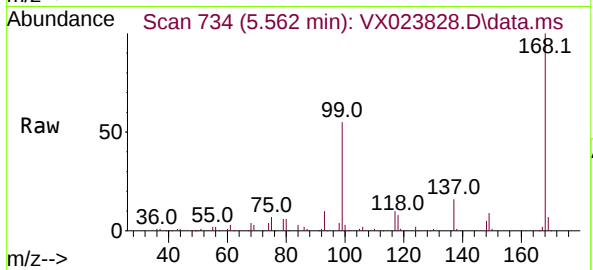



Tgt Ion:117 Resp: 13760
Ion Ratio Lower Upper
117 100
119 6.0 76.2 114.2#
121 0.0 24.8 37.2#

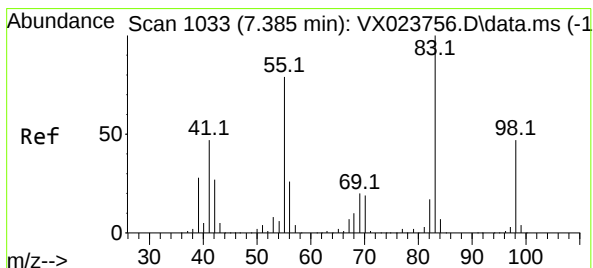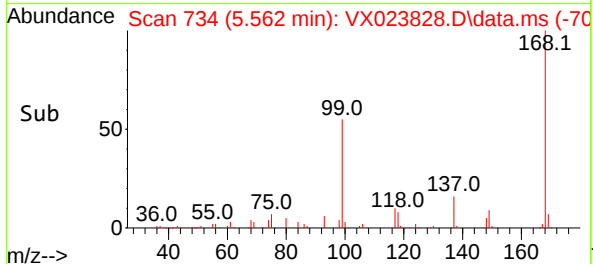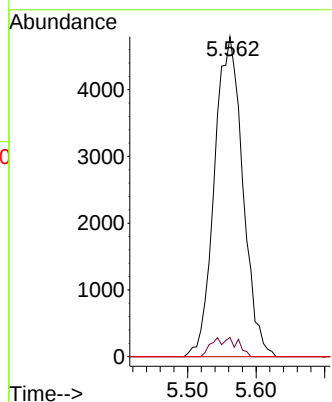

#39
Methylcyclohexane
Concen: 1.901 ug/l
RT: 7.385 min Scan# 1033
Delta R.T. -0.000 min
Lab File: VX023828.D
Acq: 18 Aug 2021 19:46

Tgt Ion: 83 Resp: 4940
Ion Ratio Lower Upper
83 100
55 86.6 58.9 88.3
98 48.6 38.1 57.1


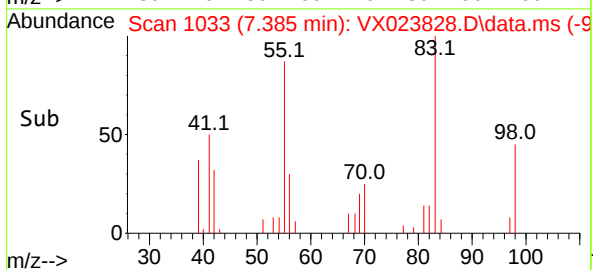
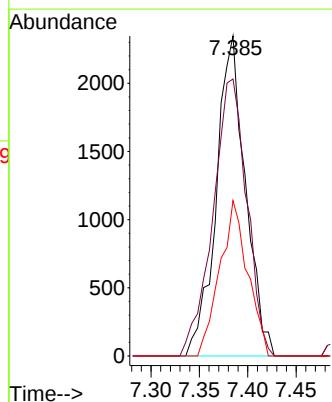
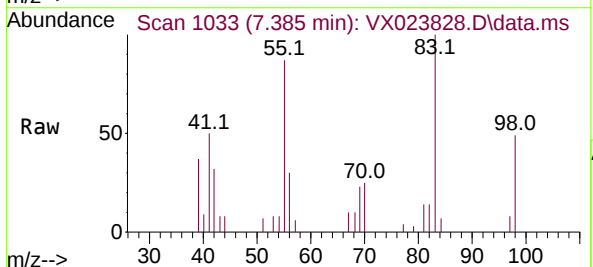


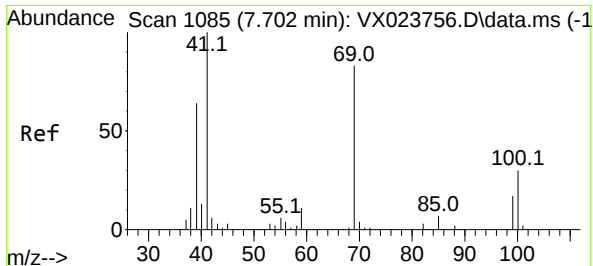

#48
Methyl methacrylate
Concen: 0.435 ug/l
RT: 7.665 min Scan# 1079
Delta R.T. -0.037 min
Lab File: VX023828.D
Acq: 18 Aug 2021 19:46




Instrument :
MSVOA_X
ClientSampled :
B-1DL


Tgt Ion: 41 Resp: 870
Ion Ratio Lower Upper
41 100
69 117.4 76.0 114.0#
39 90.3 44.6 67.0#

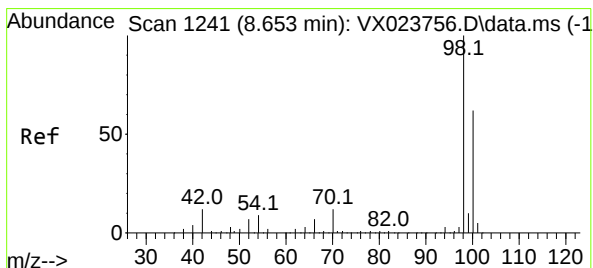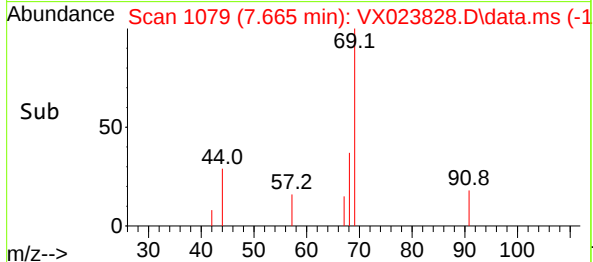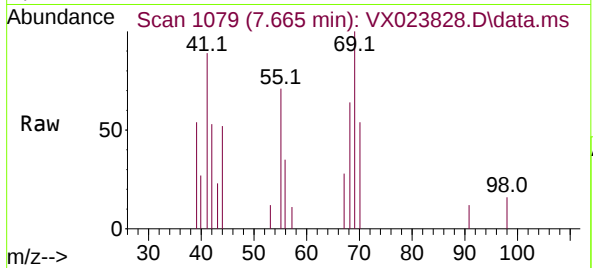

#50
Toluene-d8
Concen: 49.680 ug/l
RT: 8.653 min Scan# 1241
Delta R.T. -0.000 min
Lab File: VX023828.D
Acq: 18 Aug 2021 19:46

Tgt Ion: 98 Resp: 288439
Ion Ratio Lower Upper
98 100
100 63.6 51.9 77.9


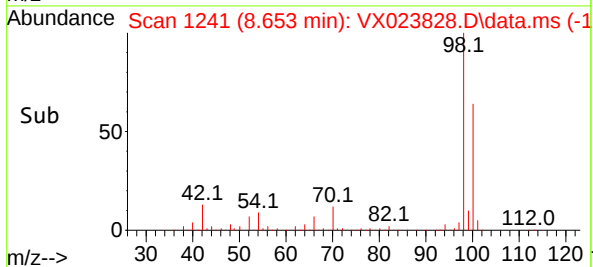

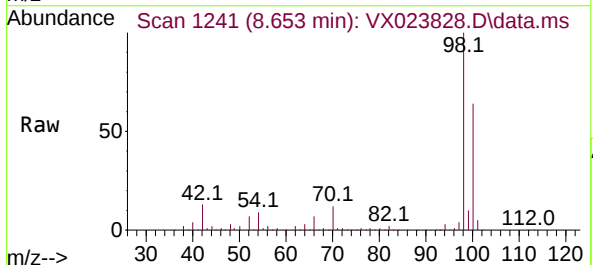


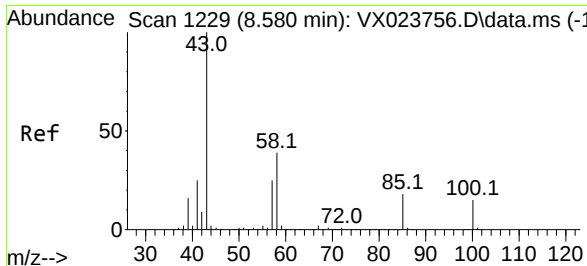

#51
4-Methyl-2-Pentanone
Concen: 0.906 ug/l
RT: 8.653 min Scan# 1241
Delta R.T. 0.073 min
Lab File: VX023828.D
Acq: 18 Aug 2021 19:46




Instrument :
MSVOA_X
ClientSampled :
B-1DL


Tgt Ion: 43 Resp: 2404
Ion Ratio Lower Upper
43 100
58 109.2 35.4 53.0#

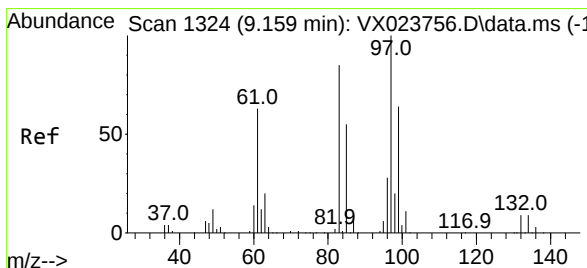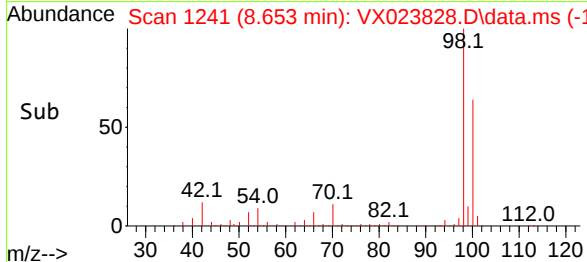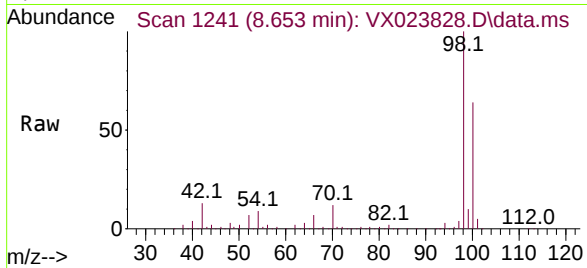

#55
1,1,2-Trichloroethane
Concen: 1.374 ug/l
RT: 9.104 min Scan# 1315
Delta R.T. -0.055 min
Lab File: VX023828.D
Acq: 18 Aug 2021 19:46

Tgt Ion: 97 Resp: 2314
Ion Ratio Lower Upper
97 100
83 9.5 69.3 103.9#
85 0.0 44.3 66.5#
99 0.0 50.3 75.5#

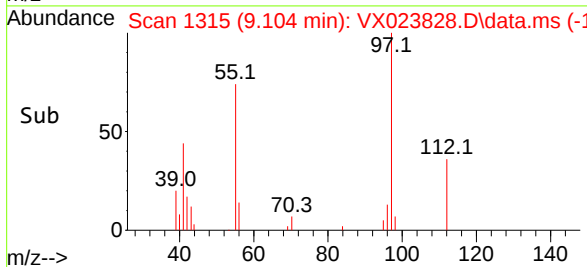
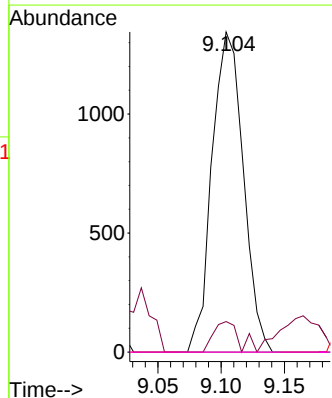
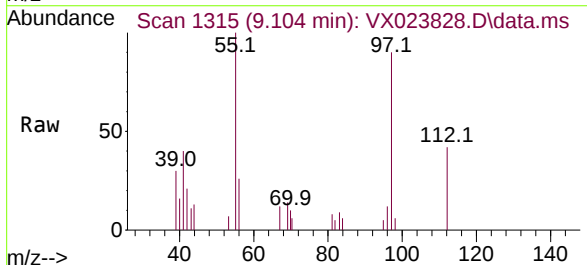


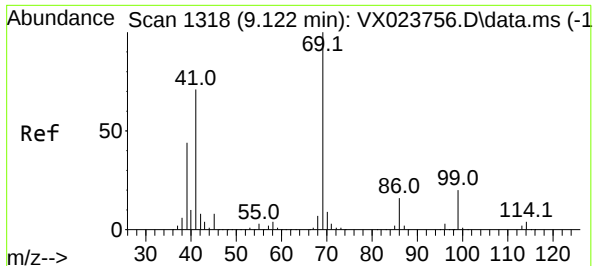

#56
Ethyl methacrylate
Concen: 0.835 ug/l
RT: 9.134 min Scan# 1320
Delta R.T. 0.012 min
Lab File: VX023828.D
Acq: 18 Aug 2021 19:46




Instrument :
MSVOA_X
ClientSampled :
B-1DL


Tgt Ion: 69	Resp: 221
Ion Ratio	Lower Upper
69	100
41	0.0 46.8 70.2#
39	0.0 24.7 37.1#

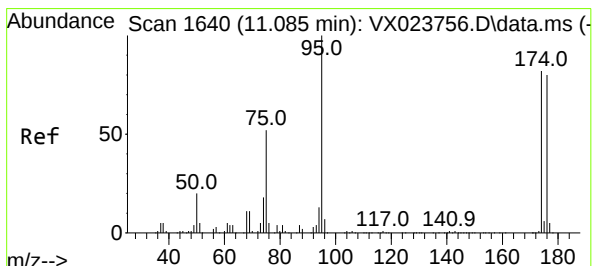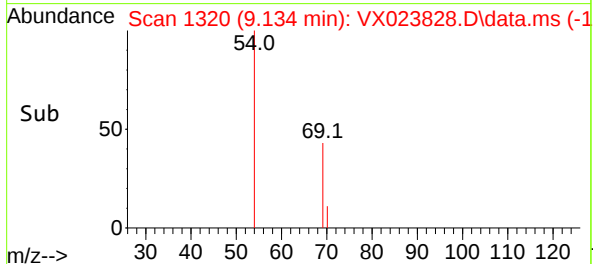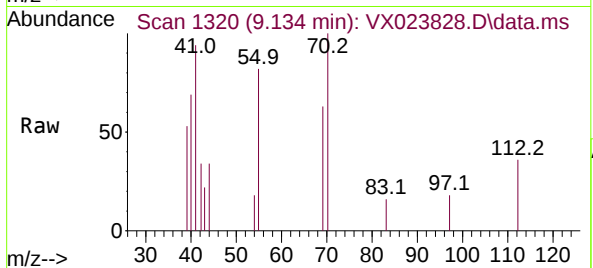

#62
4-Bromofluorobenzene
Concen: 47.168 ug/l
RT: 11.085 min Scan# 1640
Delta R.T. 0.000 min
Lab File: VX023828.D
Acq: 18 Aug 2021 19:46

Tgt Ion: 95	Resp: 100812
Ion Ratio	Lower Upper
95	100
174	79.9 0.0 154.6
176	76.5 0.0 155.8


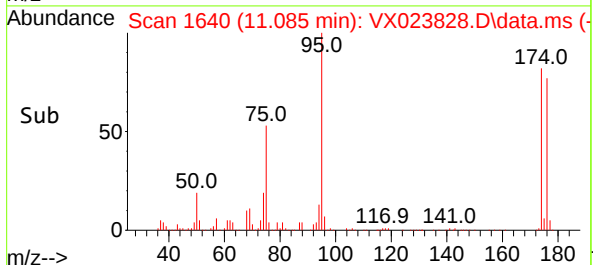

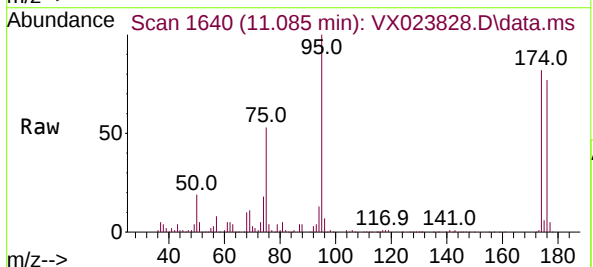




#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 10.055 min Scan# 1471
Delta R.T. -0.006 min
Lab File: VX023828.D
Acq: 18 Aug 2021 19:46




Instrument :
MSVOA_X
ClientSampled :
B-1DL


Tgt Ion:117 Resp: 218745
Ion Ratio Lower Upper
117 100
82 58.3 47.4 71.2
119 33.6 26.6 39.8

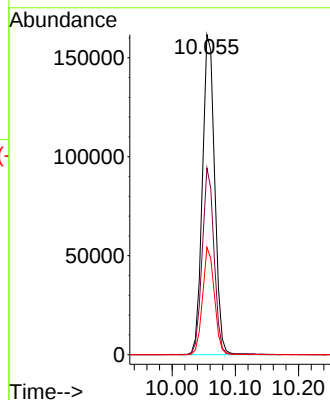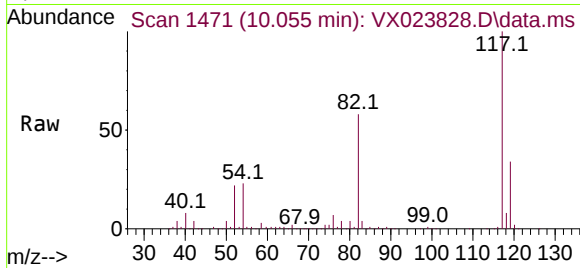

#67
Ethyl Benzene
Concen: 4.475 ug/l
RT: 10.195 min Scan# 1494
Delta R.T. 0.000 min
Lab File: VX023828.D
Acq: 18 Aug 2021 19:46

Tgt Ion: 91 Resp: 35671
Ion Ratio Lower Upper
91 100
106 31.7 24.6 37.0



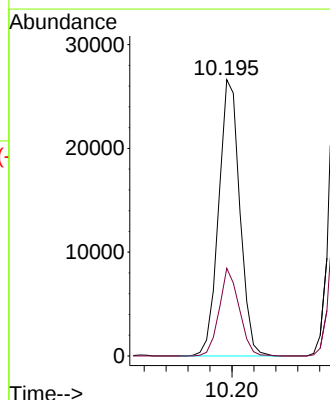
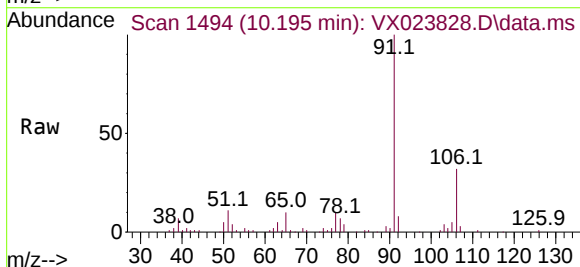




#68
m/p-Xylenes
Concen: 15.301 ug/l
RT: 10.305 min Scan# 1512
Delta R.T. -0.000 min
Lab File: VX023828.D
Acq: 18 Aug 2021 19:46




Instrument :
MSVOA_X
ClientSampleId :
B-1DL


Tgt Ion:106 Resp: 46456
Ion Ratio Lower Upper
106 100
91 209.2 162.8 244.2

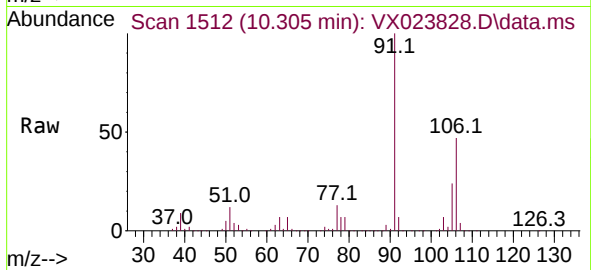

#69
o-Xylene
Concen: 0.238 ug/l
RT: 10.646 min Scan# 1568
Delta R.T. 0.000 min
Lab File: VX023828.D
Acq: 18 Aug 2021 19:46

Tgt Ion:106 Resp: 709
Ion Ratio Lower Upper
106 100
91 248.7 108.1 324.2


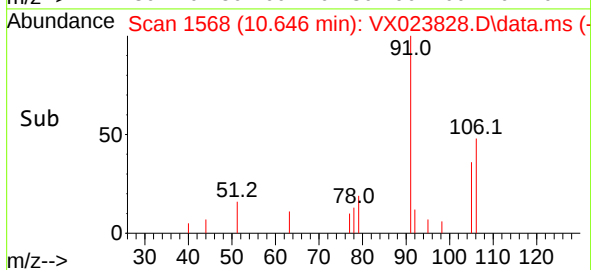

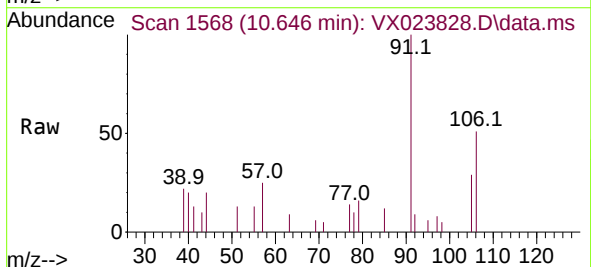




#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 12.024 min Scan# 1794
Delta R.T. 0.000 min
Lab File: VX023828.D
Acq: 18 Aug 2021 19:46




Instrument :
MSVOA_X
ClientSampled :
B-1DL


Tgt Ion:152 Resp: 87258
Ion Ratio Lower Upper
152 100
115 58.9 41.1 123.3
150 156.3 0.0 349.0

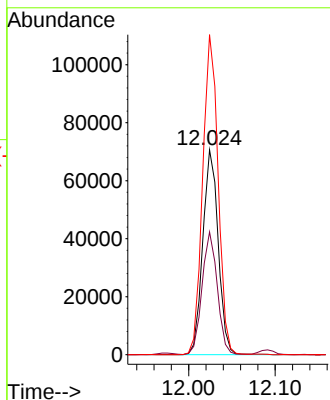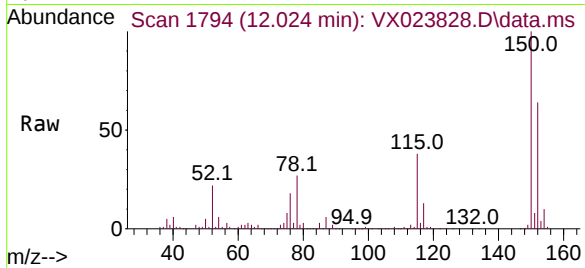

#73
Isopropylbenzene
Concen: 1.368 ug/l
RT: 10.963 min Scan# 1620
Delta R.T. 0.000 min
Lab File: VX023828.D
Acq: 18 Aug 2021 19:46

Tgt Ion:105 Resp: 9107
Ion Ratio Lower Upper
105 100
120 27.5 13.2 39.6


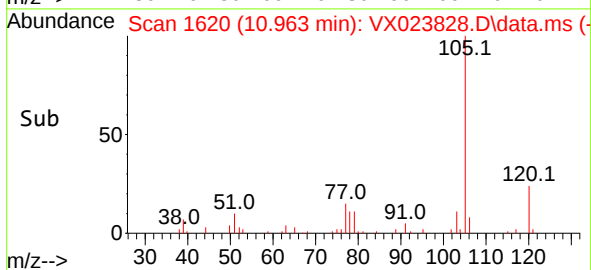
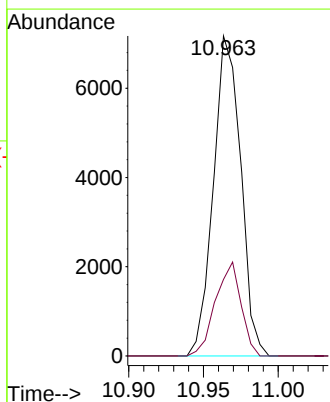
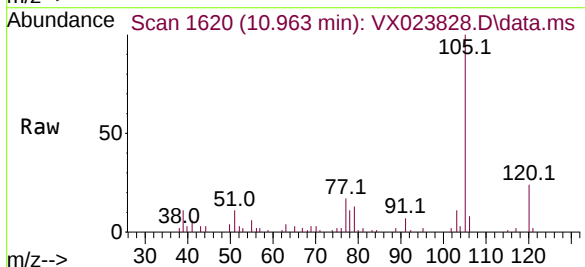




#75
1,1,2,2-Tetrachloroethane
Concen: 0.248 ug/l
RT: 11.195 min Scan# 1658
Delta R.T. -0.018 min
Lab File: VX023828.D
Acq: 18 Aug 2021 19:46




Instrument :
MSVOA_X
ClientSampled :
B-1DL


Tgt Ion: 83 Resp: 540
Ion Ratio Lower Upper
83 100
131 0.0 5.1 15.2#
85 80.0 31.8 95.4

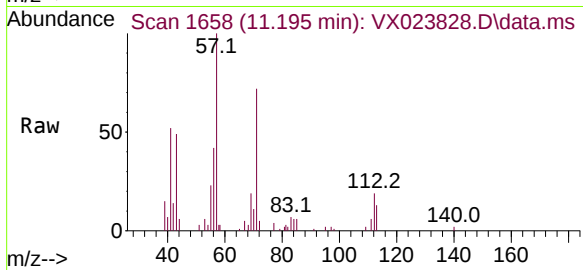

#76
1,2,3-Trichloropropane
Concen: 26.487 ug/l
RT: 11.085 min Scan# 1640
Delta R.T. -0.159 min
Lab File: VX023828.D
Acq: 18 Aug 2021 19:46

Tgt Ion: 75 Resp: 53915
Ion Ratio Lower Upper
75 100
77 1.4 19.1 57.5#




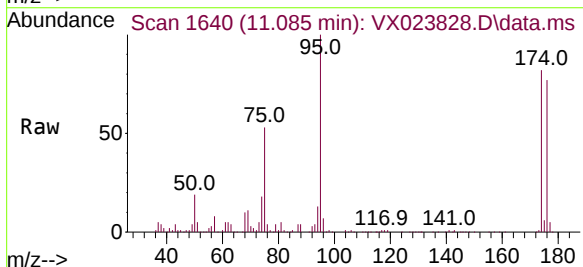




#78
n-propylbenzene
Concen: 4.324 ug/l
RT: 11.305 min Scan# 1676
Delta R.T. -0.000 min
Lab File: VX023828.D
Acq: 18 Aug 2021 19:46




Instrument :
MSVOA_X
ClientSampled :
B-1DL


Tgt Ion: 91 Resp: 32915
Ion Ratio Lower Upper
91 100
120 22.9 11.5 34.5

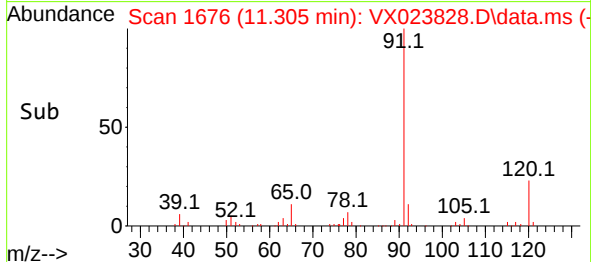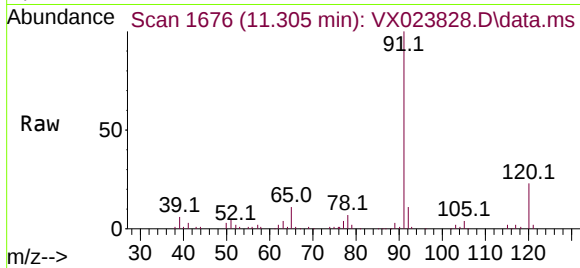

#79
2-Chlorotoluene
Concen: 1.889 ug/l
RT: 11.402 min Scan# 1692
Delta R.T. 0.036 min
Lab File: VX023828.D
Acq: 18 Aug 2021 19:46

Tgt Ion: 91 Resp: 8690
Ion Ratio Lower Upper
91 100
126 0.0 16.6 49.8#


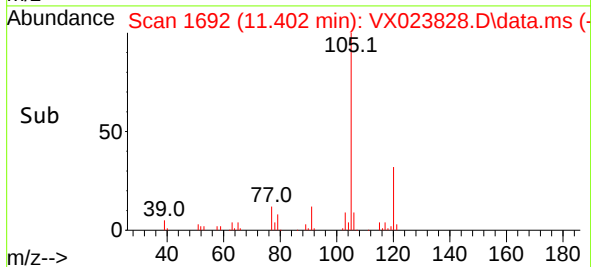

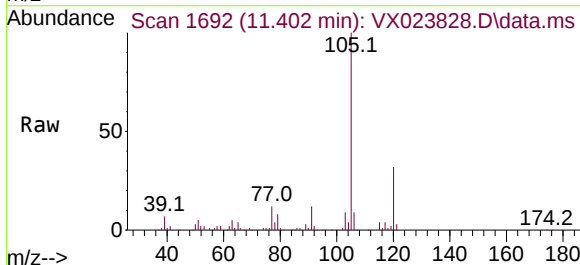




#80
1,3,5-Trimethylbenzene
Concen: 9.581 ug/l
RT: 11.457 min Scan# 1701
Delta R.T. 0.006 min
Lab File: VX023828.D
Acq: 18 Aug 2021 19:46




Instrument :
MSVOA_X
ClientSampled :
B-1DL


Tgt Ion:105 Resp: 52406
Ion Ratio Lower Upper
105 100
120 48.2 23.8 71.5

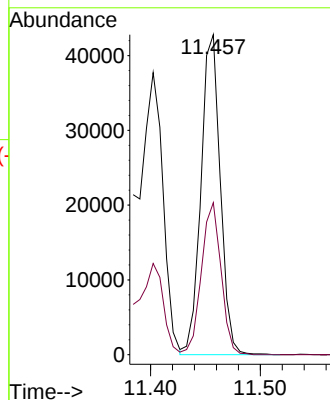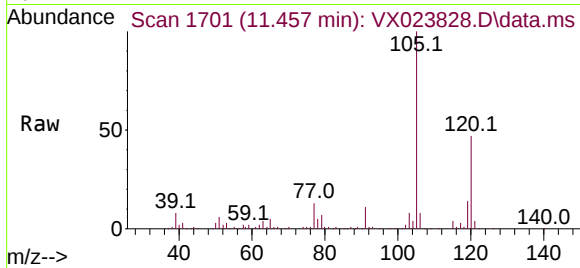

#81
trans-1,4-Dichloro-2-butene
Concen: 77.914 ug/l
RT: 11.085 min Scan# 1640
Delta R.T. 0.061 min
Lab File: VX023828.D
Acq: 18 Aug 2021 19:46

Tgt Ion: 75 Resp: 53915
Ion Ratio Lower Upper
75 100
53 0.5 74.5 111.7#
89 0.0 37.9 56.9#


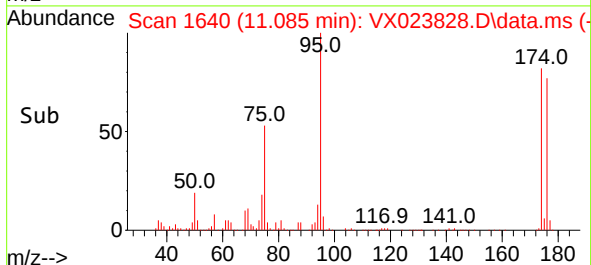
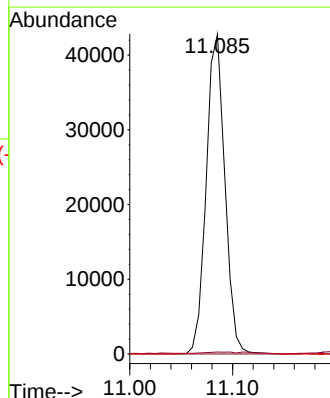
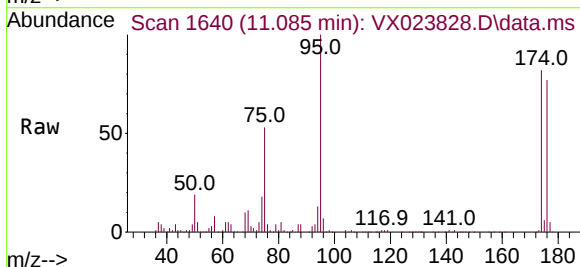




#82
4-Chlorotoluene
Concen: 1.170 ug/l
RT: 11.451 min Scan# 1700
Delta R.T. -0.006 min
Lab File: VX023828.D
Acq: 18 Aug 2021 19:46




Instrument :
MSVOA_X
ClientSampleId :
B-1DL


Tgt Ion: 91 Resp: 6109
Ion Ratio Lower Upper
91 100
126 1.1 14.9 44.5#

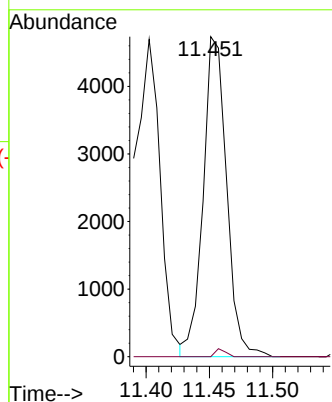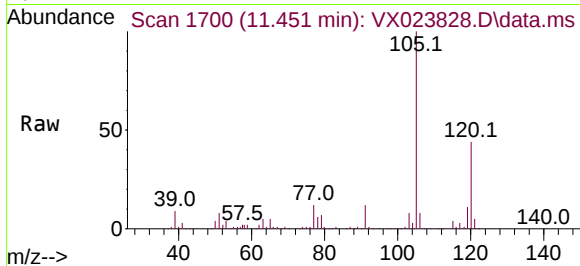

#83
tert-Butylbenzene
Concen: 4.296 ug/l
RT: 11.756 min Scan# 1750
Delta R.T. 0.037 min
Lab File: VX023828.D
Acq: 18 Aug 2021 19:46

Tgt Ion: 119 Resp: 22822
Ion Ratio Lower Upper
119 100
91 93.2 27.9 83.7#
134 0.5 11.3 33.9#


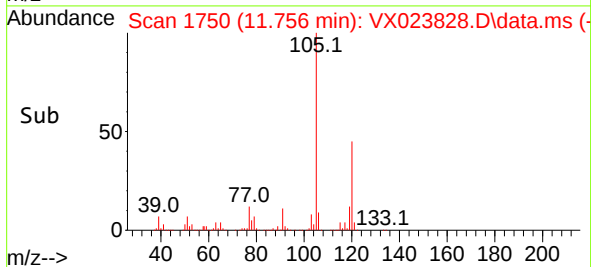

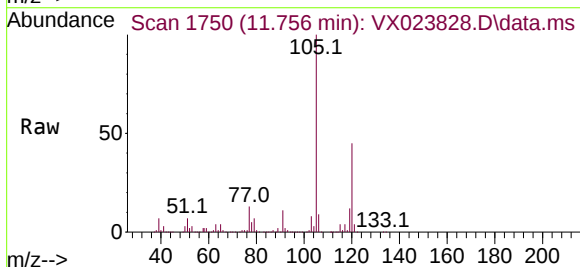




#84
1,2,4-Trimethylbenzene
Concen: 34.650 ug/l
RT: 11.756 min Scan# 1750
Delta R.T. -0.000 min
Lab File: VX023828.D
Acq: 18 Aug 2021 19:46




Instrument :
MSVOA_X
ClientSampled :
B-1DL


Tgt Ion:105 Resp: 188967
Ion Ratio Lower Upper
105 100
120 45.0 22.4 67.3

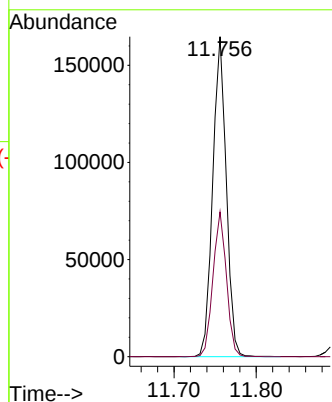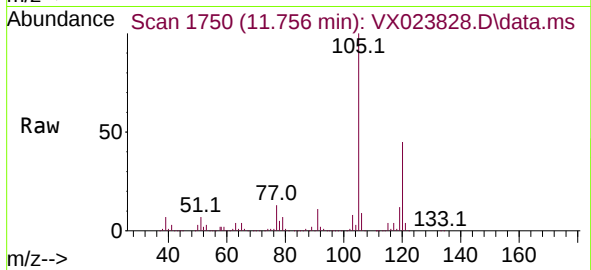

#85
sec-Butylbenzene
Concen: 0.971 ug/l
RT: 11.896 min Scan# 1773
Delta R.T. 0.000 min
Lab File: VX023828.D
Acq: 18 Aug 2021 19:46

Tgt Ion:105 Resp: 6532
Ion Ratio Lower Upper
105 100
134 15.1 10.0 29.8




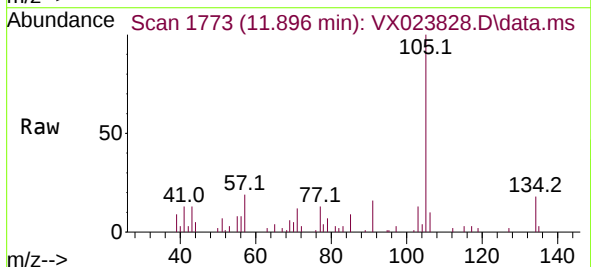




#86
p-Isopropyltoluene
Concen: 0.728 ug/l
RT: 12.012 min Scan# 1792
Delta R.T. -0.000 min
Lab File: VX023828.D
Acq: 18 Aug 2021 19:46




Instrument :
MSVOA_X
ClientSampled :
B-1DL


Tgt Ion:	119	Resp:	4028
Ion	Ratio	Lower	Upper
119	100		
134	31.4	12.9	38.7
91	33.5	11.7	35.0

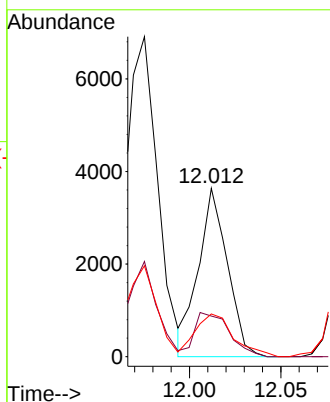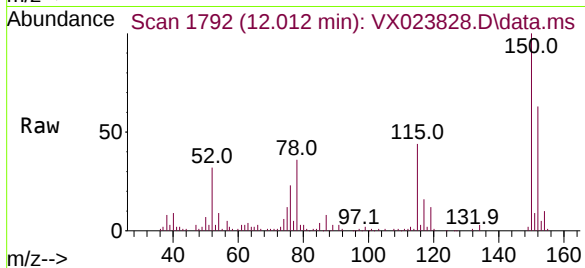

#89
n-Butylbenzene
Concen: 5.021 ug/l
RT: 12.329 min Scan# 1844
Delta R.T. -0.006 min
Lab File: VX023828.D
Acq: 18 Aug 2021 19:46

Tgt Ion:	91	Resp:	24817
Ion	Ratio	Lower	Upper
91	100		
92	33.5	27.4	82.0
134	99.3	13.2	39.5#


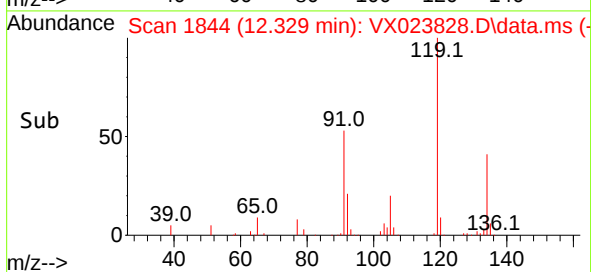
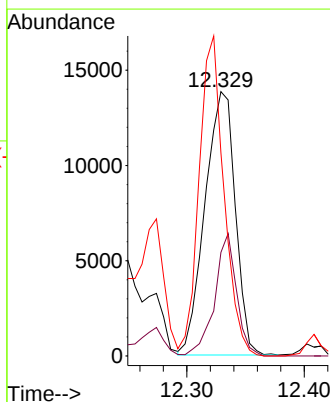
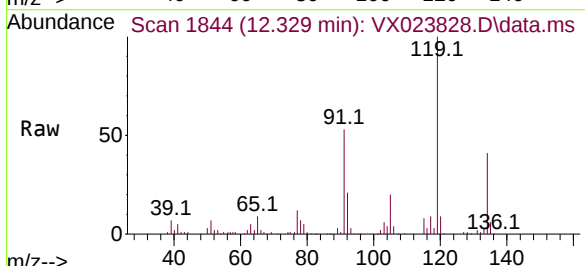




#90
Hexachloroethane
Concen: 5.260 ug/l
RT: 12.536 min Scan# 1878
Delta R.T. -0.006 min
Lab File: VX023828.D
Acq: 18 Aug 2021 19:46




Instrument :
MSVOA_X
ClientSampled :
B-1DL


Tgt Ion:117 Resp: 3771
Ion Ratio Lower Upper
117 100
201 0.0 40.4 121.2#

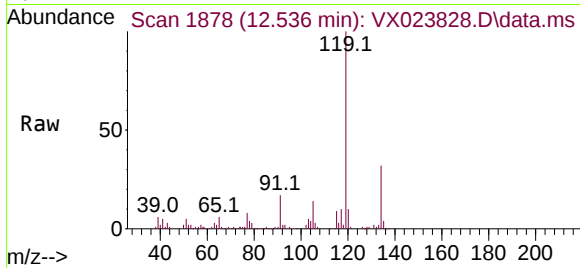

#92
1,2-Dibromo-3-Chloropropane
Concen: 2.742 ug/l
RT: 12.926 min Scan# 1942
Delta R.T. -0.019 min
Lab File: VX023828.D
Acq: 18 Aug 2021 19:46

Tgt Ion: 75 Resp: 310
Ion Ratio Lower Upper
75 100
155 0.0 45.3 135.9#
157 0.0 57.7 173.1#

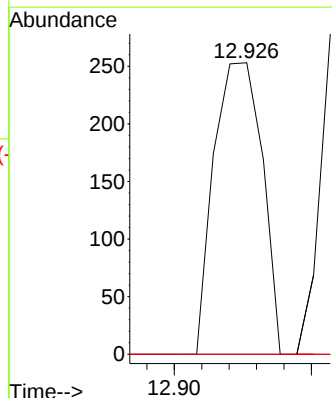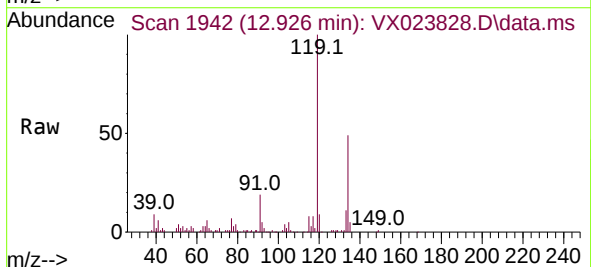

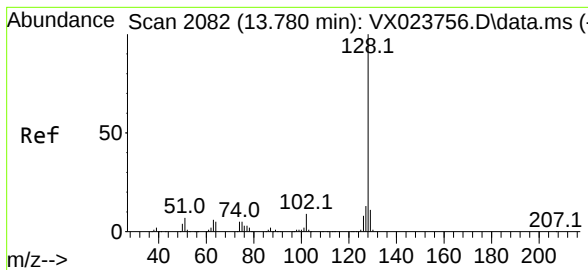

#95
Naphthalene
Concen: 7.470 ug/l
RT: 13.780 min Scan# 2082
Delta R.T. -0.000 min
Lab File: VX023828.D
Acq: 18 Aug 2021 19:46

Instrument :
MSVOA_X
ClientSampleId :
B-1DL

Tgt Ion:128 Resp: 40533
Ion Ratio Lower Upper
128 100
127 13.5 10.3 15.5
129 12.4 8.8 13.2

