

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX081822\
 Data File : VX030678.D
 Acq On : 18 Aug 2022 12:15
 Operator : JC/MD
 Sample : VX0818WBL01
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :

Quant Time: Aug 18 14:44:39 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML080422WMA.M
 Quant Title : VOC Analysis
 QLast Update : Thu Aug 18 04:21:09 2022
 Response via : Initial Calibration

Compound	R.T. QIon		Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	6.763	114	296898	50.000	ug/L	0.00
28) Chlorobenzene-d5	10.055	117	271652	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	12.024	152	124268	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.368	65	95385	50.028	ug/L	0.00
Spiked Amount	50.000	Range	60 - 135	Recovery	= 100.060%	
7) Chloroethane-d5	1.666	69	73607	54.764	ug/L	0.00
Spiked Amount	50.000	Range	70 - 130	Recovery	= 109.520%	
11) 1,1-Dichloroethene-d2	2.306	63	146338	40.575	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	= 81.160%	
21) 2-Butanone-d5	4.465	46	187414	106.088	ug/L	0.00
Spiked Amount	100.000	Range	40 - 130	Recovery	= 106.090%	
24) Chloroform-d	5.062	84	206659	52.654	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	= 105.300%	
26) 1,2-Dichloroethane-d4	5.958	65	133347	50.037	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	= 100.080%	
32) Benzene-d6	5.977	84	425595	54.694	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	= 109.380%	
36) 1,2-Dichloropropane-d6	7.312	67	141513	56.053	ug/L	0.00
Spiked Amount	50.000	Range	70 - 120	Recovery	= 112.100%	
41) Toluene-d8	8.653	98	382801	52.190	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	= 104.380%	
43) trans-1,3-Dichloroprop...	8.952	79	61999	49.364	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	= 98.720%	
47) 2-Hexanone-d5	9.384	63	139769	108.613	ug/L	0.00
Spiked Amount	100.000	Range	45 - 130	Recovery	= 108.610%	
56) 1,1,2,2-Tetrachloroeth...	11.195	84	194071	58.516	ug/L	0.00
Spiked Amount	50.000	Range	65 - 120	Recovery	= 117.040%	
66) 1,2-Dichlorobenzene-d4	12.323	152	140062	58.110	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	= 116.220%	
Target Compounds						
44) trans-1,3-Dichloropropene	8.952	75	2421	0.716	ug/L	Qvalue 93


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX081822\
Data File : VX030678.D
Acq On : 18 Aug 2022 12:15
Operator : JC/MD
Sample : VX0818WBL01
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :


Quant Time: Aug 18 14:44:39 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM080422WMA.M
Quant Title : VOC Analysis
QLast Update : Thu Aug 18 04:21:09 2022
Response via : Initial Calibration

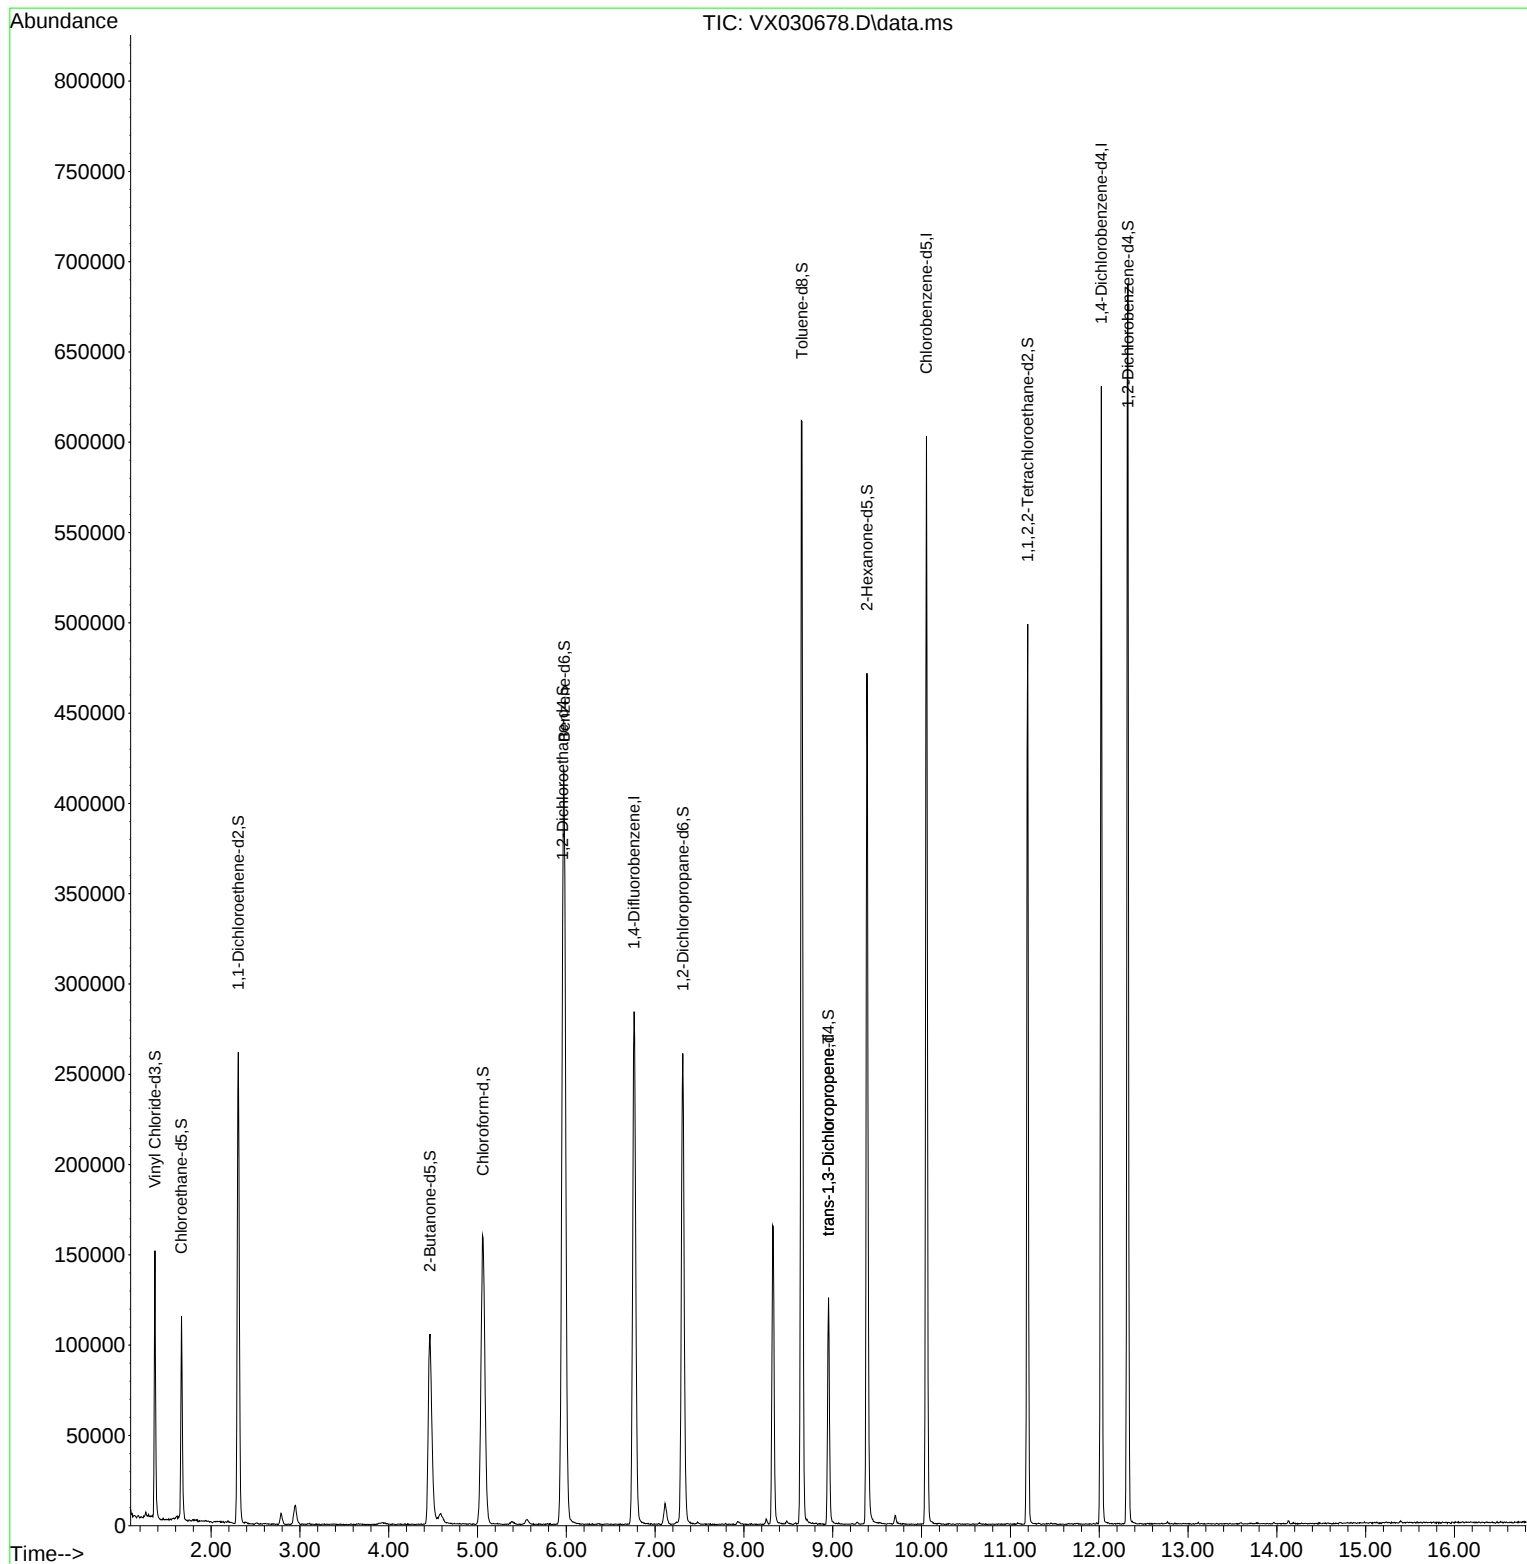

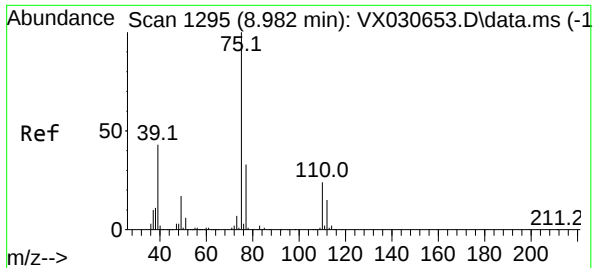

#44
 trans-1,3-Dichloropropene
 Concen: 0.716 ug/L
 RT: 8.952 min Scan# 11
 Delta R.T. -0.030 min
 Lab File: VX030678.D
 Acq: 18 Aug 2022 12:15

Instrument :
 MSVOA_X
 ClientSampleId :

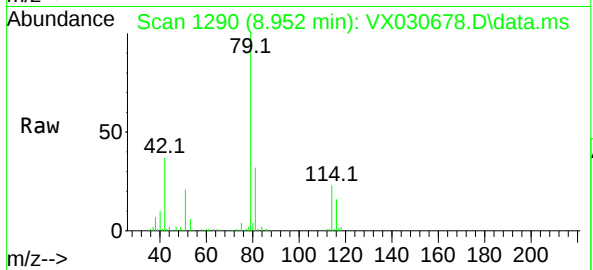

Tgt Ion: 75 Resp: 2421
 Ion Ratio Lower Upper
 75 100
 77 28.3 22.5 41.7

