

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX081822\
 Data File : VX030679.D
 Acq On : 18 Aug 2022 12:47
 Operator : JC/MD
 Sample : N4221-16DL 10X
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 C0KN8DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML080422WMA.M
 Title : VOC Analysis

Signal : TIC: VX030679.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.368	42	46	56	rVB	184487	192243	13.79%	1.746%
2	1.666	91	95	106	rVB	133923	167373	12.00%	1.520%
3	2.306	194	200	211	rVB	326898	507252	36.38%	4.606%
4	2.477	226	228	229	rVB2	462	319	0.02%	0.003%
5	2.501	229	232	233	rBV3	867	883	0.06%	0.008%
6	2.587	242	246	248	rBV3	523	436	0.03%	0.004%
7	2.697	263	264	266	rVB2	561	353	0.03%	0.003%
8	2.727	266	269	271	rVB2	397	337	0.02%	0.003%
9	2.788	274	279	285	rVV2	5028	8273	0.59%	0.075%
10	2.940	295	304	314	rBV2	21834	50118	3.59%	0.455%
11	3.087	326	328	331	rBV3	410	389	0.03%	0.004%
12	3.215	347	349	352	rVB	386	356	0.03%	0.003%
13	3.337	366	369	372	rVB	280	324	0.02%	0.003%
14	3.361	372	373	377	rVB	402	383	0.03%	0.003%
15	3.398	377	379	381	rBV2	401	392	0.03%	0.004%
16	3.483	390	393	394	rVV2	432	369	0.03%	0.003%
17	3.611	408	414	417	rVV3	871	1466	0.11%	0.013%
18	3.763	435	439	443	rBV2	270	488	0.04%	0.004%
19	3.971	469	473	475	rVB2	414	350	0.03%	0.003%
20	4.013	477	480	482	rBV2	357	442	0.03%	0.004%
21	4.239	513	517	518	rBV2	338	352	0.03%	0.003%
22	4.324	528	531	533	rBV	289	328	0.02%	0.003%
23	4.391	540	542	544	rBV2	356	428	0.03%	0.004%
24	4.465	544	554	568	rBV2	120555	406800	29.18%	3.694%
25	4.958	632	635	636	rBV2	465	470	0.03%	0.004%
26	5.062	639	652	669	rVV	180462	559966	40.16%	5.085%
27	5.184	670	672	674	rVV2	940	936	0.07%	0.008%
28	5.214	675	677	682	rVV4	724	1175	0.08%	0.011%
29	5.263	682	685	687	rVB2	778	763	0.05%	0.007%
30	5.349	696	699	700	rBV2	768	671	0.05%	0.006%
31	5.385	700	705	713	rVV6	2852	6682	0.48%	0.061%
32	5.562	726	734	738	rVV4	1665	3939	0.28%	0.036%
33	5.848	780	781	784	rBV2	419	375	0.03%	0.003%
34	5.970	789	801	819	rBV2	477316	1394225	100.00%	12.661%
35	6.257	844	848	849	rBV3	335	352	0.03%	0.003%
36	6.464	880	882	885	rVB2	521	558	0.04%	0.005%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX081822\
 Data File : VX030679.D
 Acq On : 18 Aug 2022 12:47
 Operator : JC/MD
 Sample : N4221-16DL 10X
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 C0KN8DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML080422WMA.M
 Title : VOC Analysis

37	6.495	885	887	888	rBV	531	387	0.03%	0.004%
38	6.763	921	931	944	rBV2	325117	766818	55.00%	6.963%
39	6.940	958	960	963	rBV2	408	417	0.03%	0.004%
40	7.031	974	975	978	rVB	488	409	0.03%	0.004%
41	7.123	981	990	1000	rBV3	44376	109290	7.84%	0.992%
42	7.312	1010	1021	1037	rBV	283657	629811	45.17%	5.719%
43	7.482	1047	1049	1052	rBV3	738	735	0.05%	0.007%
44	7.531	1056	1057	1059	rBV	583	325	0.02%	0.003%
45	7.610	1065	1070	1075	rBV2	472	778	0.06%	0.007%
46	7.927	1119	1122	1123	rBV	1076	878	0.06%	0.008%
47	8.080	1144	1147	1149	rVV2	447	491	0.04%	0.004%
48	8.165	1159	1161	1162	rBV	593	318	0.02%	0.003%
49	8.324	1180	1187	1197	rBV	191271	315277	22.61%	2.863%
50	8.476	1207	1212	1221	rBV6	1487	3702	0.27%	0.034%
51	8.653	1233	1241	1256	rBV	711243	1139827	81.75%	10.351%
52	8.793	1263	1264	1266	rBV2	434	391	0.03%	0.004%
53	8.952	1284	1290	1303	rBV	136944	207472	14.88%	1.884%
54	9.073	1308	1310	1312	rVV2	769	657	0.05%	0.006%
55	9.104	1312	1315	1317	rVB2	453	530	0.04%	0.005%
56	9.183	1324	1328	1332	rBV2	609	823	0.06%	0.007%
57	9.275	1336	1343	1354	rVB	310148	438510	31.45%	3.982%
58	9.384	1354	1361	1373	rBV	495906	702850	50.41%	6.383%
59	9.634	1400	1402	1404	rVV2	568	429	0.03%	0.004%
60	10.055	1465	1471	1484	rVV	671541	901038	64.63%	8.182%
61	10.207	1493	1496	1499	rVB2	521	670	0.05%	0.006%
62	10.348	1518	1519	1520	rBV	787	368	0.03%	0.003%
63	10.409	1527	1529	1530	rBV2	416	332	0.02%	0.003%
64	10.470	1537	1539	1542	rBV2	382	377	0.03%	0.003%
65	10.561	1552	1554	1558	rBV2	527	466	0.03%	0.004%
66	10.640	1563	1567	1568	rBV2	548	659	0.05%	0.006%
67	10.683	1573	1574	1578	rVB2	594	703	0.05%	0.006%
68	10.878	1602	1606	1610	rBV2	392	743	0.05%	0.007%
69	10.927	1612	1614	1617	rVV2	306	340	0.02%	0.003%
70	11.012	1624	1628	1629	rVB2	383	363	0.03%	0.003%
71	11.030	1629	1631	1633	rBV	455	438	0.03%	0.004%
72	11.085	1639	1640	1643	rBV2	542	533	0.04%	0.005%
73	11.116	1643	1645	1647	rVB2	527	380	0.03%	0.003%
74	11.146	1647	1650	1652	rBV	430	442	0.03%	0.004%
75	11.195	1652	1658	1667	rBV	526152	647530	46.44%	5.880%
76	11.305	1674	1676	1677	rBV2	403	321	0.02%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX081822\
 Data File : VX030679.D
 Acq On : 18 Aug 2022 12:47
 Operator : JC/MD
 Sample : N4221-16DL 10X
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 C0KN8DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXMLM080422WMA.M
 Title : VOC Analysis

77	11.445	1698	1699	1700	rBV	596	349	0.03%	0.003%
78	11.488	1704	1706	1708	rVB	492	342	0.02%	0.003%
79	11.762	1748	1751	1754	rBV2	683	800	0.06%	0.007%
80	11.896	1771	1773	1777	rVB2	483	381	0.03%	0.003%
81	11.969	1780	1785	1789	rBV3	594	1103	0.08%	0.010%
82	12.024	1789	1794	1803	rBV	707361	849420	60.92%	7.714%
83	12.189	1819	1821	1822	rBV2	768	356	0.03%	0.003%
84	12.323	1837	1843	1853	rBV	738661	955066	68.50%	8.673%
85	12.445	1861	1863	1866	rVB2	556	384	0.03%	0.003%
86	12.585	1885	1886	1890	rBV2	396	446	0.03%	0.004%
87	12.768	1913	1916	1918	rBV2	929	1110	0.08%	0.010%
88	13.195	1985	1986	1991	rBV	518	541	0.04%	0.005%
89	13.524	2037	2040	2043	rBV2	527	662	0.05%	0.006%
90	13.756	2075	2078	2080	rBV	443	629	0.05%	0.006%
91	13.786	2080	2083	2086	rVV2	667	841	0.06%	0.008%
92	13.853	2092	2094	2097	rVB	502	345	0.02%	0.003%
93	13.963	2110	2112	2114	rBV2	618	557	0.04%	0.005%
94	13.981	2114	2115	2117	rVB	578	363	0.03%	0.003%
95	14.109	2133	2136	2137	rBV2	540	620	0.04%	0.006%
96	14.127	2137	2139	2148	rVB3	2588	3883	0.28%	0.035%
97	14.463	2193	2194	2197	rBV	593	493	0.04%	0.004%
98	15.395	2343	2347	2354	rVB5	2162	4165	0.30%	0.038%
99	15.572	2374	2376	2380	rBV3	843	1017	0.07%	0.009%
100	16.115	2463	2465	2470	rVB4	785	854	0.06%	0.008%




Sum of corrected areas: 11012121

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX081822\
Data File : VX030679.D
Acq On : 18 Aug 2022 12:47
Operator : JC/MD
Sample : N4221-16DL 10X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
C0KN8DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML080422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

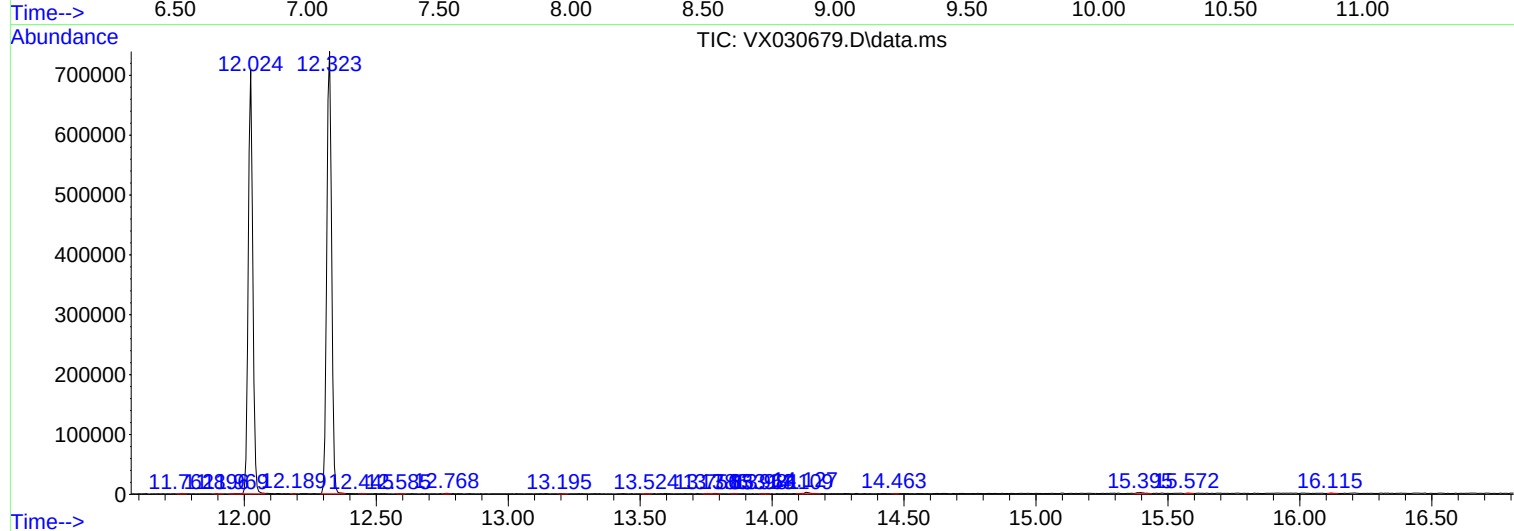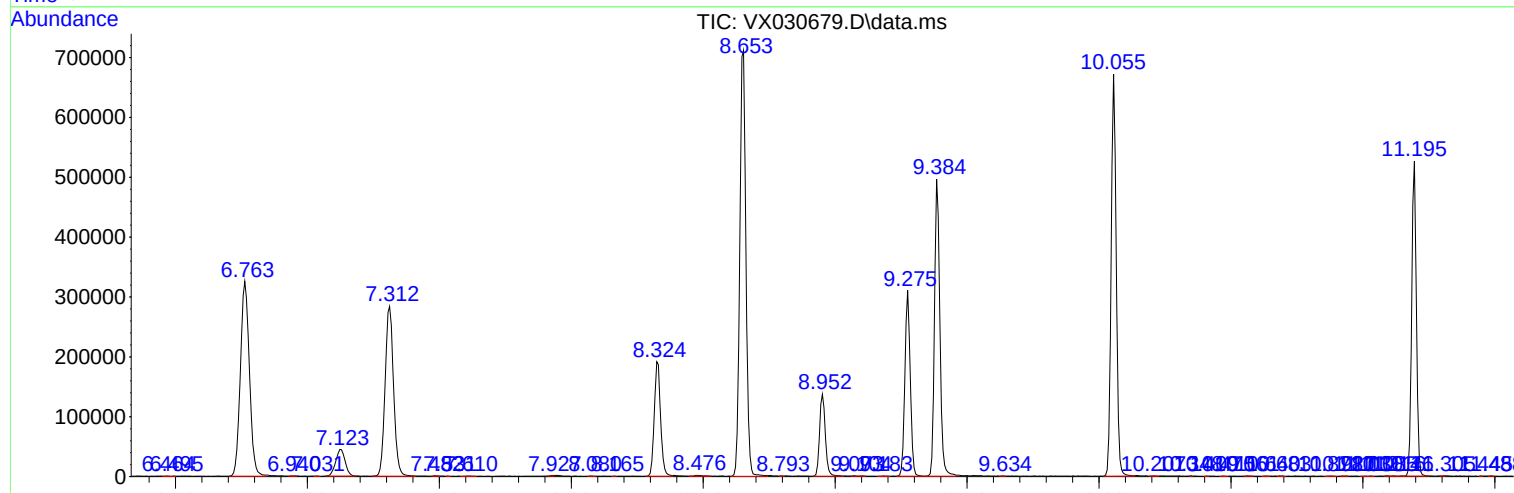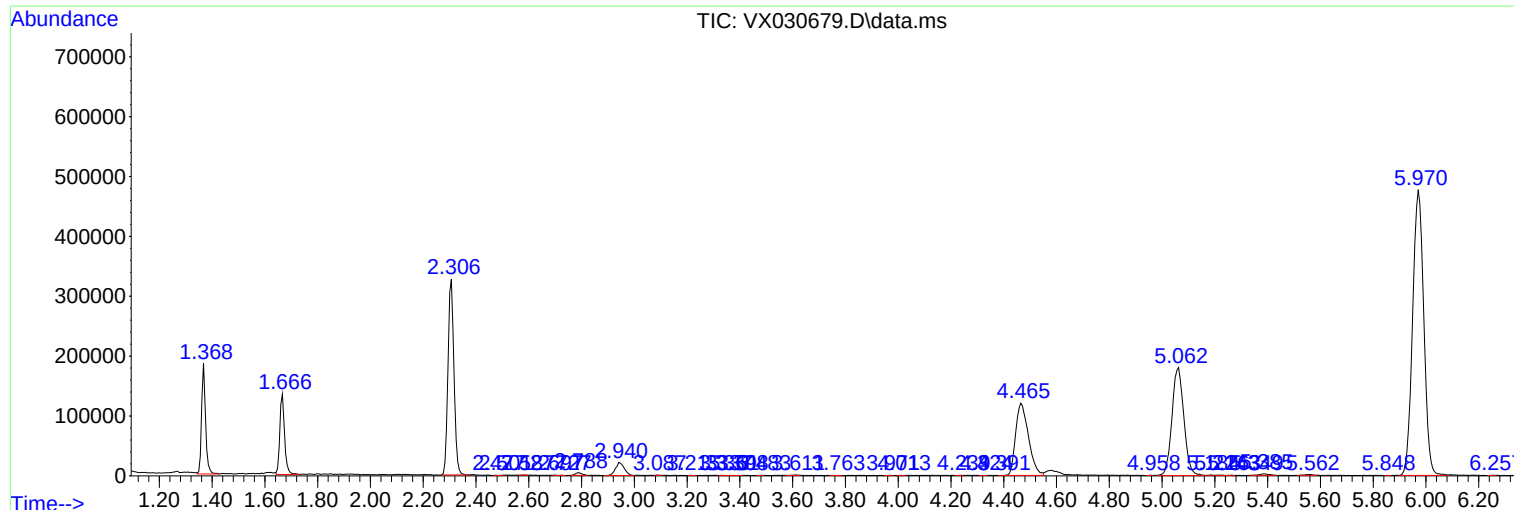

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX081822\
Data File : VX030679.D
Acq On : 18 Aug 2022 12:47
Operator : JC/MD
Sample : N4221-16DL 10X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
C0KN8DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML080422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX081822\
Data File : VX030679.D
Acq On : 18 Aug 2022 12:47
Operator : JC/MD
Sample : N4221-16DL 10X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
C0KN8DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML080422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc