

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX081822\
 Data File : VX030680.D
 Acq On : 18 Aug 2022 13:17
 Operator : JC/MD
 Sample : N4221-18DL 10X
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 C0KP0DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML080422WMA.M

Title : VOC Analysis

Signal : TIC: VX030680.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.368	42	46	54	rVB	150515	157695	14.36%	1.594%
2	1.666	91	95	103	rVB	107279	132570	12.07%	1.340%
3	2.307	193	200	209	rBV	258554	413874	37.70%	4.183%
4	2.557	239	241	243	rVB3	614	518	0.05%	0.005%
5	2.611	248	250	253	rBV3	733	672	0.06%	0.007%
6	2.697	262	264	266	rVB2	446	312	0.03%	0.003%
7	2.715	266	267	269	rBV	692	499	0.05%	0.005%
8	2.794	274	280	284	rBV4	4309	8759	0.80%	0.089%
9	2.843	286	288	290	rBV2	445	413	0.04%	0.004%
10	2.947	298	305	314	rVB	14046	32597	2.97%	0.329%
11	3.032	317	319	321	rVB	520	348	0.03%	0.004%
12	3.099	323	330	333	rBV3	908	1462	0.13%	0.015%
13	3.447	384	387	390	rVB2	271	369	0.03%	0.004%
14	3.611	408	414	421	rBV5	2254	5654	0.51%	0.057%
15	3.812	444	447	449	rVV2	415	423	0.04%	0.004%
16	3.989	474	476	479	rVB2	379	453	0.04%	0.005%
17	4.050	484	486	489	rBV2	359	495	0.05%	0.005%
18	4.117	494	497	498	rBV2	416	374	0.03%	0.004%
19	4.190	507	509	511	rVB2	361	330	0.03%	0.003%
20	4.209	511	512	515	rBV2	383	335	0.03%	0.003%
21	4.245	515	518	519	rVB2	526	444	0.04%	0.004%
22	4.257	519	520	525	rVB2	320	484	0.04%	0.005%
23	4.300	525	527	530	rBV	441	419	0.04%	0.004%
24	4.349	533	535	538	rBV	394	415	0.04%	0.004%
25	4.471	545	555	568	rBV3	119053	440464	40.12%	4.452%
26	4.824	611	613	619	rVB	460	591	0.05%	0.006%
27	4.952	632	634	636	rBV	597	339	0.03%	0.003%
28	5.062	639	652	668	rVV	140014	432959	39.44%	4.376%
29	5.391	695	706	714	rBV4	4324	12315	1.12%	0.124%
30	5.556	727	733	741	rVB4	2173	5301	0.48%	0.054%
31	5.660	748	750	754	rBV2	519	612	0.06%	0.006%
32	5.727	758	761	762	rBV	363	371	0.03%	0.004%
33	5.745	762	764	767	rVB2	310	370	0.03%	0.004%
34	5.861	780	783	786	rBV2	307	384	0.03%	0.004%
35	5.971	788	801	823	rVV2	377772	1097891	100.00%	11.097%
36	6.367	865	866	868	rBV	624	378	0.03%	0.004%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX081822\
 Data File : VX030680.D
 Acq On : 18 Aug 2022 13:17
 Operator : JC/MD
 Sample : N4221-18DL 10X
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 C0KP0DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML080422WMA.M
 Title : VOC Analysis

37	6.556	893	897	900	rVV2	457	839	0.08%	0.008%
38	6.598	902	904	905	rVB	438	285	0.03%	0.003%
39	6.635	905	910	912	rBV2	352	562	0.05%	0.006%
40	6.763	921	931	946	rBV	321965	759567	69.18%	7.677%
41	6.989	966	968	969	rVB2	592	401	0.04%	0.004%
42	7.013	969	972	974	rBV3	713	602	0.05%	0.006%
43	7.129	981	991	1002	rBV3	72047	169812	15.47%	1.716%
44	7.312	1012	1021	1033	rBV	227590	494626	45.05%	4.999%
45	7.617	1069	1071	1075	rVB	541	633	0.06%	0.006%
46	7.787	1096	1099	1100	rBV	485	537	0.05%	0.005%
47	7.940	1119	1124	1127	rBV3	1448	2071	0.19%	0.021%
48	8.190	1162	1165	1169	rBV2	370	539	0.05%	0.005%
49	8.238	1169	1173	1175	rVV	267	409	0.04%	0.004%
50	8.330	1181	1188	1199	rBV	147091	246580	22.46%	2.492%
51	8.482	1209	1213	1218	rVB2	1244	1734	0.16%	0.018%
52	8.586	1225	1230	1233	rBV3	443	902	0.08%	0.009%
53	8.653	1233	1241	1253	rBV	562487	884363	80.55%	8.938%
54	8.952	1284	1290	1302	rBV	108628	161955	14.75%	1.637%
55	9.275	1336	1343	1353	rVV	589364	847989	77.24%	8.571%
56	9.385	1355	1361	1375	rBV	382468	550801	50.17%	5.567%
57	9.653	1403	1405	1407	rVB	484	283	0.03%	0.003%
58	9.860	1435	1439	1440	rBV	462	552	0.05%	0.006%
59	10.055	1465	1471	1486	rBV	678654	895859	81.60%	9.055%
60	10.195	1493	1494	1496	rVB	588	348	0.03%	0.004%
61	10.244	1500	1502	1505	rVB2	515	402	0.04%	0.004%
62	10.409	1528	1529	1531	rBV	447	310	0.03%	0.003%
63	10.573	1551	1556	1557	rBV2	386	639	0.06%	0.006%
64	10.671	1570	1572	1573	rBV2	364	286	0.03%	0.003%
65	10.775	1587	1589	1592	rVB	645	415	0.04%	0.004%
66	10.976	1619	1622	1624	rBV	551	736	0.07%	0.007%
67	11.012	1626	1628	1630	rVB	439	394	0.04%	0.004%
68	11.067	1634	1637	1638	rBV2	305	307	0.03%	0.003%
69	11.085	1638	1640	1642	rVB2	619	401	0.04%	0.004%
70	11.195	1652	1658	1666	rVV	390721	506230	46.11%	5.117%
71	11.317	1674	1678	1681	rBV4	751	1291	0.12%	0.013%
72	11.579	1718	1721	1724	rBV2	391	622	0.06%	0.006%
73	11.677	1736	1737	1740	rBV2	319	322	0.03%	0.003%
74	11.707	1740	1742	1746	rVV	902	761	0.07%	0.008%
75	11.756	1748	1750	1752	rVV	490	359	0.03%	0.004%
76	11.787	1752	1755	1762	rVB2	648	1072	0.10%	0.011%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX081822\
 Data File : VX030680.D
 Acq On : 18 Aug 2022 13:17
 Operator : JC/MD
 Sample : N4221-18DL 10X
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 C0KP0DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML080422WMA.M
 Title : VOC Analysis

77	11.866	1764	1768	1773	rBV2	538	984	0.09%	0.010%
78	11.957	1780	1783	1784	rBV2	410	390	0.04%	0.004%
79	12.024	1788	1794	1802	rVV	692486	831377	75.72%	8.403%
80	12.152	1814	1815	1817	rVB	613	364	0.03%	0.004%
81	12.232	1823	1828	1832	rBV3	3787	6649	0.61%	0.067%
82	12.323	1837	1843	1854	rVV	597371	753373	68.62%	7.615%
83	12.506	1871	1873	1875	rBV2	561	497	0.05%	0.005%
84	12.610	1888	1890	1892	rBV	403	326	0.03%	0.003%
85	12.707	1903	1906	1907	rBV2	383	378	0.03%	0.004%
86	13.116	1971	1973	1977	rVB	714	815	0.07%	0.008%
87	13.536	2041	2042	2045	rVB	601	435	0.04%	0.004%
88	13.676	2062	2065	2066	rBV	582	568	0.05%	0.006%
89	13.835	2089	2091	2093	rBV3	524	628	0.06%	0.006%
90	13.914	2102	2104	2106	rBV	467	406	0.04%	0.004%
91	13.981	2113	2115	2118	rBV	318	384	0.03%	0.004%
92	14.036	2122	2124	2125	rBV	654	365	0.03%	0.004%
93	14.128	2136	2139	2144	rBV	2095	2962	0.27%	0.030%
94	14.548	2205	2208	2210	rBV2	511	643	0.06%	0.006%
95	14.634	2220	2222	2223	rBV	670	414	0.04%	0.004%
96	14.652	2223	2225	2226	rBV2	744	500	0.05%	0.005%
97	14.902	2264	2266	2269	rBV3	692	706	0.06%	0.007%
98	14.957	2274	2275	2276	rBV	618	351	0.03%	0.004%
99	15.042	2285	2289	2290	rBV2	934	1130	0.10%	0.011%
100	16.024	2448	2450	2453	rVB2	889	568	0.05%	0.006%


Sum of corrected areas: 9893898

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX081822\
Data File : VX030680.D
Acq On : 18 Aug 2022 13:17
Operator : JC/MD
Sample : N4221-18DL 10X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
C0KP0DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML080422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

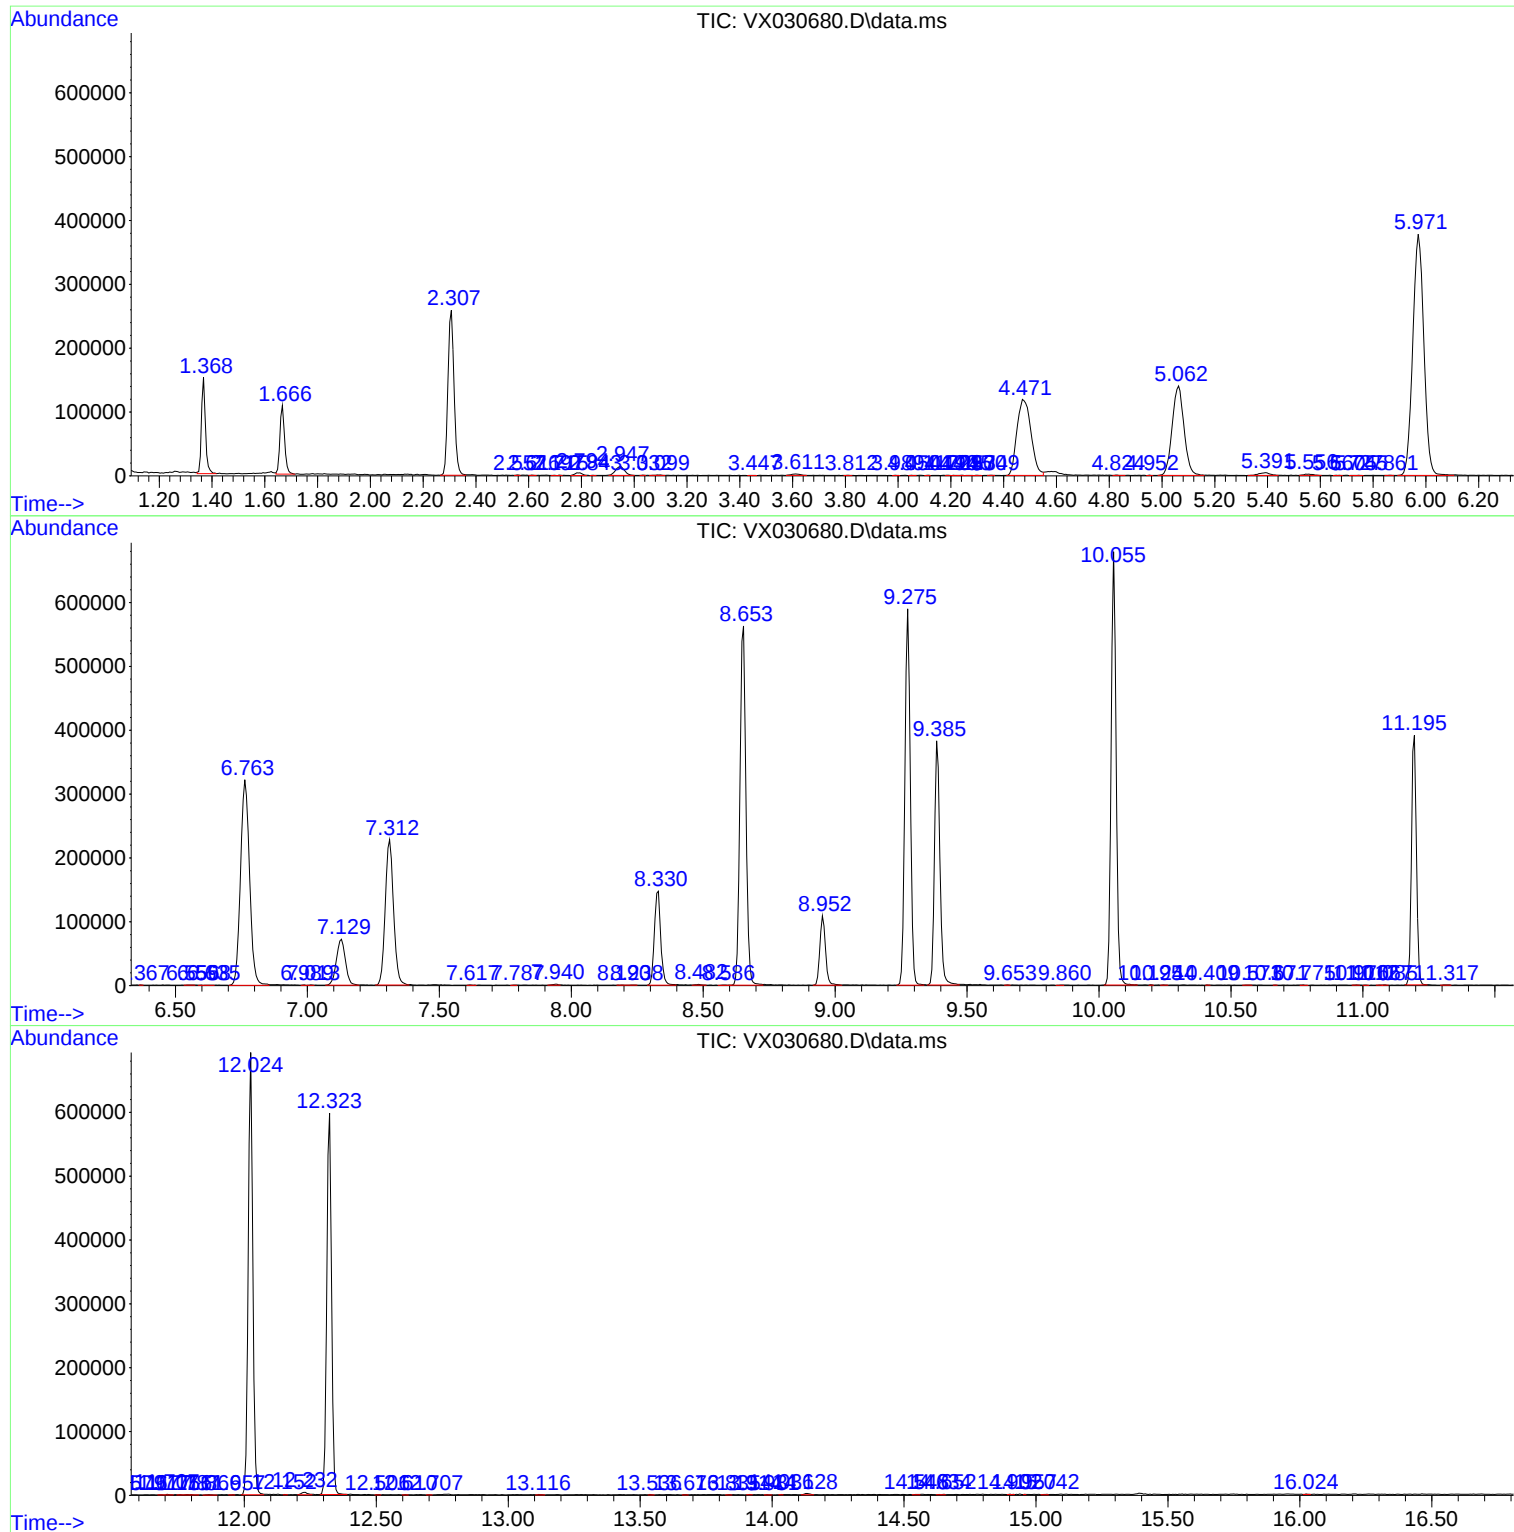

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX081822\
Data File : VX030680.D
Acq On : 18 Aug 2022 13:17
Operator : JC/MD
Sample : N4221-18DL 10X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
C0KP0DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML080422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX081822\
Data File : VX030680.D
Acq On : 18 Aug 2022 13:17
Operator : JC/MD
Sample : N4221-18DL 10X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
C0KP0DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML080422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc