

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX081822\
 Data File : VX030681.D
 Acq On : 18 Aug 2022 13:40
 Operator : JC/MD
 Sample : N4221-12DL 20X
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 C0KN2DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML080422WMA.M

Title : VOC Analysis

Signal : TIC: VX030681.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.142	7	9	12	rBV	5392	5136	0.38%	0.044%
2	1.368	42	46	56	rVB	207792	215468	15.74%	1.827%
3	1.666	91	95	102	rVB	136509	164525	12.02%	1.395%
4	2.313	193	201	214	rBV2	430900	803354	58.70%	6.813%
5	2.502	230	232	235	rBV3	512	443	0.03%	0.004%
6	2.794	274	280	288	rVB3	2751	4934	0.36%	0.042%
7	2.947	297	305	315	rBV	10933	25624	1.87%	0.217%
8	3.093	324	329	335	rVV4	1157	2381	0.17%	0.020%
9	3.282	358	360	362	rVB2	486	404	0.03%	0.003%
10	3.312	362	365	366	rBV2	442	466	0.03%	0.004%
11	3.343	369	370	372	rBV	446	315	0.02%	0.003%
12	3.471	387	391	392	rBV2	407	572	0.04%	0.005%
13	3.611	406	414	424	rBV2	12203	28907	2.11%	0.245%
14	3.684	424	426	431	rVB2	507	750	0.05%	0.006%
15	3.733	431	434	436	rVB2	396	447	0.03%	0.004%
16	3.898	459	461	466	rVV2	300	478	0.03%	0.004%
17	4.093	491	493	496	rBV	567	395	0.03%	0.003%
18	4.227	513	515	522	rVB2	525	662	0.05%	0.006%
19	4.282	522	524	527	rBV	417	350	0.03%	0.003%
20	4.471	545	555	568	rBV2	122113	425620	31.10%	3.609%
21	4.861	616	619	624	rBV2	525	997	0.07%	0.008%
22	4.904	624	626	629	rVB2	795	1026	0.07%	0.009%
23	4.928	629	630	632	rBV	605	456	0.03%	0.004%
24	4.952	632	634	636	rVB	752	566	0.04%	0.005%
25	5.062	636	652	668	rBV	175737	549851	40.18%	4.663%
26	5.342	696	698	699	rBV	445	351	0.03%	0.003%
27	5.397	699	707	717	rVB6	4670	12872	0.94%	0.109%
28	5.556	728	733	744	rVB5	3492	9208	0.67%	0.078%
29	5.647	744	748	749	rBV2	337	389	0.03%	0.003%
30	5.702	754	757	758	rVB	491	439	0.03%	0.004%
31	5.977	788	802	817	rBV2	472656	1368626	100.00%	11.606%
32	6.245	844	846	849	rVB2	507	449	0.03%	0.004%
33	6.391	868	870	873	rVB3	530	481	0.04%	0.004%
34	6.440	876	878	880	rBV2	349	293	0.02%	0.002%
35	6.489	883	886	887	rBV2	488	352	0.03%	0.003%
36	6.556	892	897	899	rBV	446	548	0.04%	0.005%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX081822\
 Data File : VX030681.D
 Acq On : 18 Aug 2022 13:40
 Operator : JC/MD
 Sample : N4221-12DL 20X
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 C0KN2DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML080422WMA.M
 Title : VOC Analysis

37	6.696	919	920	922	rVB2	533	353	0.03%	0.003%
38	6.763	922	931	947	rBV	309933	743111	54.30%	6.302%
39	7.068	978	981	982	rBV2	557	496	0.04%	0.004%
40	7.129	982	991	1009	rVV	407912	891605	65.15%	7.561%
41	7.312	1012	1021	1037	rVB	284552	615124	44.94%	5.216%
42	7.476	1045	1048	1049	rBV2	1032	946	0.07%	0.008%
43	7.684	1074	1082	1088	rBV4	2425	6203	0.45%	0.053%
44	7.940	1117	1124	1127	rBV2	2057	3612	0.26%	0.031%
45	8.055	1139	1143	1147	rVB	474	840	0.06%	0.007%
46	8.116	1151	1153	1155	rVB	543	366	0.03%	0.003%
47	8.165	1159	1161	1163	rBV2	411	361	0.03%	0.003%
48	8.330	1181	1188	1200	rVV	186277	310746	22.70%	2.635%
49	8.421	1200	1203	1206	rVB3	850	1132	0.08%	0.010%
50	8.482	1210	1213	1220	rBV5	1346	2545	0.19%	0.022%
51	8.653	1234	1241	1251	rBV	712035	1106306	80.83%	9.382%
52	8.805	1263	1266	1269	rBV3	686	908	0.07%	0.008%
53	8.952	1284	1290	1300	rBV	134834	198917	14.53%	1.687%
54	9.275	1335	1343	1351	rBV	277738	397265	29.03%	3.369%
55	9.384	1356	1361	1381	rVV	498795	707791	51.72%	6.002%
56	9.890	1443	1444	1446	rVB	558	359	0.03%	0.003%
57	9.964	1452	1456	1458	rBV	414	627	0.05%	0.005%
58	10.055	1465	1471	1482	rBV	639257	855514	62.51%	7.255%
59	10.244	1500	1502	1506	rBV3	529	633	0.05%	0.005%
60	10.299	1509	1511	1515	rVB2	679	720	0.05%	0.006%
61	10.372	1521	1523	1528	rVB3	1209	1710	0.12%	0.015%
62	10.433	1531	1533	1536	rBV2	396	337	0.02%	0.003%
63	10.500	1542	1544	1546	rBV	398	384	0.03%	0.003%
64	10.665	1569	1571	1573	rVB	614	323	0.02%	0.003%
65	10.793	1590	1592	1595	rBV2	351	415	0.03%	0.004%
66	10.945	1616	1617	1622	rVB3	328	388	0.03%	0.003%
67	11.012	1627	1628	1631	rBV2	417	288	0.02%	0.002%
68	11.195	1652	1658	1676	rVB	494517	635828	46.46%	5.392%
69	11.317	1676	1678	1681	rBV2	546	607	0.04%	0.005%
70	11.591	1722	1723	1724	rBV	502	307	0.02%	0.003%
71	11.640	1729	1731	1733	rVV	437	345	0.03%	0.003%
72	11.713	1740	1743	1744	rBV2	440	425	0.03%	0.004%
73	11.756	1749	1750	1755	rVB3	555	532	0.04%	0.005%
74	11.823	1759	1761	1763	rBV	461	358	0.03%	0.003%
75	11.969	1783	1785	1788	rVB2	752	551	0.04%	0.005%
76	12.024	1789	1794	1806	rVV	647165	776227	56.72%	6.583%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX081822\
 Data File : VX030681.D
 Acq On : 18 Aug 2022 13:40
 Operator : JC/MD
 Sample : N4221-12DL 20X
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 C0KN2DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML080422WMA.M
 Title : VOC Analysis

77	12.164	1814	1817	1818	rBV2	473	398	0.03%	0.003%
78	12.207	1823	1824	1825	rBV	573	416	0.03%	0.004%
79	12.225	1825	1827	1831	rVB3	1183	1066	0.08%	0.009%
80	12.323	1837	1843	1850	rBV	702314	881043	64.37%	7.472%
81	12.756	1913	1914	1919	rVB4	940	1187	0.09%	0.010%
82	12.811	1921	1923	1925	rBV2	485	575	0.04%	0.005%
83	12.908	1937	1939	1941	rBV2	595	504	0.04%	0.004%
84	13.055	1961	1963	1964	rBV	362	334	0.02%	0.003%
85	13.420	2021	2023	2026	rVB2	480	454	0.03%	0.004%
86	13.512	2034	2038	2039	rVB2	500	593	0.04%	0.005%
87	13.530	2039	2041	2044	rBV	513	455	0.03%	0.004%
88	13.585	2047	2050	2052	rBV	487	446	0.03%	0.004%
89	13.707	2067	2070	2072	rBV3	428	600	0.04%	0.005%
90	13.780	2077	2082	2085	rBV3	597	939	0.07%	0.008%
91	13.920	2103	2105	2106	rBV	436	396	0.03%	0.003%
92	13.969	2111	2113	2115	rBV2	326	279	0.02%	0.002%
93	14.134	2136	2140	2143	rBV4	1975	2959	0.22%	0.025%
94	14.390	2180	2182	2184	rBV2	505	444	0.03%	0.004%
95	14.518	2201	2203	2204	rBV	603	450	0.03%	0.004%
96	15.335	2335	2337	2339	rBV2	859	914	0.07%	0.008%
97	15.383	2343	2345	2349	rVV3	1034	1488	0.11%	0.013%
98	15.774	2408	2409	2411	rBV	1093	942	0.07%	0.008%
99	16.523	2530	2532	2535	rVB	1193	919	0.07%	0.008%
100	16.548	2535	2536	2537	rBV	1080	458	0.03%	0.004%




Sum of corrected areas: 11791899

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX081822\
Data File : VX030681.D
Acq On : 18 Aug 2022 13:40
Operator : JC/MD
Sample : N4221-12DL 20X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
C0KN2DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML080422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

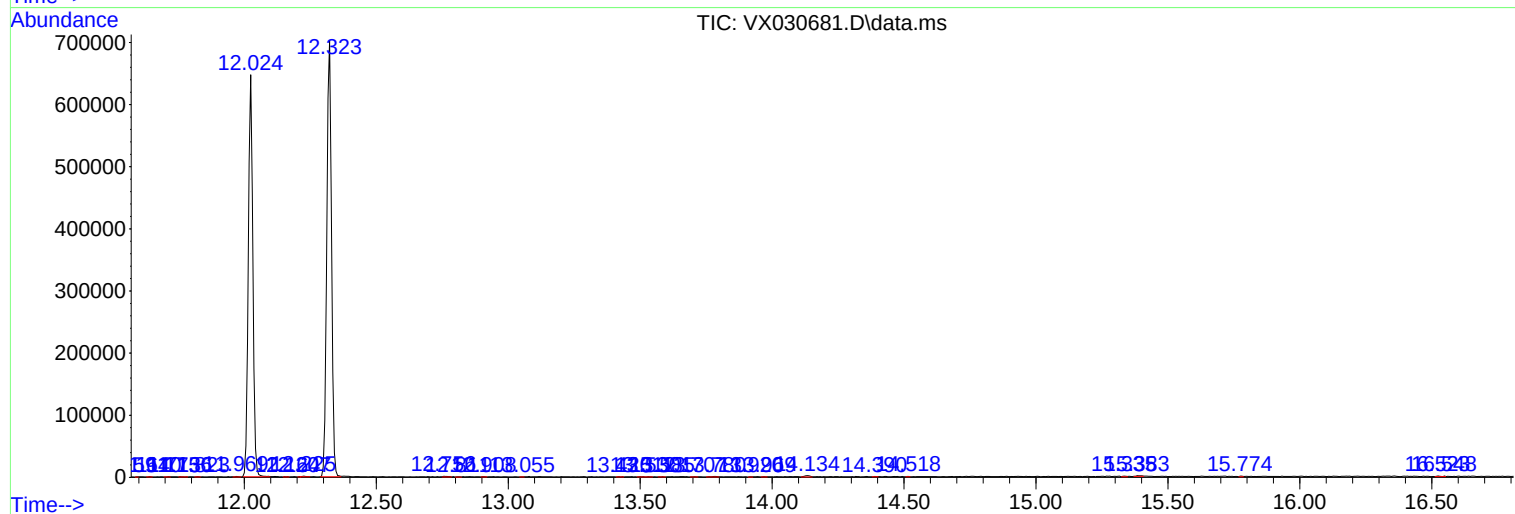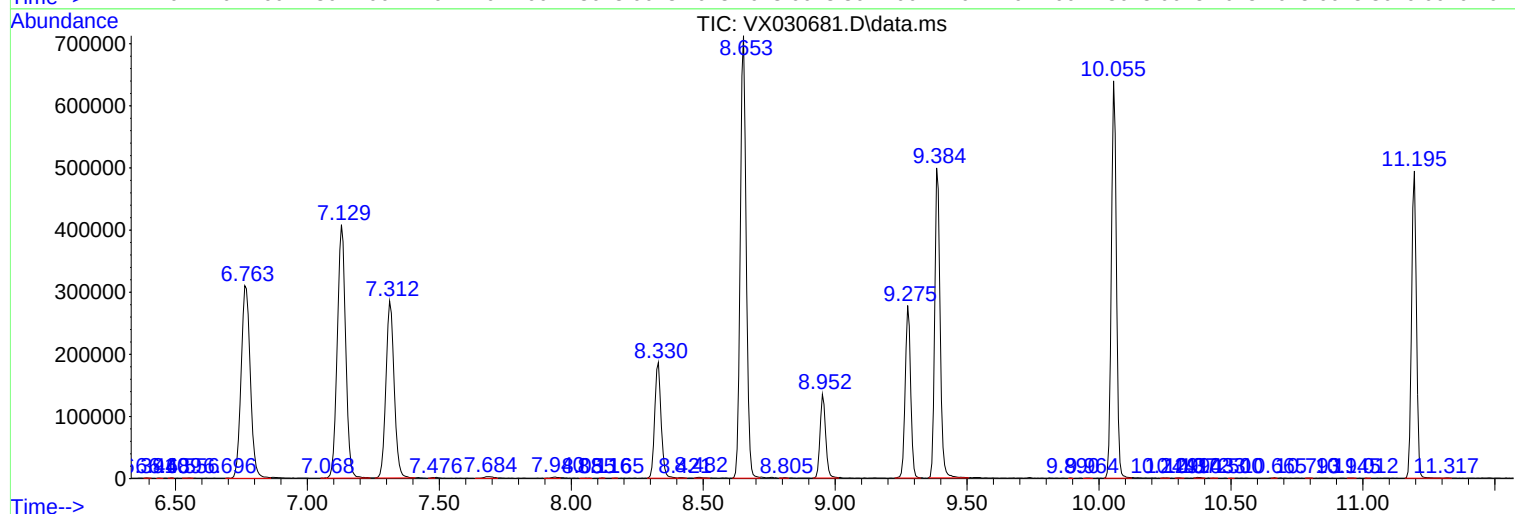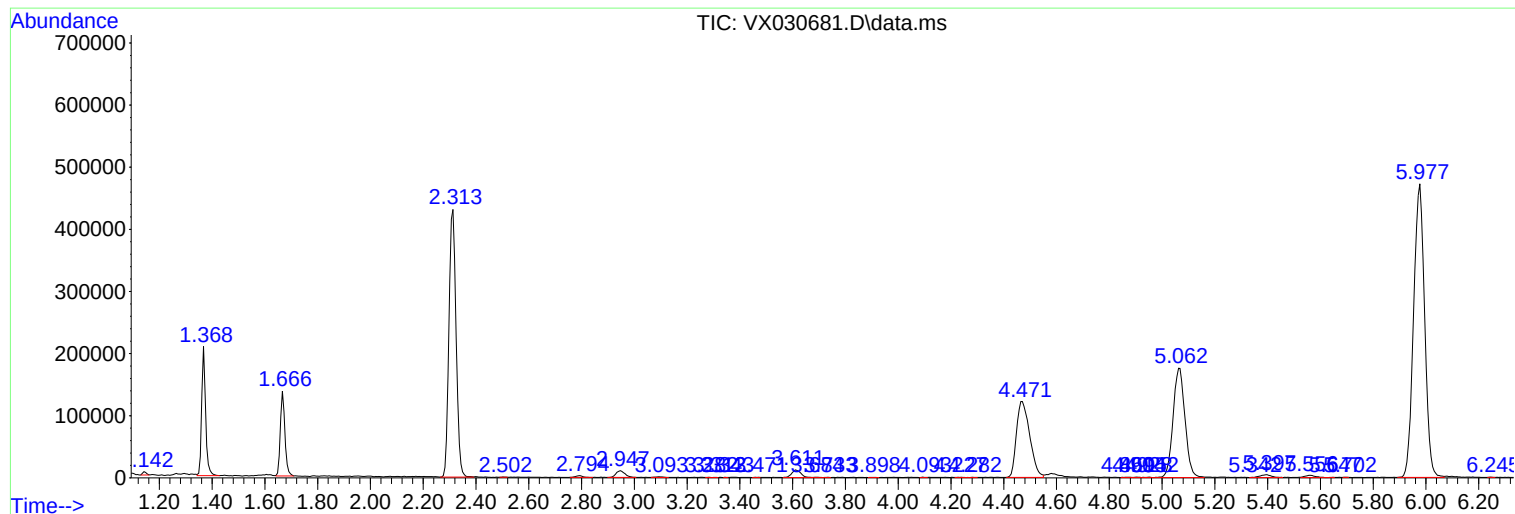

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX081822\
Data File : VX030681.D
Acq On : 18 Aug 2022 13:40
Operator : JC/MD
Sample : N4221-12DL 20X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
C0KN2DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML080422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX081822\
Data File : VX030681.D
Acq On : 18 Aug 2022 13:40
Operator : JC/MD
Sample : N4221-12DL 20X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
C0KN2DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML080422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc