

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX081822\
 Data File : VX030682.D
 Acq On : 18 Aug 2022 14:03
 Operator : JC/MD
 Sample : N4221-14DL 20X
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 C0KN6DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML080422WMA.M

Title : VOC Analysis

Signal : TIC: VX030682.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.368	42	46	59	rVB2	221667	238749	17.83%	1.850%
2	1.666	91	95	102	rVB	131944	161073	12.03%	1.248%
3	2.313	194	201	213	rBV3	541168	1033728	77.20%	8.010%
4	2.508	229	233	234	rBV3	432	445	0.03%	0.003%
5	2.715	265	267	269	rVV2	467	324	0.02%	0.003%
6	2.794	274	280	285	rVB5	3314	6470	0.48%	0.050%
7	2.874	290	293	296	rVB2	562	691	0.05%	0.005%
8	2.947	296	305	313	rBV	21802	48827	3.65%	0.378%
9	3.032	317	319	322	rVB2	346	345	0.03%	0.003%
10	3.099	325	330	333	rBV4	981	1537	0.11%	0.012%
11	3.221	349	350	352	rVV2	548	327	0.02%	0.003%
12	3.239	352	353	356	rVV	435	398	0.03%	0.003%
13	3.288	359	361	363	rBV2	265	312	0.02%	0.002%
14	3.331	366	368	370	rBV2	456	437	0.03%	0.003%
15	3.380	375	376	381	rVB2	416	501	0.04%	0.004%
16	3.434	381	385	387	rBV2	489	681	0.05%	0.005%
17	3.483	391	393	397	rBV2	329	566	0.04%	0.004%
18	3.611	406	414	422	rBV	9412	22782	1.70%	0.177%
19	3.745	433	436	440	rBV2	378	582	0.04%	0.005%
20	3.916	463	464	467	rVB2	442	360	0.03%	0.003%
21	3.959	470	471	474	rBV2	401	320	0.02%	0.002%
22	4.001	474	478	481	rVB2	393	479	0.04%	0.004%
23	4.075	488	490	493	rVB2	322	302	0.02%	0.002%
24	4.306	525	528	534	rVB3	515	996	0.07%	0.008%
25	4.349	534	535	537	rBV	511	367	0.03%	0.003%
26	4.477	545	556	569	rBV3	149539	574951	42.94%	4.455%
27	4.757	601	602	605	rVB2	903	613	0.05%	0.005%
28	4.788	605	607	608	rBV2	523	347	0.03%	0.003%
29	4.818	610	612	613	rBV2	462	304	0.02%	0.002%
30	4.855	616	618	619	rBV	467	419	0.03%	0.003%
31	5.068	640	653	667	rBV	174211	538744	40.23%	4.174%
32	5.227	677	679	687	rVB4	666	1139	0.09%	0.009%
33	5.318	693	694	696	rBV	459	400	0.03%	0.003%
34	5.385	696	705	715	rVB3	8026	22192	1.66%	0.172%
35	5.556	727	733	742	rVB6	2928	7258	0.54%	0.056%
36	5.763	764	767	768	rVV2	440	368	0.03%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX081822\
 Data File : VX030682.D
 Acq On : 18 Aug 2022 14:03
 Operator : JC/MD
 Sample : N4221-14DL 20X
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 C0KN6DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML080422WMA.M
 Title : VOC Analysis

37	5.977	789	802	819	rBV3	458935	1339002	100.00%	10.375%
38	6.257	847	848	851	rBV	304	332	0.02%	0.003%
39	6.330	858	860	863	rVB2	399	364	0.03%	0.003%
40	6.385	864	869	875	rVB4	964	2144	0.16%	0.017%
41	6.629	906	909	911	rBV2	315	351	0.03%	0.003%
42	6.763	921	931	947	rBV	295750	715633	53.45%	5.545%
43	6.995	965	969	970	rBV2	456	577	0.04%	0.004%
44	7.056	976	979	981	rBV2	289	354	0.03%	0.003%
45	7.129	981	991	1006	rBV	563082	1227201	91.65%	9.509%
46	7.312	1012	1021	1034	rBV	271167	604971	45.18%	4.688%
47	7.550	1059	1060	1064	rVB2	432	449	0.03%	0.003%
48	7.684	1077	1082	1092	rBV3	3213	6803	0.51%	0.053%
49	7.769	1094	1096	1098	rVV2	318	359	0.03%	0.003%
50	7.836	1104	1107	1108	rBV2	374	334	0.02%	0.003%
51	7.946	1118	1125	1127	rBV3	1553	3223	0.24%	0.025%
52	8.141	1155	1157	1160	rBV2	340	373	0.03%	0.003%
53	8.184	1160	1164	1166	rVB2	574	803	0.06%	0.006%
54	8.330	1181	1188	1200	rBV	181130	301917	22.55%	2.339%
55	8.482	1209	1213	1215	rBV3	1257	1631	0.12%	0.013%
56	8.537	1220	1222	1224	rVB2	413	297	0.02%	0.002%
57	8.562	1224	1226	1228	rBV3	476	480	0.04%	0.004%
58	8.653	1233	1241	1259	rBV	707090	1092855	81.62%	8.468%
59	8.952	1283	1290	1301	rBV	138246	200107	14.94%	1.551%
60	9.275	1337	1343	1352	rVB	587711	854489	63.82%	6.621%
61	9.385	1356	1361	1376	rBV	481034	700260	52.30%	5.426%
62	9.738	1415	1419	1421	rBV4	819	1060	0.08%	0.008%
63	9.842	1433	1436	1440	rVB2	662	965	0.07%	0.007%
64	9.872	1440	1441	1443	rBV	559	467	0.03%	0.004%
65	9.891	1443	1444	1446	rBV	493	460	0.03%	0.004%
66	10.055	1465	1471	1485	rBV	602718	831495	62.10%	6.443%
67	10.201	1493	1495	1497	rBV3	500	628	0.05%	0.005%
68	10.329	1514	1516	1518	rVB3	743	623	0.05%	0.005%
69	10.378	1518	1524	1528	rBV3	4167	6426	0.48%	0.050%
70	10.525	1546	1548	1550	rBV3	434	482	0.04%	0.004%
71	10.714	1574	1579	1580	rBV2	484	695	0.05%	0.005%
72	10.768	1585	1588	1590	rBV	326	426	0.03%	0.003%
73	10.854	1600	1602	1605	rBV	519	365	0.03%	0.003%
74	10.909	1610	1611	1613	rBV	476	424	0.03%	0.003%
75	11.012	1627	1628	1630	rBV	440	339	0.03%	0.003%
76	11.092	1636	1641	1642	rBV2	466	713	0.05%	0.006%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX081822\
 Data File : VX030682.D
 Acq On : 18 Aug 2022 14:03
 Operator : JC/MD
 Sample : N4221-14DL 20X
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 C0KN6DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML080422WMA.M
 Title : VOC Analysis

77	11.195	1652	1658	1666	rBV	502101	636535	47.54%	4.932%
78	11.482	1703	1705	1708	rVV2	620	378	0.03%	0.003%
79	11.622	1726	1728	1729	rVB	575	315	0.02%	0.002%
80	11.646	1729	1732	1734	rBV2	391	598	0.04%	0.005%
81	11.713	1742	1743	1746	rBV3	660	546	0.04%	0.004%
82	11.762	1750	1751	1754	rVB3	619	523	0.04%	0.004%
83	11.890	1771	1772	1775	rVB2	503	328	0.02%	0.003%
84	12.024	1788	1794	1807	rBV	637241	772942	57.73%	5.989%
85	12.219	1825	1826	1830	rVB3	983	1205	0.09%	0.009%
86	12.274	1834	1835	1837	rBV	594	307	0.02%	0.002%
87	12.323	1837	1843	1858	rVV	738559	913481	68.22%	7.078%
88	13.189	1984	1985	1990	rBV2	566	838	0.06%	0.006%
89	13.292	2000	2002	2003	rBV2	389	382	0.03%	0.003%
90	13.408	2019	2021	2022	rBV2	459	299	0.02%	0.002%
91	13.500	2034	2036	2038	rBV2	580	531	0.04%	0.004%
92	13.811	2086	2087	2089	rBV	559	461	0.03%	0.004%
93	14.042	2123	2125	2127	rBV	520	341	0.03%	0.003%
94	14.134	2134	2140	2143	rBV2	1996	3011	0.22%	0.023%
95	14.298	2166	2167	2169	rBV	704	332	0.02%	0.003%
96	14.609	2217	2218	2221	rBV2	681	638	0.05%	0.005%
97	14.999	2281	2282	2286	rVB2	939	661	0.05%	0.005%
98	16.011	2446	2448	2451	rBV2	890	1060	0.08%	0.008%
99	16.292	2493	2494	2496	rBV	835	384	0.03%	0.003%
100	16.603	2543	2545	2546	rBV2	666	387	0.03%	0.003%




Sum of corrected areas: 12905694

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX081822\
Data File : VX030682.D
Acq On : 18 Aug 2022 14:03
Operator : JC/MD
Sample : N4221-14DL 20X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
C0KN6DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML080422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

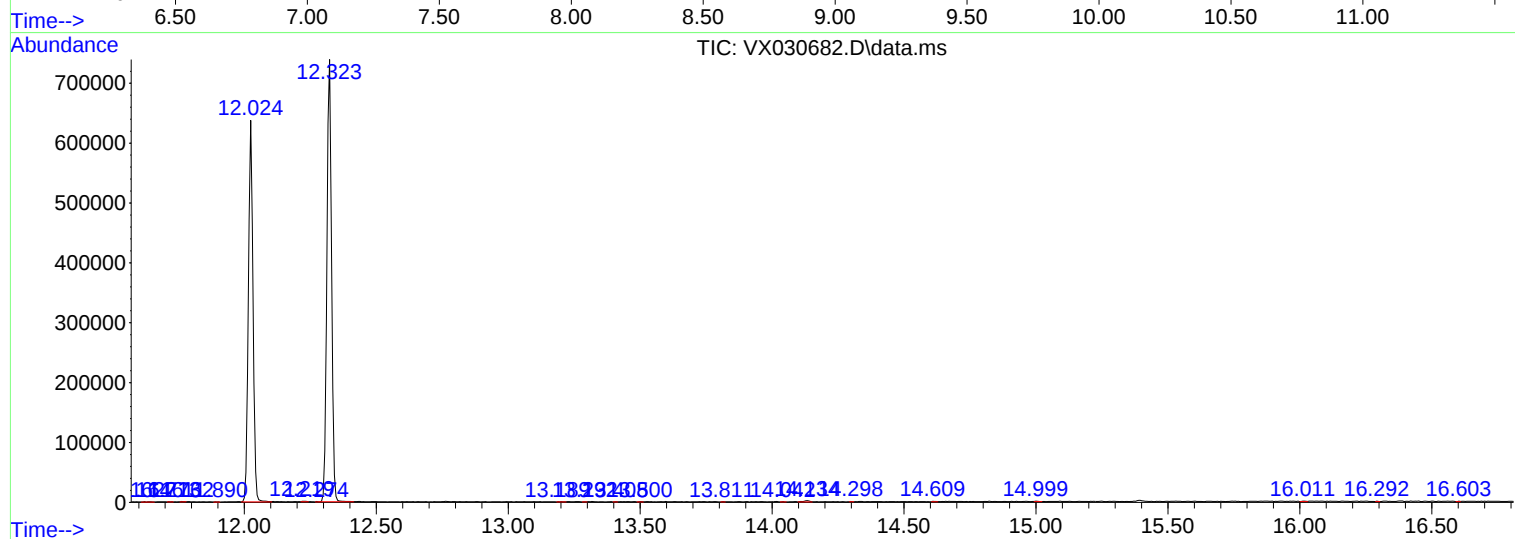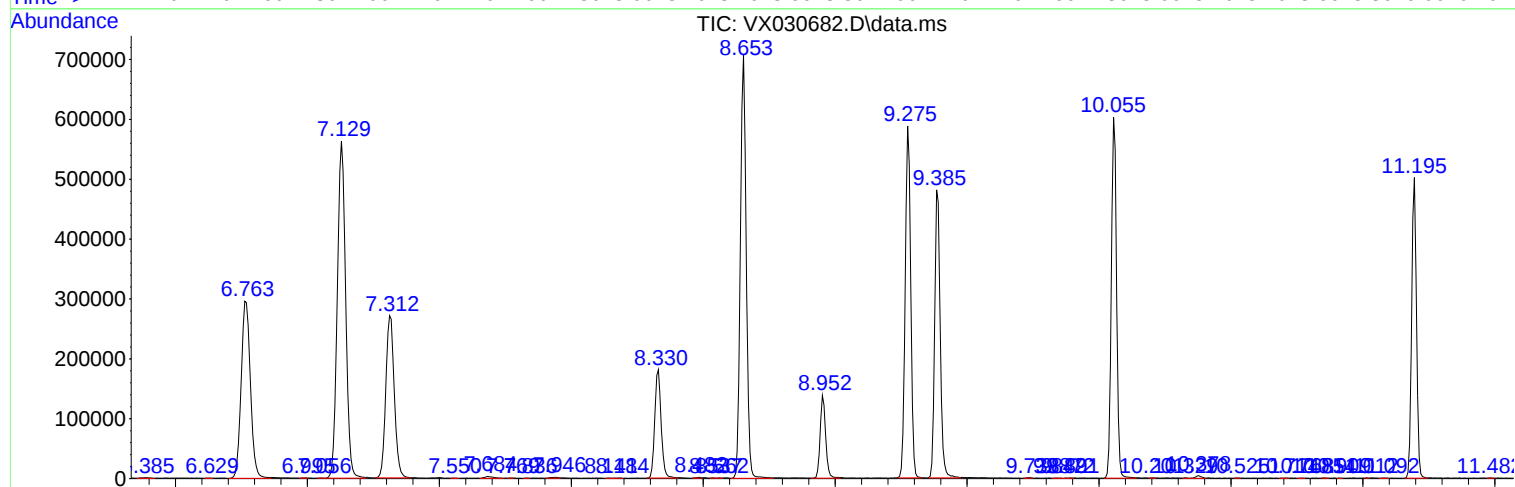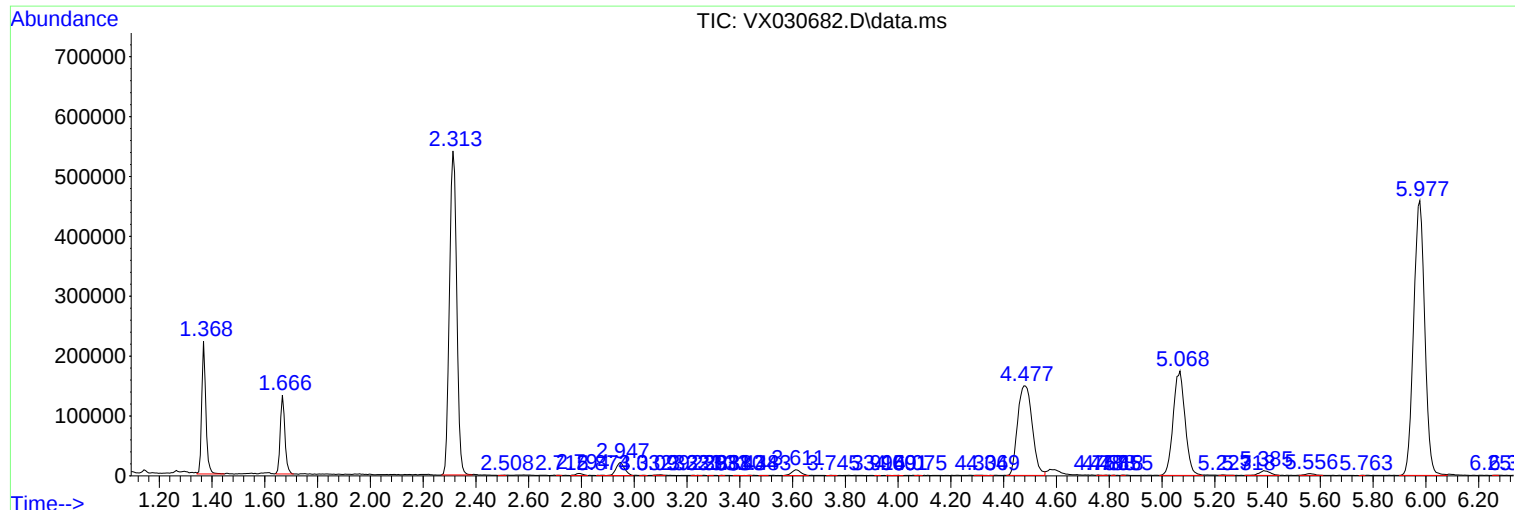

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX081822\
Data File : VX030682.D
Acq On : 18 Aug 2022 14:03
Operator : JC/MD
Sample : N4221-14DL 20X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
C0KN6DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML080422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX081822\
Data File : VX030682.D
Acq On : 18 Aug 2022 14:03
Operator : JC/MD
Sample : N4221-14DL 20X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
C0KN6DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML080422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc