

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX081822\
 Data File : VX030683.D
 Acq On : 18 Aug 2022 14:27
 Operator : JC/MD
 Sample : N4221-15DL 20X
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 C0KN7DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML080422WMA.M
 Title : VOC Analysis

Signal : TIC: VX030683.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.142	7	9	13	rVB	5858	5102	0.38%	0.040%
2	1.368	42	46	56	rVB2	223666	234356	17.64%	1.851%
3	1.666	91	95	103	rVB	129146	157583	11.86%	1.245%
4	2.124	169	170	173	rBV3	921	1098	0.08%	0.009%
5	2.313	194	201	211	rBV2	530466	996753	75.03%	7.873%
6	2.483	227	229	231	rBV2	617	475	0.04%	0.004%
7	2.502	231	232	233	rBV	640	327	0.02%	0.003%
8	2.605	247	249	252	rVB2	682	553	0.04%	0.004%
9	2.648	252	256	257	rBV2	555	609	0.05%	0.005%
10	2.684	261	262	266	rBV2	513	473	0.04%	0.004%
11	2.788	275	279	286	rBV4	3115	6003	0.45%	0.047%
12	2.947	296	305	316	rBV2	18617	45055	3.39%	0.356%
13	3.087	324	328	333	rBV3	1388	2633	0.20%	0.021%
14	3.123	333	334	337	rVV	607	354	0.03%	0.003%
15	3.166	339	341	344	rVB2	462	331	0.02%	0.003%
16	3.459	387	389	393	rVB2	460	464	0.03%	0.004%
17	3.611	408	414	424	rVV	9385	20969	1.58%	0.166%
18	3.727	432	433	437	rBV	307	336	0.03%	0.003%
19	3.910	461	463	467	rVB2	363	379	0.03%	0.003%
20	3.989	472	476	478	rBV2	287	394	0.03%	0.003%
21	4.020	478	481	486	rVV2	373	521	0.04%	0.004%
22	4.062	486	488	491	rVB2	470	424	0.03%	0.003%
23	4.087	491	492	495	rBV2	564	417	0.03%	0.003%
24	4.349	531	535	536	rBV2	784	750	0.06%	0.006%
25	4.477	544	556	569	rBV2	145596	558746	42.06%	4.414%
26	4.830	612	614	616	rBV	610	375	0.03%	0.003%
27	4.946	631	633	634	rBV	394	331	0.02%	0.003%
28	5.062	639	652	667	rBV	170346	531041	39.98%	4.195%
29	5.221	676	678	682	rVB4	732	757	0.06%	0.006%
30	5.269	684	686	688	rBV3	552	389	0.03%	0.003%
31	5.294	688	690	693	rVB	586	610	0.05%	0.005%
32	5.330	693	696	697	rBV	527	445	0.03%	0.004%
33	5.391	699	706	715	rVB6	6951	19702	1.48%	0.156%
34	5.562	726	734	740	rBV5	2618	6811	0.51%	0.054%
35	5.977	790	802	815	rBV2	457130	1328425	100.00%	10.493%
36	6.263	845	849	852	rVB3	607	1094	0.08%	0.009%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX081822\
 Data File : VX030683.D
 Acq On : 18 Aug 2022 14:27
 Operator : JC/MD
 Sample : N4221-15DL 20X
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 C0KN7DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML080422WMA.M
 Title : VOC Analysis

37	6.294	852	854	855	rBV	414	342	0.03%	0.003%
38	6.342	859	862	865	rBV2	372	701	0.05%	0.006%
39	6.379	865	868	870	rBV3	548	750	0.06%	0.006%
40	6.519	889	891	893	rBV2	348	485	0.04%	0.004%
41	6.769	922	932	945	rBV	309934	736764	55.46%	5.820%
42	7.129	980	991	1008	rBV	521153	1143704	86.09%	9.034%
43	7.312	1013	1021	1037	rVB	272503	599582	45.13%	4.736%
44	7.482	1047	1049	1055	rVB3	875	936	0.07%	0.007%
45	7.629	1072	1073	1076	rBV2	596	517	0.04%	0.004%
46	7.684	1076	1082	1089	rBV4	2512	6268	0.47%	0.050%
47	7.805	1100	1102	1105	rVB	468	392	0.03%	0.003%
48	7.946	1119	1125	1127	rBV3	1401	2818	0.21%	0.022%
49	8.031	1136	1139	1140	rBV2	919	691	0.05%	0.005%
50	8.116	1152	1153	1156	rVB2	655	558	0.04%	0.004%
51	8.147	1156	1158	1159	rBV2	541	353	0.03%	0.003%
52	8.196	1163	1166	1167	rBV2	384	395	0.03%	0.003%
53	8.263	1173	1177	1180	rBV2	360	497	0.04%	0.004%
54	8.330	1182	1188	1196	rBV	179810	296612	22.33%	2.343%
55	8.476	1209	1212	1221	rVB4	1018	2390	0.18%	0.019%
56	8.555	1224	1225	1227	rBV2	376	348	0.03%	0.003%
57	8.574	1227	1228	1230	rBV2	490	334	0.03%	0.003%
58	8.653	1234	1241	1249	rBV	708320	1086125	81.76%	8.579%
59	8.952	1284	1290	1298	rBV	132930	194635	14.65%	1.537%
60	9.275	1334	1343	1356	rBV	524580	752765	56.67%	5.946%
61	9.384	1356	1361	1373	rBV	476948	695237	52.34%	5.492%
62	9.598	1394	1396	1397	rBV	542	464	0.03%	0.004%
63	9.708	1412	1414	1415	rBV2	404	356	0.03%	0.003%
64	9.732	1416	1418	1424	rVV3	1078	1313	0.10%	0.010%
65	9.890	1442	1444	1448	rBV2	427	583	0.04%	0.005%
66	9.945	1451	1453	1456	rBV2	312	351	0.03%	0.003%
67	10.055	1465	1471	1484	rBV	650784	856939	64.51%	6.769%
68	10.378	1520	1524	1529	rBV3	3700	5300	0.40%	0.042%
69	10.494	1541	1543	1544	rBV	493	346	0.03%	0.003%
70	10.561	1552	1554	1555	rBV	394	331	0.02%	0.003%
71	10.622	1563	1564	1566	rBV	598	349	0.03%	0.003%
72	10.720	1578	1580	1582	rBV	440	445	0.03%	0.004%
73	10.884	1605	1607	1614	rVB2	538	1011	0.08%	0.008%
74	11.091	1639	1641	1644	rBV	732	743	0.06%	0.006%
75	11.195	1652	1658	1665	rBV	488138	620887	46.74%	4.904%
76	11.274	1669	1671	1674	rVB2	818	639	0.05%	0.005%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX081822\
 Data File : VX030683.D
 Acq On : 18 Aug 2022 14:27
 Operator : JC/MD
 Sample : N4221-15DL 20X
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 C0KN7DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML080422WMA.M
 Title : VOC Analysis

77	11.408	1690	1693	1694	rBV	319	383	0.03%	0.003%
78	11.549	1714	1716	1717	rBV	560	318	0.02%	0.003%
79	11.811	1757	1759	1761	rBV	395	403	0.03%	0.003%
80	12.024	1788	1794	1805	rBV	669158	800436	60.25%	6.323%
81	12.128	1809	1811	1814	rVB2	1065	731	0.06%	0.006%
82	12.225	1823	1827	1829	rBV2	1439	1826	0.14%	0.014%
83	12.323	1837	1843	1852	rBV	709208	905187	68.14%	7.150%
84	12.457	1863	1865	1866	rVB2	656	436	0.03%	0.003%
85	12.585	1884	1886	1891	rBV3	580	851	0.06%	0.007%
86	12.622	1891	1892	1895	rVV2	487	405	0.03%	0.003%
87	13.372	2013	2015	2018	rBV2	590	405	0.03%	0.003%
88	13.652	2059	2061	2063	rBV	547	666	0.05%	0.005%
89	13.932	2105	2107	2108	rBV	586	412	0.03%	0.003%
90	14.127	2137	2139	2146	rVB2	2093	2811	0.21%	0.022%
91	14.335	2171	2173	2176	rVB2	633	709	0.05%	0.006%
92	14.371	2176	2179	2180	rBV	458	543	0.04%	0.004%
93	14.524	2202	2204	2205	rBV	471	348	0.03%	0.003%
94	15.127	2302	2303	2304	rBV	945	356	0.03%	0.003%
95	15.243	2320	2322	2324	rVB2	709	352	0.03%	0.003%
96	15.298	2329	2331	2332	rVB2	912	423	0.03%	0.003%
97	15.316	2332	2334	2337	rBV2	848	955	0.07%	0.008%
98	15.719	2399	2400	2401	rBV	725	400	0.03%	0.003%
99	15.902	2428	2430	2432	rBV3	859	725	0.05%	0.006%
100	16.481	2523	2525	2526	rBV	760	318	0.02%	0.003%




Sum of corrected areas: 12659740

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX081822\
Data File : VX030683.D
Acq On : 18 Aug 2022 14:27
Operator : JC/MD
Sample : N4221-15DL 20X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
C0KN7DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML080422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

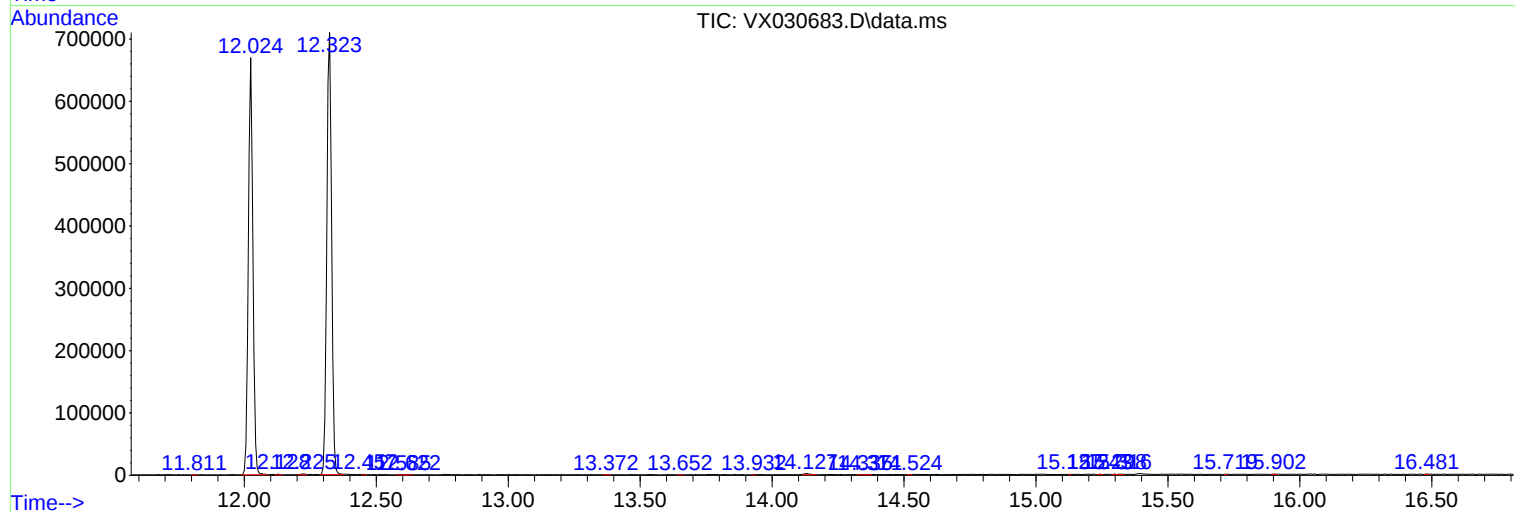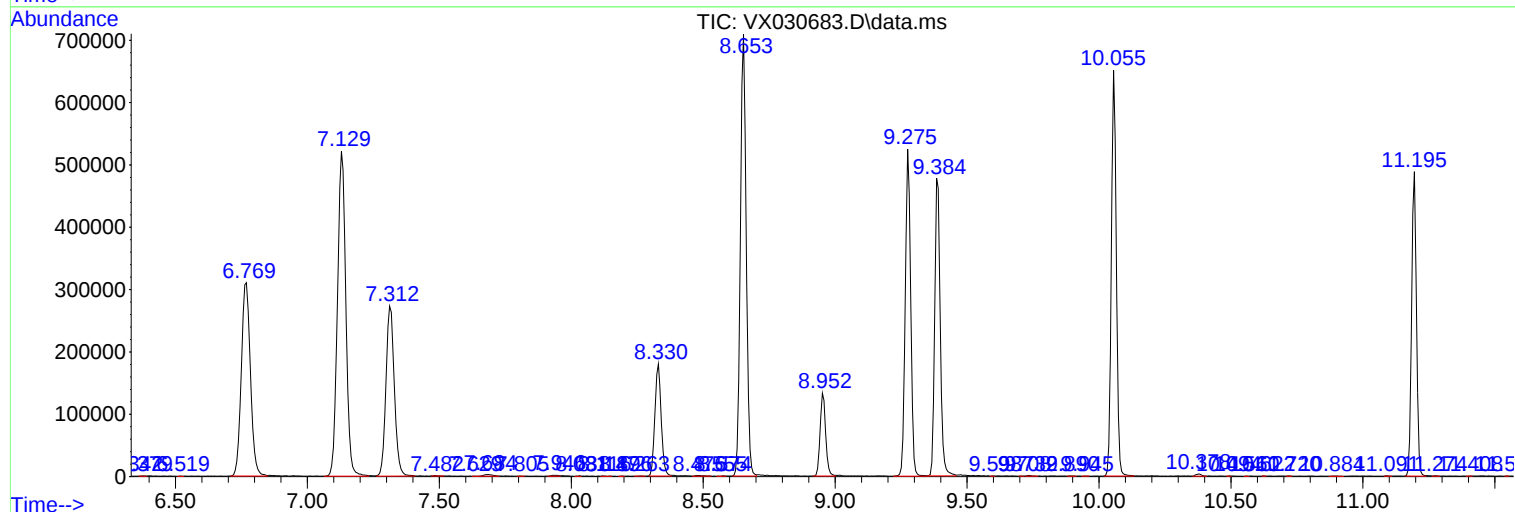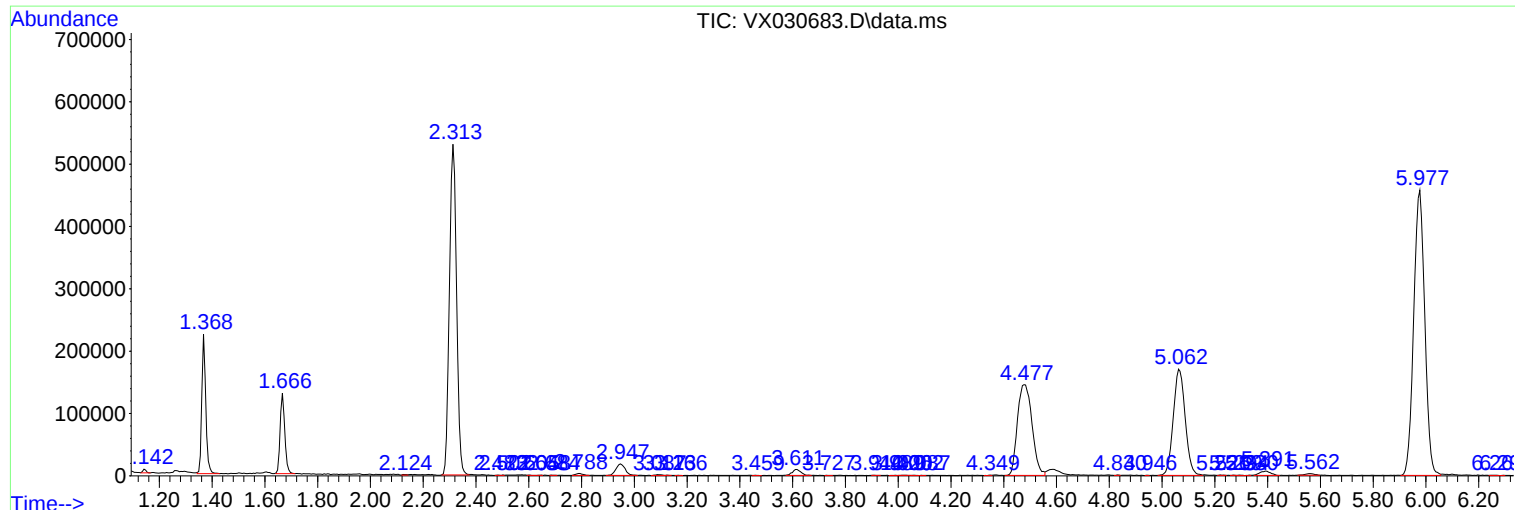

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX081822\
Data File : VX030683.D
Acq On : 18 Aug 2022 14:27
Operator : JC/MD
Sample : N4221-15DL 20X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
C0KN7DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML080422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX081822\
Data File : VX030683.D
Acq On : 18 Aug 2022 14:27
Operator : JC/MD
Sample : N4221-15DL 20X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
C0KN7DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML080422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc