

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX081822\
 Data File : VX030684.D
 Acq On : 18 Aug 2022 14:50
 Operator : JC/MD
 Sample : N4221-13 40X
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 C0KN3

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML080422WMA.M

Title : VOC Analysis

Signal : TIC: VX030684.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.368	42	46	53	rVB	197389	199096	14.71%	1.724%
2	1.666	90	95	105	rVB	135640	165178	12.21%	1.430%
3	2.307	194	200	210	rBV3	362898	633435	46.81%	5.484%
4	2.557	239	241	243	rBV2	720	634	0.05%	0.005%
5	2.630	250	253	255	rBV2	667	784	0.06%	0.007%
6	2.788	273	279	285	rBV3	5717	10522	0.78%	0.091%
7	2.947	297	305	316	rVB	21006	48028	3.55%	0.416%
8	3.038	319	320	324	rBV	389	296	0.02%	0.003%
9	3.093	326	329	331	rBV	593	680	0.05%	0.006%
10	3.166	339	341	343	rVB	353	281	0.02%	0.002%
11	3.191	343	345	347	rBV2	208	252	0.02%	0.002%
12	3.294	360	362	364	rVB2	423	348	0.03%	0.003%
13	3.325	364	367	368	rBV2	362	385	0.03%	0.003%
14	3.343	368	370	371	rVV	525	302	0.02%	0.003%
15	3.361	371	373	375	rVB2	363	276	0.02%	0.002%
16	3.386	375	377	379	rBV2	309	271	0.02%	0.002%
17	3.489	391	394	398	rBV2	399	562	0.04%	0.005%
18	3.526	398	400	401	rBV2	409	357	0.03%	0.003%
19	3.611	408	414	422	rVV2	5907	12197	0.90%	0.106%
20	3.794	443	444	446	rBV	433	287	0.02%	0.002%
21	3.837	450	451	455	rVB	367	268	0.02%	0.002%
22	3.886	457	459	461	rVV	315	281	0.02%	0.002%
23	3.995	474	477	478	rBV2	374	430	0.03%	0.004%
24	4.318	529	530	533	rVB2	538	322	0.02%	0.003%
25	4.379	538	540	543	rBV2	428	401	0.03%	0.003%
26	4.465	546	554	569	rBV2	119124	381261	28.18%	3.301%
27	4.751	600	601	605	rBV2	602	575	0.04%	0.005%
28	4.867	619	620	622	rBV2	509	275	0.02%	0.002%
29	5.062	640	652	669	rBV	180266	540580	39.95%	4.680%
30	5.294	686	690	691	rBV2	649	443	0.03%	0.004%
31	5.391	699	706	712	rBV5	1991	5224	0.39%	0.045%
32	5.458	715	717	718	rBV	413	300	0.02%	0.003%
33	5.477	718	720	722	rBV	517	449	0.03%	0.004%
34	5.556	726	733	740	rBV4	3204	7745	0.57%	0.067%
35	5.690	753	755	757	rBV	318	273	0.02%	0.002%
36	5.708	757	758	760	rBV2	437	300	0.02%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX081822\
 Data File : VX030684.D
 Acq On : 18 Aug 2022 14:50
 Operator : JC/MD
 Sample : N4221-13 40X
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 C0KN3

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML080422WMA.M
 Title : VOC Analysis

37	5.977	790	802	815	rBV2	465279	1353152	100.00%	11.715%
38	6.373	864	867	869	rVB4	688	652	0.05%	0.006%
39	6.428	874	876	879	rVB2	435	496	0.04%	0.004%
40	6.452	879	880	881	rBV	440	227	0.02%	0.002%
41	6.647	909	912	913	rBV	379	296	0.02%	0.003%
42	6.769	922	932	944	rBV	314211	743008	54.91%	6.433%
43	6.970	964	965	968	rBV2	272	244	0.02%	0.002%
44	7.129	980	991	1009	rBV	459603	1000884	73.97%	8.665%
45	7.312	1013	1021	1038	rVV	277087	613715	45.35%	5.313%
46	7.635	1071	1074	1075	rBV	284	295	0.02%	0.003%
47	7.684	1078	1082	1088	rVV2	1310	2919	0.22%	0.025%
48	7.769	1092	1096	1097	rBV2	450	500	0.04%	0.004%
49	7.842	1105	1108	1111	rBV2	459	642	0.05%	0.006%
50	7.934	1120	1123	1125	rBV2	1339	1958	0.14%	0.017%
51	8.037	1137	1140	1141	rBV	422	350	0.03%	0.003%
52	8.135	1154	1156	1159	rVB	356	305	0.02%	0.003%
53	8.165	1159	1161	1162	rBV	423	254	0.02%	0.002%
54	8.330	1181	1188	1198	rBV	183839	301218	22.26%	2.608%
55	8.586	1226	1230	1233	rVB3	589	765	0.06%	0.007%
56	8.653	1233	1241	1253	rBV	710112	1097065	81.07%	9.498%
57	8.848	1272	1273	1274	rBV	612	269	0.02%	0.002%
58	8.952	1285	1290	1300	rBV	128237	194194	14.35%	1.681%
59	9.074	1309	1310	1311	rBV	428	231	0.02%	0.002%
60	9.220	1329	1334	1336	rBV3	646	1015	0.08%	0.009%
61	9.275	1336	1343	1353	rVV	192157	276805	20.46%	2.396%
62	9.385	1355	1361	1375	rBV	494833	711020	52.55%	6.156%
63	9.817	1430	1432	1435	rVB	902	648	0.05%	0.006%
64	9.854	1435	1438	1440	rBV2	464	619	0.05%	0.005%
65	10.055	1465	1471	1482	rBV	658047	869975	64.29%	7.532%
66	10.378	1522	1524	1526	rVB	959	682	0.05%	0.006%
67	10.451	1534	1536	1538	rBV	358	229	0.02%	0.002%
68	10.616	1561	1563	1564	rVB	445	231	0.02%	0.002%
69	10.701	1575	1577	1581	rBV2	381	457	0.03%	0.004%
70	10.903	1608	1610	1612	rBV2	326	248	0.02%	0.002%
71	10.939	1614	1616	1617	rVB2	514	290	0.02%	0.003%
72	11.018	1627	1629	1633	rVB	722	691	0.05%	0.006%
73	11.195	1652	1658	1669	rBV	491820	626748	46.32%	5.426%
74	11.348	1682	1683	1685	rVB	492	242	0.02%	0.002%
75	11.421	1693	1695	1696	rBV	523	291	0.02%	0.003%
76	11.677	1735	1737	1738	rBV2	548	548	0.04%	0.005%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX081822\
 Data File : VX030684.D
 Acq On : 18 Aug 2022 14:50
 Operator : JC/MD
 Sample : N4221-13 40X
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 C0KN3

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML080422WMA.M
 Title : VOC Analysis

77	11.945	1780	1781	1784	rBV2	751	955	0.07%	0.008%
78	12.024	1789	1794	1803	rVV	668388	799185	59.06%	6.919%
79	12.165	1815	1817	1818	rBV	625	381	0.03%	0.003%
80	12.226	1825	1827	1831	rVB3	984	1081	0.08%	0.009%
81	12.256	1831	1832	1834	rBV	445	361	0.03%	0.003%
82	12.323	1837	1843	1850	rBV	732386	918539	67.88%	7.952%
83	12.616	1889	1891	1892	rVB	502	248	0.02%	0.002%
84	12.939	1943	1944	1947	rBV2	345	318	0.02%	0.003%
85	13.024	1955	1958	1959	rBV	357	266	0.02%	0.002%
86	13.128	1973	1975	1979	rBV2	643	766	0.06%	0.007%
87	13.164	1979	1981	1983	rVV2	619	490	0.04%	0.004%
88	13.207	1986	1988	1989	rBV	407	271	0.02%	0.002%
89	13.335	2007	2009	2011	rBV2	434	447	0.03%	0.004%
90	13.378	2014	2016	2018	rVB	516	350	0.03%	0.003%
91	13.408	2019	2021	2024	rBV2	523	502	0.04%	0.004%
92	13.524	2038	2040	2041	rBV	379	306	0.02%	0.003%
93	13.817	2086	2088	2089	rBV	551	298	0.02%	0.003%
94	14.134	2137	2140	2146	rVB3	2004	2745	0.20%	0.024%
95	14.689	2228	2231	2232	rBV	887	953	0.07%	0.008%
96	14.737	2238	2239	2240	rBV	532	234	0.02%	0.002%
97	14.884	2262	2263	2265	rBV2	831	456	0.03%	0.004%
98	15.237	2319	2321	2322	rBV	802	444	0.03%	0.004%
99	15.390	2344	2346	2351	rVB3	1942	2671	0.20%	0.023%
100	16.609	2544	2546	2548	rBV2	914	750	0.06%	0.006%


Sum of corrected areas: 11550693

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX081822\
Data File : VX030684.D
Acq On : 18 Aug 2022 14:50
Operator : JC/MD
Sample : N4221-13 40X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
COKN3

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML080422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

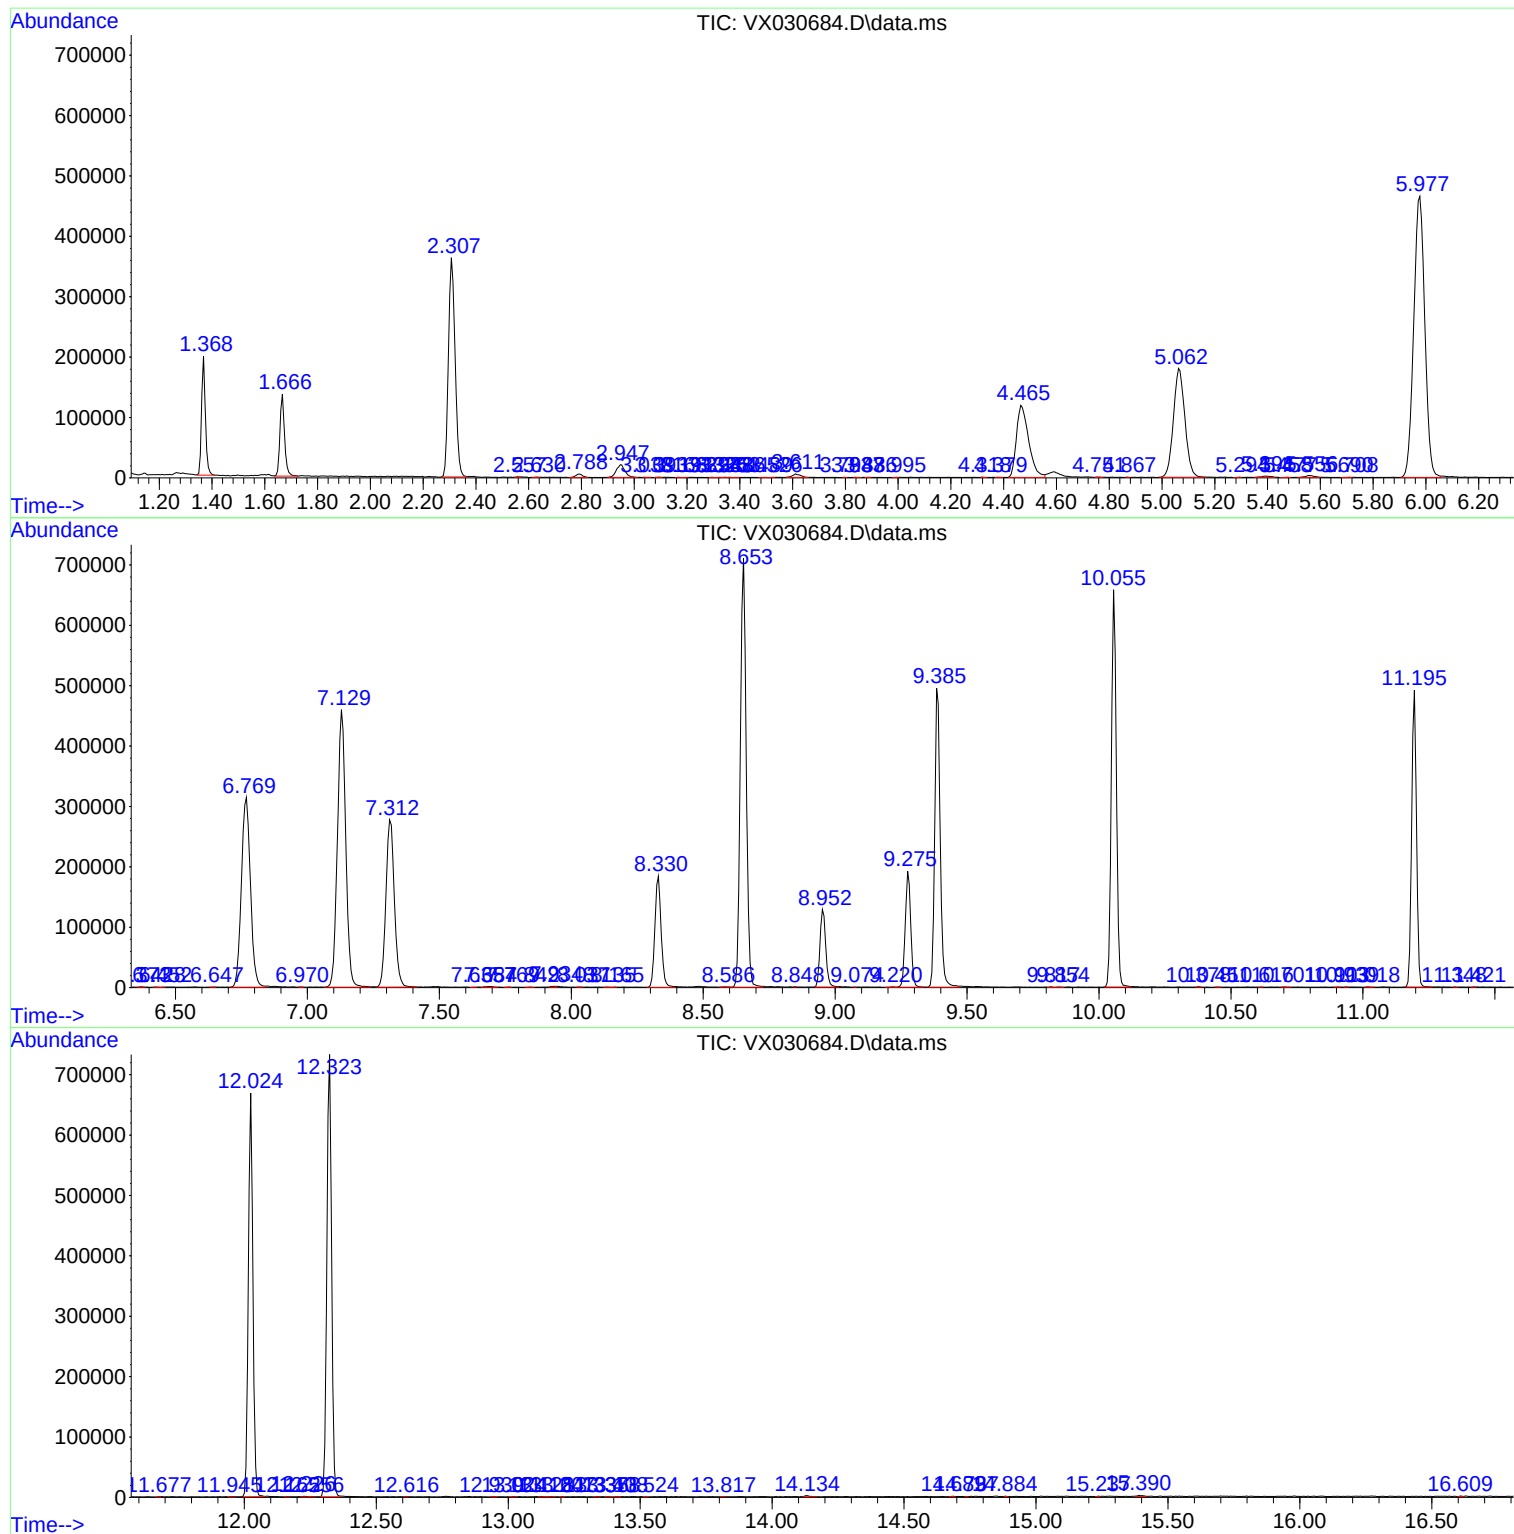

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX081822\
Data File : VX030684.D
Acq On : 18 Aug 2022 14:50
Operator : JC/MD
Sample : N4221-13 40X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
C0KN3

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML080422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX081822\
Data File : VX030684.D
Acq On : 18 Aug 2022 14:50
Operator : JC/MD
Sample : N4221-13 40X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
C0KN3

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML080422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc