
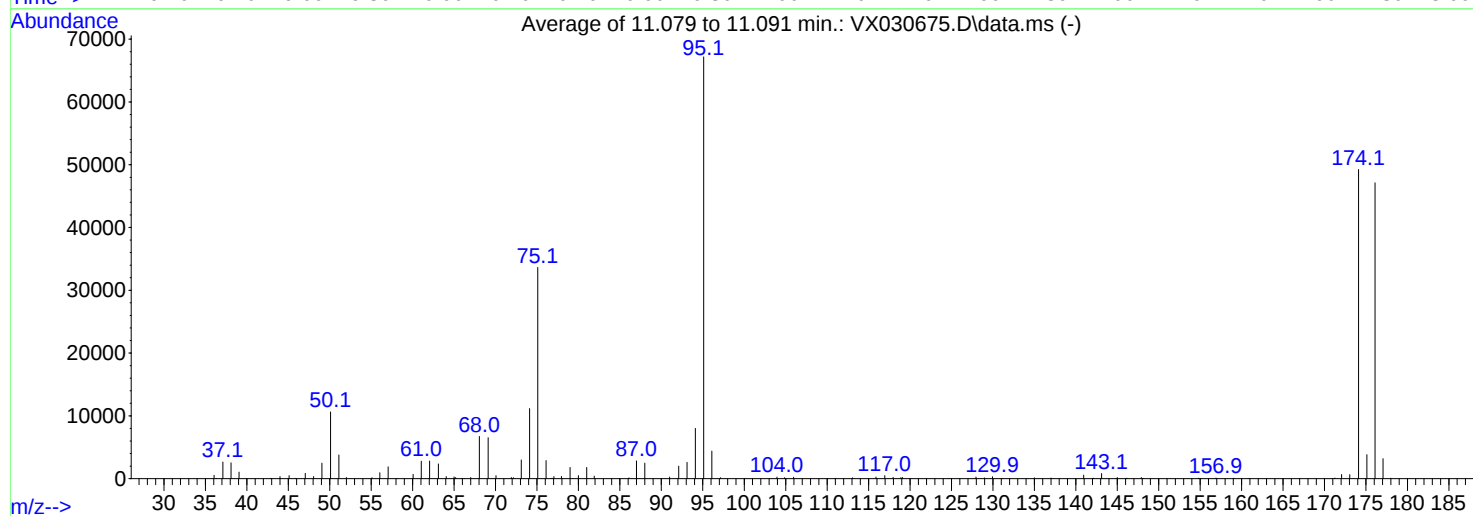


Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX081822\
 Data File : VX030675.D
 Acq On : 18 Aug 2022 10:42
 Operator : JC/MD
 Sample : BFB682
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 BFB682

Integration File: LSCINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM080422WMA.M
 Title : VOC Analysis
 Last Update : Tue Aug 23 02:05:32 2022

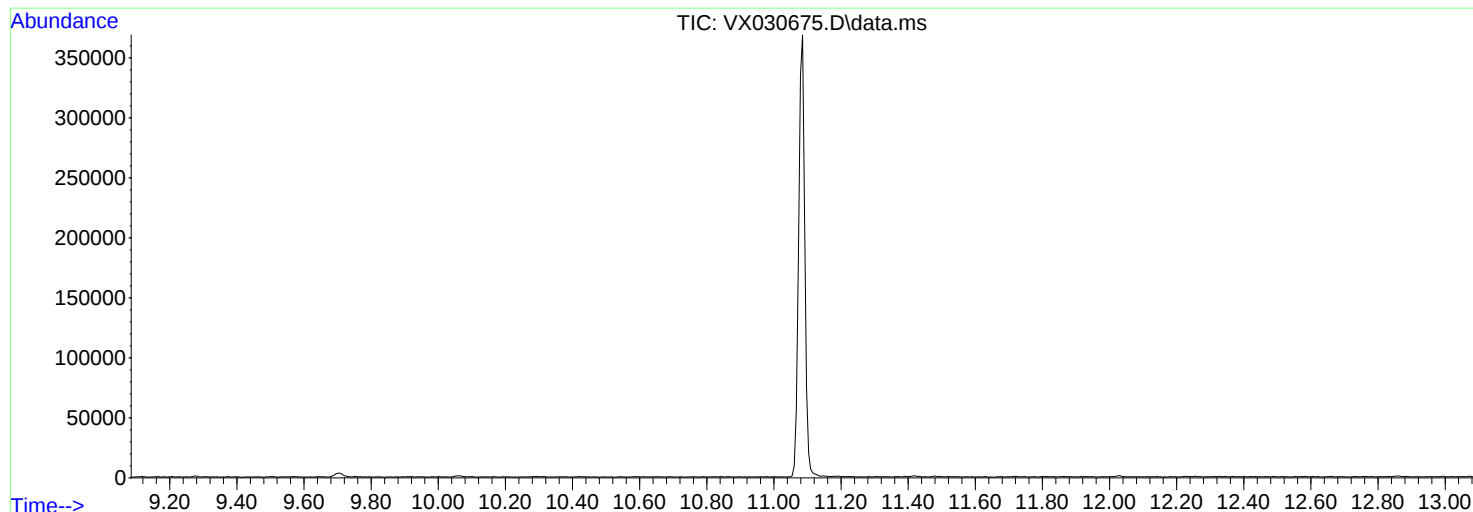

AutoFind: Scans 1639, 1640, 1641; Background Corrected with Scan 1633

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	15.8	10622	PASS
75	95	30	80	50.1	33629	PASS
95	95	100	100	100.0	67181	PASS
96	95	5	9	6.5	4381	PASS
173	174	0.00	2	1.3	631	PASS
174	95	50	120	73.3	49240	PASS
175	174	5	9	7.8	3825	PASS
176	174	95	101	95.7	47131	PASS
177	176	5	9	6.8	3193	PASS

m/z	Abundance
40.10	555.0
44.00	256.0
118.90	77.0

Instrument :
MSVOA_X
ClientSampleId :
BFB682

m/z	Abundance
36.00	739.0
37.10	3071.0
38.10	3111.0
39.10	1272.0
40.10	597.0
42.90	57.0
44.00	631.0
45.10	606.0
46.00	80.0
47.00	912.0
48.10	459.0
49.10	2933.0
50.10	13021.0
51.10	4217.0
52.00	249.0
55.00	102.0
56.00	1156.0
57.10	2229.0
60.10	768.0
61.00	3388.0
62.10	3276.0
63.10	2626.0
64.00	363.0
65.00	589.0
66.30	53.0
67.00	215.0
68.00	7444.0
69.10	7751.0
70.10	638.0
71.90	526.0
73.10	3280.0
74.10	12385.0
75.10	38008.0
76.10	3153.0
77.10	457.0
78.00	298.0
79.00	2089.0
79.90	523.0
81.00	2140.0
82.00	574.0
86.10	64.0
87.00	3269.0
88.00	2483.0
91.00	290.0
92.10	2060.0
93.10	2934.0
94.10	8805.0
95.10	75592.0
96.10	5374.0
97.20	261.0
104.00	389.0
104.80	168.0
106.00	242.0
113.00	114.0
116.00	345.0
116.90	489.0
118.00	186.0
118.90	418.0
127.90	290.0
128.90	148.0
130.00	497.0
135.00	123.0
137.00	91.0
141.00	502.0
142.10	85.0
143.10	1052.0
145.10	170.0
146.10	97.0
147.90	255.0
154.80	80.0
156.90	136.0
159.00	78.0
171.30	134.0
172.00	558.0
173.10	590.0
174.10	47792.0
175.10	3394.0
176.10	46208.0
177.00	3459.0
178.10	85.0

Instrument :
MSVOA_X
ClientSampleId :
BFB682

m/z	Abundance
36.10	621.0
37.10	3329.0
38.10	2860.0
39.00	1256.0
40.10	514.0
42.90	81.0
44.00	611.0
45.10	590.0
47.10	909.0
48.00	314.0
49.00	2873.0
50.10	12760.0
51.10	4631.0
52.00	168.0
55.10	257.0
56.10	1189.0
57.00	2458.0
58.10	75.0
60.00	757.0
61.10	3507.0
62.00	3254.0
63.10	2751.0
64.00	297.0
65.20	557.0
65.90	87.0
67.00	212.0
68.10	8175.0
69.10	7686.0
70.00	465.0
72.10	197.0
73.10	3773.0
74.10	13706.0
75.10	40448.0
76.10	3756.0
77.00	331.0
78.00	463.0
79.00	2219.0
80.00	580.0
81.00	2144.0
81.90	336.0
86.20	86.0
87.00	3412.0
88.00	3063.0
91.00	308.0
92.10	2272.0
93.10	3141.0
94.10	9714.0
95.10	80136.0
96.10	4721.0
97.10	136.0
103.90	206.0
104.80	139.0
105.90	325.0
111.00	90.0
113.10	159.0
115.90	270.0
117.00	539.0
118.00	272.0
119.10	522.0
124.70	56.0
128.00	219.0
129.00	111.0
130.00	298.0
131.20	77.0
134.90	207.0
137.00	169.0
141.00	706.0
142.10	165.0
143.10	763.0
144.90	219.0
146.20	66.0
147.90	308.0
154.80	155.0
156.90	129.0
159.10	70.0
160.80	72.0
171.30	86.0
172.10	641.0
173.00	812.0
174.10	58384.0
175.10	4628.0
176.10	56080.0
177.10	3799.0
177.90	115.0

Instrument :
MSVOA_X
ClientSampleId :
BFB682

m/z	Abundance
35.90	218.0
36.30	200.0
37.10	1563.0
38.10	1577.0
39.00	626.0
40.00	342.0
44.00	533.0
45.20	301.0
45.80	50.0
47.10	691.0
48.00	253.0
49.00	1599.0
50.10	6086.0
51.10	2475.0
52.00	139.0
55.20	95.0
56.20	458.0
57.10	1002.0
60.10	516.0
61.00	1412.0
62.00	1892.0
63.10	1694.0
64.10	336.0
65.00	226.0
66.00	73.0
67.10	133.0
68.10	4532.0
69.00	4154.0
70.00	381.0
72.20	289.0
73.10	1865.0
74.10	7404.0
75.10	22432.0
76.10	1732.0
76.80	218.0
77.10	228.0
77.90	294.0
78.90	1089.0
80.10	366.0
80.90	1042.0
81.80	311.0
86.10	210.0
87.00	1807.0
88.00	1854.0
90.90	143.0
92.10	1639.0
93.10	1721.0
94.10	5511.0
95.10	45816.0
96.10	3049.0
97.00	60.0
103.90	185.0
104.90	128.0
105.90	155.0
110.80	53.0
113.00	128.0
115.80	188.0
117.00	443.0
117.90	194.0
118.90	379.0
127.90	293.0
129.00	117.0
129.80	157.0
135.10	80.0
137.00	69.0
140.80	454.0
143.10	650.0
145.00	134.0
146.10	95.0
148.10	132.0
155.10	103.0
157.00	78.0
159.10	64.0
171.20	99.0
172.10	800.0
173.10	490.0
174.10	41544.0
175.10	3453.0
176.10	39104.0
177.10	2321.0
178.10	50.0

Instrument :
MSVOA_X
ClientSampleId :
BFB682