

Data Path : Z:\voasrv\HPCHEM1\MSVOA\_X\Data\VX081823\  
 Data File : VX037071.D  
 Acq On : 18 Aug 2023 09:54  
 Operator : JC/MD  
 Sample : VX0818MBL01  
 Misc : 5.00g/10mL/100uL/5.00mL/MSVOA\_X/MEOH  
 ALS Vial : 3 Sample Multiplier: 1

Instrument :  
 MSVOA\_X  
 ClientSampleId :  
 VX0818MBL01

Quant Time: Aug 19 05:12:40 2023  
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA\_X\Method\82X081723W.M  
 Quant Title : SW846 8260  
 QLast Update : Fri Aug 18 09:30:38 2023  
 Response via : Initial Calibration


| Compound                      | R.T.           | QIon | Response   | Conc     | Units  | Dev(Min) |
|-------------------------------|----------------|------|------------|----------|--------|----------|
| -----                         |                |      |            |          |        |          |
| Internal Standards            |                |      |            |          |        |          |
| 1) Pentafluorobenzene         | 5.550          | 168  | 122145     | 50.000   | ug/l   | 0.00     |
| 34) 1,4-Difluorobenzene       | 6.757          | 114  | 223202     | 50.000   | ug/l   | 0.00     |
| 63) Chlorobenzene-d5          | 10.055         | 117  | 217130     | 50.000   | ug/l   | 0.00     |
| 72) 1,4-Dichlorobenzene-d4    | 12.024         | 152  | 99721      | 50.000   | ug/l   | 0.00     |
|                               |                |      |            |          |        |          |
| System Monitoring Compounds   |                |      |            |          |        |          |
| 33) 1,2-Dichloroethane-d4     | 5.952          | 65   | 84340      | 47.895   | ug/l   | 0.00     |
| Spiked Amount 50.000          | Range 78 - 117 |      | Recovery = | 95.780%  |        |          |
| 35) Dibromofluoromethane      | 5.379          | 113  | 70493      | 47.688   | ug/l   | 0.00     |
| Spiked Amount 50.000          | Range 75 - 124 |      | Recovery = | 95.380%  |        |          |
| 50) Toluene-d8                | 8.647          | 98   | 266750     | 49.748   | ug/l   | 0.00     |
| Spiked Amount 50.000          | Range 92 - 112 |      | Recovery = | 99.500%  |        |          |
| 62) 4-Bromofluorobenzene      | 11.079         | 95   | 109316     | 51.877   | ug/l   | 0.00     |
| Spiked Amount 50.000          | Range 83 - 123 |      | Recovery = | 103.760% |        |          |
|                               |                |      |            |          |        |          |
| Target Compounds              |                |      |            |          | Qvalue |          |
| 5) Bromomethane               | 1.611          | 94   | 492        | 0.731    | ug/l   | 91       |
| 11) Tert butyl alcohol        | 2.953          | 59   | 327        | 0.792    | ug/l # | 78       |
| 13) Acrolein                  | 2.239          | 56   | 482        | 1.534    | ug/l # | 68       |
| 15) Acrylonitrile             | 3.075          | 53   | 426        | 0.578    | ug/l # | 81       |
| 16) Acetone                   | 2.386          | 43   | 716        | 1.039    | ug/l   | 96       |
| 17) Carbon Disulfide          | 2.508          | 76   | 2605       | 0.815    | ug/l # | 94       |
| 18) Methyl Acetate            | 2.709          | 43   | 542        | 0.209    | ug/l # | 88       |
| 20) Methylene Chloride        | 2.788          | 84   | 669        | 0.434    | ug/l # | 80       |
| 21) trans-1,2-Dichloroethene  | 3.087          | 96   | 397        | 0.278    | ug/l # | 60       |
| 25) 2-Butanone                | 4.574          | 43   | 384        | 0.370    | ug/l # | 51       |
| 38) Carbon Tetrachloride      | 5.550          | 117  | 13065      | 5.727    | ug/l # | 16       |
| 59) 2-Hexanone                | 9.439          | 43   | 491        | 0.311    | ug/l   | 89       |
| 68) m/p-Xylenes               | 10.299         | 106  | 787        | 0.252    | ug/l   | 95       |
| 76) 1,2,3-Trichloropropane    | 11.079         | 75   | 56739      | 26.717   | ug/l # | 38       |
| 81) trans-1,4-Dichloro-2-b... | 11.079         | 75   | 56739      | 74.621   | ug/l # | 5        |
| 82) 4-Chlorotoluene           | 11.451         | 91   | 1191       | 0.200    | ug/l   | 93       |
| 85) sec-Butylbenzene          | 11.890         | 105  | 2149       | 0.319    | ug/l   | 99       |
| 86) p-Isopropyltoluene        | 12.012         | 119  | 1834       | 0.316    | ug/l # | 85       |
| 87) 1,3-Dichlorobenzene       | 11.969         | 146  | 842        | 0.254    | ug/l   | 96       |
| 88) 1,4-Dichlorobenzene       | 11.969         | 146  | 842        | 0.246    | ug/l   | 97       |
| 89) n-Butylbenzene            | 12.335         | 91   | 2839       | 0.591    | ug/l   | 97       |
| 91) 1,2-Dichlorobenzene       | 12.335         | 146  | 692        | 0.213    | ug/l   | 90       |
| 93) 1,2,4-Trichlorobenzene    | 13.591         | 180  | 1275       | 0.671    | ug/l   | 99       |
| 94) Hexachlorobutadiene       | 13.725         | 225  | 1602       | 2.184    | ug/l   | 96       |
| 95) Naphthalene               | 13.774         | 128  | 6630       | 0.797    | ug/l   | 97       |
| 96) 1,2,3-Trichlorobenzene    | 13.963         | 180  | 1408       | 0.746    | ug/l   | 94       |
| -----                         |                |      |            |          |        |          |


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA\_X\Data\VX081823\  
Data File : VX037071.D  
Acq On : 18 Aug 2023 09:54  
Operator : JC/MD  
Sample : VX0818MBL01  
Misc : 5.00g/10mL/100uL/5.00mL/MSVOA\_X/MEOH  
ALS Vial : 3 Sample Multiplier: 1

Instrument :  
MSVOA\_X  
ClientSampleId :  
VX0818MBL01

Quant Time: Aug 19 05:12:40 2023  
Quant Method : Z:\voasrv\HPCHEM1\MSVOA\_X\Method\82X081723W.M  
Quant Title : SW846 8260  
QLast Update : Fri Aug 18 09:30:38 2023  
Response via : Initial Calibration

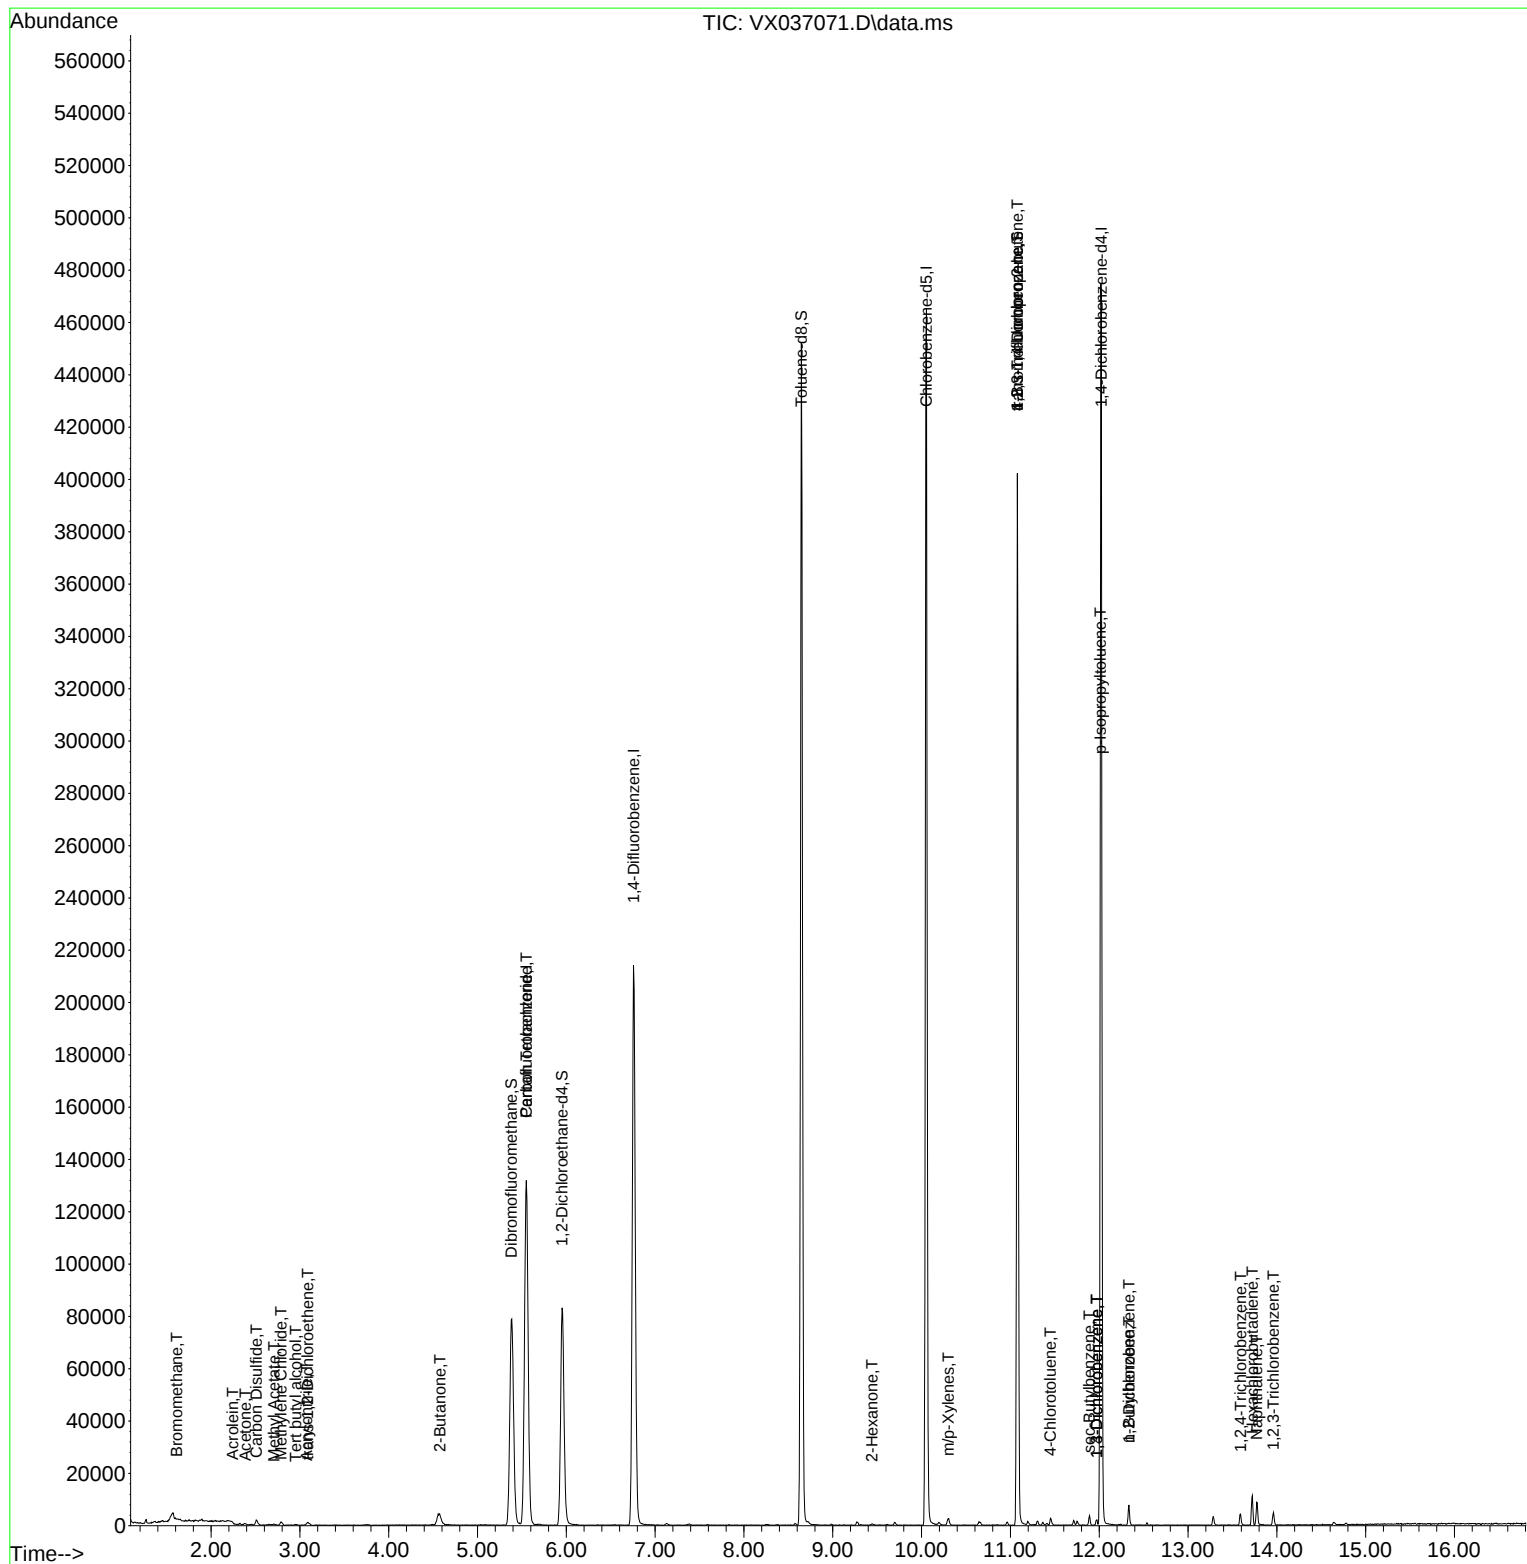



#1  
Pentafluorobenzene

Concen: 50.000 ug/l

RT: 5.550 min Scan# 71

Delta R.T. -0.000 min

Lab File: VX037071.D

Acq: 18 Aug 2023 09:54

Instrument :

MSVOA\_X

ClientSampleId :





VX0818MBL01

Tgt Ion:168 Resp: 122145

Ion Ratio Lower Upper

168 100

99 62.7 56.6 85.0

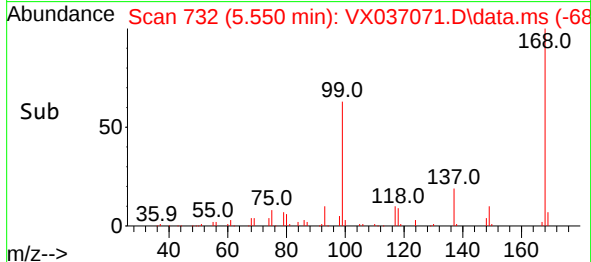

#5

Bromomethane

Concen: 0.731 ug/l

RT: 1.611 min Scan# 86

Delta R.T. 0.012 min

Lab File: VX037071.D




Acq: 18 Aug 2023 09:54


Tgt Ion: 94 Resp: 492

Ion Ratio Lower Upper

94 100

96 102.2 74.6 111.8

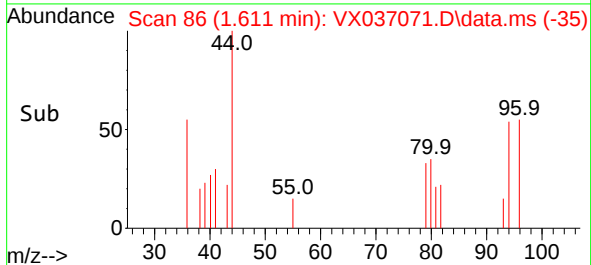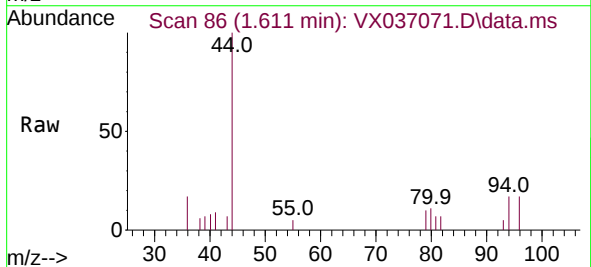

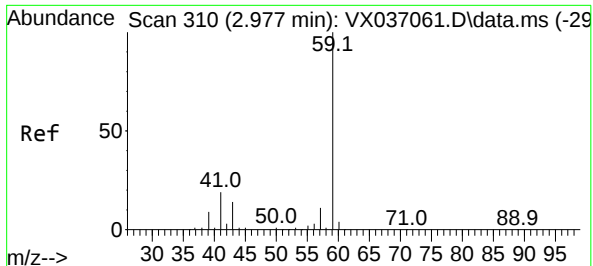

#11

Tert butyl alcohol

Concen: 0.792 ug/l

RT: 2.953 min Scan# 306

Delta R.T. -0.024 min

Lab File: VX037071.D

Acq: 18 Aug 2023 09:54

Instrument :

MSVOA\_X

ClientSampleId :





VX0818MBL01

Tgt Ion: 59 Resp: 327

Ion Ratio Lower Upper

59 100

57 0.0 6.0 9.0#

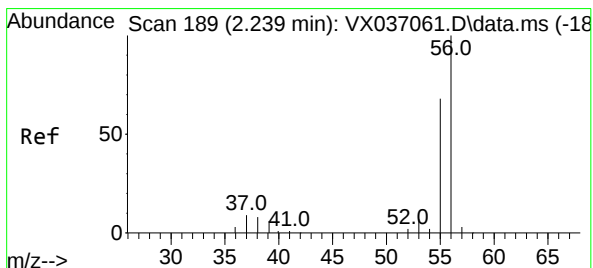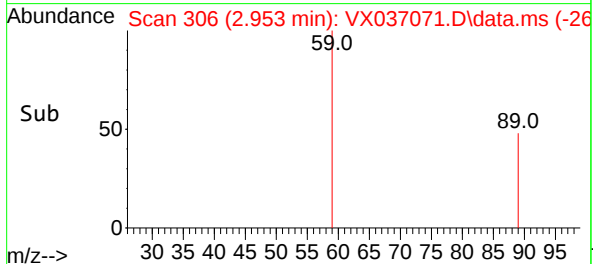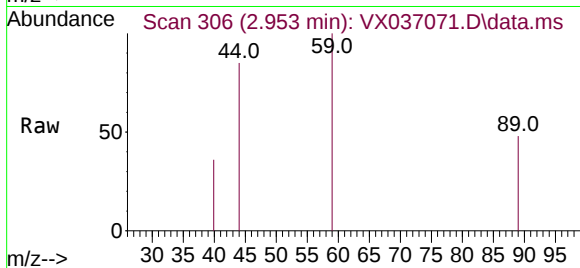

#13

Acrolein

Concen: 1.534 ug/l

RT: 2.239 min Scan# 189

Delta R.T. -0.000 min

Lab File: VX037071.D




Acq: 18 Aug 2023 09:54


Tgt Ion: 56 Resp: 482

Ion Ratio Lower Upper

56 100

55 98.3 57.1 85.7#

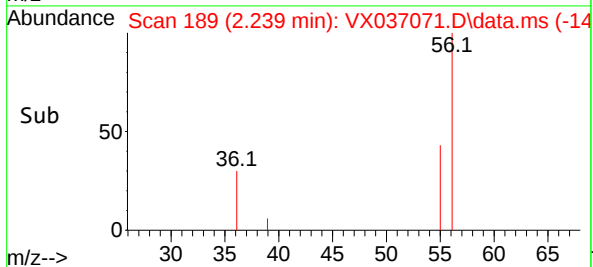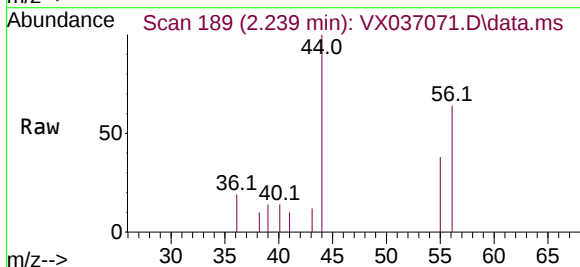



#15

Acrylonitrile

Concen: 0.578 ug/l

RT: 3.075 min Scan# 31

Delta R.T. 0.012 min

Lab File: VX037071.D

Acq: 18 Aug 2023 09:54

Instrument :

MSVOA\_X

ClientSampleId :

VX0818MBL01





Tgt Ion: 53 Resp: 426

Ion Ratio Lower Upper

53 100

52 71.6 66.0 99.0

51 17.4 29.8 44.6#

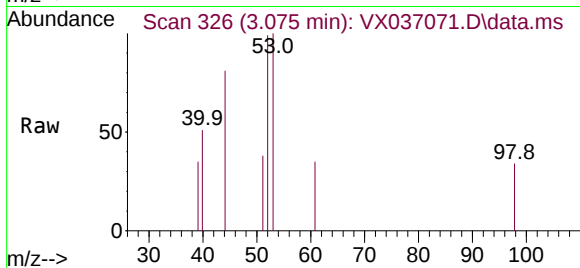

#16

Acetone

Concen: 1.039 ug/l

RT: 2.386 min Scan# 213

Delta R.T. -0.000 min

Lab File: VX037071.D




Acq: 18 Aug 2023 09:54


Tgt Ion: 43 Resp: 716

Ion Ratio Lower Upper

43 100

58 25.1 21.9 32.9


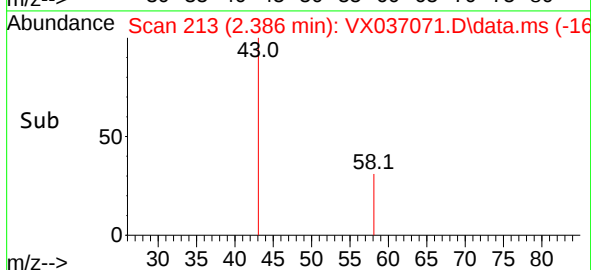

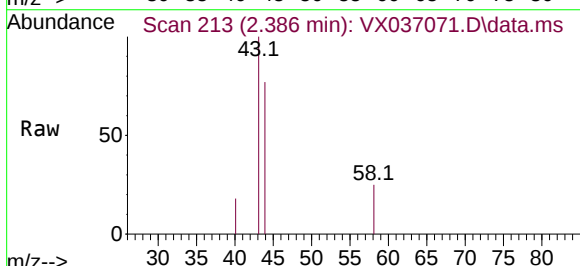


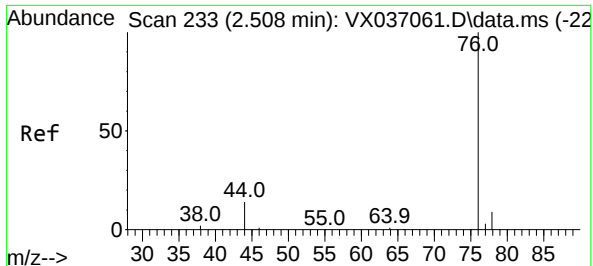

#17  
Carbon Disulfide  
Concen: 0.815 ug/l  
RT: 2.508 min Scan# 211  
Delta R.T. -0.000 min  
Lab File: VX037071.D  
Acq: 18 Aug 2023 09:54




Instrument :  
MSVOA\_X  
ClientSampleId :  
VX0818MBL01


Tgt Ion: 76 Resp: 2605  
Ion Ratio Lower Upper  
76 100  
78 10.8 7.0 10.6#

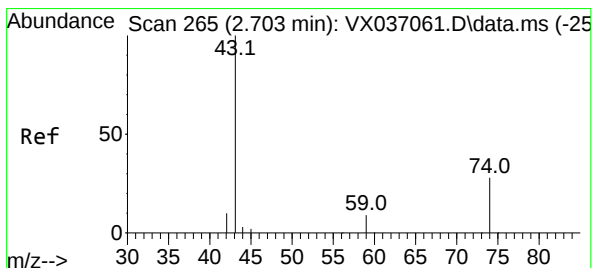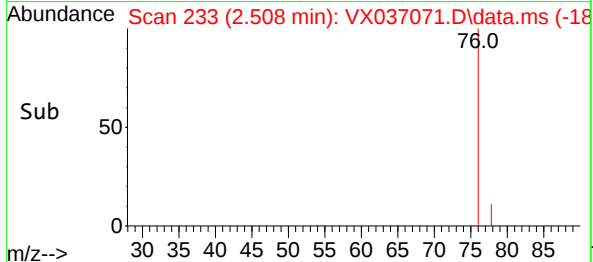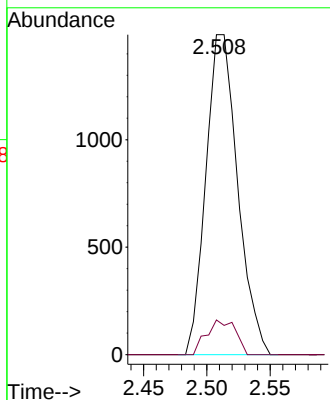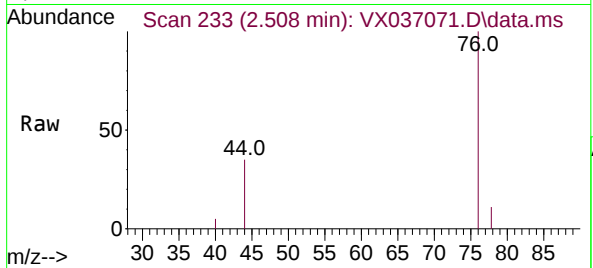

#18  
Methyl Acetate  
Concen: 0.209 ug/l  
RT: 2.709 min Scan# 266  
Delta R.T. 0.006 min  
Lab File: VX037071.D  
Acq: 18 Aug 2023 09:54

Tgt Ion: 43 Resp: 542  
Ion Ratio Lower Upper  
43 100  
74 16.6 17.8 26.8#


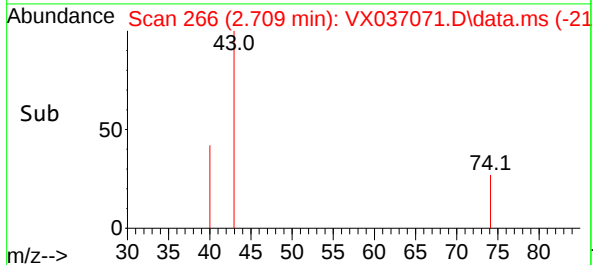
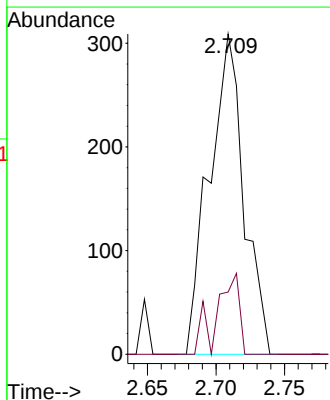
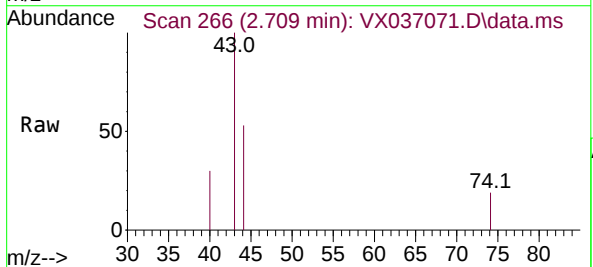




#20  
Methylene Chloride  
Concen: 0.434 ug/l  
RT: 2.788 min Scan# 21  
Delta R.T. -0.000 min  
Lab File: VX037071.D  
Acq: 18 Aug 2023 09:54




Instrument :  
MSVOA\_X  
ClientSampleId :  
VX0818MBL01


|          |       |       |        |
|----------|-------|-------|--------|
| Tgt Ion: | 84    | Resp: | 669    |
| Ion      | Ratio | Lower | Upper  |
| 84       | 100   |       |        |
| 49       | 97.9  | 103.6 | 155.4# |
| 51       | 28.9  | 33.8  | 50.6#  |
| 86       | 64.1  | 49.4  | 74.0   |

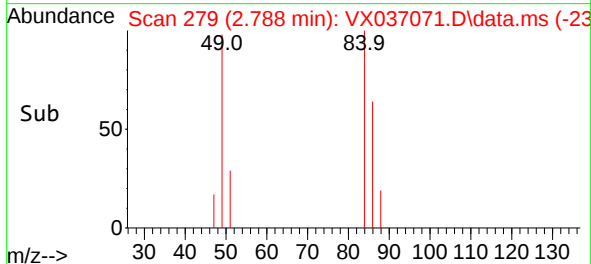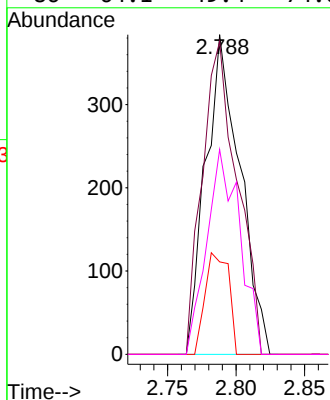

#21  
trans-1,2-Dichloroethene  
Concen: 0.278 ug/l  
RT: 3.087 min Scan# 328  
Delta R.T. -0.000 min  
Lab File: VX037071.D  
Acq: 18 Aug 2023 09:54

|          |       |       |        |
|----------|-------|-------|--------|
| Tgt Ion: | 96    | Resp: | 397    |
| Ion      | Ratio | Lower | Upper  |
| 96       | 100   |       |        |
| 61       | 95.2  | 119.2 | 178.8# |
| 98       | 34.7  | 48.7  | 73.1#  |


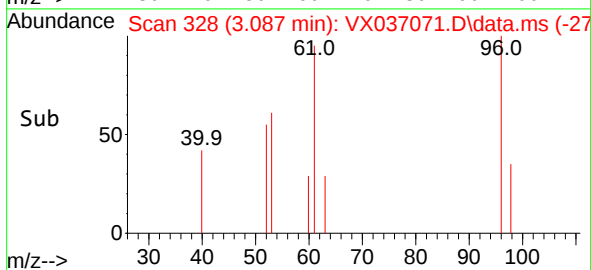
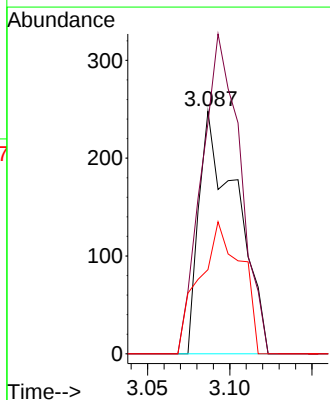
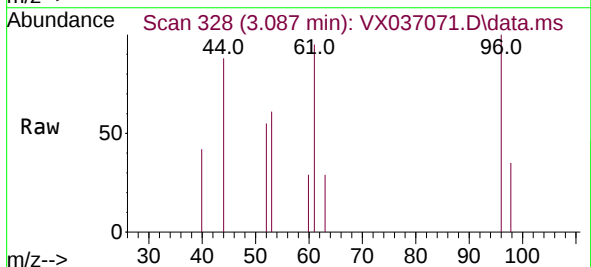




#25  
2-Butanone  
Concen: 0.370 ug/l  
RT: 4.574 min Scan# 51  
Delta R.T. 0.018 min  
Lab File: VX037071.D  
Acq: 18 Aug 2023 09:54




Instrument :  
MSVOA\_X  
ClientSampleId :  
VX0818MBL01


Tgt Ion: 43 Resp: 384  
Ion Ratio Lower Upper  
43 100  
72 0.0 19.4 29.2#

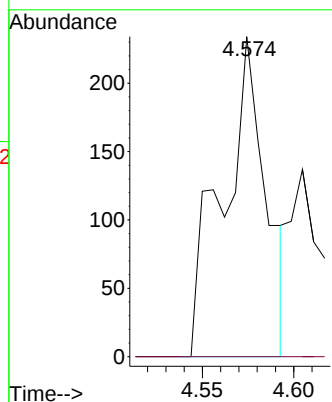

#33  
1,2-Dichloroethane-d4  
Concen: 47.895 ug/l  
RT: 5.952 min Scan# 798  
Delta R.T. -0.006 min  
Lab File: VX037071.D  
Acq: 18 Aug 2023 09:54

Tgt Ion: 65 Resp: 84340  
Ion Ratio Lower Upper  
65 100  
67 50.1 0.0 100.2


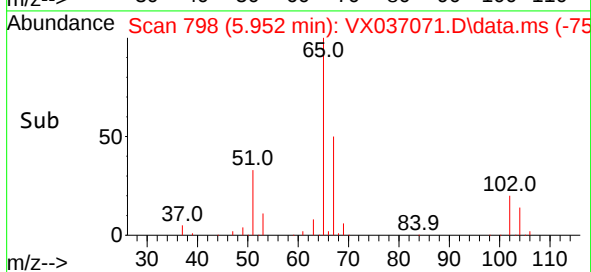
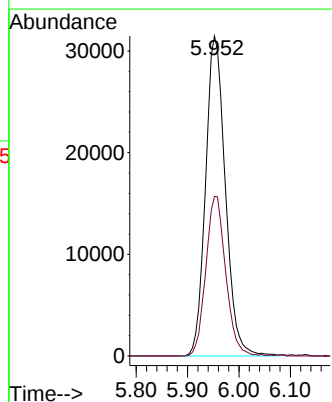





#34  
1,4-Difluorobenzene  
Concen: 50.000 ug/l  
RT: 6.757 min Scan# 911  
Delta R.T. -0.006 min  
Lab File: VX037071.D  
Acq: 18 Aug 2023 09:54




Instrument :  
MSVOA\_X  
ClientSampleId :  
VX0818MBL01


Tgt Ion:114 Resp: 223202  
Ion Ratio Lower Upper  
114 100  
63 20.7 0.0 45.0  
88 17.2 0.0 36.6

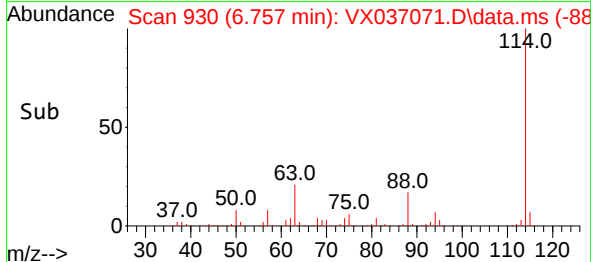

#35  
Dibromofluoromethane  
Concen: 47.688 ug/l  
RT: 5.379 min Scan# 704  
Delta R.T. -0.006 min  
Lab File: VX037071.D  
Acq: 18 Aug 2023 09:54


Tgt Ion:113 Resp: 70493  
Ion Ratio Lower Upper  
113 100  
111 103.5 82.9 124.3  
192 18.6 13.3 19.9

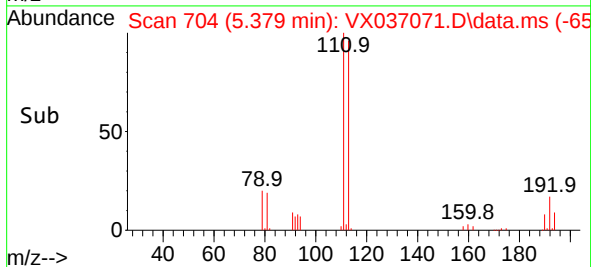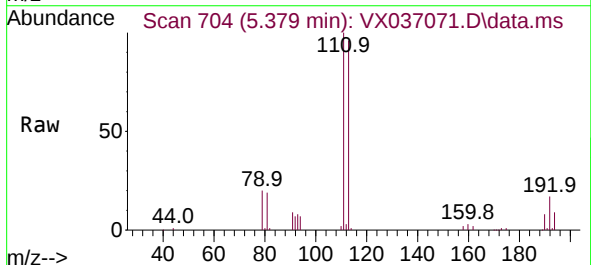






#38  
Carbon Tetrachloride  
Concen: 5.727 ug/l  
RT: 5.550 min Scan# 71  
Delta R.T. -0.122 min  
Lab File: VX037071.D  
Acq: 18 Aug 2023 09:54

Instrument :  
MSVOA\_X  
ClientSampleId :  
VX0818MBL01







Tgt Ion:117 Resp: 13065  
Ion Ratio Lower Upper  
117 100  
119 6.8 78.2 117.2#  
121 0.0 24.4 36.6#

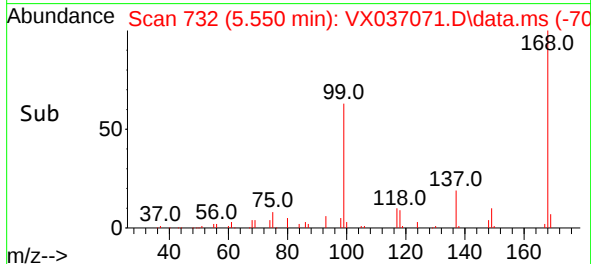

#50  
Toluene-d8  
Concen: 49.748 ug/l  
RT: 8.647 min Scan# 1240  
Delta R.T. -0.000 min  
Lab File: VX037071.D  
Acq: 18 Aug 2023 09:54

Tgt Ion: 98 Resp: 266750  
Ion Ratio Lower Upper  
98 100  
100 66.7 53.1 79.7


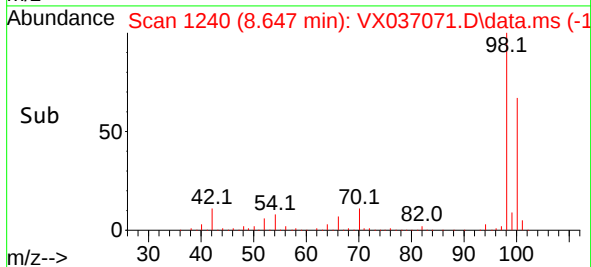

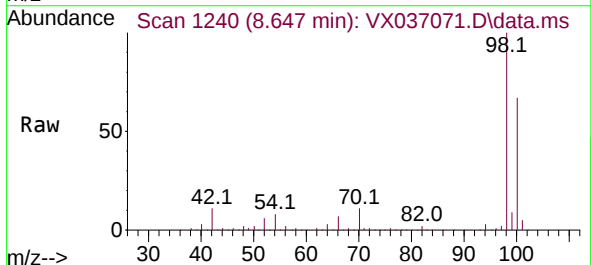


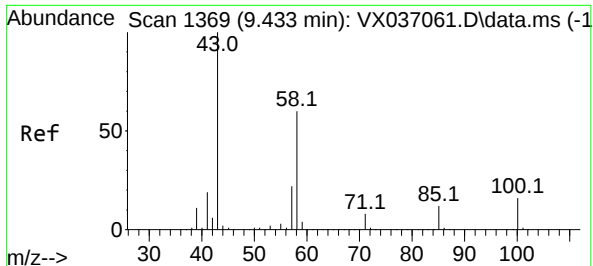

#59  
2-Hexanone  
Concen: 0.311 ug/l  
RT: 9.439 min Scan# 11  
Delta R.T. 0.006 min  
Lab File: VX037071.D  
Acq: 18 Aug 2023 09:54




Instrument :  
MSVOA\_X  
ClientSampleId :  
VX0818MBL01


Tgt Ion: 43 Resp: 491  
Ion Ratio Lower Upper  
43 100  
58 60.3 26.2 78.5

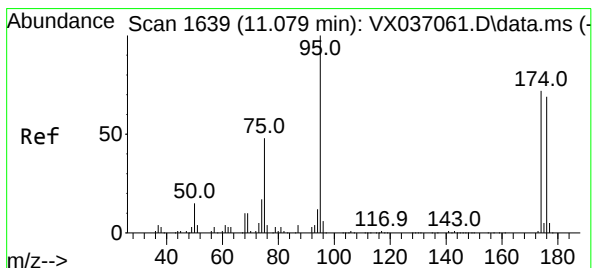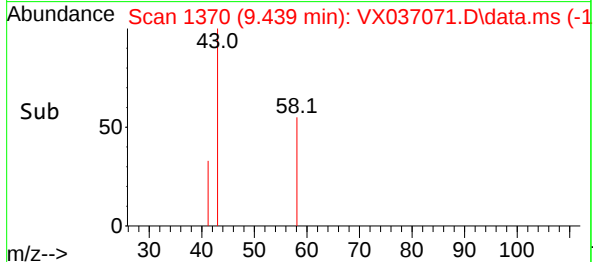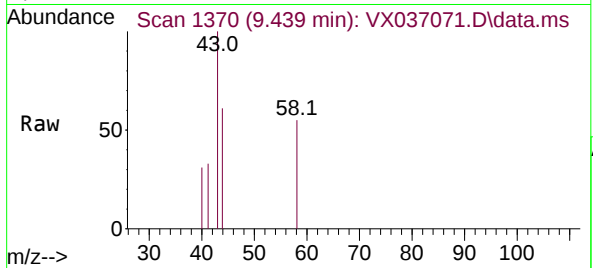

#62  
4-Bromofluorobenzene  
Concen: 51.877 ug/l  
RT: 11.079 min Scan# 1639  
Delta R.T. -0.000 min  
Lab File: VX037071.D  
Acq: 18 Aug 2023 09:54

Tgt Ion: 95 Resp: 109316  
Ion Ratio Lower Upper  
95 100  
174 71.9 0.0 135.6  
176 71.3 0.0 131.0


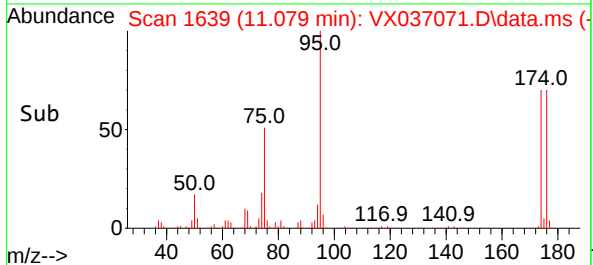

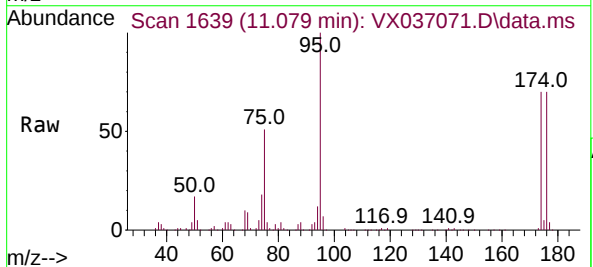




#63  
Chlorobenzene-d5  
Concen: 50.000 ug/l  
RT: 10.055 min Scan# 1471  
Delta R.T. -0.000 min  
Lab File: VX037071.D  
Acq: 18 Aug 2023 09:54




Instrument :  
MSVOA\_X  
ClientSampleId :  
VX0818MBL01


Tgt Ion:117 Resp: 217130  
Ion Ratio Lower Upper  
117 100  
82 55.7 46.2 69.4  
119 32.3 25.5 38.3

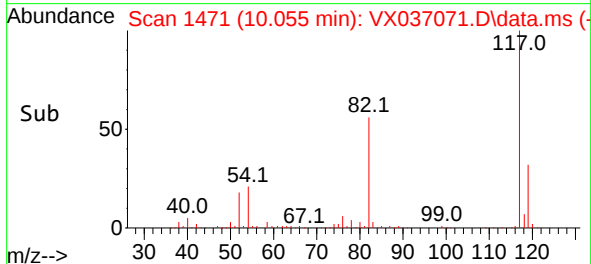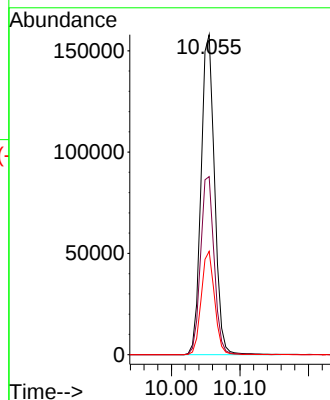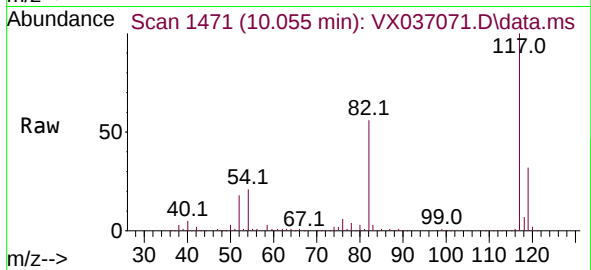

#68  
m/p-Xylenes  
Concen: 0.252 ug/l  
RT: 10.299 min Scan# 1511  
Delta R.T. -0.000 min  
Lab File: VX037071.D  
Acq: 18 Aug 2023 09:54

Tgt Ion:106 Resp: 787  
Ion Ratio Lower Upper  
106 100  
91 199.5 165.5 248.3


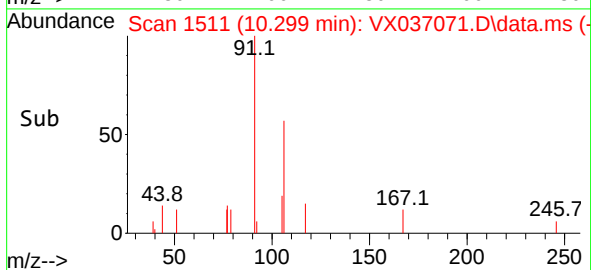
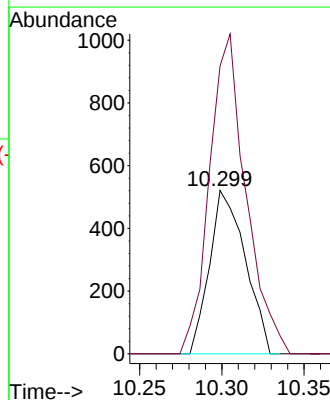
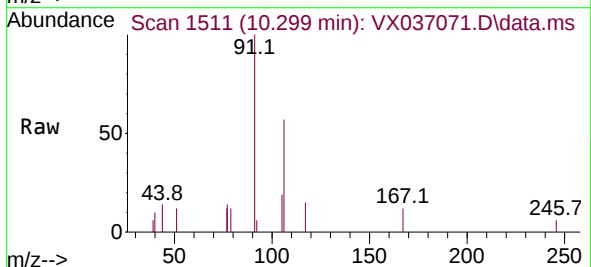




#72  
1,4-Dichlorobenzene-d4  
Concen: 50.000 ug/l  
RT: 12.024 min Scan# 11  
Delta R.T. -0.000 min  
Lab File: VX037071.D  
Acq: 18 Aug 2023 09:54




Instrument :  
MSVOA\_X  
ClientSampleId :  
VX0818MBL01


Tgt Ion:152 Resp: 99721  
Ion Ratio Lower Upper  
152 100  
115 64.0 43.3 129.9  
150 157.0 0.0 345.0

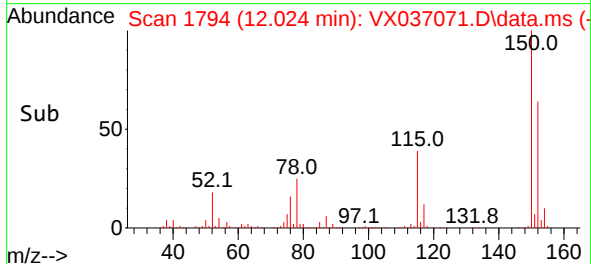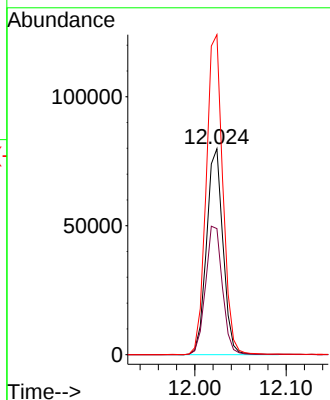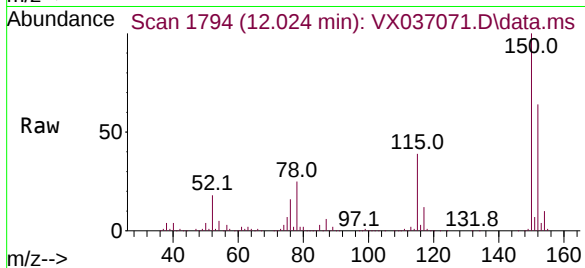

#76  
1,2,3-Trichloropropane  
Concen: 26.717 ug/l  
RT: 11.079 min Scan# 1639  
Delta R.T. -0.159 min  
Lab File: VX037071.D  
Acq: 18 Aug 2023 09:54

Tgt Ion: 75 Resp: 56739  
Ion Ratio Lower Upper  
75 100  
77 0.9 19.1 57.5#


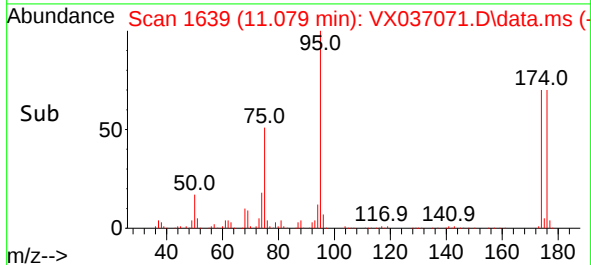
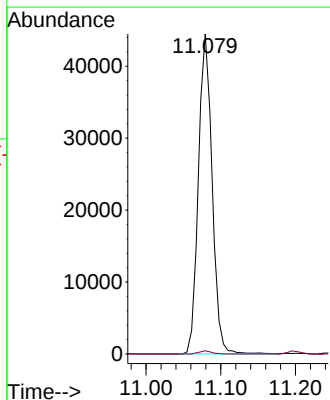
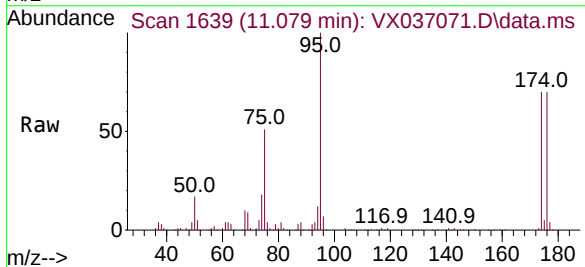




#81  
trans-1,4-Dichloro-2-butene  
Concen: 74.621 ug/l  
RT: 11.079 min Scan# 1639  
Delta R.T. 0.061 min  
Lab File: VX037071.D  
Acq: 18 Aug 2023 09:54




Instrument :  
MSVOA\_X  
ClientSampleId :  
VX0818MBL01


Tgt Ion: 75 Resp: 56739  
Ion Ratio Lower Upper  
75 100  
53 0.0 90.5 135.7#  
89 0.1 36.9 55.3#

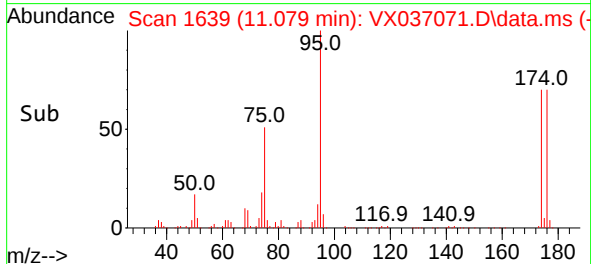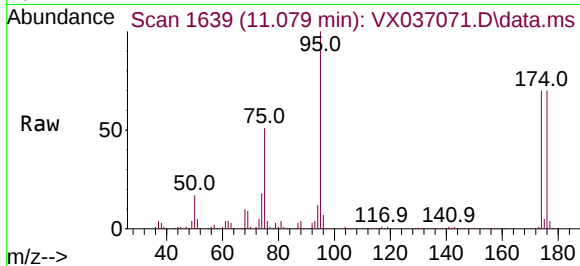

#82  
4-Chlorotoluene  
Concen: 0.200 ug/l  
RT: 11.451 min Scan# 1700  
Delta R.T. -0.000 min  
Lab File: VX037071.D  
Acq: 18 Aug 2023 09:54

Tgt Ion: 91 Resp: 1191  
Ion Ratio Lower Upper  
91 100  
126 24.9 14.2 42.6


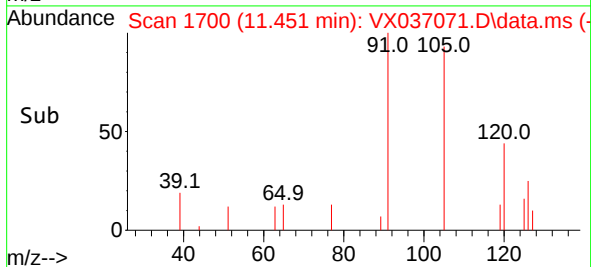

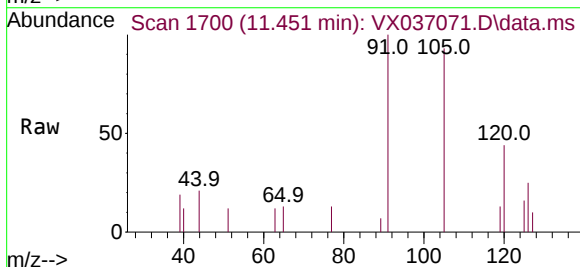




#85  
 sec-Butylbenzene  
 Concen: 0.319 ug/l  
 RT: 11.890 min Scan# 1772  
 Delta R.T. -0.000 min  
 Lab File: VX037071.D  
 Acq: 18 Aug 2023 09:54




Instrument :  
 MSVOA\_X  
 ClientSampleId :  
 VX0818MBL01


Tgt Ion:105 Resp: 2149  
 Ion Ratio Lower Upper  
 105 100  
 134 20.0 9.8 29.4

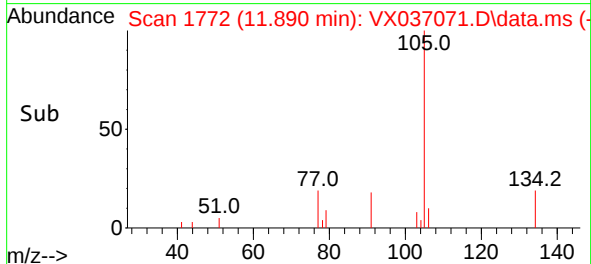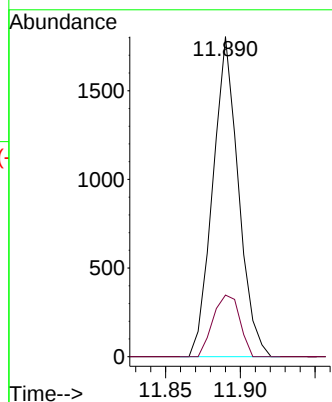

#86  
 p-Isopropyltoluene  
 Concen: 0.316 ug/l  
 RT: 12.012 min Scan# 1792  
 Delta R.T. 0.006 min  
 Lab File: VX037071.D  
 Acq: 18 Aug 2023 09:54

Tgt Ion:119 Resp: 1834  
 Ion Ratio Lower Upper  
 119 100  
 134 26.4 12.8 38.3  
 91 40.9 13.1 39.3#

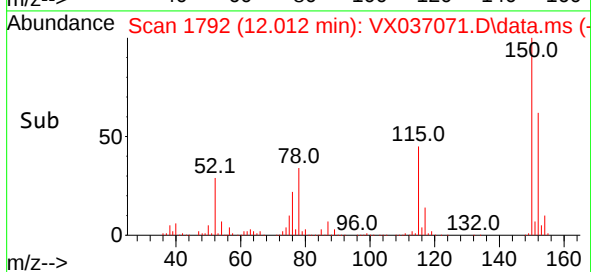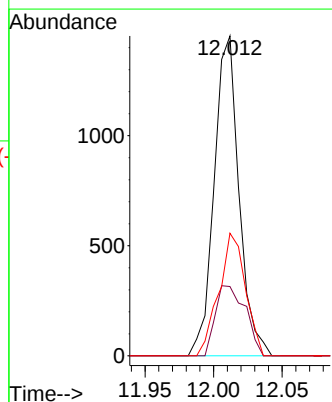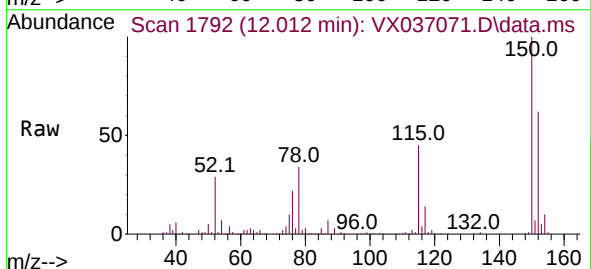



#87

1,3-Dichlorobenzene

Concen: 0.254 ug/l

RT: 11.969 min Scan# 1785

Delta R.T. -0.000 min

Lab File: VX037071.D

Acq: 18 Aug 2023 09:54

Instrument :

MSVOA\_X

ClientSampleId :

VX0818MBL01





Tgt Ion:146 Resp: 842

Ion Ratio Lower Upper

146 100

111 41.1 22.1 66.1

148 60.5 31.8 95.3

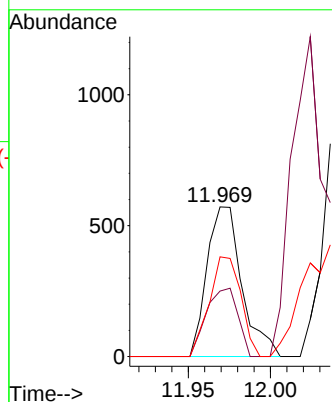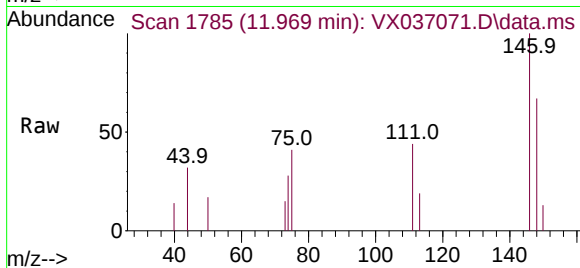

#88

1,4-Dichlorobenzene

Concen: 0.246 ug/l

RT: 11.969 min Scan# 1785

Delta R.T. -0.073 min

Lab File: VX037071.D

Acq: 18 Aug 2023 09:54




Tgt Ion:146 Resp: 842


Ion Ratio Lower Upper

146 100

111 41.1 21.3 63.7

148 60.5 31.8 95.4

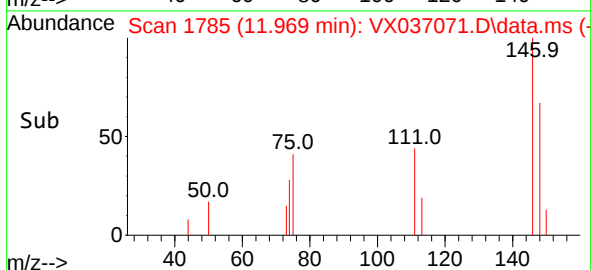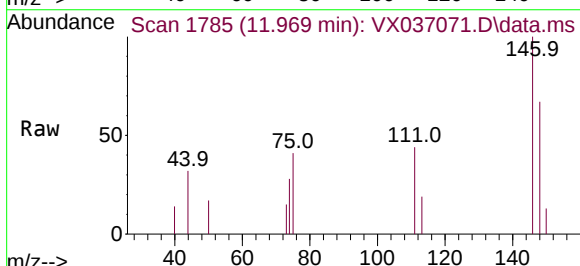



#89

n-Butylbenzene

Concen: 0.591 ug/l

RT: 12.335 min Scan# 1845

Delta R.T. 0.006 min

Lab File: VX037071.D

Acq: 18 Aug 2023 09:54

Instrument :

MSVOA\_X

ClientSampleId :

VX0818MBL01





Tgt Ion: 91 Resp: 2839

Ion Ratio Lower Upper

91 100

92 51.3 27.4 82.0

134 25.3 12.6 37.8

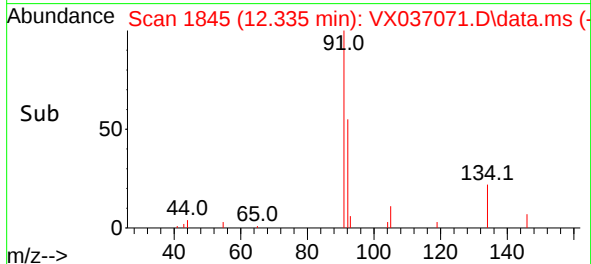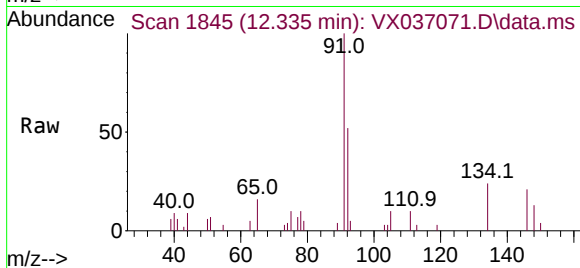

#91

1,2-Dichlorobenzene

Concen: 0.213 ug/l

RT: 12.335 min Scan# 1845

Delta R.T. -0.000 min

Lab File: VX037071.D

Acq: 18 Aug 2023 09:54




Tgt Ion:146 Resp: 692


Ion Ratio Lower Upper

146 100

111 34.4 22.4 67.0

148 58.8 31.6 95.0

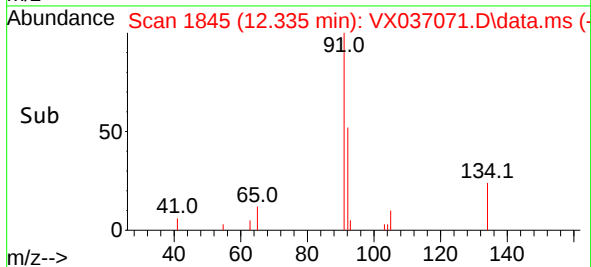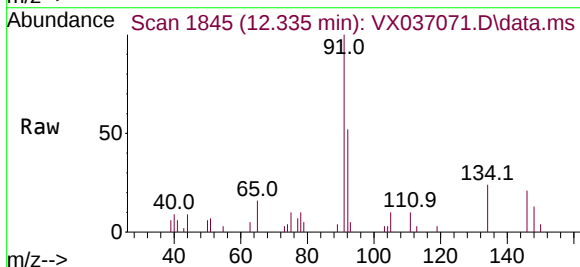



#93

1,2,4-Trichlorobenzene

Concen: 0.671 ug/l

RT: 13.591 min Scan# 2050

Delta R.T. 0.006 min

Lab File: VX037071.D

Acq: 18 Aug 2023 09:54

Instrument :

MSVOA\_X

ClientSampleId :

VX0818MBL01





Tgt Ion:180 Resp: 1275

Ion Ratio Lower Upper

180 100

182 96.7 48.3 144.8

145 36.9 18.0 54.0

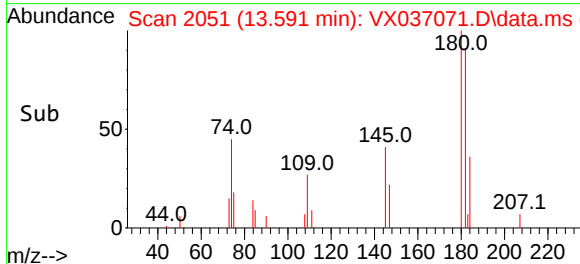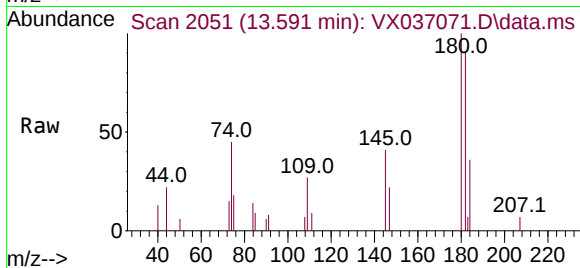

#94

Hexachlorobutadiene

Concen: 2.184 ug/l

RT: 13.725 min Scan# 2073

Delta R.T. -0.000 min

Lab File: VX037071.D

Acq: 18 Aug 2023 09:54




Tgt Ion:225 Resp: 1602


Ion Ratio Lower Upper

225 100

223 66.8 31.1 93.2

227 63.1 32.5 97.5

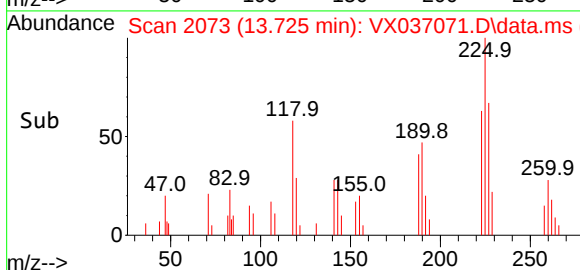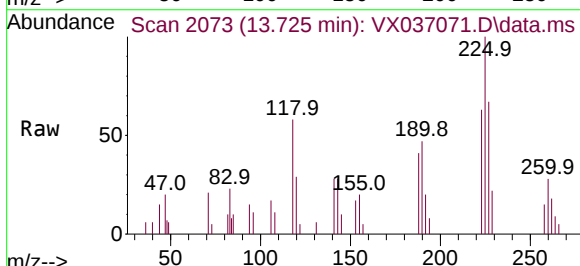



#95

Naphthalene

Concen: 0.797 ug/l

RT: 13.774 min Scan# 2081

Delta R.T. -0.000 min

Lab File: VX037071.D

Acq: 18 Aug 2023 09:54

Instrument :

MSVOA\_X

ClientSampleId :

VX0818MBL01





Tgt Ion:128 Resp: 6630

Ion Ratio Lower Upper

128 100

127 10.8 10.3 15.5

129 11.2 8.8 13.2

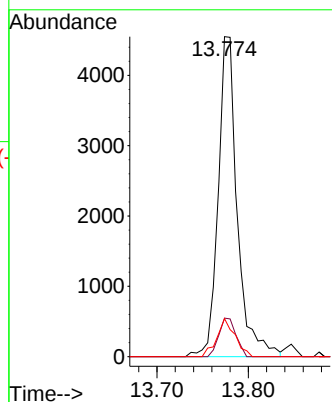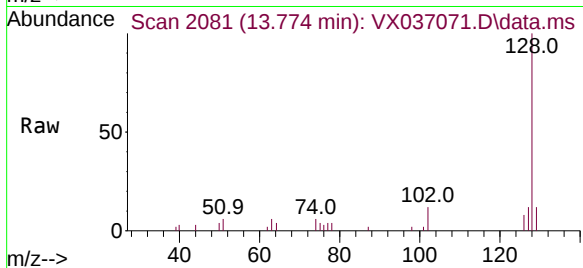

#96

1,2,3-Trichlorobenzene

Concen: 0.746 ug/l

RT: 13.963 min Scan# 2112

Delta R.T. -0.000 min

Lab File: VX037071.D

Acq: 18 Aug 2023 09:54

Tgt Ion:180 Resp: 1408

Ion Ratio Lower Upper

180 100

182 101.3 46.9 140.6

145 35.4 17.8 53.5

